

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 06:42
 Operator : AR\AJ
 Sample : M3318-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 07:48:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.640	5.570	8555498	22033793	20.683	21.701
28)	SA Decachlor...	10.408	11.491	10586037	18290471	18.420	18.851
Target Compounds							
8)	B Heptachlo...	0.000	8.037	0	2613731	N.D.	2.261 #
10)	B gamma-Chl...	0.000	8.324f	0	338359	N.D.	0.295 #
12)	B 4,4'-DDE	0.000	8.567	0	294700	N.D.	0.279 #
13)	MA Dieldrin	7.779	0.000	833813	0	1.612	N.D. #
14)	MA Endrin	8.084f	8.964	658473	1427064	1.366	1.572
15)	B Endosulfa...	0.000	9.218f	0	382081	N.D.	0.417 #
22)	Mirex	0.000	10.564f	0	215368	N.D.	0.272 #
25)	Chlordane-3	0.000	8.324f	0	338359	N.D.	2.071 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 06:42
Operator : AR\AJ
Sample : M3318-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 07:48:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

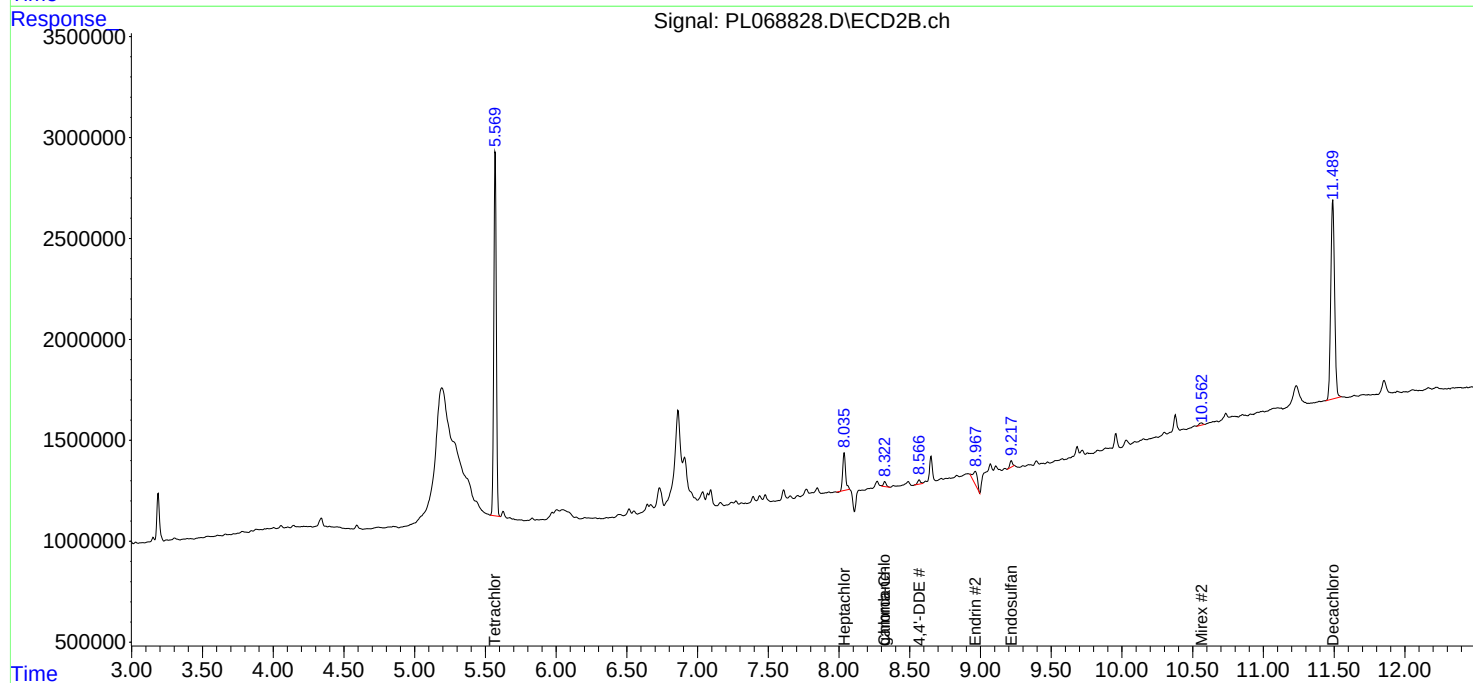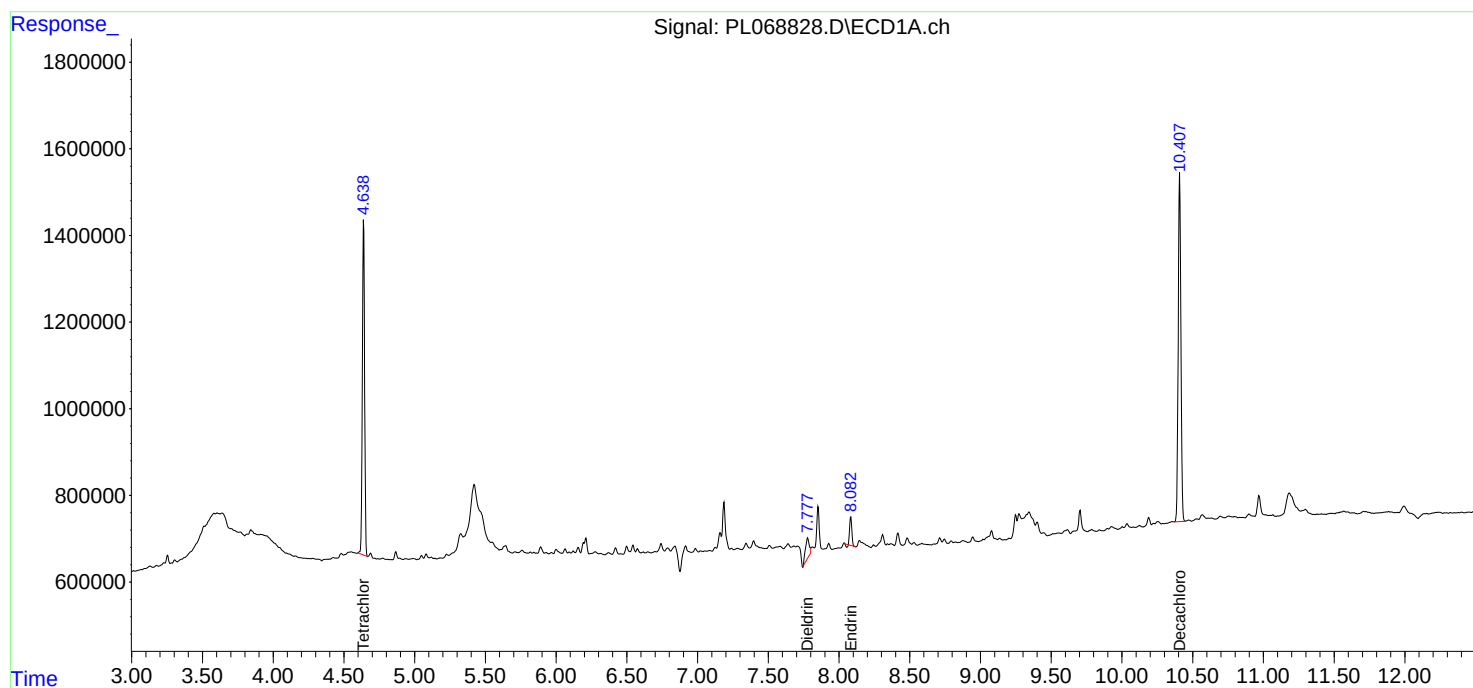


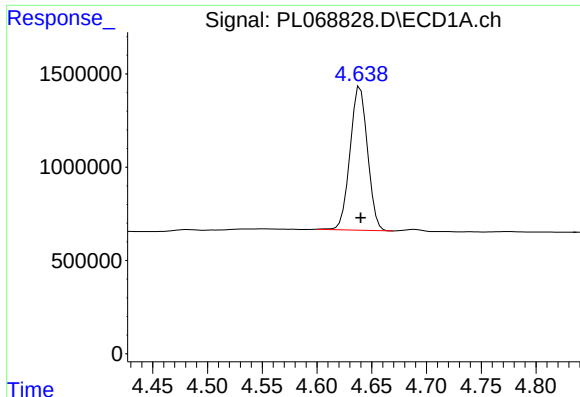

#1 Tetrachloro-m-xylene


R.T.: 4.640 min
Delta R.T.: 0.000 min
Response: 8555498
Conc: 20.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

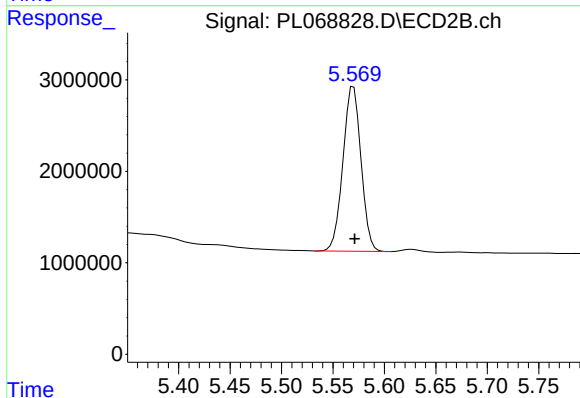


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 22033793
Conc: 21.70 ng/ml

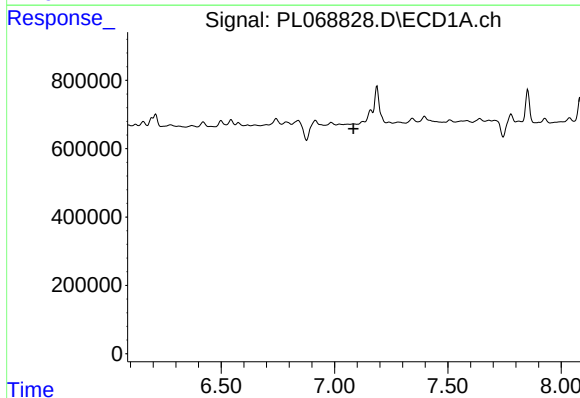


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

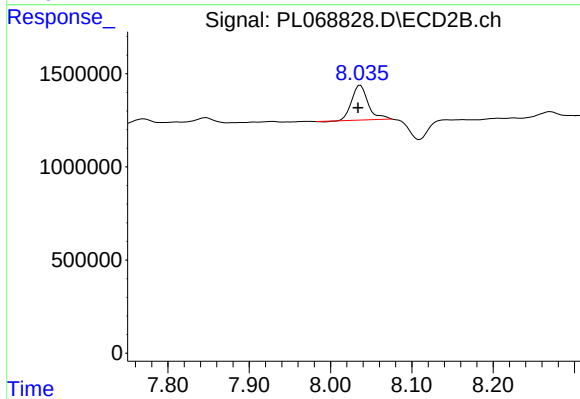

#8 Heptachlor epoxide


R.T.: 8.037 min
Delta R.T.: 0.003 min
Response: 2613731
Conc: 2.26 ng/ml

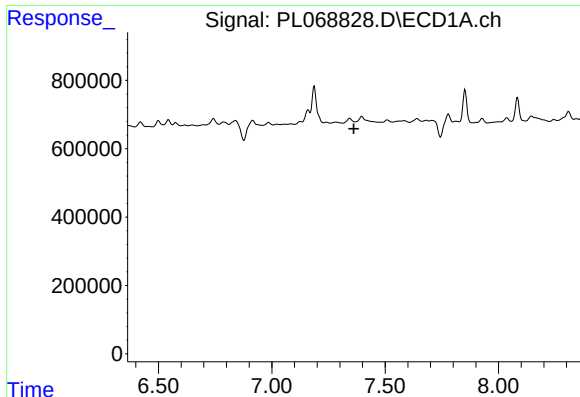

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

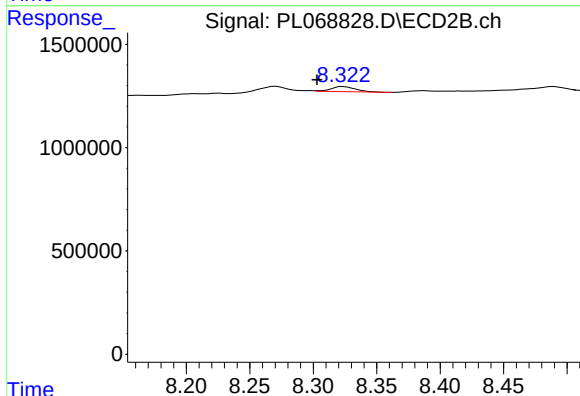


#10 gamma-Chlordane

R.T.: 8.324 min
Delta R.T.: 0.021 min
Response: 338359
Conc: 0.30 ng/ml

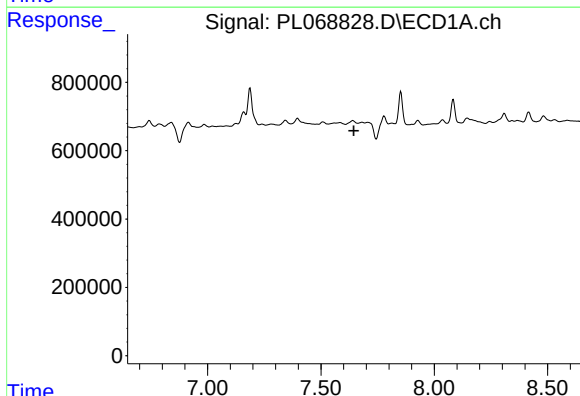


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

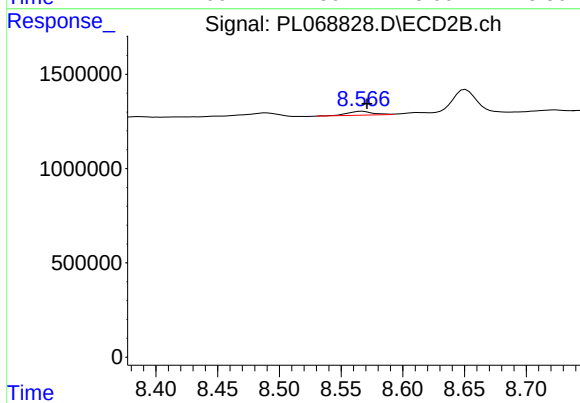

#12 4,4'-DDE


R.T.: 8.567 min
Delta R.T.: -0.004 min
Response: 294700
Conc: 0.28 ng/ml

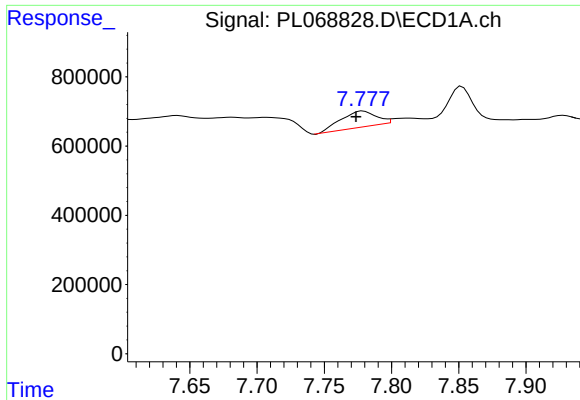

#13 Dieldrin


R.T.: 7.779 min
Delta R.T.: 0.005 min
Response: 833813
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

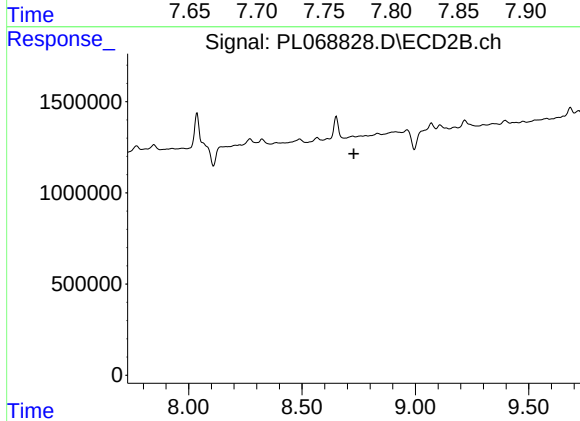


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.729 min
Response: 0
Conc: N.D.

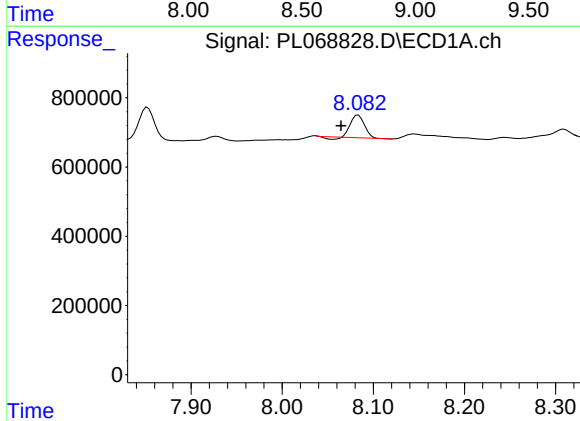


#14 Endrin

R.T.: 8.084 min
Delta R.T.: 0.019 min
Response: 658473
Conc: 1.37 ng/ml

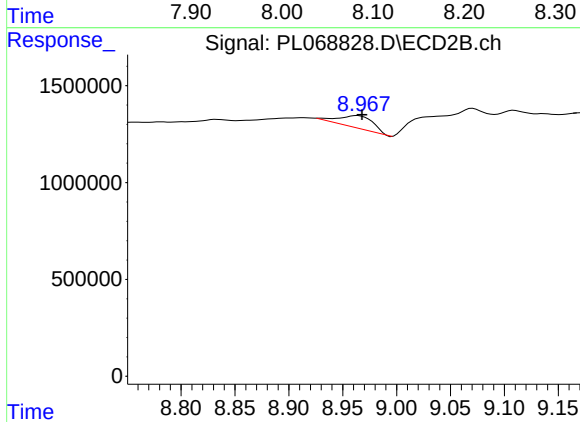

#14 Endrin


R.T.: 8.964 min
Delta R.T.: -0.004 min
Response: 1427064
Conc: 1.57 ng/ml

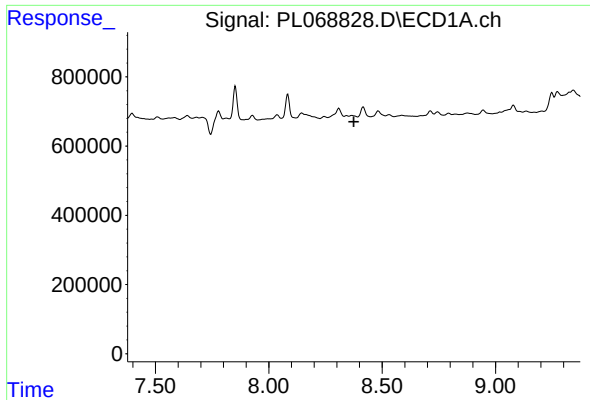

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

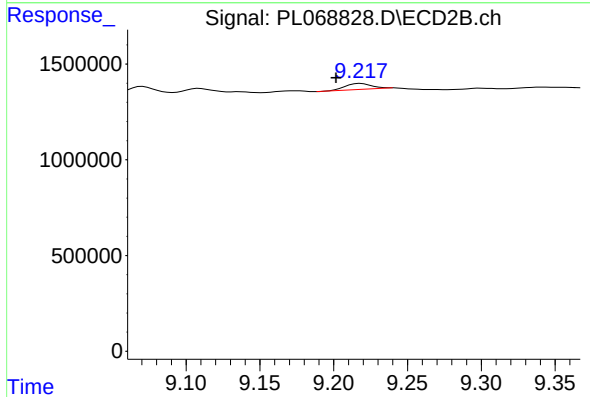


#15 Endosulfan II

R.T.: 9.218 min
Delta R.T.: 0.016 min
Response: 382081
Conc: 0.42 ng/ml

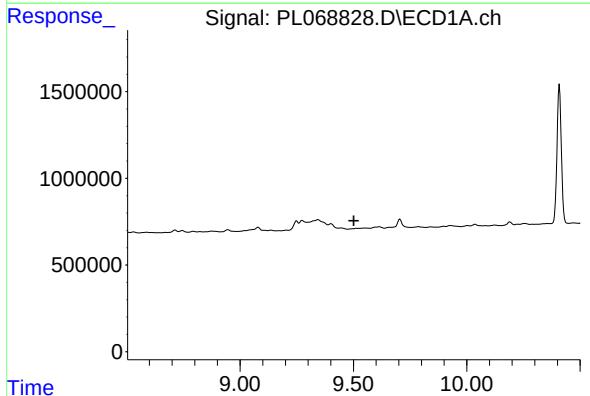


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

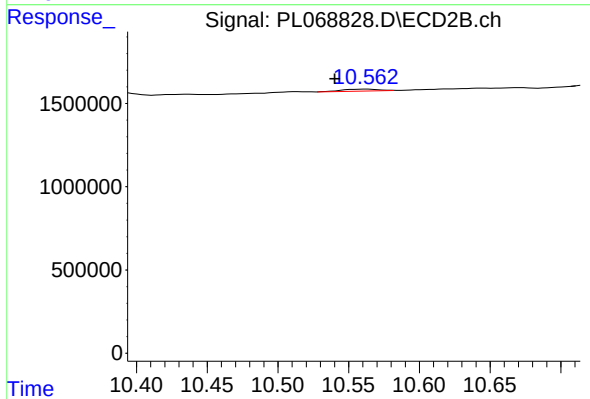

#22 Mirex


R.T.: 10.564 min
Delta R.T.: 0.023 min
Response: 215368
Conc: 0.27 ng/ml

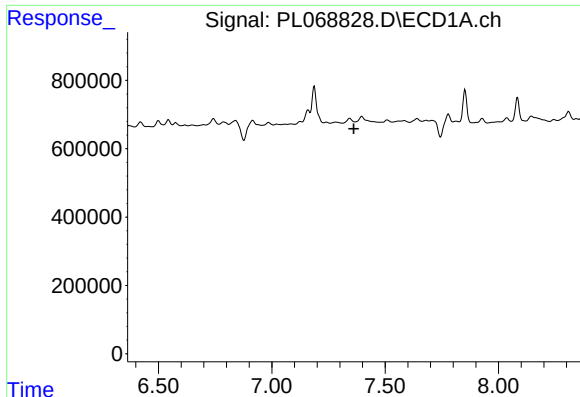

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

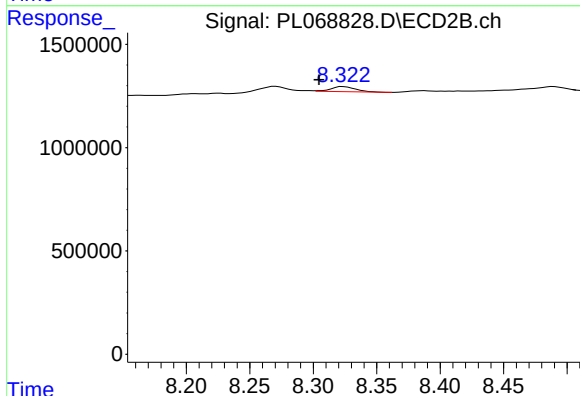


#25 Chlordane-3

R.T.: 8.324 min
Delta R.T.: 0.019 min
Response: 338359
Conc: 2.07 ng/ml

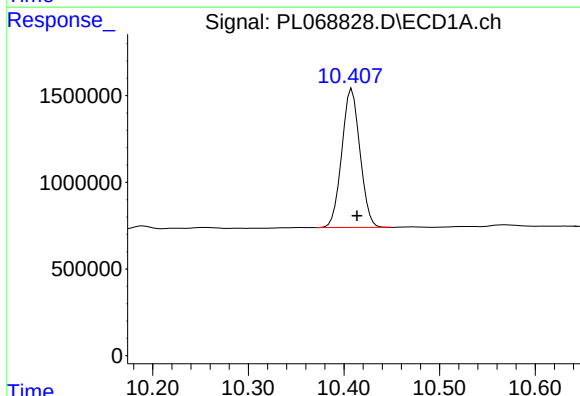

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: -0.005 min
Response: 10586037
Conc: 18.42 ng/ml

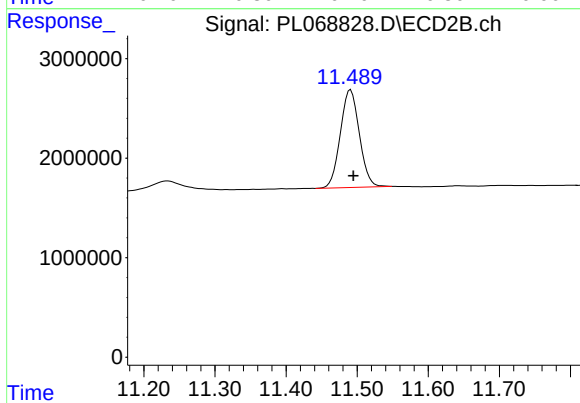

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.004 min
Response: 18290471
Conc: 18.85 ng/ml