

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 06:59
 Operator : AR\AJ
 Sample : M3318-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 07:49:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.570	8825310	22472192	21.336	22.133
28)	SA Decachlor...	10.408	11.490	10323678	17433776	17.964	17.968
Target Compounds							
4)	MA Heptachlor	6.210f	0.000	496679	0	0.846	N.D. #
8)	B Heptachlo...	0.000	8.032	0	198305	N.D.	0.172 #
10)	B gamma-Chl...	0.000	8.323f	0	783599	N.D.	0.684 #
12)	B 4,4'-DDE	0.000	8.569	0	280069	N.D.	0.265 #
15)	B Endosulfa...	0.000	9.216	0	349776	N.D.	0.381 #
20)	A Methoxychlor	9.079	0.000	579638	0	1.852	N.D. #
23)	Chlordane-1	0.000	6.973f	0	789543	N.D.	18.723 #
25)	Chlordane-3	0.000	8.323f	0	783599	N.D.	4.797 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 06:59
Operator : AR\AJ
Sample : M3318-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 07:49:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

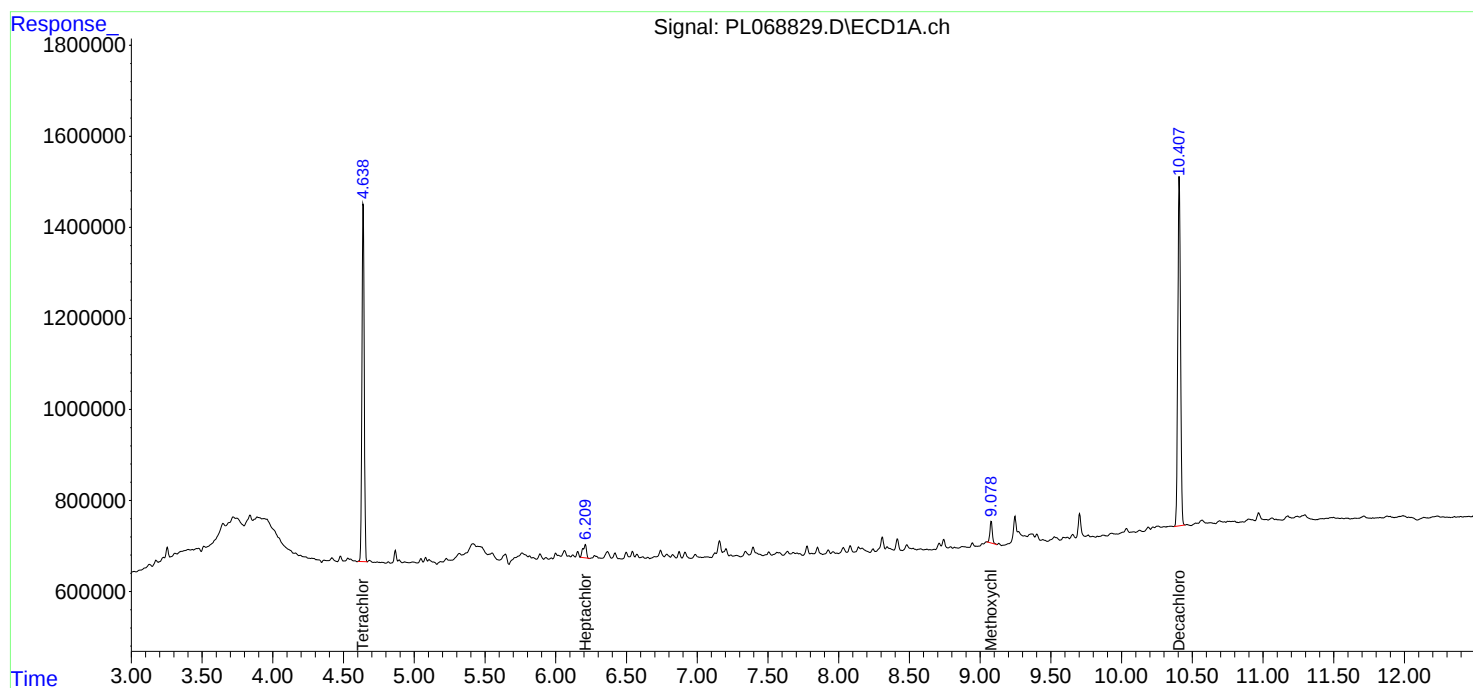


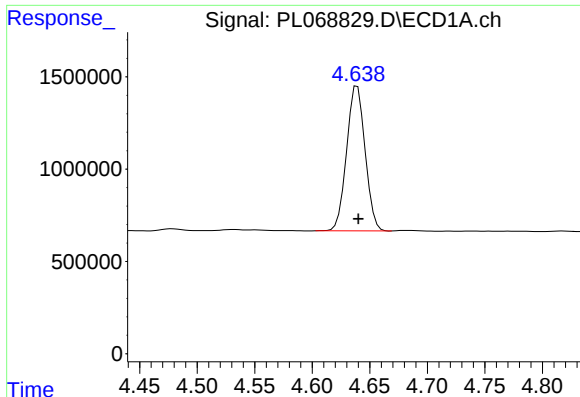

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 8825310
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

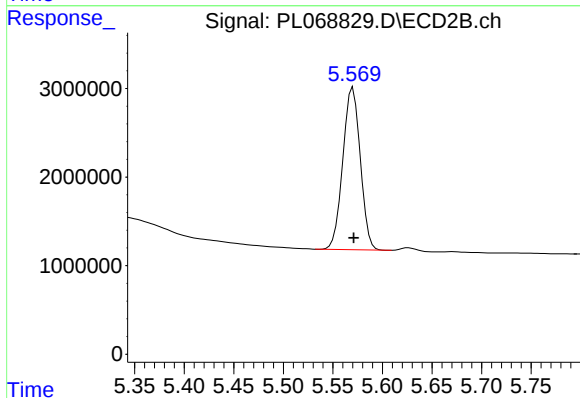


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 22472192
Conc: 22.13 ng/ml

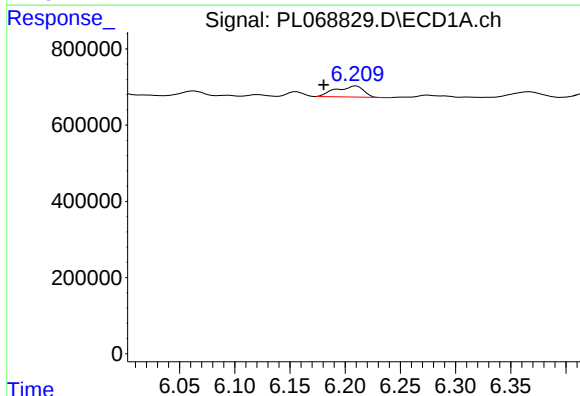


#4 Heptachlor

R.T.: 6.210 min
Delta R.T.: 0.030 min
Response: 496679
Conc: 0.85 ng/ml

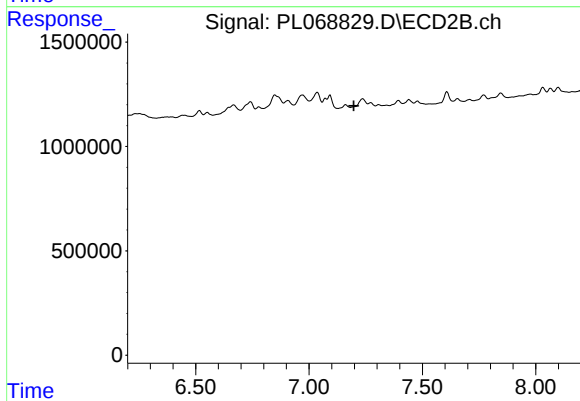

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.197 min
Response: 0
Conc: N.D.

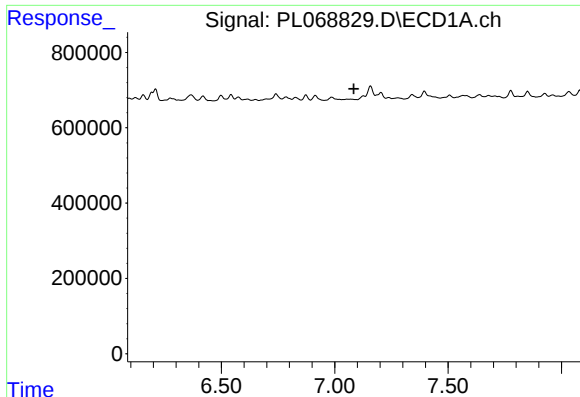

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

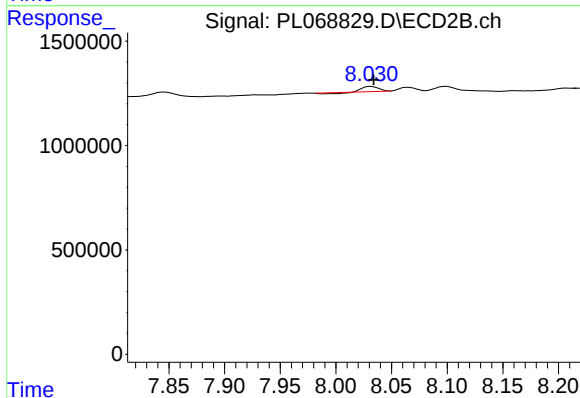


#8 Heptachlor epoxide

R.T.: 8.032 min
Delta R.T.: -0.002 min
Response: 198305
Conc: 0.17 ng/ml

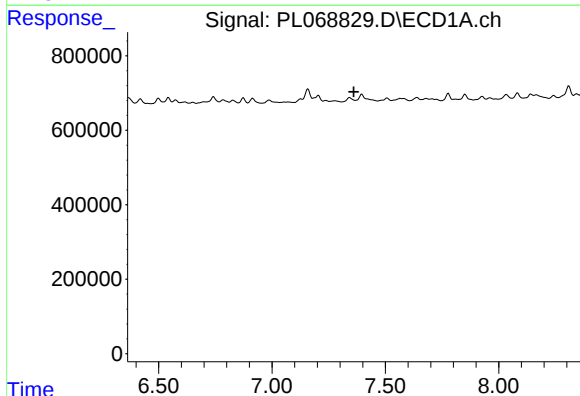


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

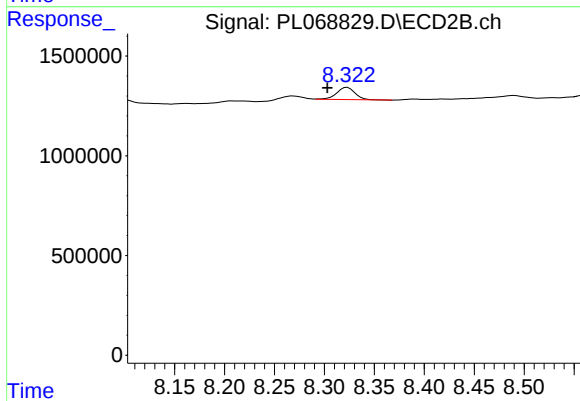

#10 gamma-Chlordane


R.T.: 8.323 min
Delta R.T.: 0.020 min
Response: 783599
Conc: 0.68 ng/ml

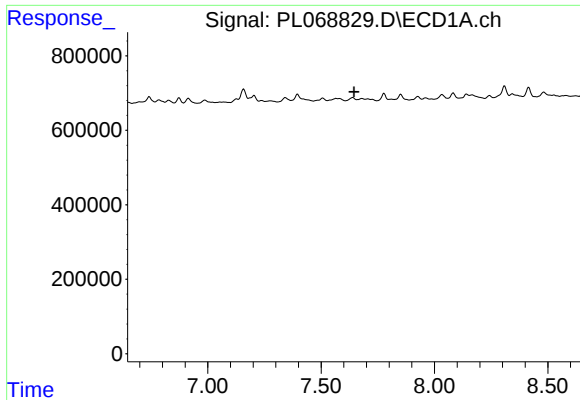

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

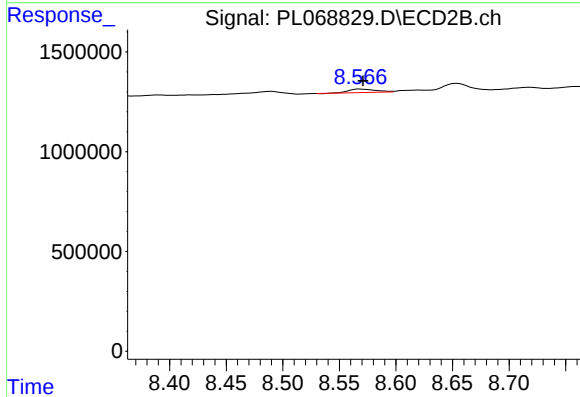


#12 4,4'-DDE

R.T.: 8.569 min
Delta R.T.: -0.002 min
Response: 280069
Conc: 0.26 ng/ml

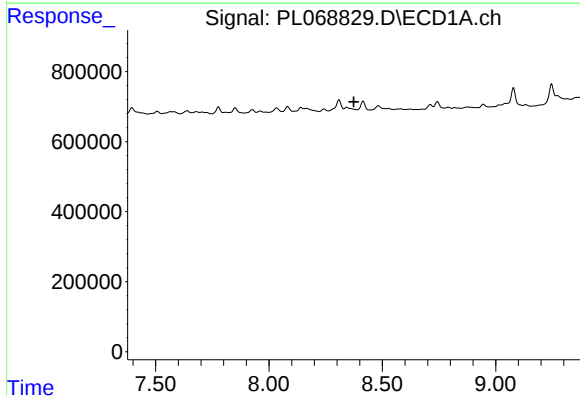


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

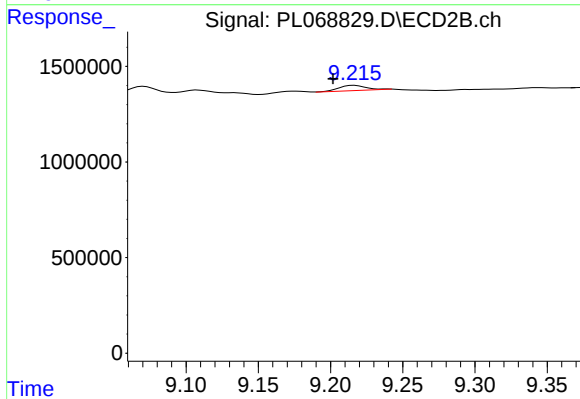

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.015 min
Response: 349776
Conc: 0.38 ng/ml

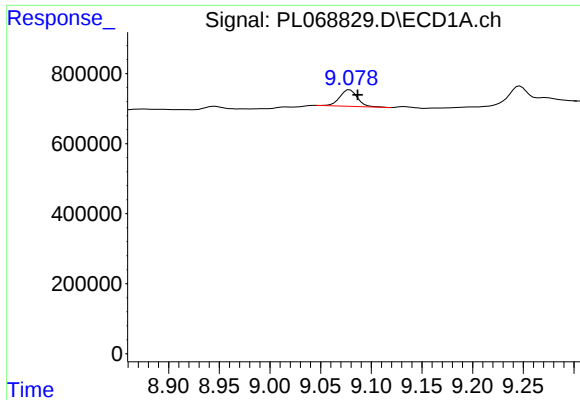

#20 Methoxychlor


R.T.: 9.079 min
Delta R.T.: -0.008 min
Response: 579638
Conc: 1.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

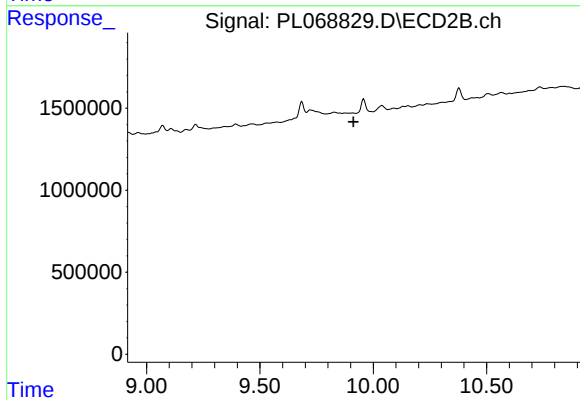


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

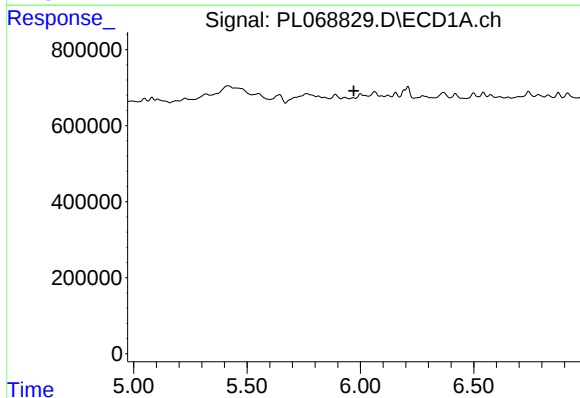


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

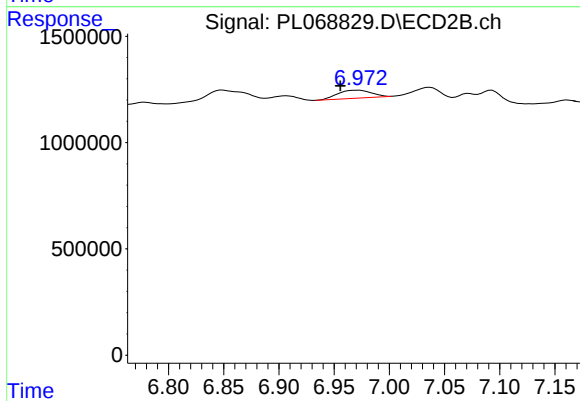

#23 Chlordane-1


R.T.: 6.973 min
Delta R.T.: 0.017 min
Response: 789543
Conc: 18.72 ng/ml

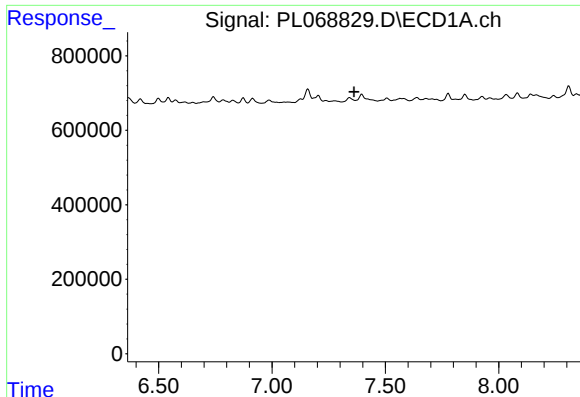

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

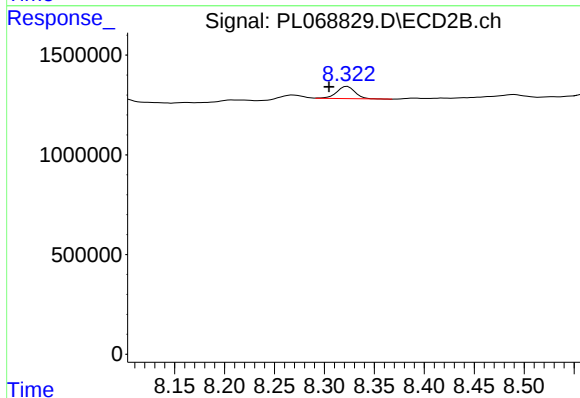


#25 Chlordane-3

R.T.: 8.323 min
Delta R.T.: 0.018 min
Response: 783599
Conc: 4.80 ng/ml

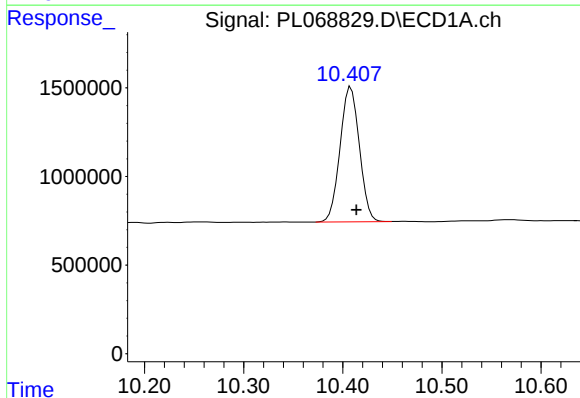

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: -0.005 min
Response: 10323678
Conc: 17.96 ng/ml

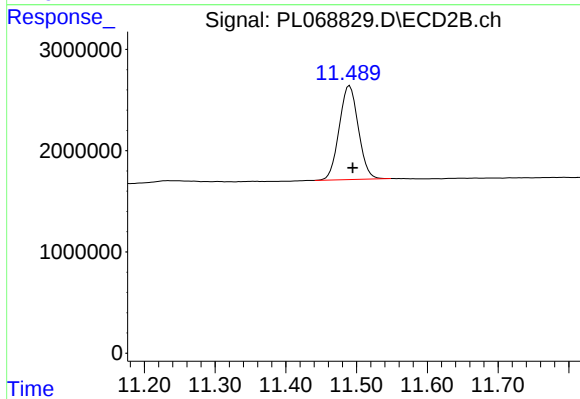

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: -0.004 min
Response: 17433776
Conc: 17.97 ng/ml