

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 13:38
 Operator : AR\AJ
 Sample : M3318-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 08:30:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.570	8146176	20437602	19.694	20.129
28)	SA Decachlor...	10.412	11.495	9890956	16968972	17.211	17.489
Target Compounds							
7)	B delta-BHC	0.000	7.094f	0	136526	N.D.	0.108 #
8)	B Heptachlo...	0.000	8.034	0	180631	N.D.	0.156 #
10)	B gamma-Chl...	0.000	8.324f	0	805626	N.D.	0.703 #
12)	B 4,4'-DDE	0.000	8.572	0	207391	N.D.	0.196 #
15)	B Endosulfa...	0.000	9.218f	0	372437	N.D.	0.406 #
20)	A Methoxychlor	9.082	0.000	362954	0	1.159	N.D. #
23)	Chlordane-1	0.000	6.974f	0	356525	N.D.	8.455 #
25)	Chlordane-3	0.000	8.324f	0	805626	N.D.	4.932 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 13:38
Operator : AR\AJ
Sample : M3318-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:30:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

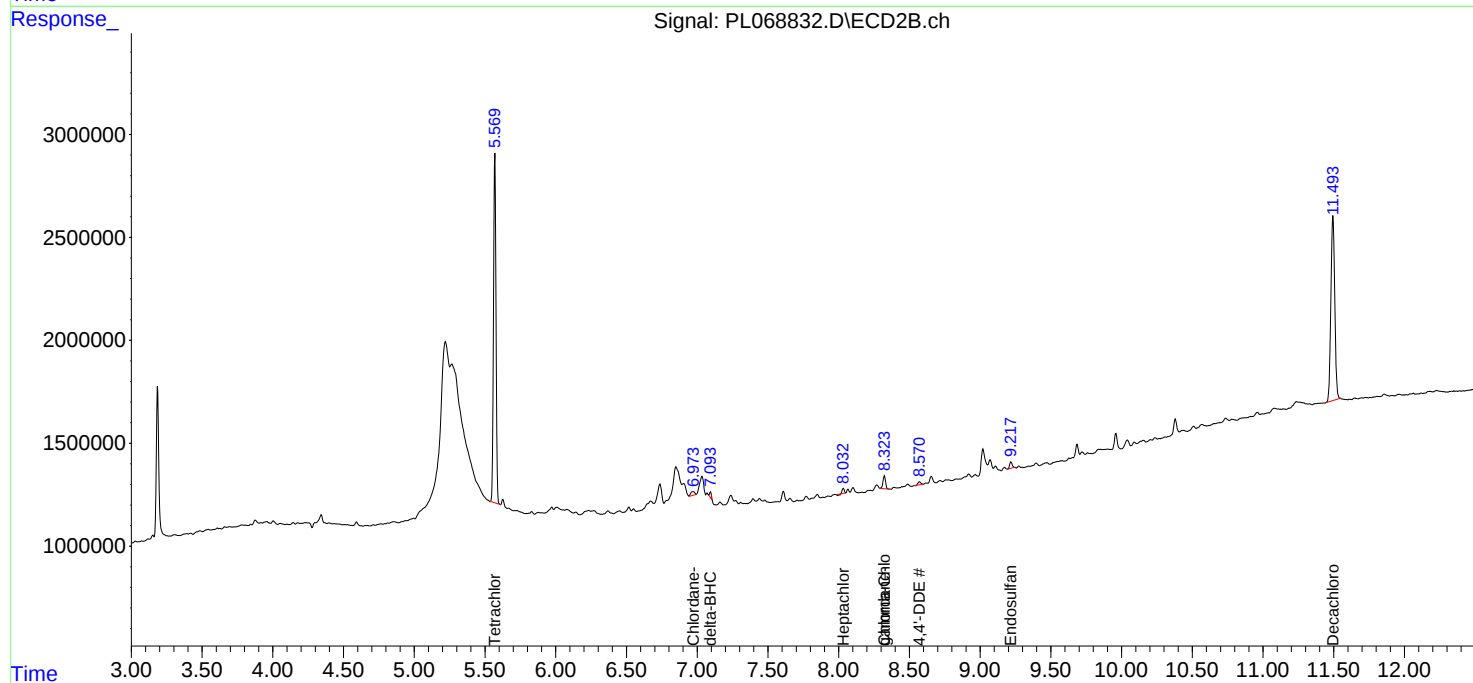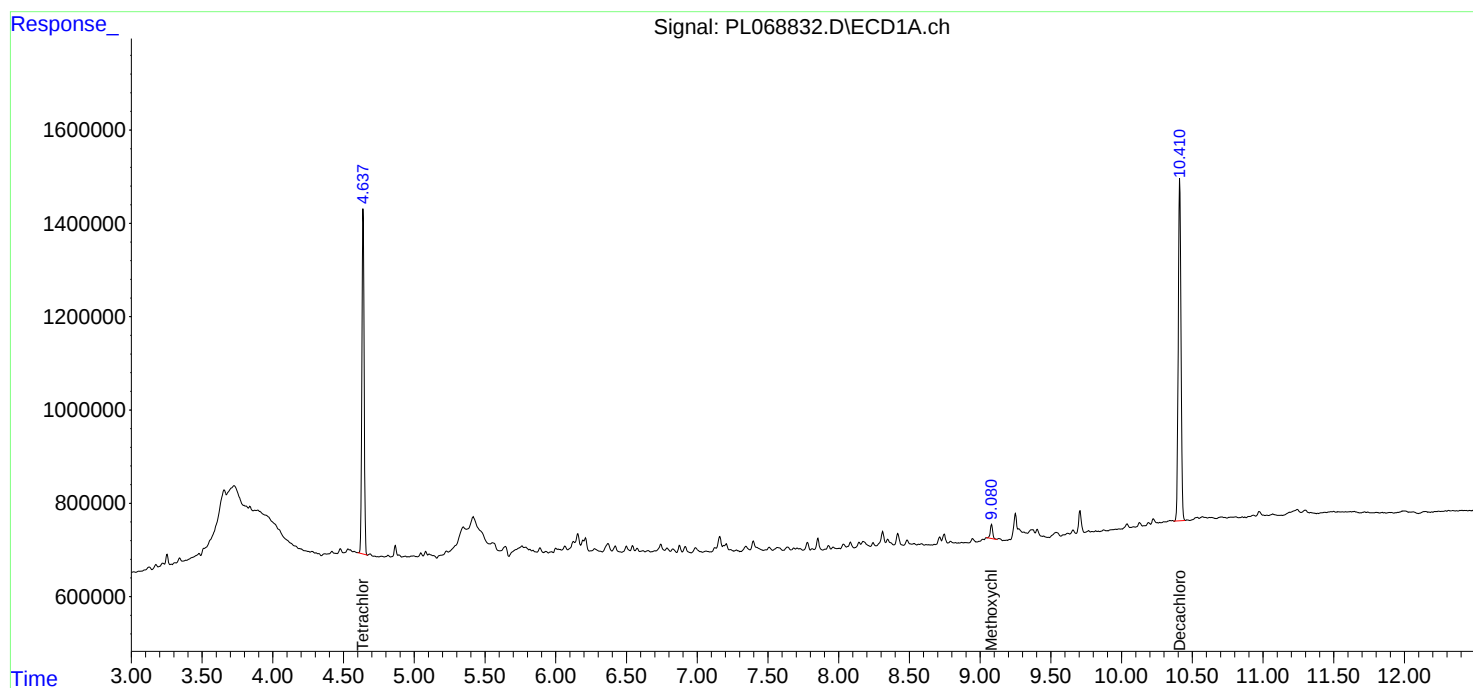


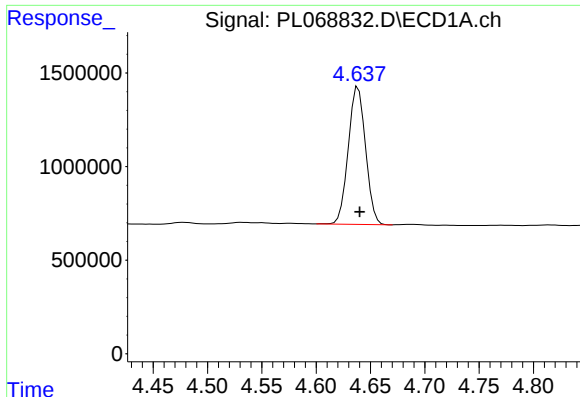

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: -0.001 min
Response: 8146176
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

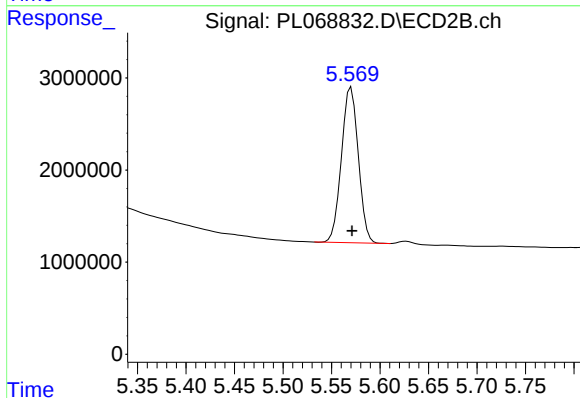


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 20437602
Conc: 20.13 ng/ml

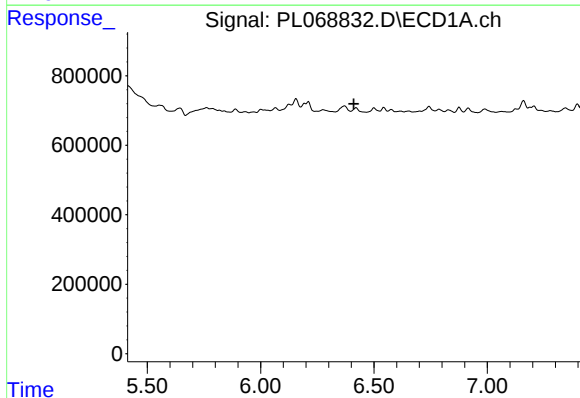


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

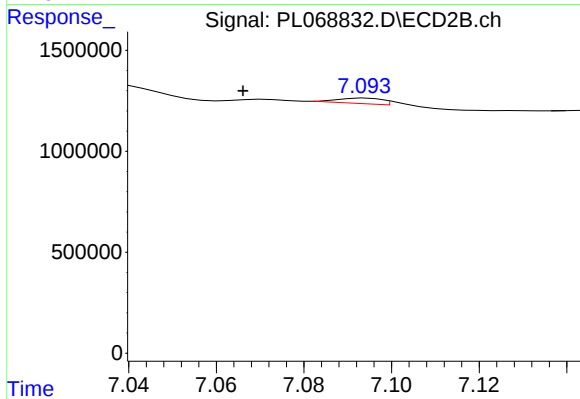

#7 delta-BHC


R.T.: 7.094 min
Delta R.T.: 0.028 min
Response: 136526
Conc: 0.11 ng/ml

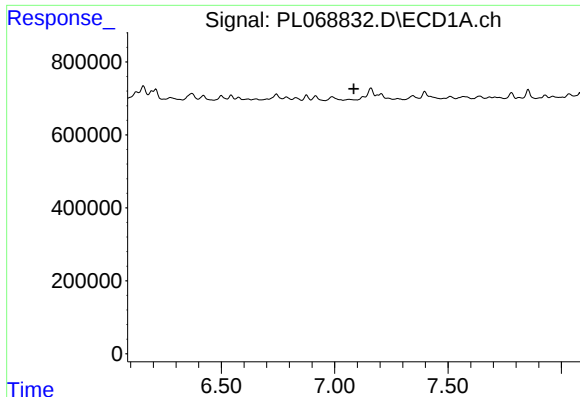

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

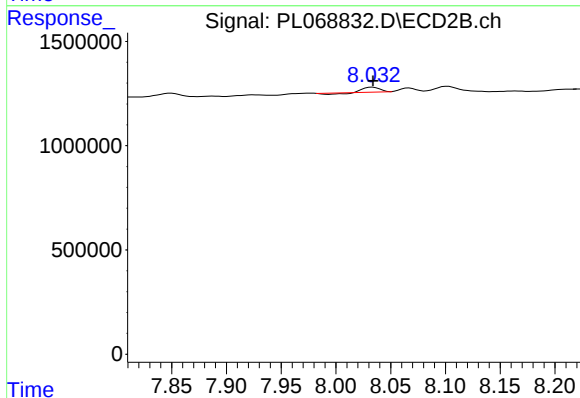


#8 Heptachlor epoxide

R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 180631
Conc: 0.16 ng/ml

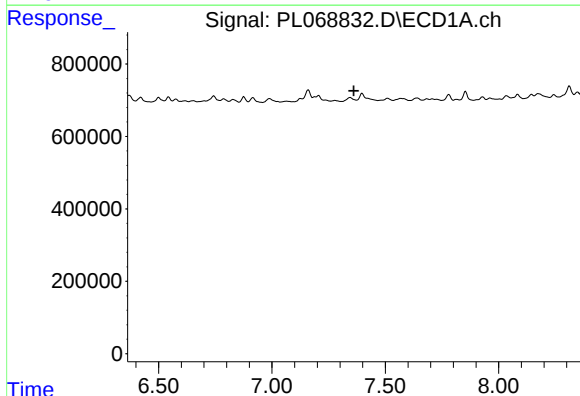


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

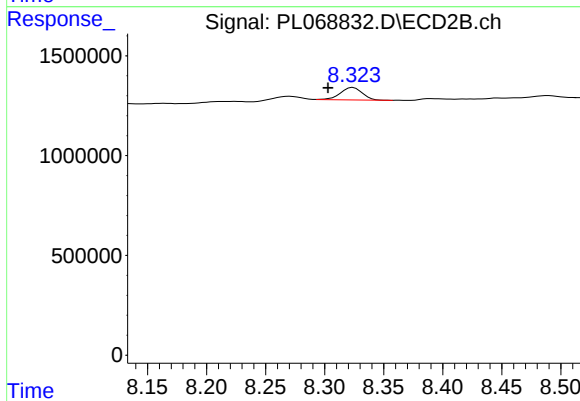

#10 gamma-Chlordane


R.T.: 8.324 min
Delta R.T.: 0.021 min
Response: 805626
Conc: 0.70 ng/ml

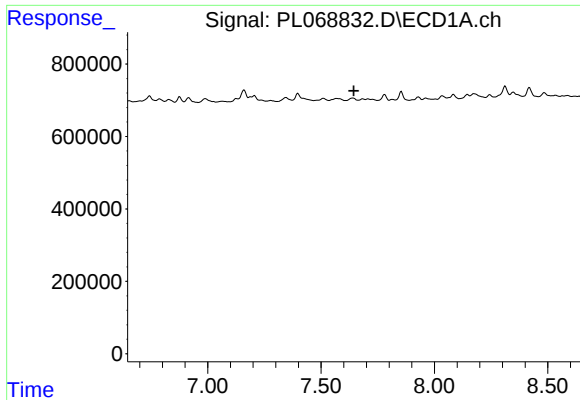

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

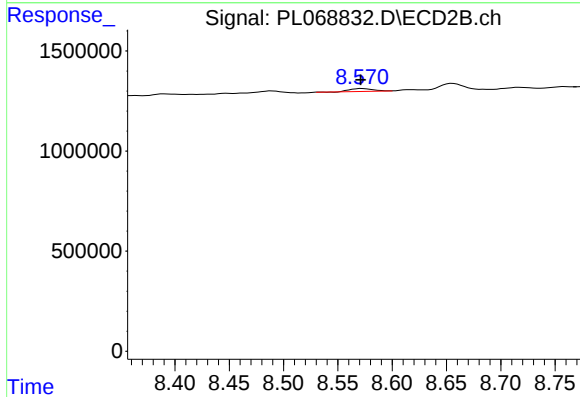


#12 4,4'-DDE

R.T.: 8.572 min
Delta R.T.: 0.001 min
Response: 207391
Conc: 0.20 ng/ml

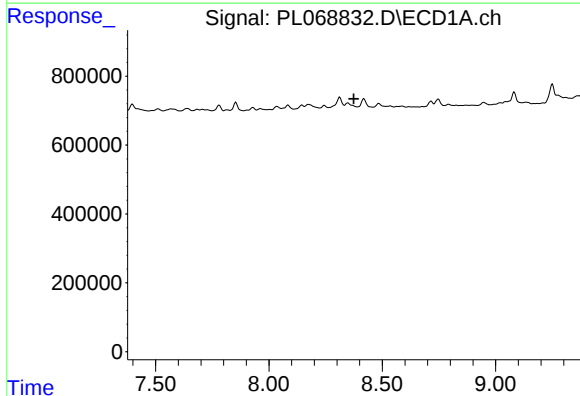


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

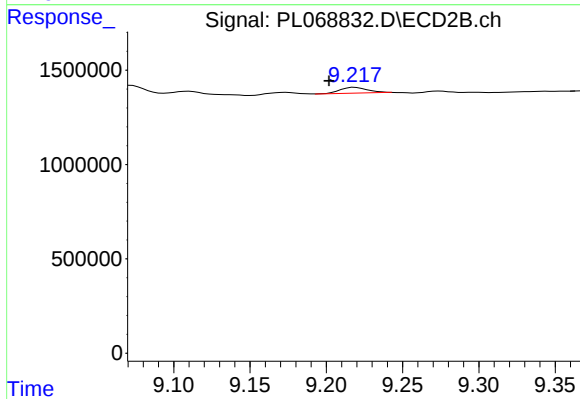

#15 Endosulfan II


R.T.: 9.218 min
Delta R.T.: 0.017 min
Response: 372437
Conc: 0.41 ng/ml

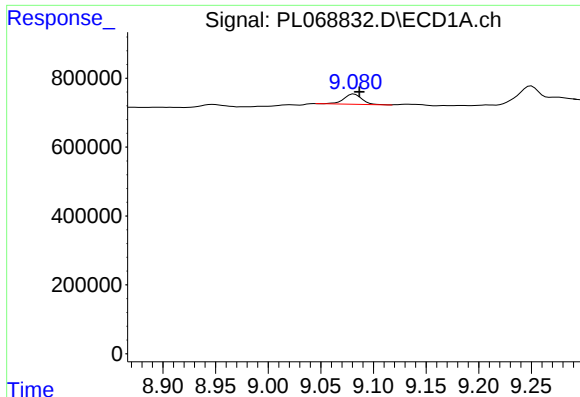

#20 Methoxychlor


R.T.: 9.082 min
Delta R.T.: -0.005 min
Response: 362954
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

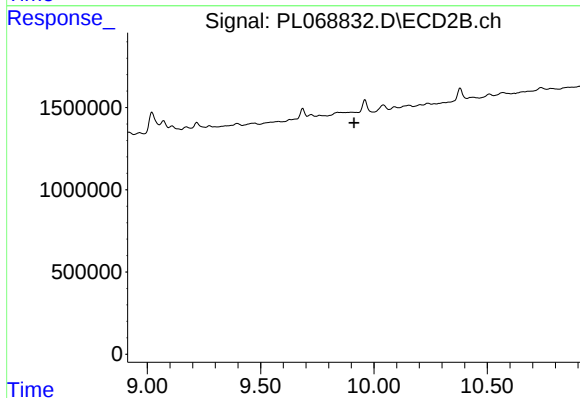


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

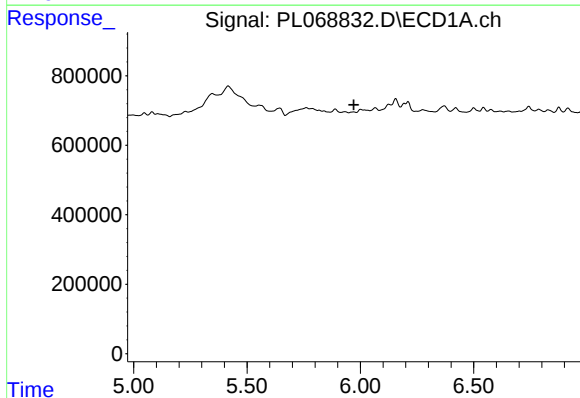


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

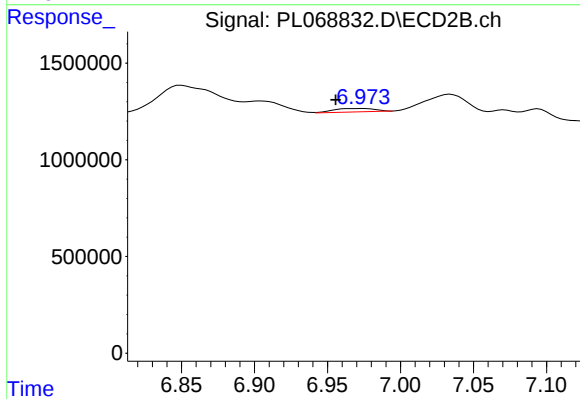

#23 Chlordane-1


R.T.: 6.974 min
Delta R.T.: 0.018 min
Response: 356525
Conc: 8.45 ng/ml

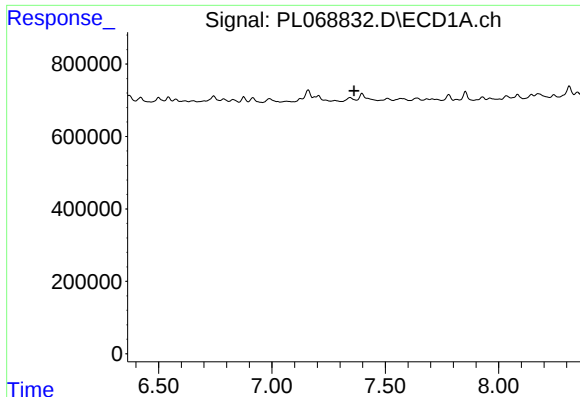

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

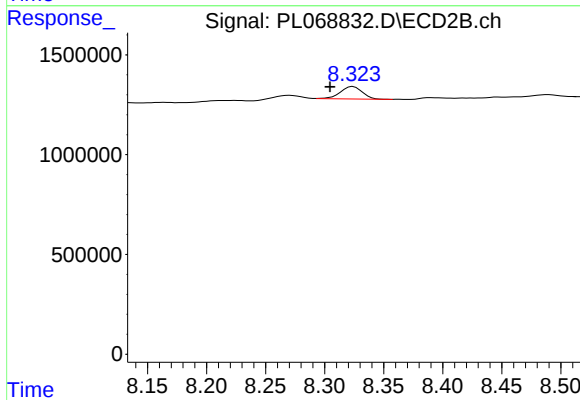


#25 Chlordane-3

R.T.: 8.324 min
Delta R.T.: 0.020 min
Response: 805626
Conc: 4.93 ng/ml

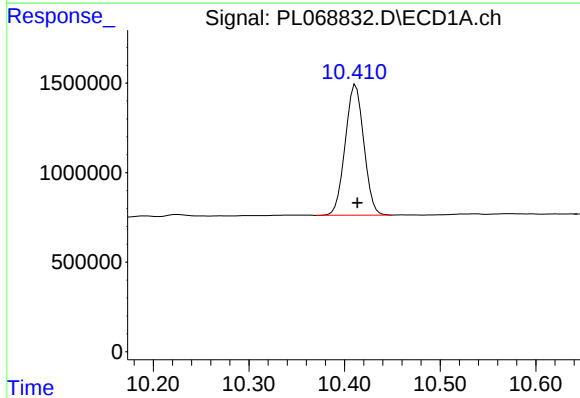

#28 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.002 min
Response: 9890956
Conc: 17.21 ng/ml

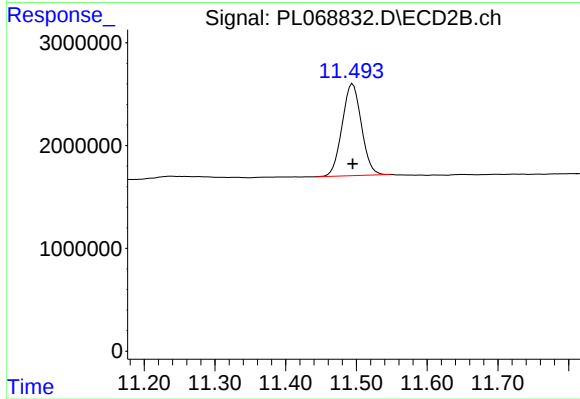

#28 Decachlorobiphenyl

R.T.: 11.495 min
Delta R.T.: 0.000 min
Response: 16968972
Conc: 17.49 ng/ml