

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 16:21
 Operator : AR\AJ
 Sample : M3316-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 08:33:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.570	7598615	19750043	18.370	19.452
28)	SA Decachlor...	10.411	11.494	11158805	19104284	19.417	19.690
Target Compounds							
3)	MA gamma-BHC...	0.000	6.574f	0	264887	N.D.	0.204 #
9)	A Endosulfan I	0.000	8.456f	0	89230	N.D.	0.085 #
11)	B alpha-Chl...	0.000	8.412f	0	117416	N.D.	0.102 #
15)	B Endosulfa...	0.000	9.217f	0	1186445	N.D.	1.294 #
23)	Chlordane-1	0.000	6.969	0	205286	N.D.	4.868 #
26)	Chlordane-4	0.000	8.412f	0	117416	N.D.	0.592 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 16:21
Operator : AR\AJ
Sample : M3316-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:33:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

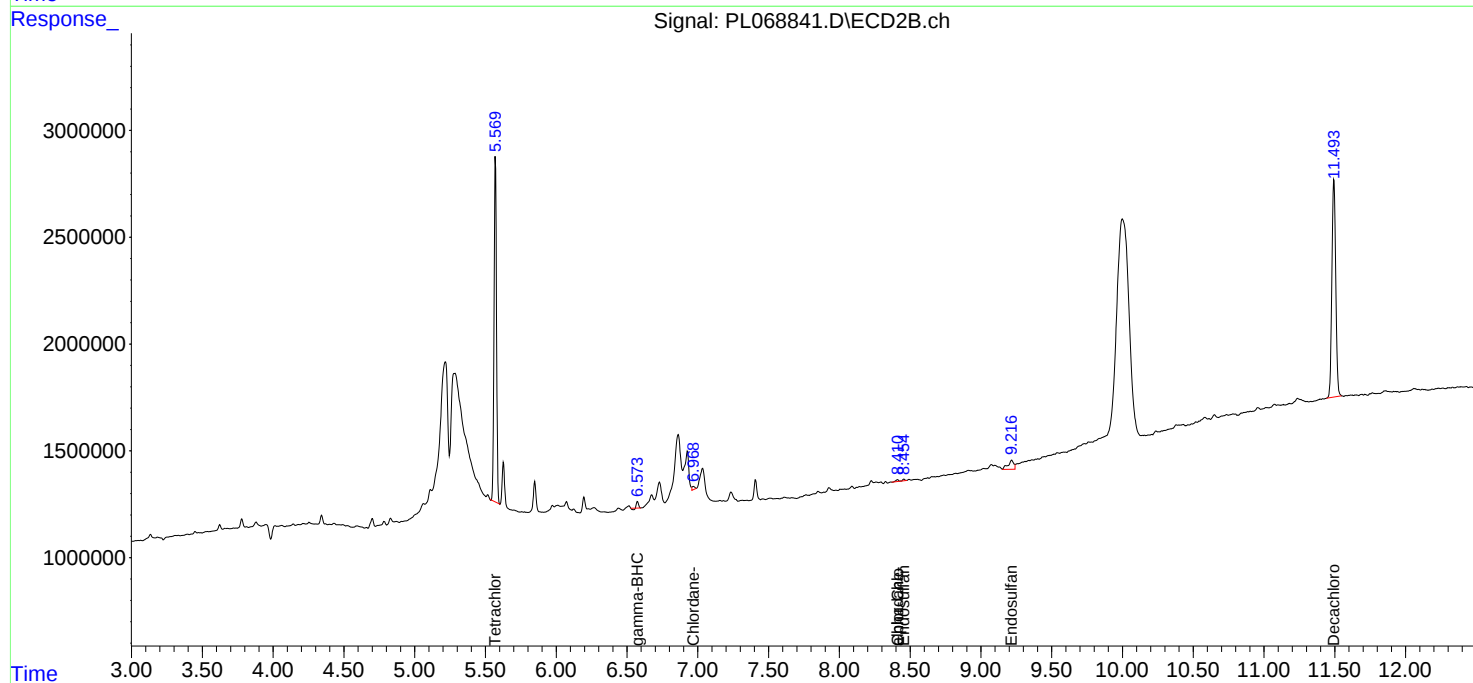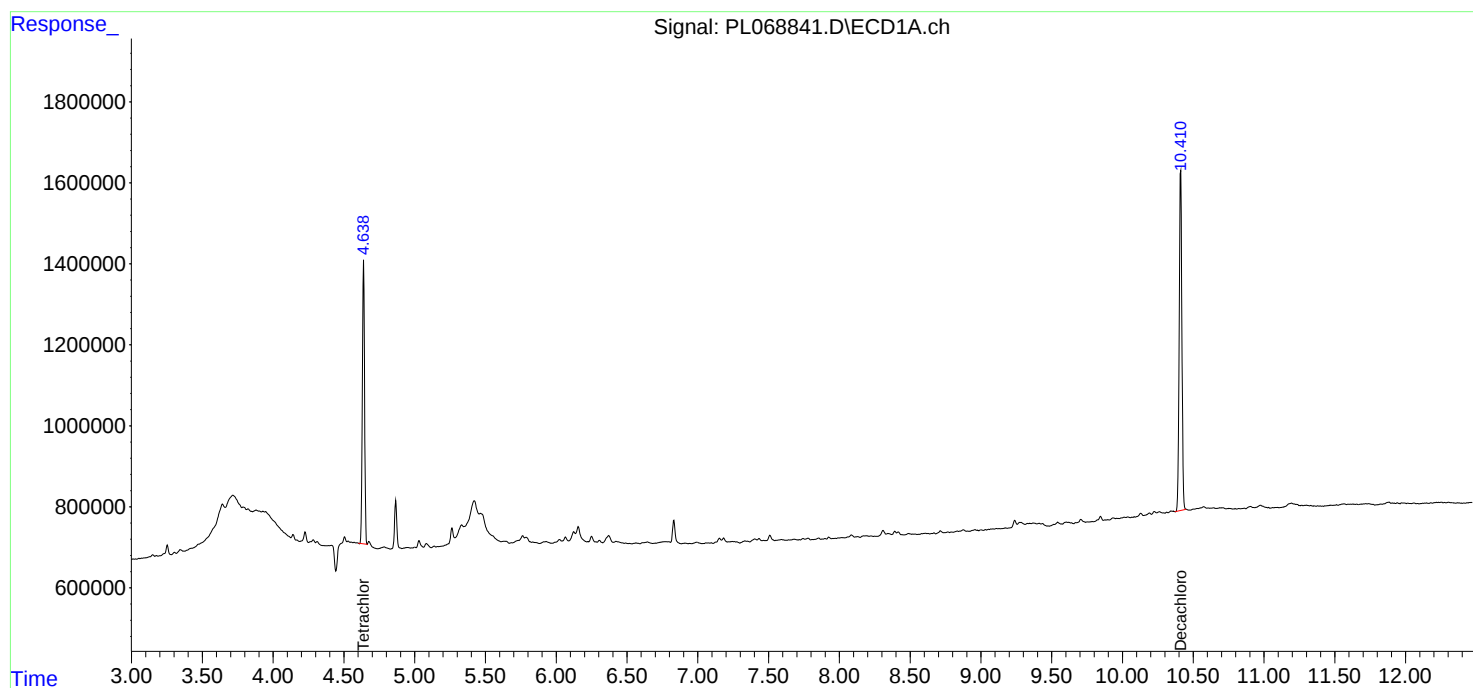


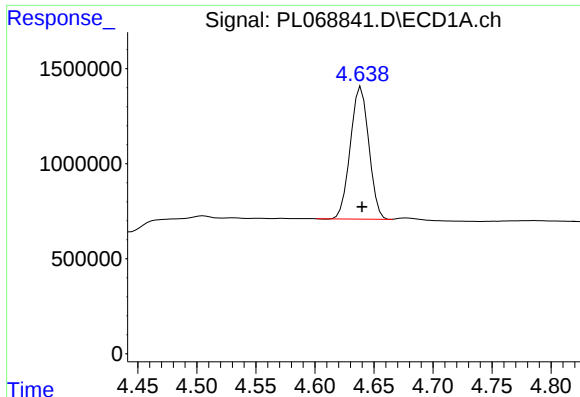

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 7598615
Conc: 18.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

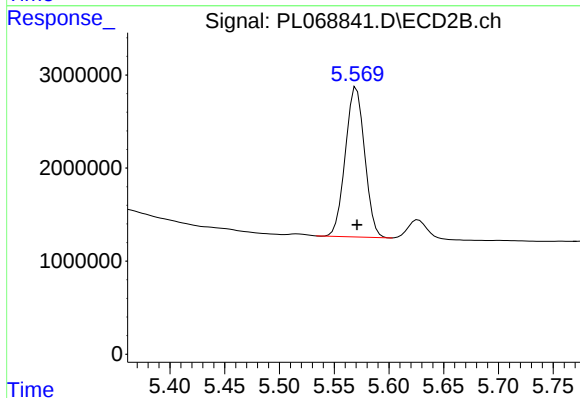


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 19750043
Conc: 19.45 ng/ml

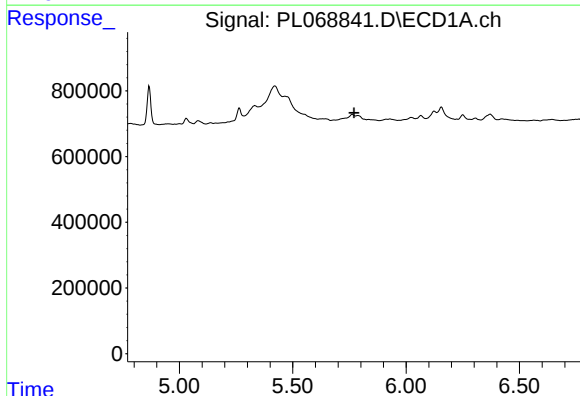


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.770 min
Response: 0
Conc: N.D.

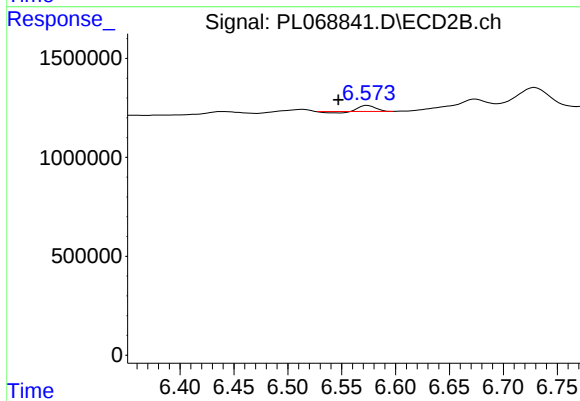

#3 gamma-BHC (Lindane)


R.T.: 6.574 min
Delta R.T.: 0.027 min
Response: 264887
Conc: 0.20 ng/ml

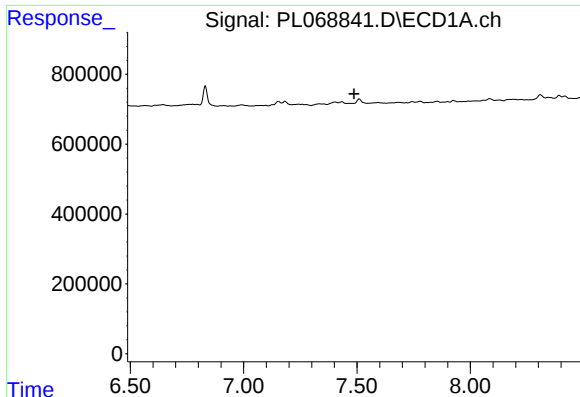

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

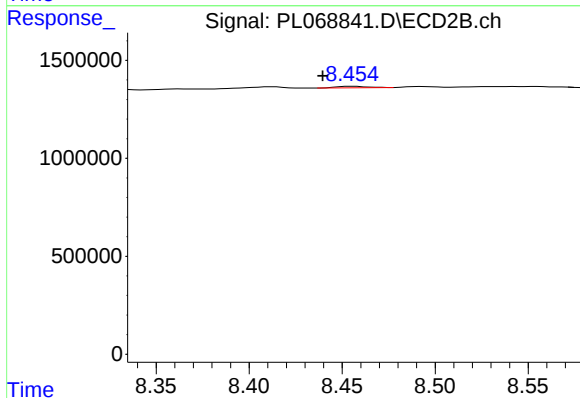


#9 Endosulfan I

R.T.: 8.456 min
Delta R.T.: 0.016 min
Response: 89230
Conc: 0.08 ng/ml

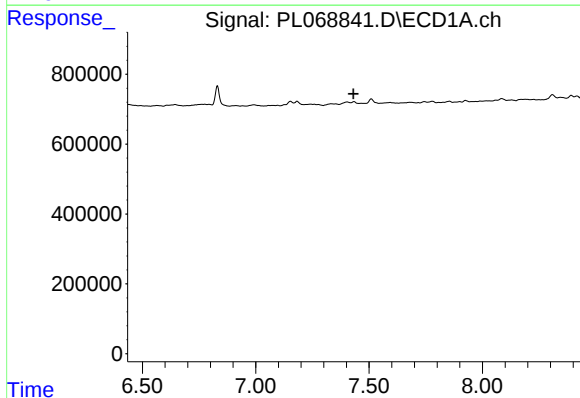


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

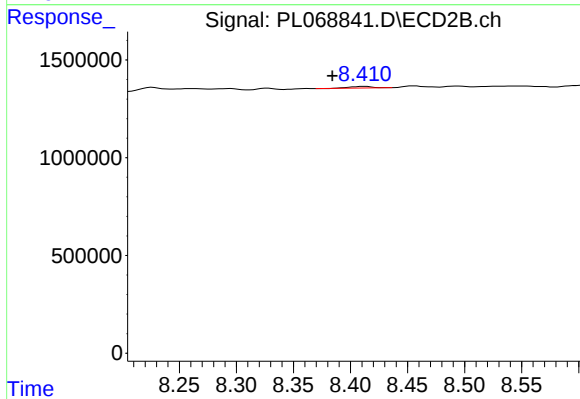

#11 alpha-Chlordane


R.T.: 8.412 min
Delta R.T.: 0.028 min
Response: 117416
Conc: 0.10 ng/ml

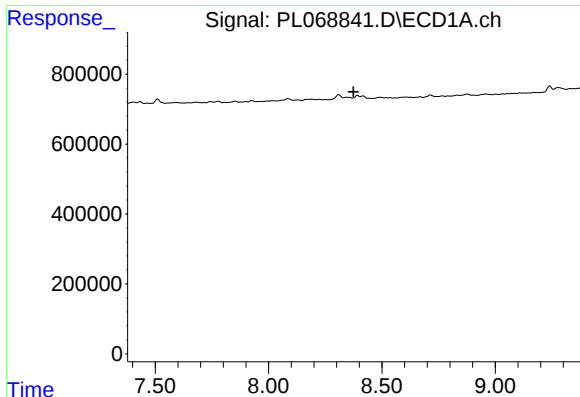

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

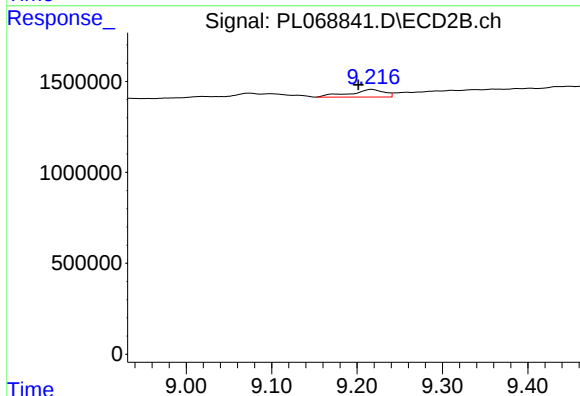


#15 Endosulfan II

R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 1186445
Conc: 1.29 ng/ml

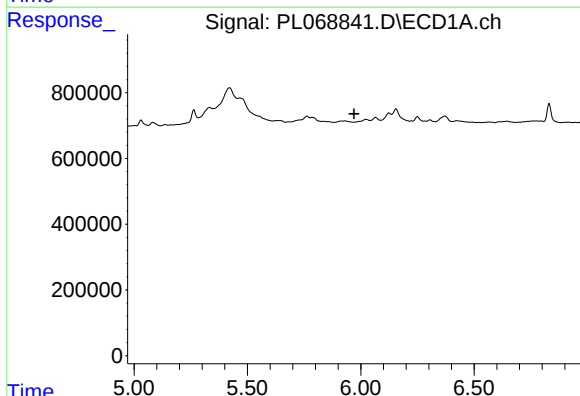


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

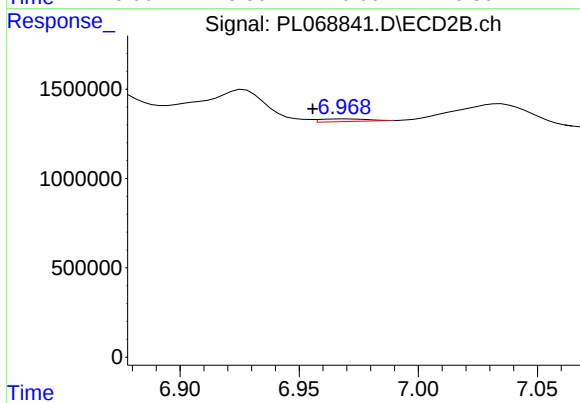

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.014 min
Response: 205286
Conc: 4.87 ng/ml

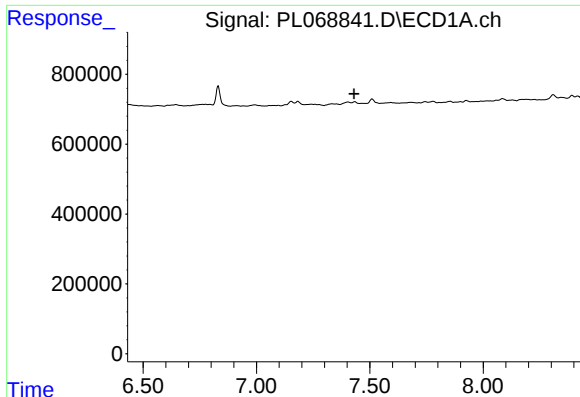

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

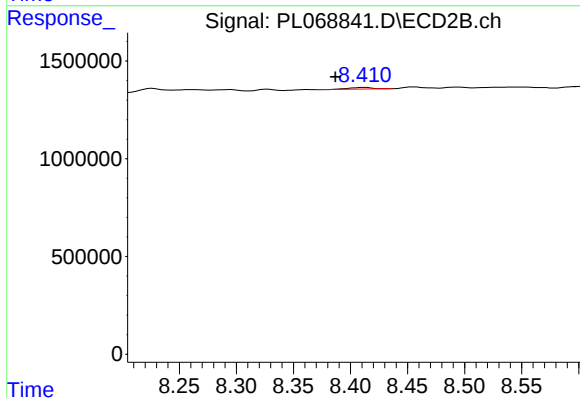


#26 Chlordane-4

R.T.: 8.412 min
Delta R.T.: 0.025 min
Response: 117416
Conc: 0.59 ng/ml

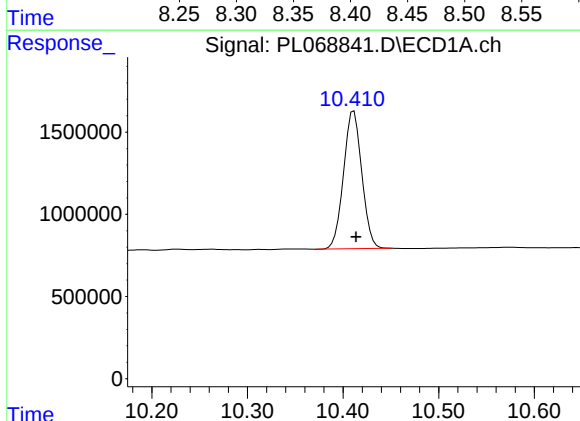

#28 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: -0.002 min
Response: 11158805
Conc: 19.42 ng/ml

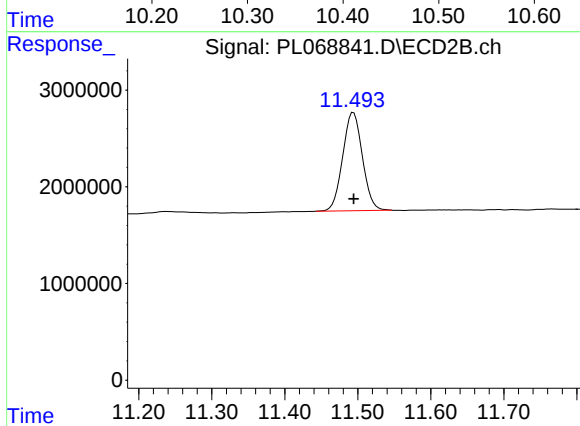

#28 Decachlorobiphenyl

R.T.: 11.494 min
Delta R.T.: 0.000 min
Response: 19104284
Conc: 19.69 ng/ml