

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 19:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 08:34:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	8487552	22280565	20.519	21.944
28)	SA Decachlor...	10.406	11.486	12436749	20666566	21.641	21.300
Target Compounds							
4)	MA Heptachlor	6.154f	0.000	557044	0	0.948	N.D. #
6)	B beta-BHC	6.154	0.000	557044	0	1.976	N.D. #
8)	B Heptachlo...	0.000	8.035	0	1086412	N.D.	0.940 #
14)	MA Endrin	8.081f	0.000	556423	0	1.155	N.D. #
15)	B Endosulfa...	0.000	9.215	0	386274	N.D.	0.421 #
17)	MA 4,4'-DDT	0.000	9.437	0	232965	N.D.	0.246 #
21)	B Endrin ke...	0.000	10.088f	0	371497	N.D.	0.365 #
23)	Chlordane-1	0.000	6.979f	0	54425	N.D.	1.291 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 19:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:34:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

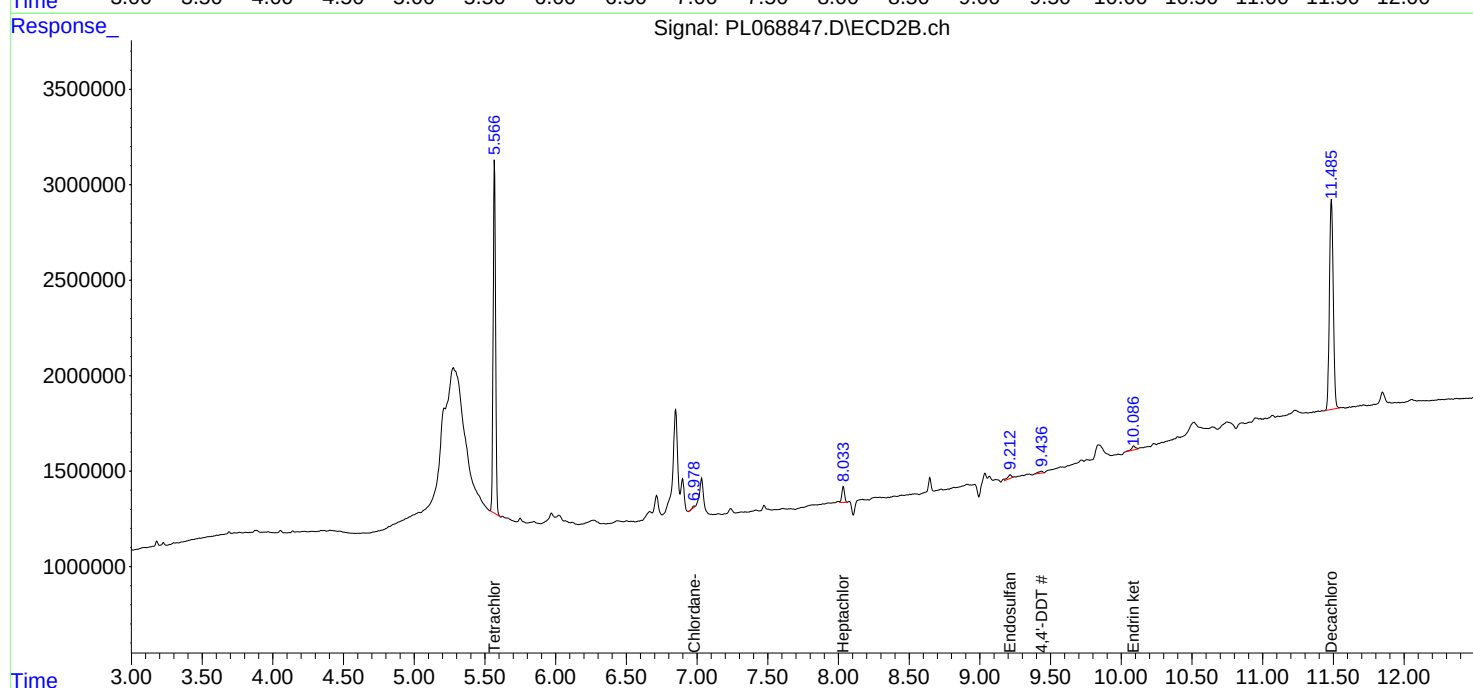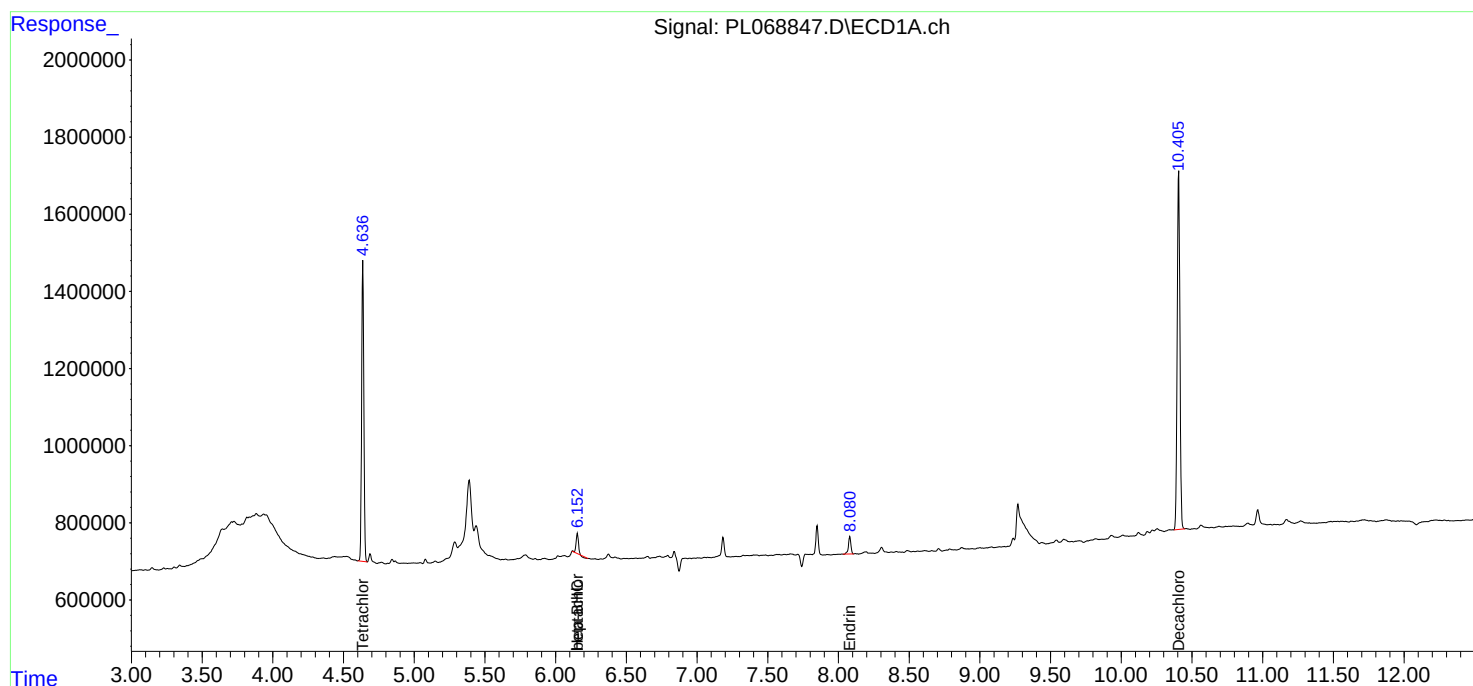


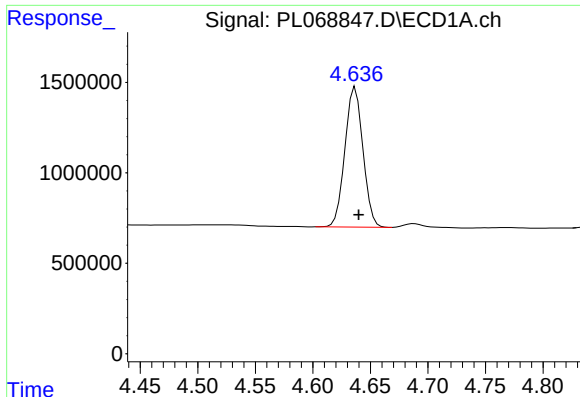

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 8487552
Conc: 20.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

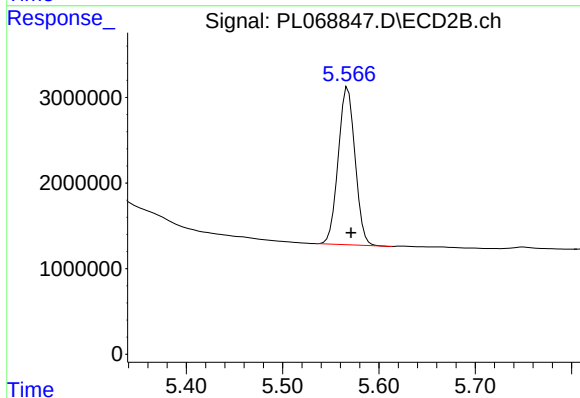


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 22280565
Conc: 21.94 ng/ml

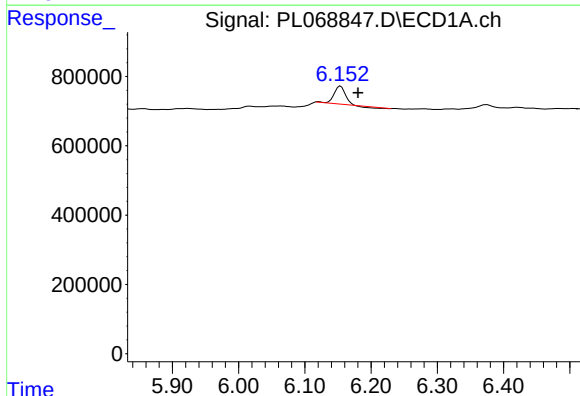


#4 Heptachlor

R.T.: 6.154 min
Delta R.T.: -0.027 min
Response: 557044
Conc: 0.95 ng/ml

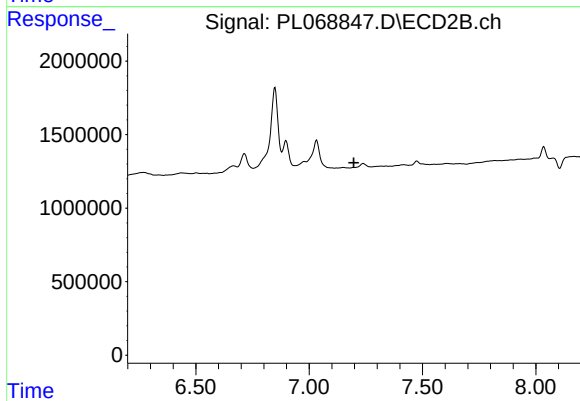

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.197 min
Response: 0
Conc: N.D.

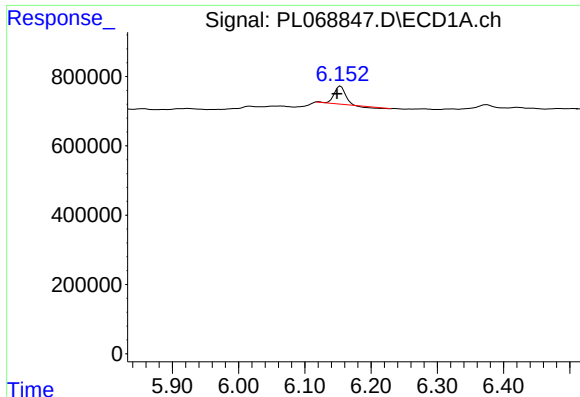

#6 beta-BHC


R.T.: 6.154 min
Delta R.T.: 0.005 min
Response: 557044
Conc: 1.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

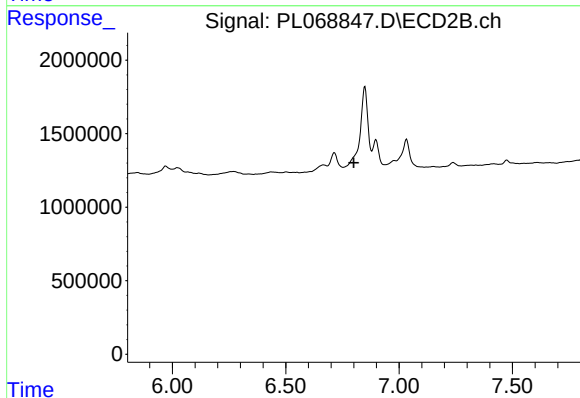


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

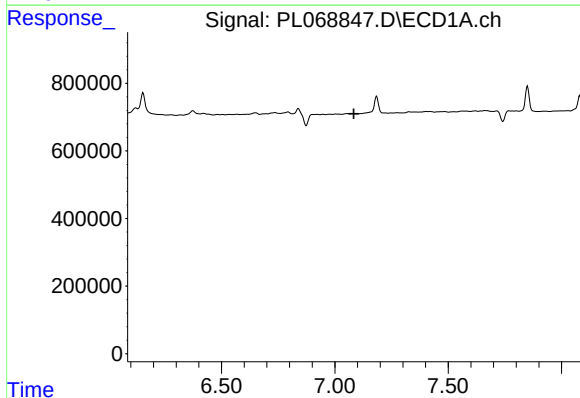


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

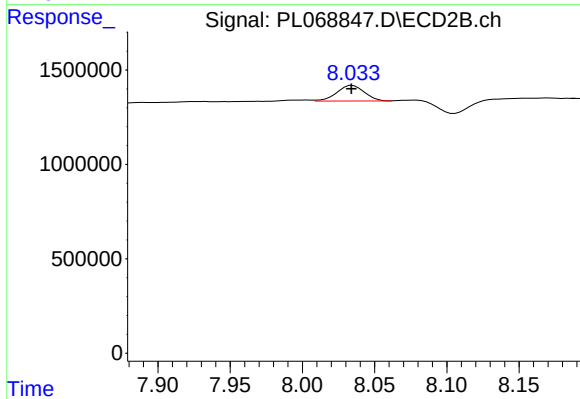

#8 Heptachlor epoxide


R.T.: 8.035 min
Delta R.T.: 0.000 min
Response: 1086412
Conc: 0.94 ng/ml

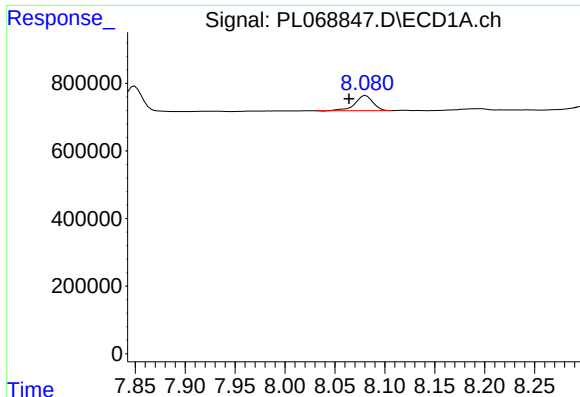

#14 Endrin


R.T.: 8.081 min
Delta R.T.: 0.017 min
Response: 556423
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

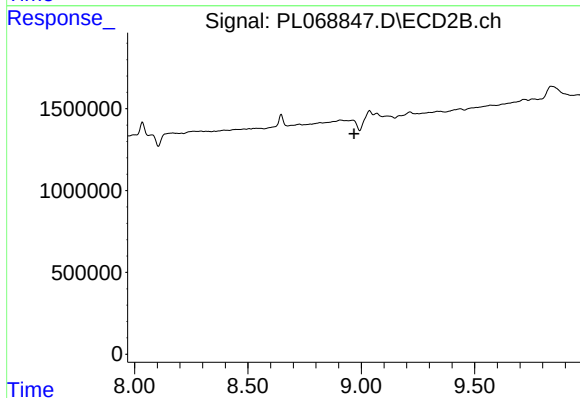


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

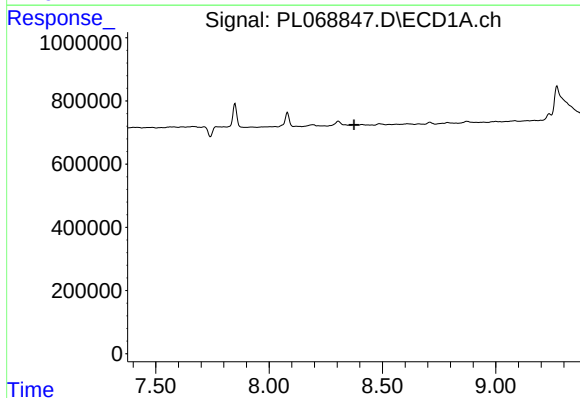


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

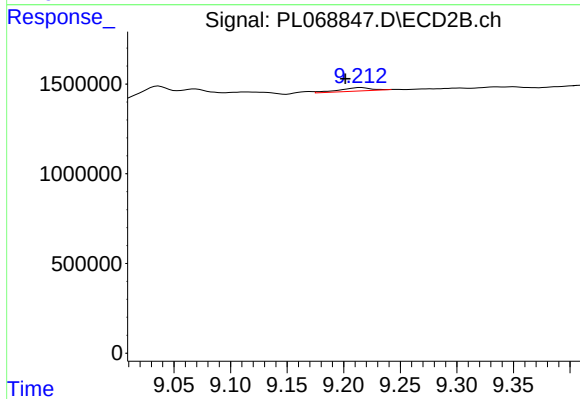

#15 Endosulfan II


R.T.: 9.215 min
Delta R.T.: 0.013 min
Response: 386274
Conc: 0.42 ng/ml

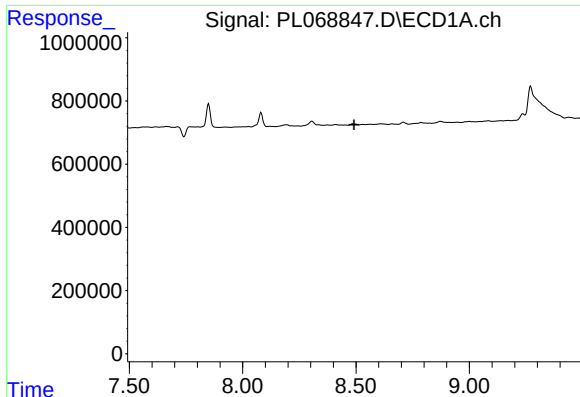

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

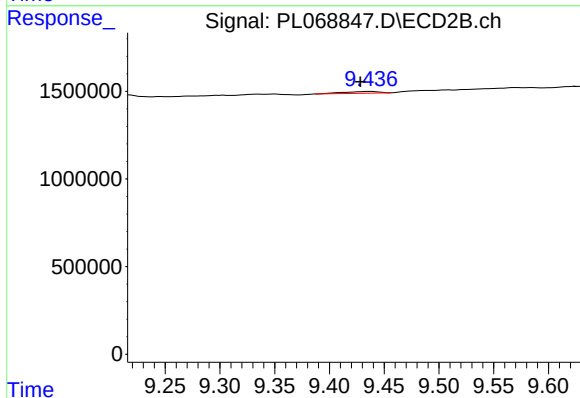


#17 4,4'-DDT

R.T.: 9.437 min
Delta R.T.: 0.009 min
Response: 232965
Conc: 0.25 ng/ml

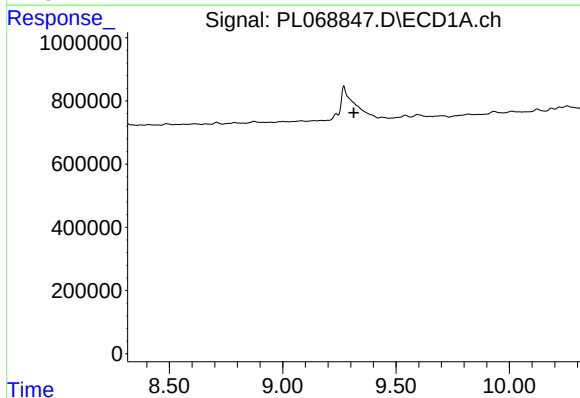


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

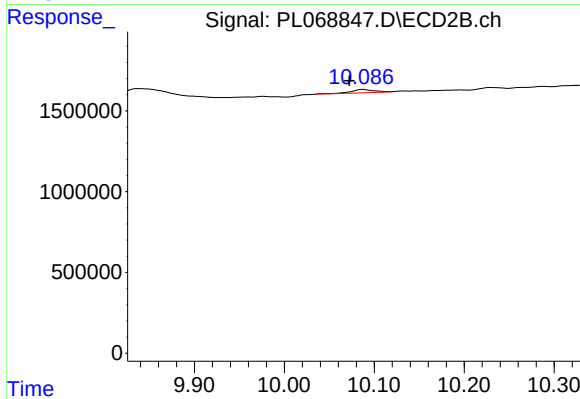

#21 Endrin ketone


R.T.: 10.088 min
Delta R.T.: 0.015 min
Response: 371497
Conc: 0.36 ng/ml

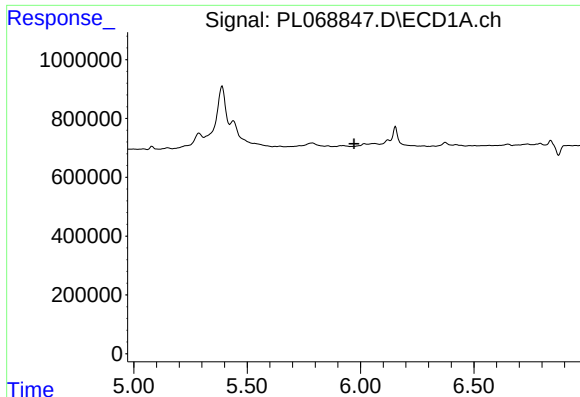

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

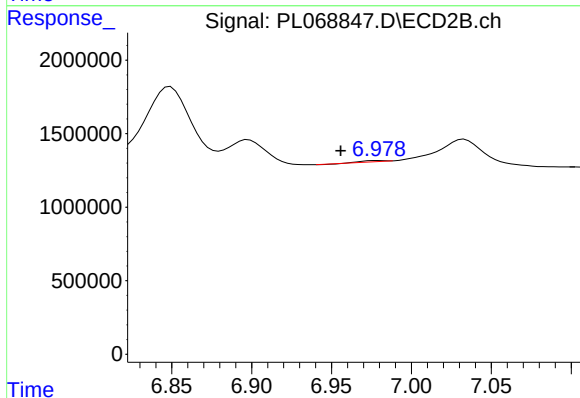


#23 Chlordane-1

R.T.: 6.979 min
Delta R.T.: 0.024 min
Response: 54425
Conc: 1.29 ng/ml

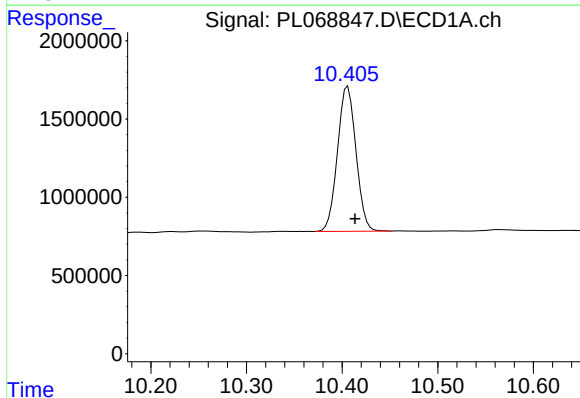

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.008 min
Response: 12436749
Conc: 21.64 ng/ml

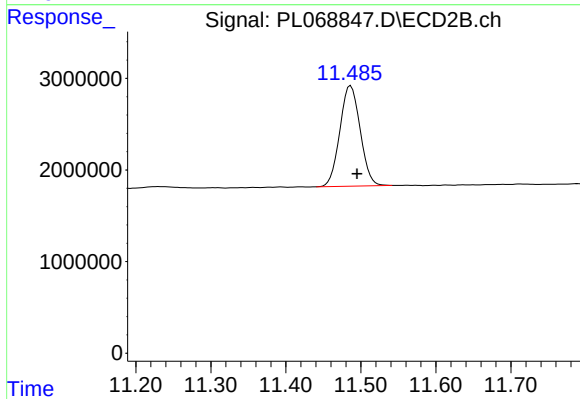

#28 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: -0.008 min
Response: 20666566
Conc: 21.30 ng/ml