

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 21:59
 Operator : AR\AJ
 Sample : PB138269BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 08:54:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.567	7437534	19940072	17.981	19.639
28)	SA Decachlor...	10.405	11.486	11213322	19293010	19.512	19.885
Target Compounds							
11)	B alpha-Chl...	0.000	8.406f	0	41774	N.D.	0.036 #
15)	B Endosulfa...	0.000	9.215	0	683929	N.D.	0.746 #
21)	B Endrin ke...	0.000	10.090f	0	562531	N.D.	0.552 #
23)	Chlordane-1	0.000	6.979f	0	20359	N.D.	0.483 #
26)	Chlordane-4	0.000	8.406f	0	41774	N.D.	0.211 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 21:59
Operator : AR\AJ
Sample : PB138269BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:54:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

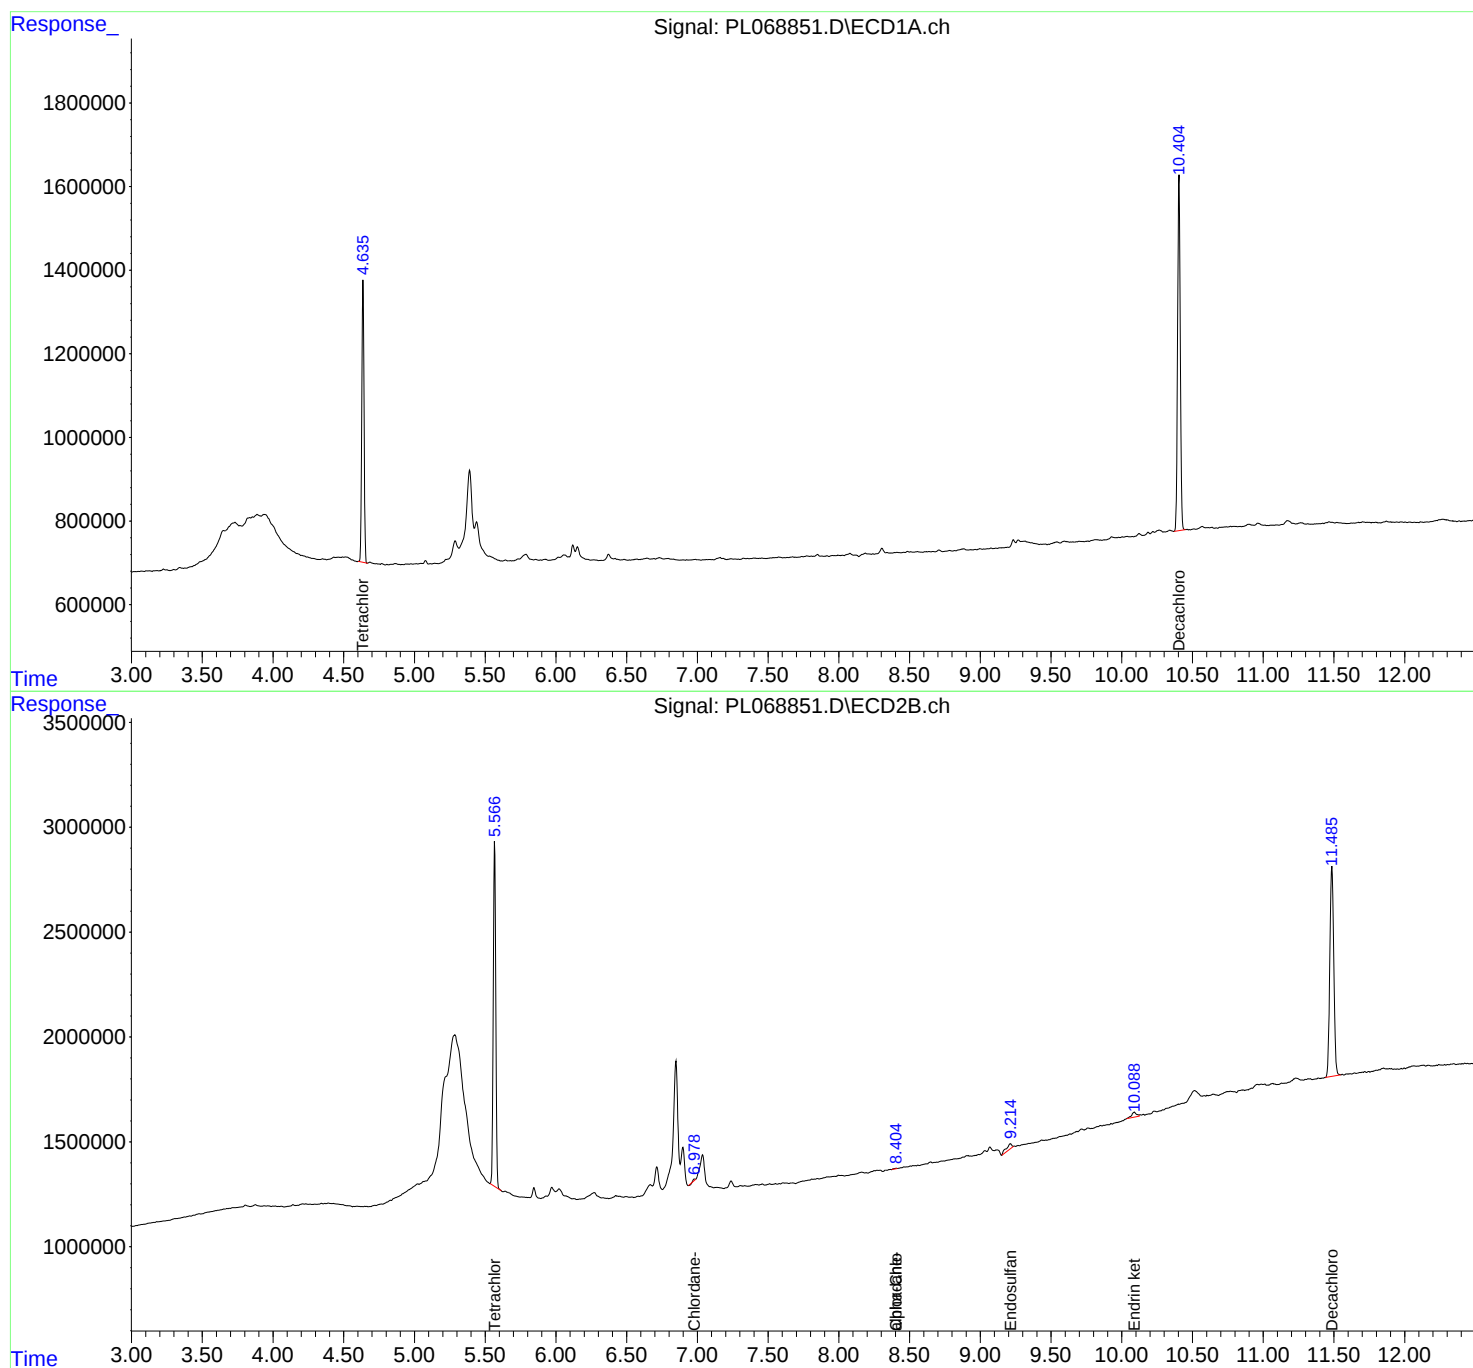


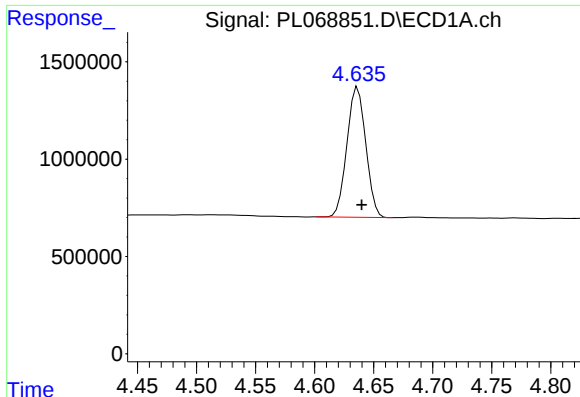

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 7437534
Conc: 17.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

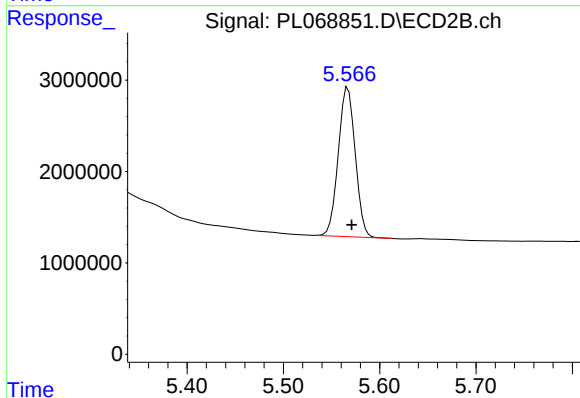


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: -0.004 min
Response: 19940072
Conc: 19.64 ng/ml

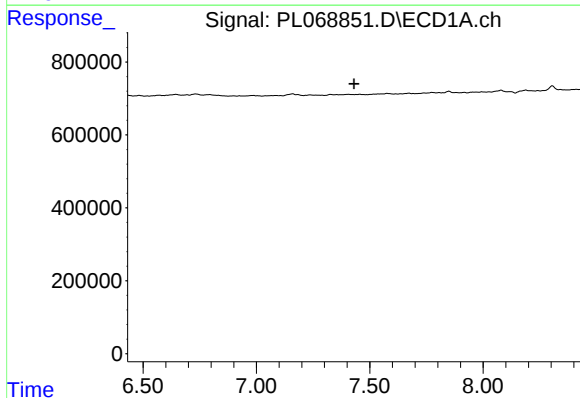


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

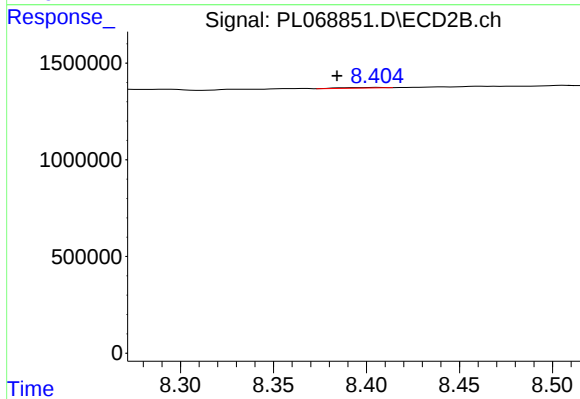

#11 alpha-Chlordane


R.T.: 8.406 min
Delta R.T.: 0.021 min
Response: 41774
Conc: 0.04 ng/ml

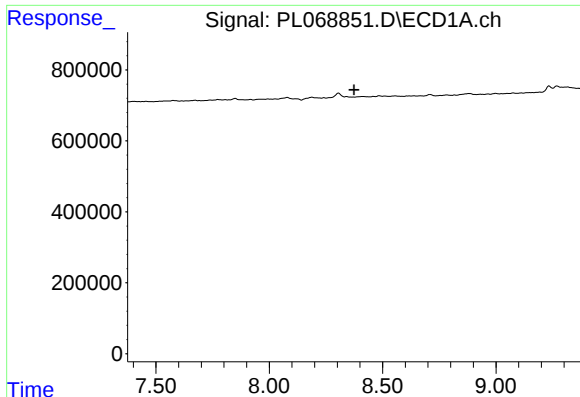

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

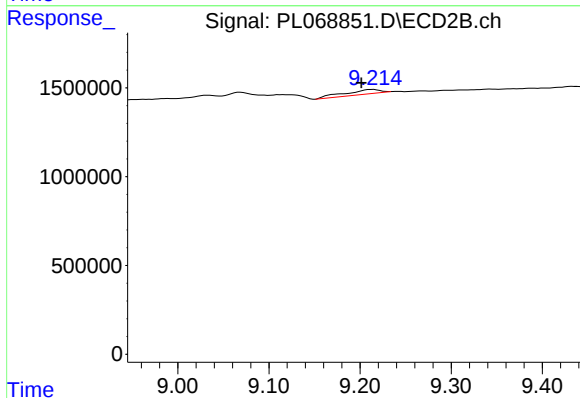


#15 Endosulfan II

R.T.: 9.215 min
Delta R.T.: 0.013 min
Response: 683929
Conc: 0.75 ng/ml

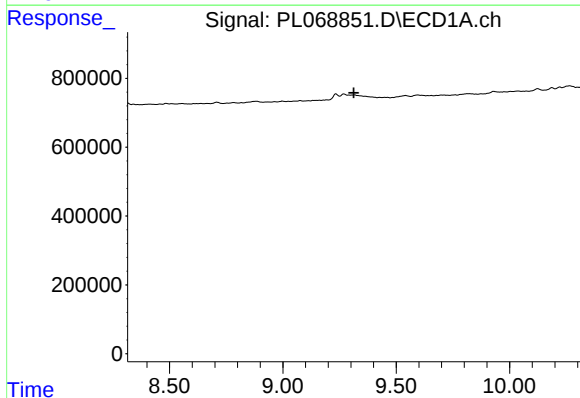


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

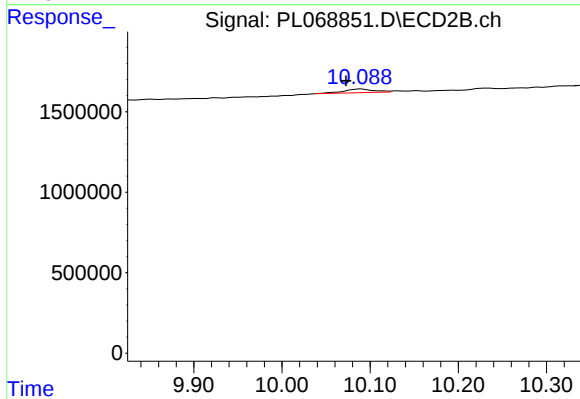

#21 Endrin ketone


R.T.: 10.090 min
Delta R.T.: 0.017 min
Response: 562531
Conc: 0.55 ng/ml

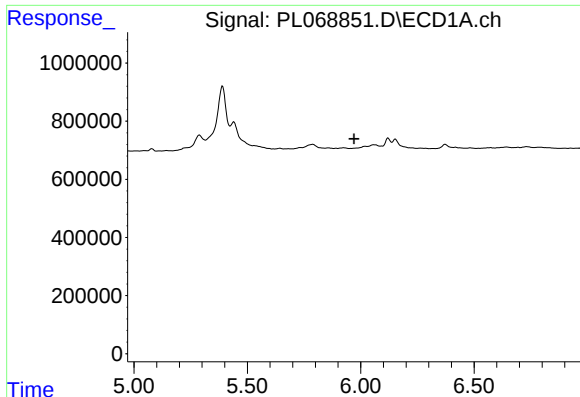

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

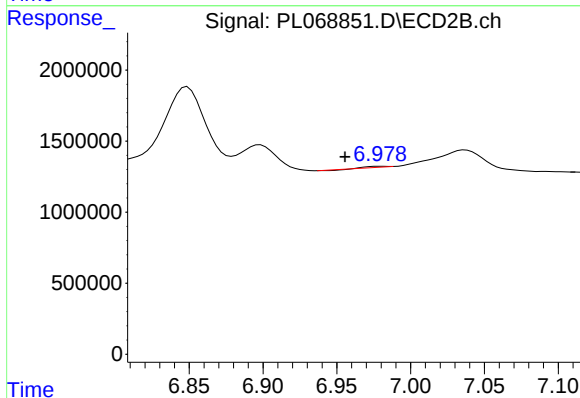


#23 Chlordane-1

R.T.: 6.979 min
Delta R.T.: 0.024 min
Response: 20359
Conc: 0.48 ng/ml

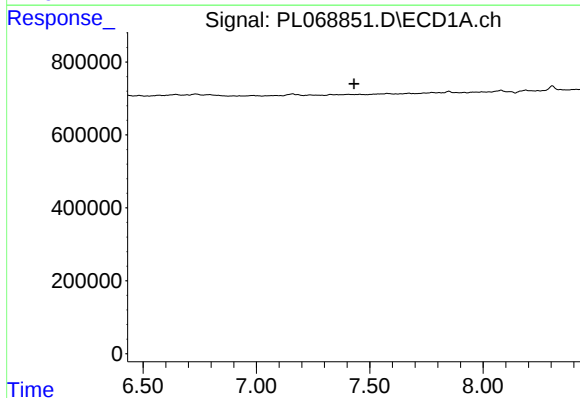


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

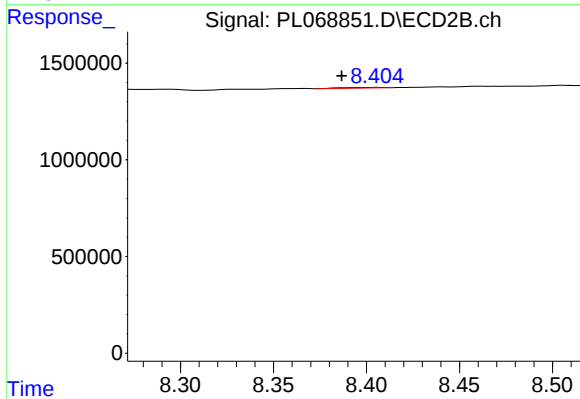

#26 Chlordane-4


R.T.: 8.406 min
Delta R.T.: 0.019 min
Response: 41774
Conc: 0.21 ng/ml

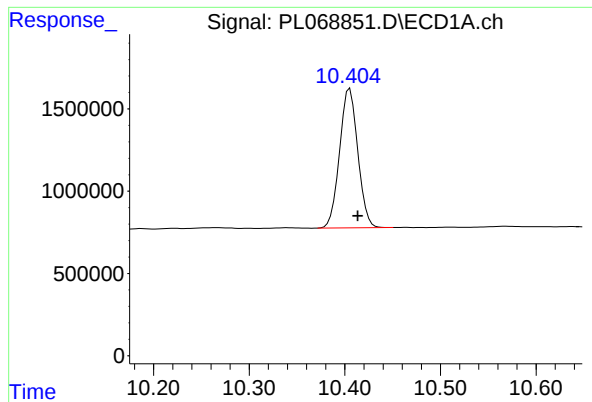

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.008 min
Response: 11213322
Conc: 19.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

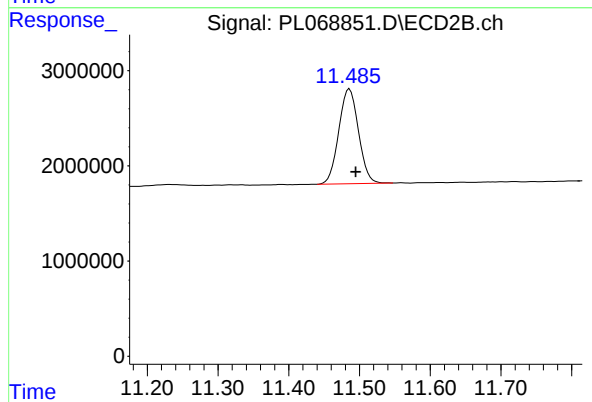

#28 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: -0.009 min
Response: 19293010
Conc: 19.88 ng/ml