

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 15:01
 Operator : AR\AJ
 Sample : M3326-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDE-NB

Manual Integrations
 APPROVED

Ankita
 8/10/2021 12:54:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 08:31:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	5856992	14295315	14.160	14.079
28)	SA Decachlor...	10.407	11.487	7926104	12987212	13.792	13.386
Target Compounds							
11)	B alpha-Chl...	7.423	8.382	708817	1426201	1.288m	1.242
12)	B 4,4'-DDE	7.639	8.561	734719	1397051	1.521m	1.322
17)	MA 4,4'-DDT	8.480	9.422	3788413	1370526	7.800	1.448m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 15:01
Operator : AR\AJ
Sample : M3326-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDE-NB


Manual Integrations
APPROVED

Ankita
8/10/2021 12:54:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:31:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

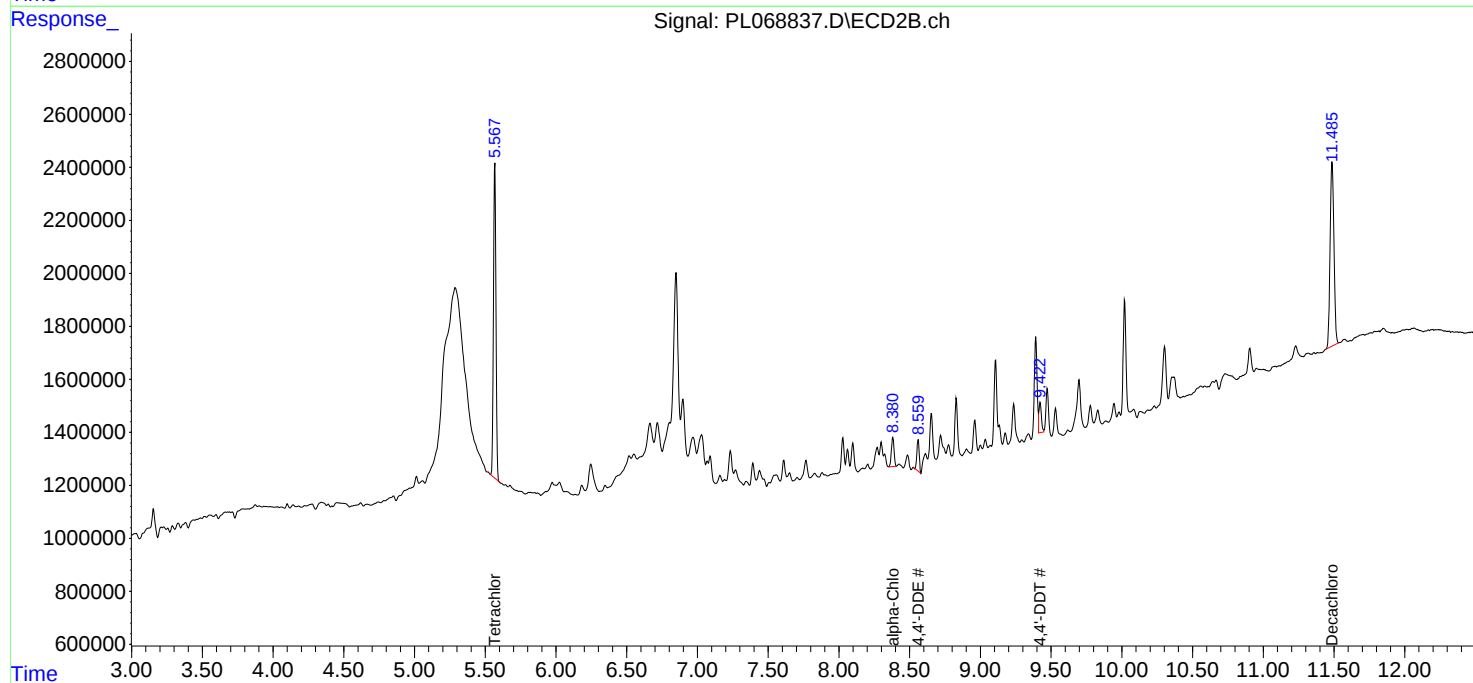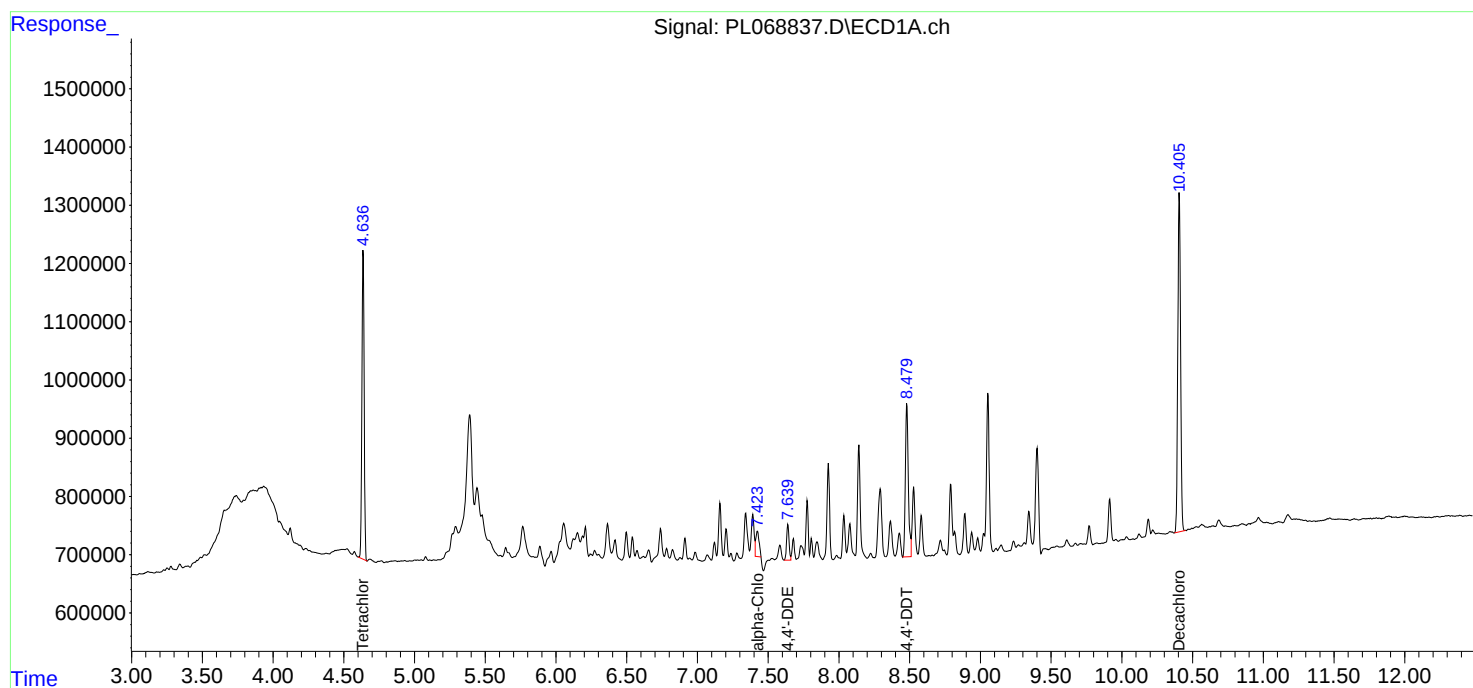

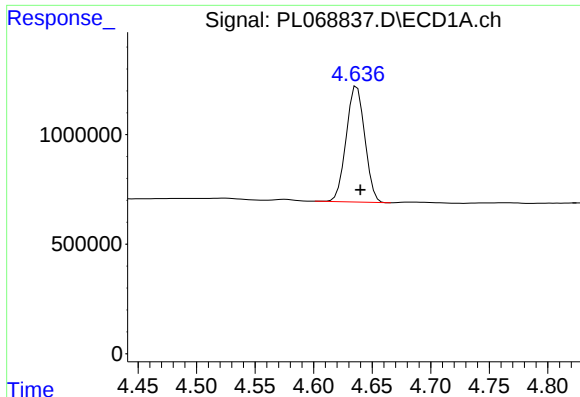


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 5856992
Conc: 14.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDE-NB


Manual Integrations
APPROVED

Ankita
8/10/2021 12:54:55 PM

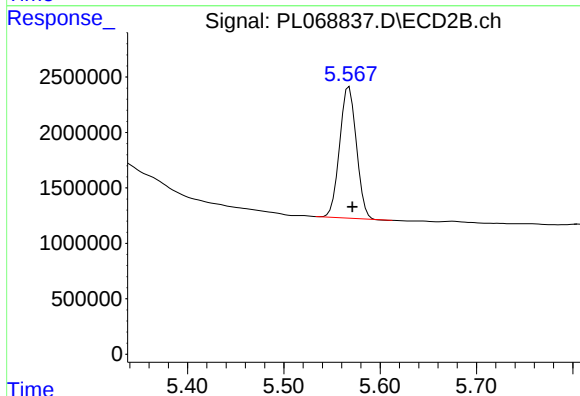


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 14295315
Conc: 14.08 ng/ml

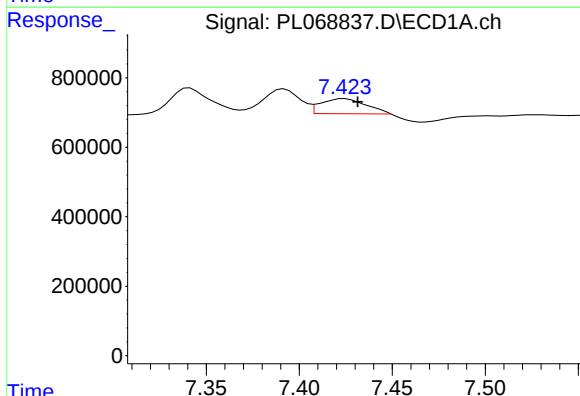


#11 alpha-Chlordane

R.T.: 7.423 min
Delta R.T.: -0.008 min
Response: 708817
Conc: 1.29 ng/ml m

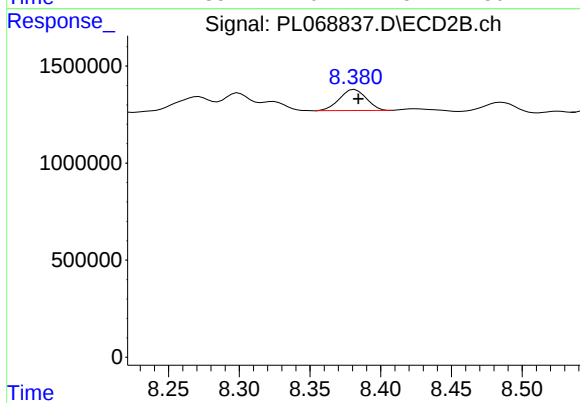

#11 alpha-Chlordane

R.T.: 8.382 min
Delta R.T.: -0.002 min
Response: 1426201
Conc: 1.24 ng/ml

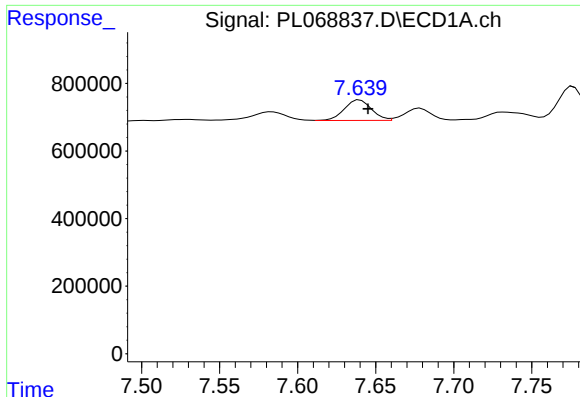


#12 4,4'-DDE

R.T.: 7.639 min
Delta R.T.: -0.006 min
Response: 734719
Conc: 1.52 ng/ml m

Instrument :
ECD_L
ClientSampleId :
MDE-NB


Manual Integrations
APPROVED

Ankita
8/10/2021 12:54:55 PM

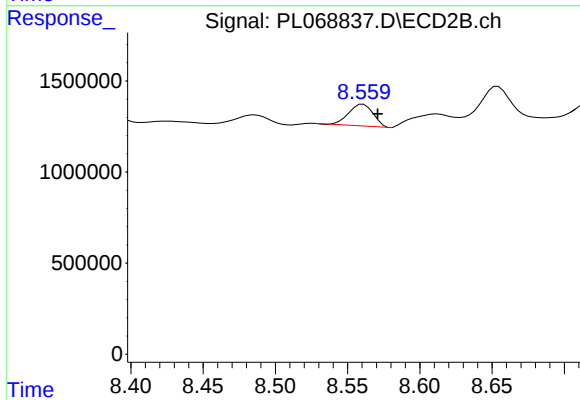


#12 4,4'-DDE

R.T.: 8.561 min
Delta R.T.: -0.010 min
Response: 1397051
Conc: 1.32 ng/ml

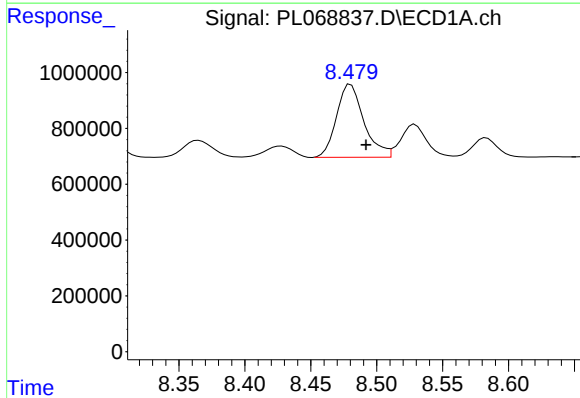


#17 4,4'-DDT

R.T.: 8.480 min
Delta R.T.: -0.012 min
Response: 3788413
Conc: 7.80 ng/ml

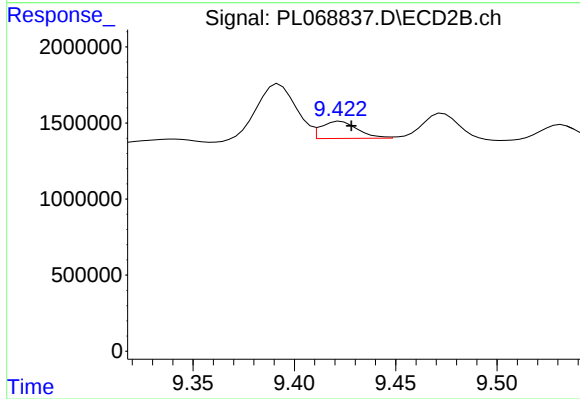

#17 4,4'-DDT

R.T.: 9.422 min
Delta R.T.: -0.007 min
Response: 1370526
Conc: 1.45 ng/ml m

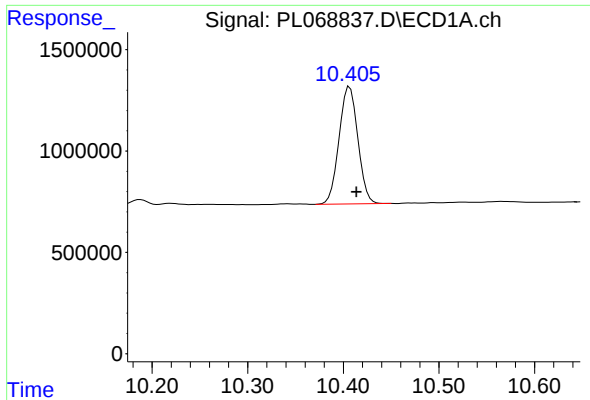


#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.007 min
Response: 7926104
Conc: 13.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDE-NB

Manual Integrations
APPROVED

Ankita
8/10/2021 12:54:55 PM

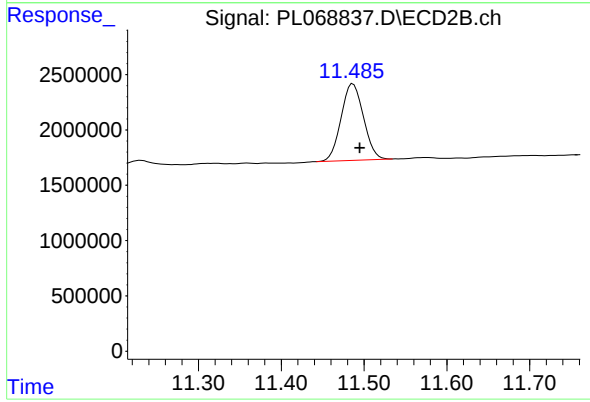

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 12987212
Conc: 13.39 ng/ml