

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 18:22
 Operator : AR\AJ
 Sample : PB138290BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138290BL

Manual Integrations
 APPROVED

Ankita
 8/10/2021 12:54:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 08:33:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.566	8118729	22794704	19.628m	22.450
28)	SA Decachlor...	10.414	11.492	12411357	20508395	21.596	21.137

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 18:22
Operator : AR\AJ
Sample : PB138290BL
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB138290BL


Manual Integrations
APPROVED

Ankita
8/10/2021 12:54:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:33:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

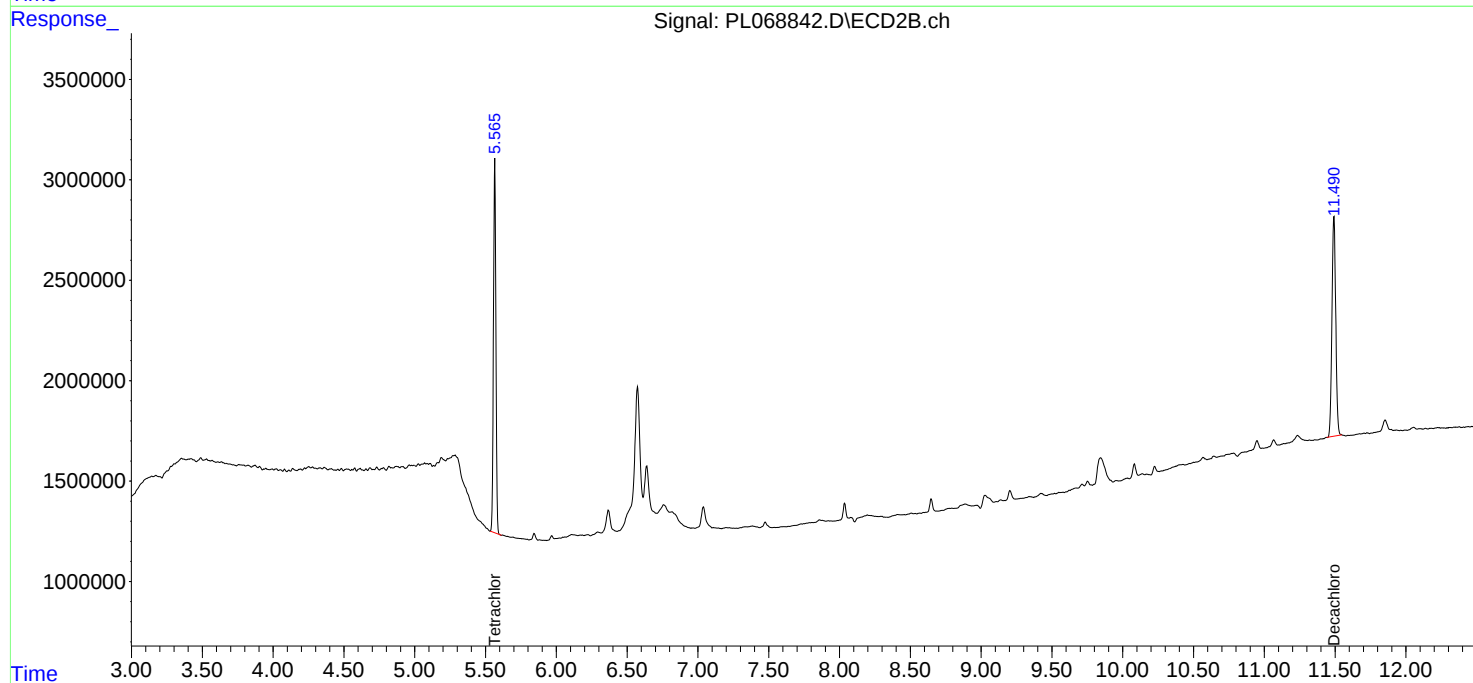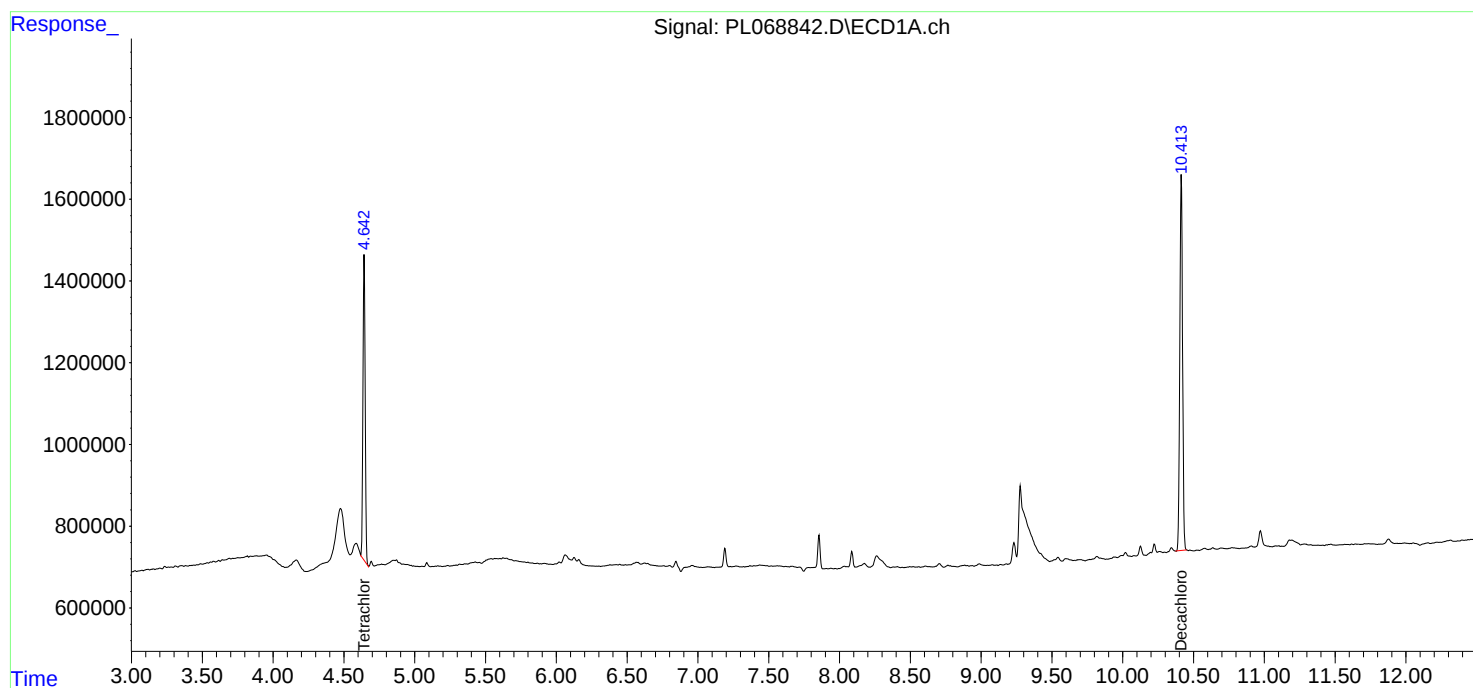

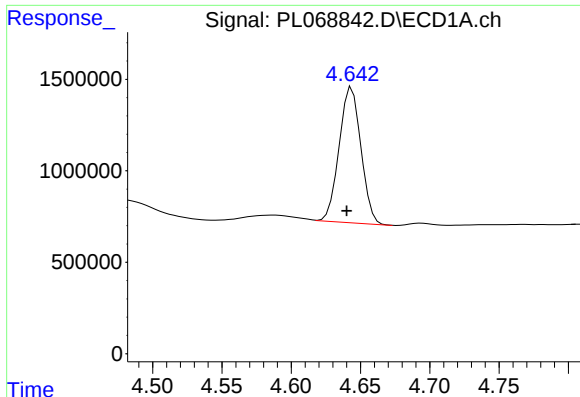


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.002 min
Response: 8118729
Conc: 19.63 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PB138290BL


Manual Integrations
APPROVED

Ankita
8/10/2021 12:54:58 PM

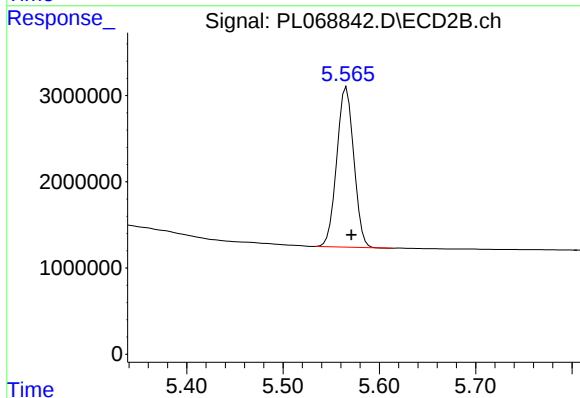


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.005 min
Response: 22794704
Conc: 22.45 ng/ml

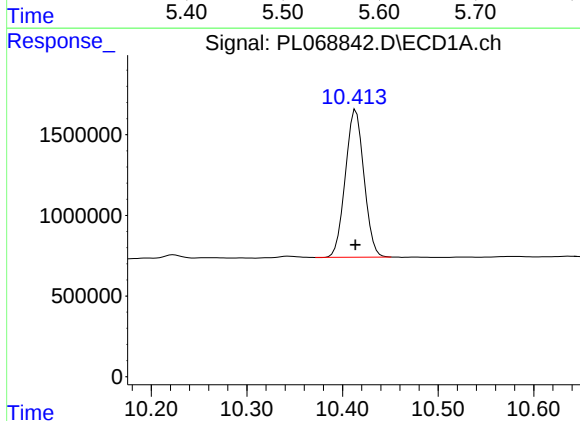

#28 Decachlorobiphenyl

R.T.: 10.414 min
Delta R.T.: 0.000 min
Response: 12411357
Conc: 21.60 ng/ml

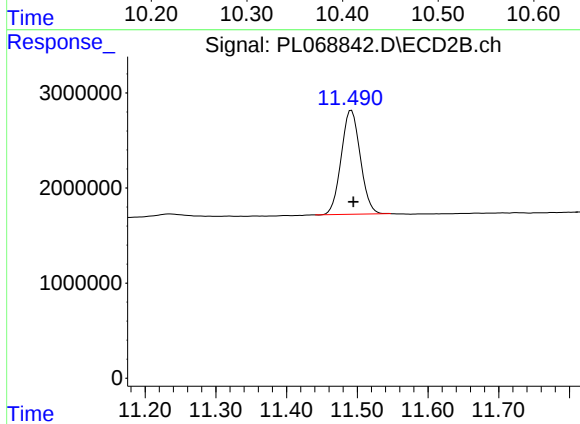

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: -0.003 min
Response: 20508395
Conc: 21.14 ng/ml