

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
 Data File : PL068852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 22:16
 Operator : AR\AJ
 Sample : M3314-01 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 72-11931

Manual Integrations
 APPROVED

Ankita
 8/10/2021 12:55:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 08:54:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.634	5.567	729469	1691070	1.764m	1.666
28) SA Decachlor...	10.404	11.485	1320213	2061800	2.297	2.125

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080921\
Data File : PL068852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 22:16
Operator : AR\AJ
Sample : M3314-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
72-11931


Manual Integrations
APPROVED

Ankita
8/10/2021 12:55:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 08:54:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

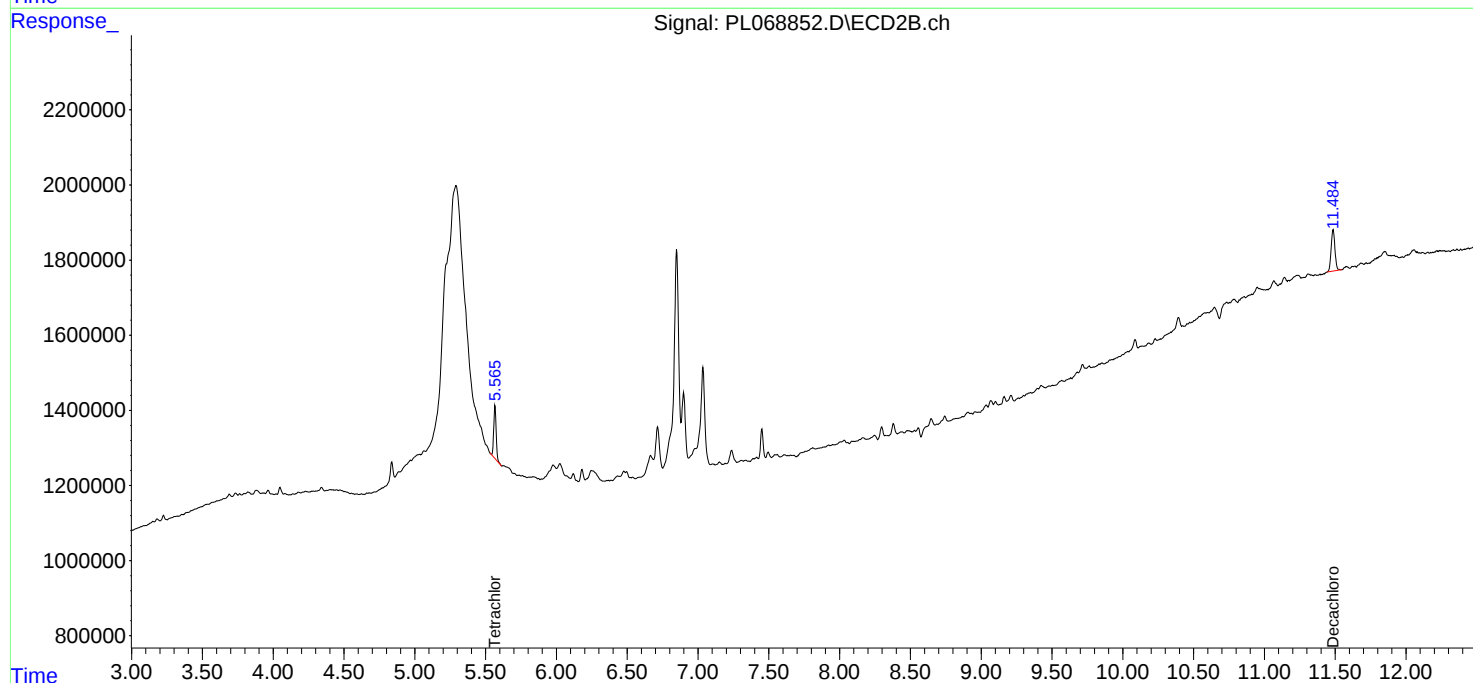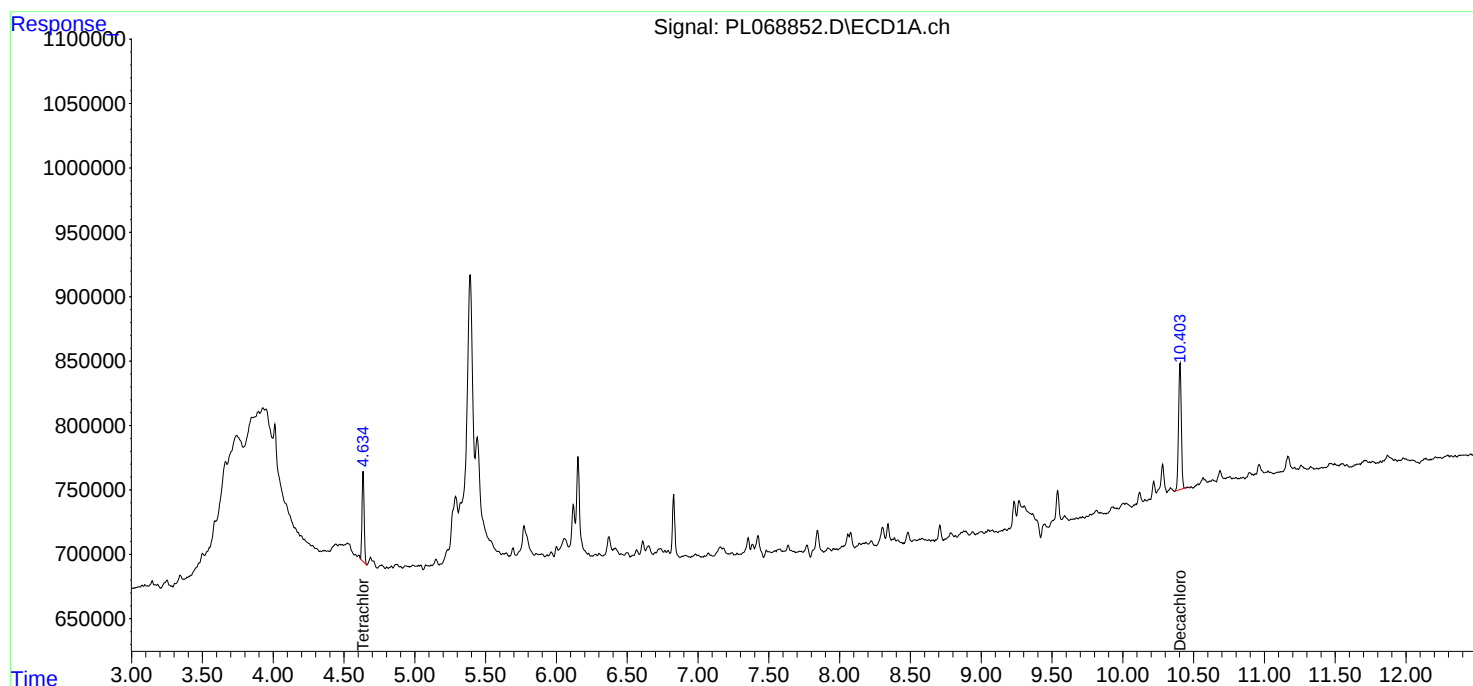

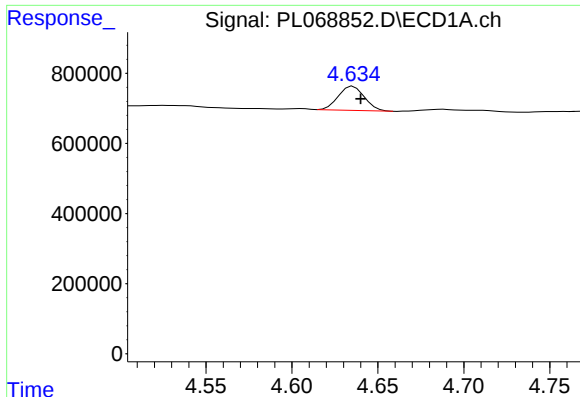


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: -0.006 min
Response: 729469
Conc: 1.76 ng/ml m

Instrument :
ECD_L
ClientSampleId :
72-11931


Manual Integrations
APPROVED

Ankita
8/10/2021 12:55:04 PM

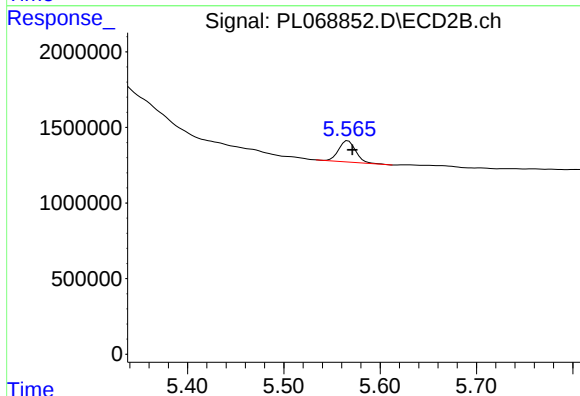


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: -0.004 min
Response: 1691070
Conc: 1.67 ng/ml

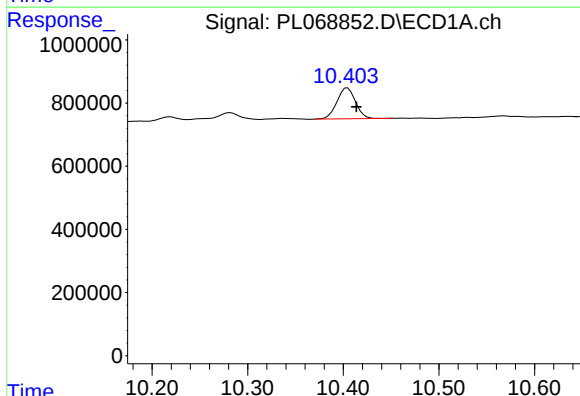

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.009 min
Response: 1320213
Conc: 2.30 ng/ml

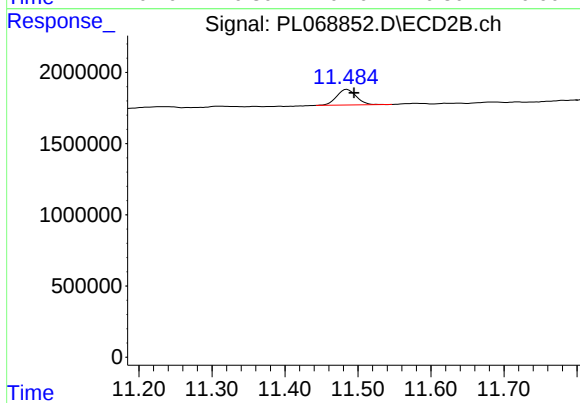

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.010 min
Response: 2061800
Conc: 2.13 ng/ml