

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081124\
 Data File : PL090953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2024 06:14
 Operator : AR\AJ
 Sample : P3478-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TS07

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/12/2024
 Supervised By :Ankita Jodhani 08/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 06:28:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 06 10:55:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.784	36753377	33136415	18.982m	19.167m
28)	SA Decachlor...	9.055	7.927	28288595	31860495	19.689	19.088

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081124\
Data File : PL090953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2024 06:14
Operator : AR\AJ
Sample : P3478-09
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TS07


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/12/2024
Supervised By : Ankita Jodhani 08/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 06:28:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Tue Aug 06 10:55:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

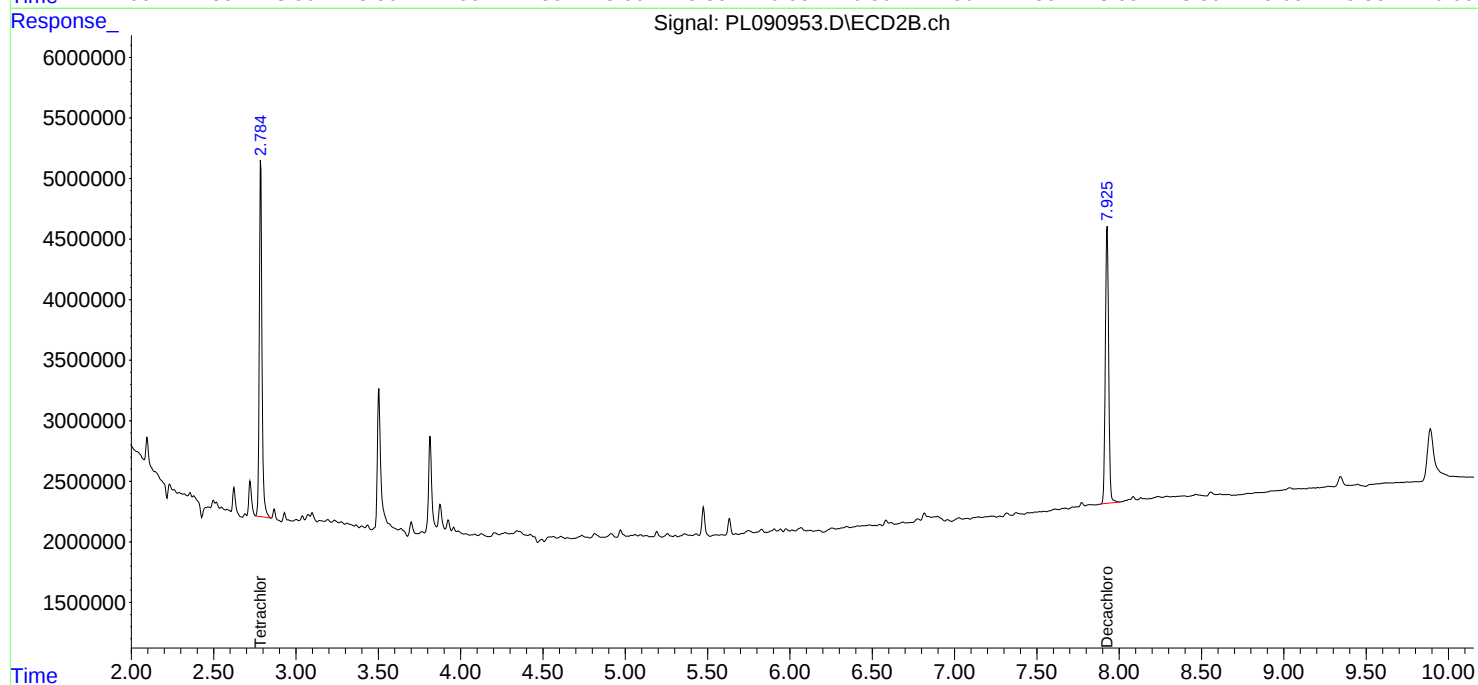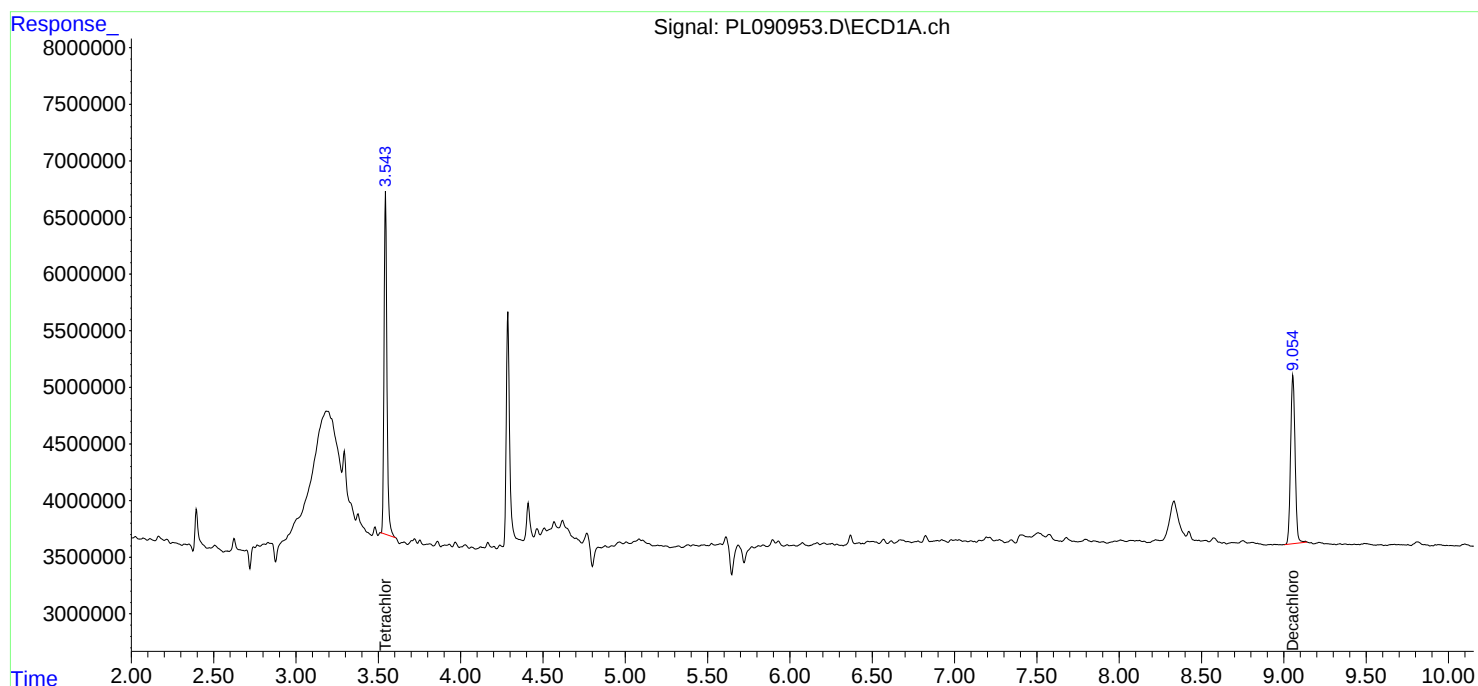

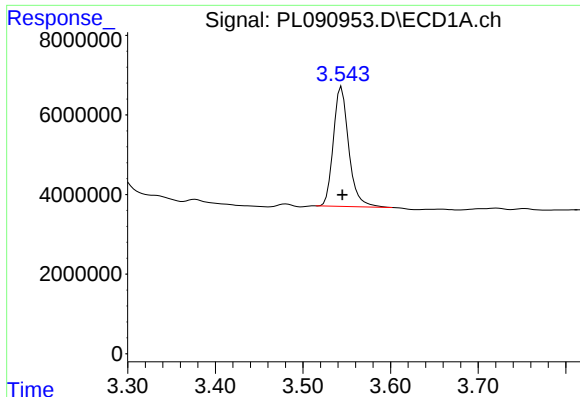


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 36753377
Conc: 18.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TS07


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/12/2024
Supervised By :Ankita Jodhani 08/12/2024

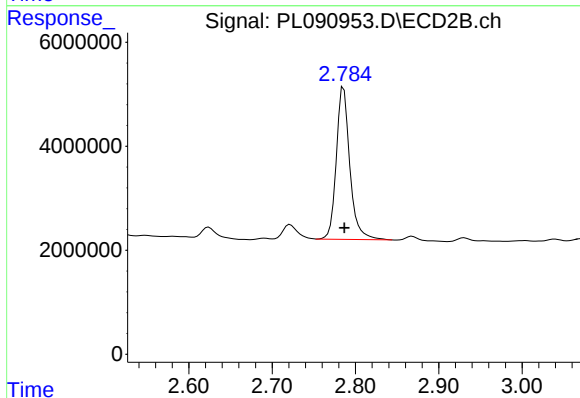


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: -0.002 min
Response: 33136415
Conc: 19.17 ng/ml m

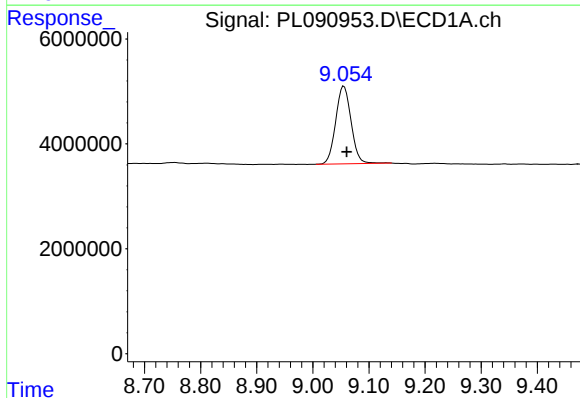

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: -0.005 min
Response: 28288595
Conc: 19.69 ng/ml

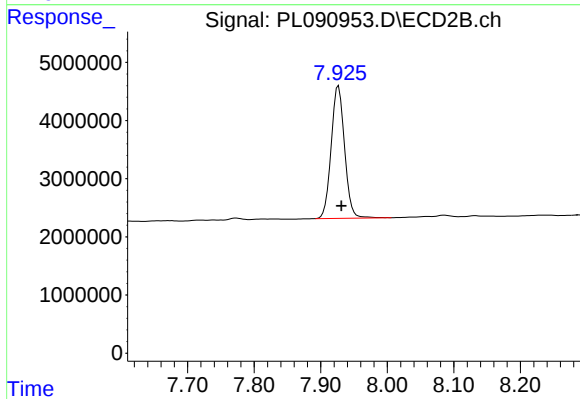

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: -0.004 min
Response: 31860495
Conc: 19.09 ng/ml