

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081124\
 Data File : PL090964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2024 09:26
 Operator : AR\AJ
 Sample : P3519-23
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU4-CF-04-080624

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/12/2024
 Supervised By : Ankita Jodhani 08/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 01:57:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 06 10:55:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.787	28897310	24570988	14.924m	14.213
2) SA Decachlor...	9.061	7.930	23366726	23490776	16.264	14.073

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081124\
Data File : PL090964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2024 09:26
Operator : AR\AJ
Sample : P3519-23
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OU4-CF-04-080624


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/12/2024
Supervised By : Ankita Jodhani 08/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 01:57:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Tue Aug 06 10:55:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

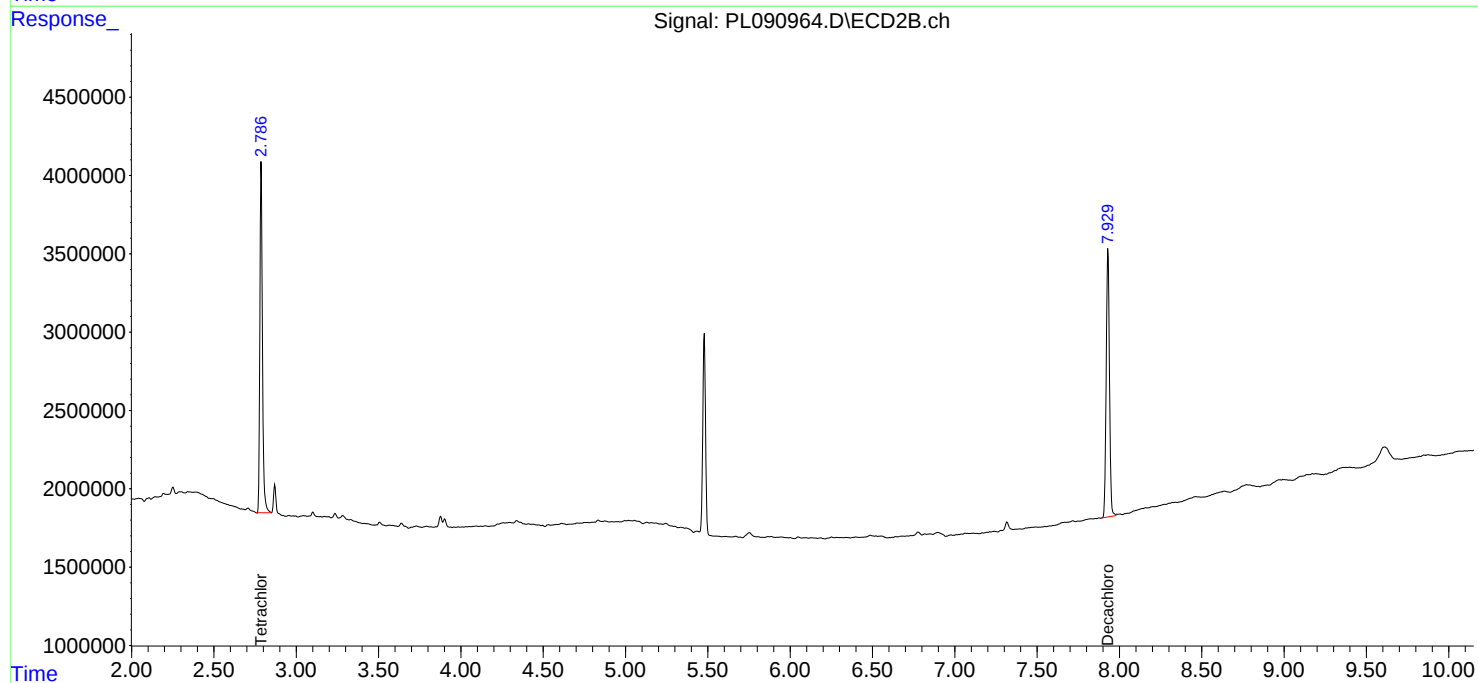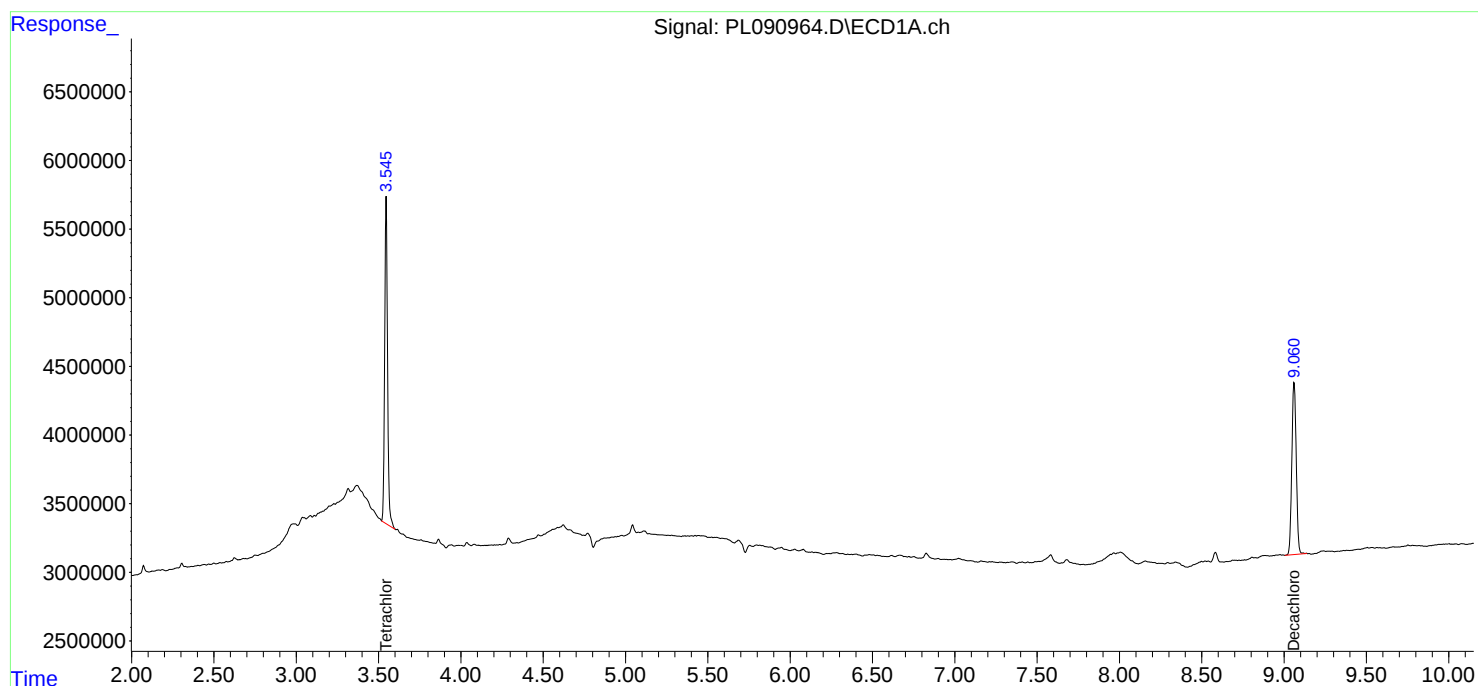

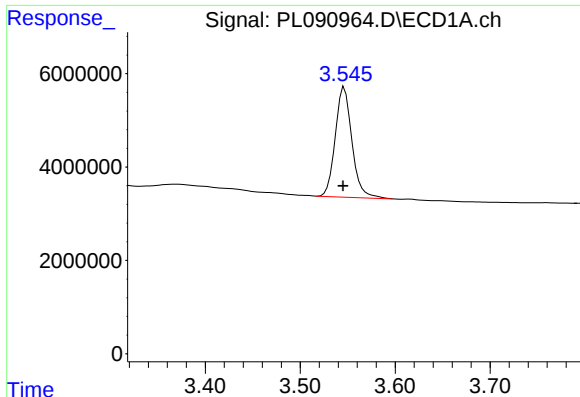


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 28897310
Conc: 14.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU4-CF-04-080624


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/12/2024
Supervised By :Ankita Jodhani 08/12/2024

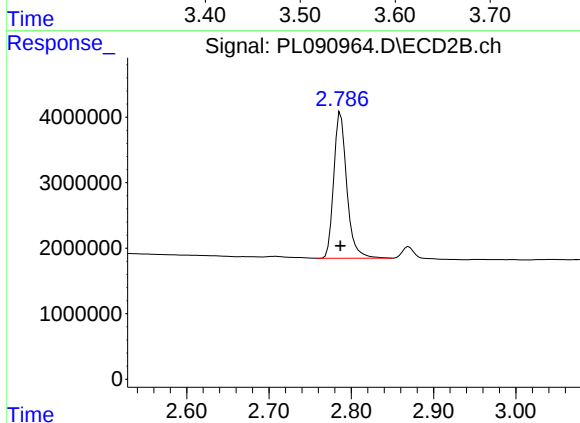


#1 Tetrachloro-m-xylene

R.T.: 2.787 min
Delta R.T.: 0.000 min
Response: 24570988
Conc: 14.21 ng/ml

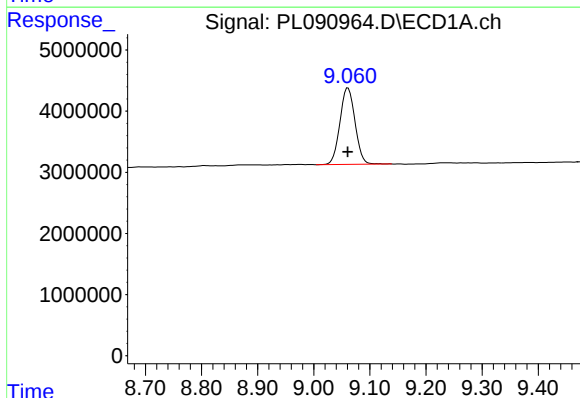

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 23366726
Conc: 16.26 ng/ml

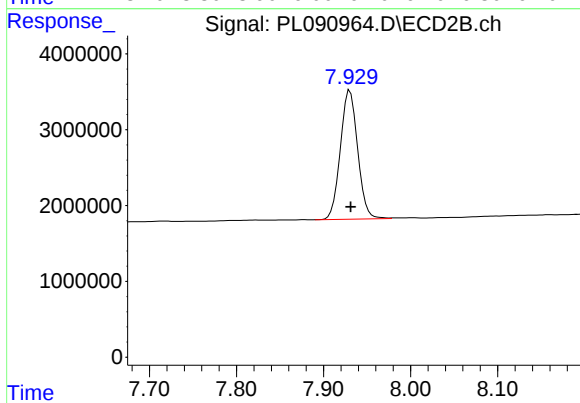

#28 Decachlorobiphenyl

R.T.: 7.930 min
Delta R.T.: 0.000 min
Response: 23490776
Conc: 14.07 ng/ml