

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081919\
 Data File : PL051615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2019 15:20
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 17:56:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 17:55:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.928	492.5E6	108.9E6	50.000	50.000
28)	SA Decachlor...	7.979	8.956	583.8E6	143.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.159	4.913	161.1E6	45343097	500.000	500.000
24)	Chlordane-2	4.649	5.380	204.4E6	50185300	500.000	500.000
25)	Chlordane-3	5.204	6.023	649.2E6	222.8E6	500.000	500.000
26)	Chlordane-4	5.258	6.096	609.7E6	271.6E6	500.000	500.000
27)	Chlordane-5	6.079	6.898	245.4E6	49291636	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081919\
Data File : PL051615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2019 15:20
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 17:56:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 17:55:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

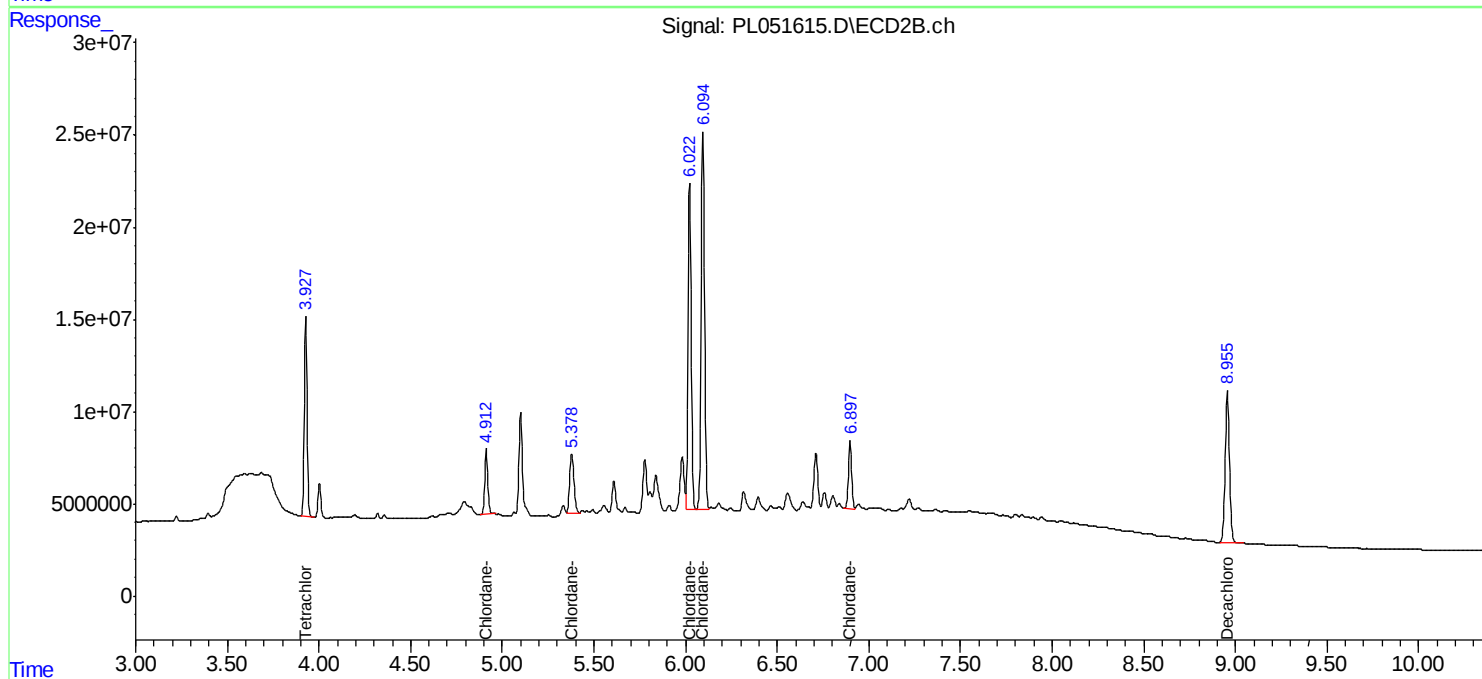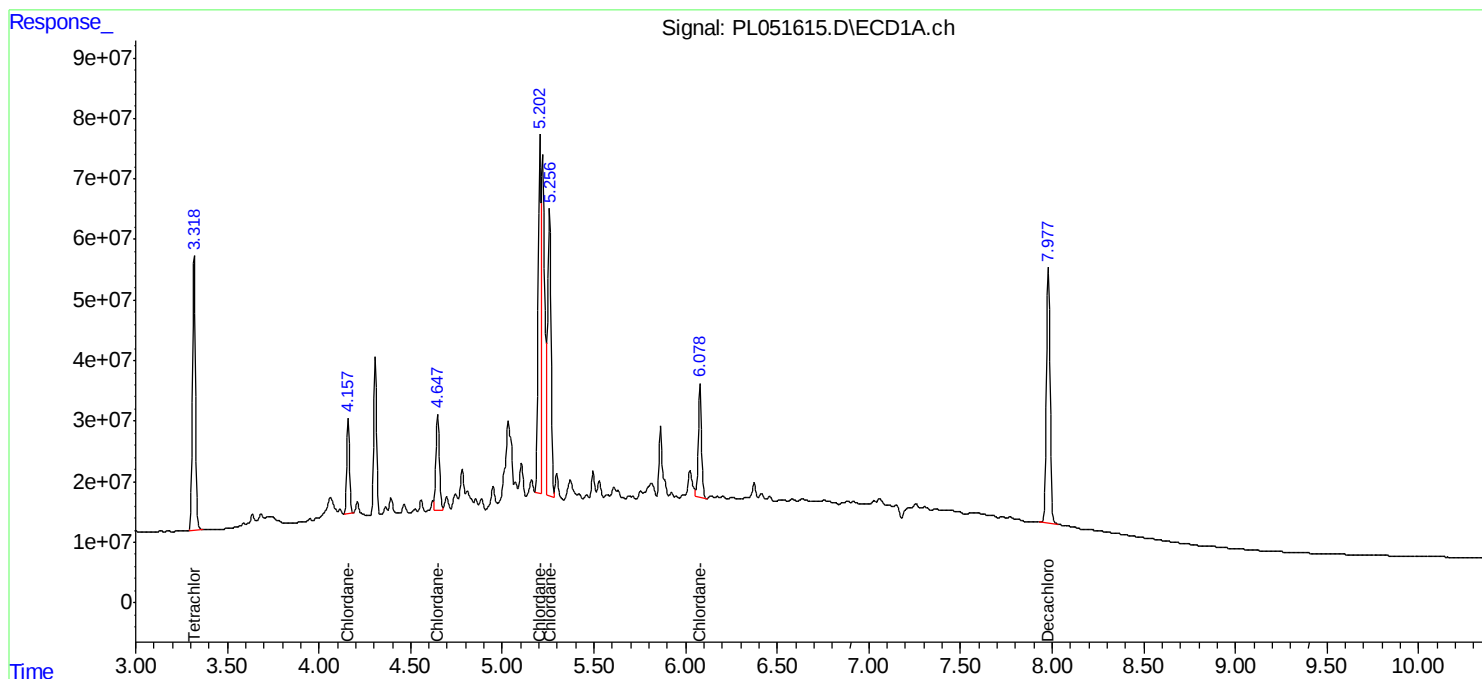


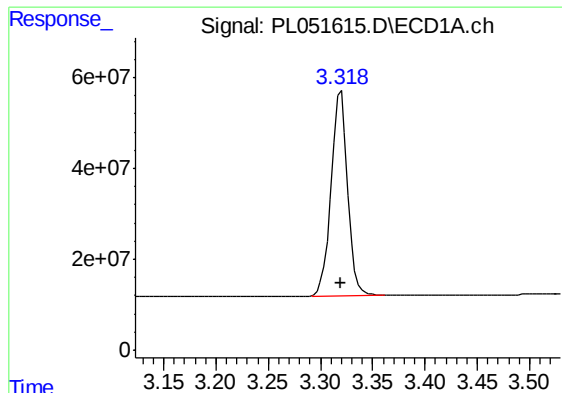

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: 0.000 min
Response: 492513195
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

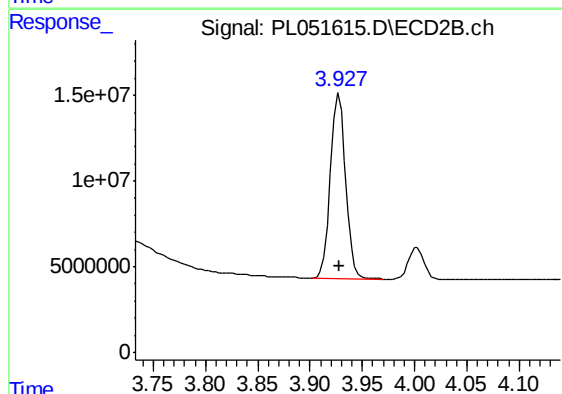


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.000 min
Response: 108865483
Conc: 50.00 ng/ml

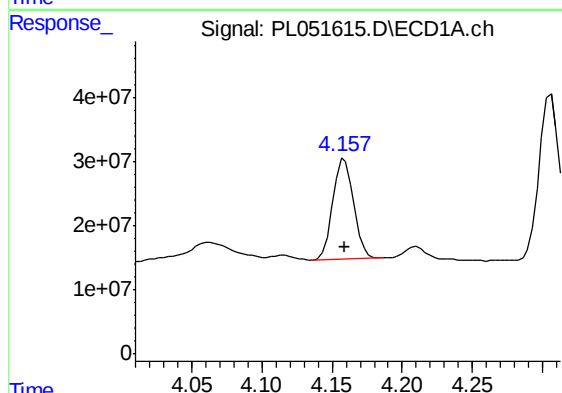


#23 Chlordane-1

R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 161084742
Conc: 500.00 ng/ml

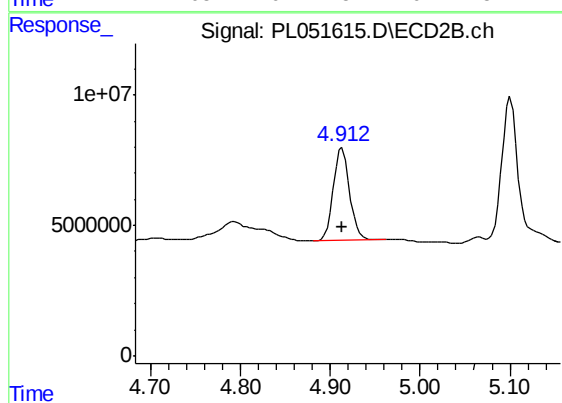

#23 Chlordane-1


R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 45343097
Conc: 500.00 ng/ml

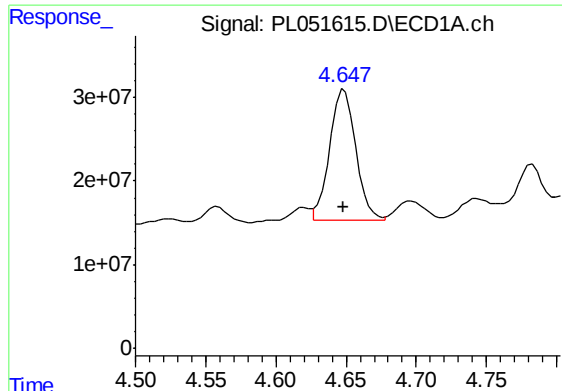

#24 Chlordane-2


R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 204358146
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

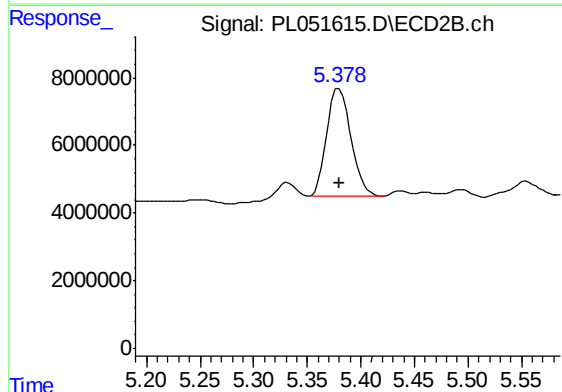


#24 Chlordane-2

R.T.: 5.380 min
Delta R.T.: 0.000 min
Response: 50185300
Conc: 500.00 ng/ml

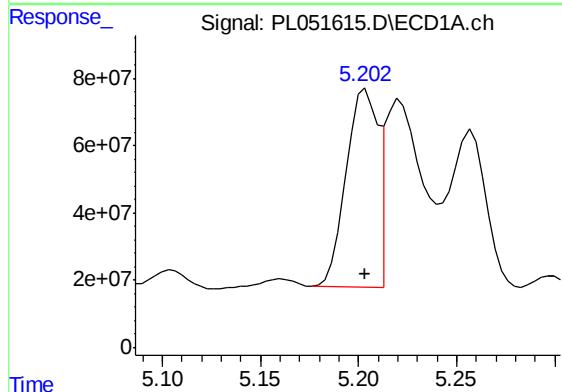


#25 Chlordane-3

R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 649170027
Conc: 500.00 ng/ml

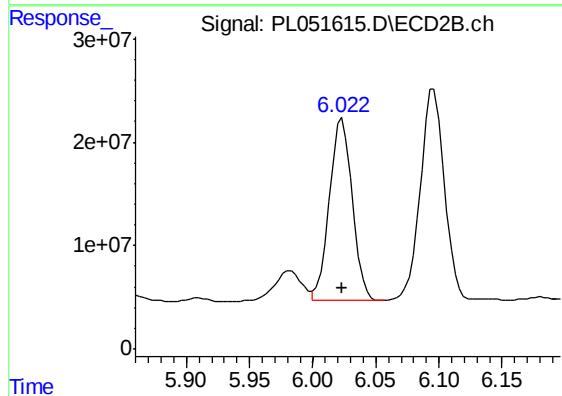

#25 Chlordane-3


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 222769947
Conc: 500.00 ng/ml

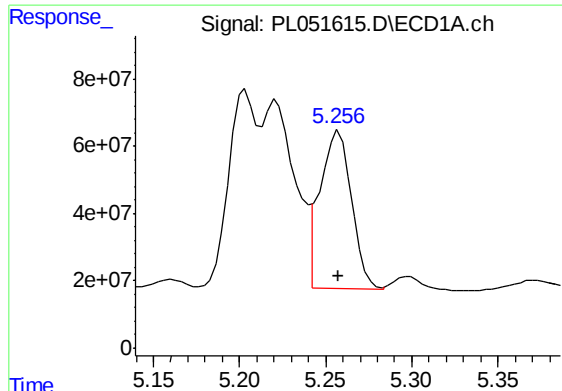

#26 Chlordane-4


R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 609678537
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

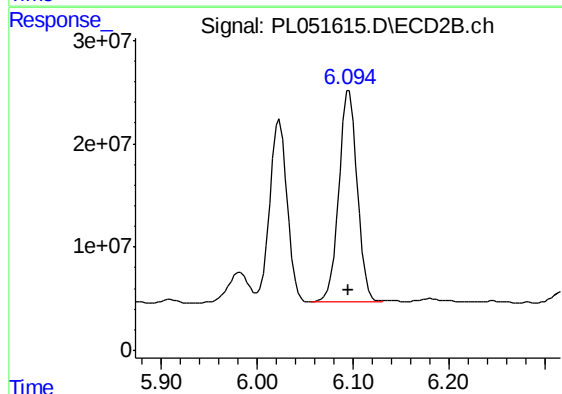


#26 Chlordane-4

R.T.: 6.096 min
Delta R.T.: 0.000 min
Response: 271555914
Conc: 500.00 ng/ml

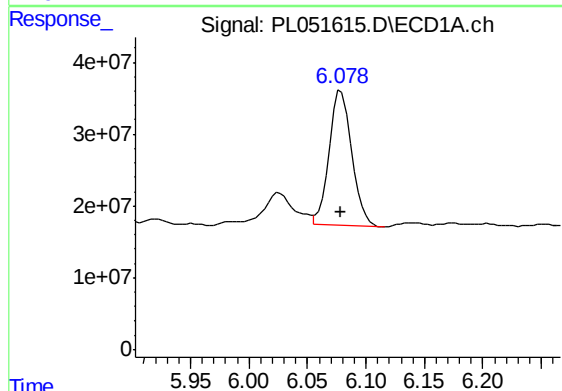


#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 245358705
Conc: 500.00 ng/ml

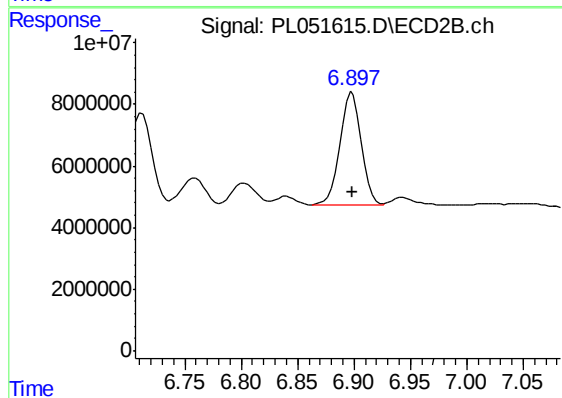

#27 Chlordane-5


R.T.: 6.898 min
Delta R.T.: 0.000 min
Response: 49291636
Conc: 500.00 ng/ml

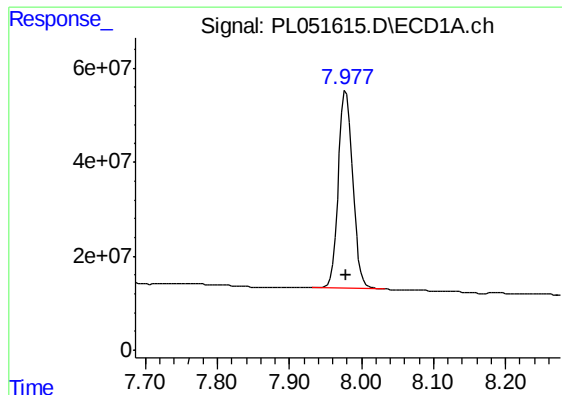

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: 0.000 min
Response: 583840610
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

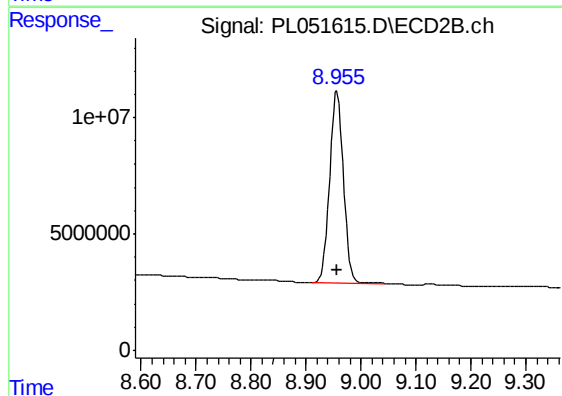

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: 0.000 min
Response: 143584517
Conc: 50.00 ng/ml