

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081919\
 Data File : PL051621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2019 17:33
 Operator : SG\AJ
 Sample : K4319-04DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TRANSFORMER-CONTAINMENT-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 18:26:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.928	28499006	7617843	3.330	3.487
28)	SA Decachlor...	7.979	8.957	32845353	8103774	2.706	2.662
Target Compounds							
15)	B Endosulfa...	6.095f	6.850f	906.1E6	253.4E6	65.122	76.876



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081919\
Data File : PL051621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2019 17:33
Operator : SG\AJ
Sample : K4319-04DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-CONTAINMENT-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 18:26:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

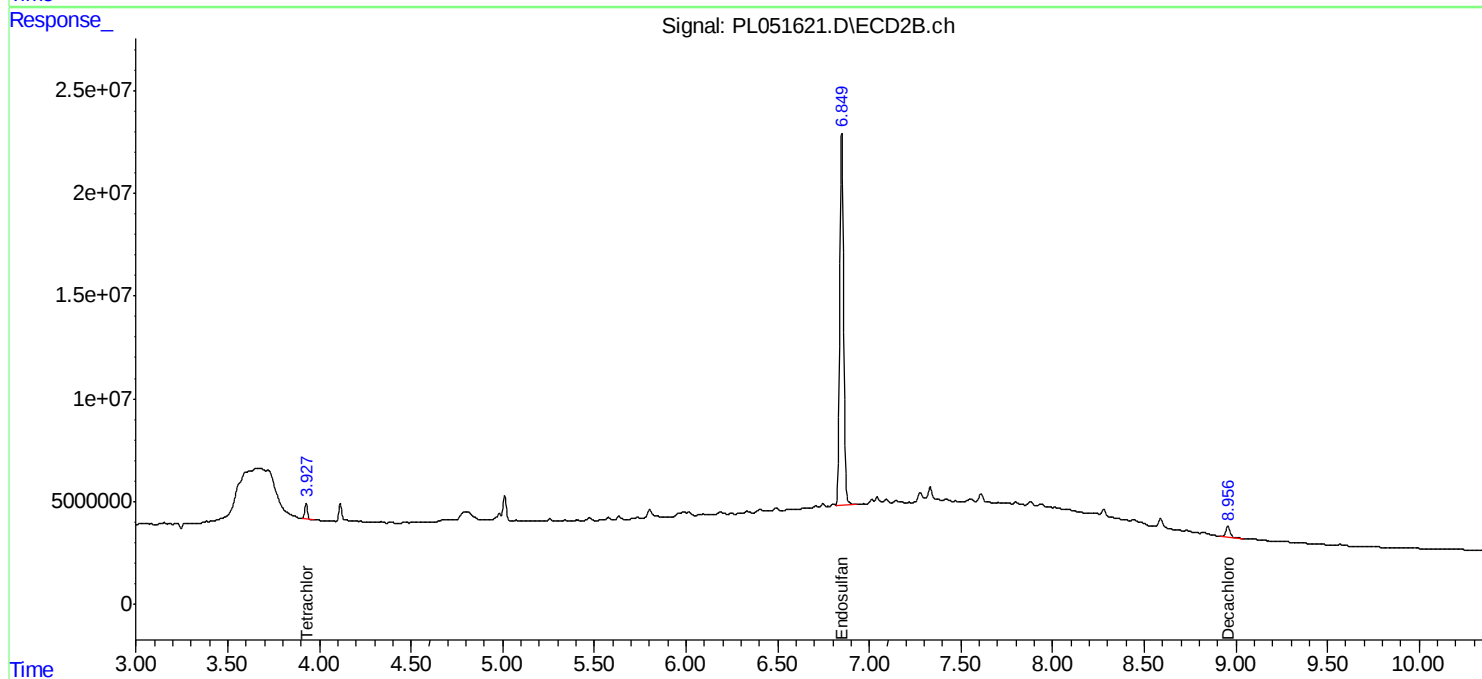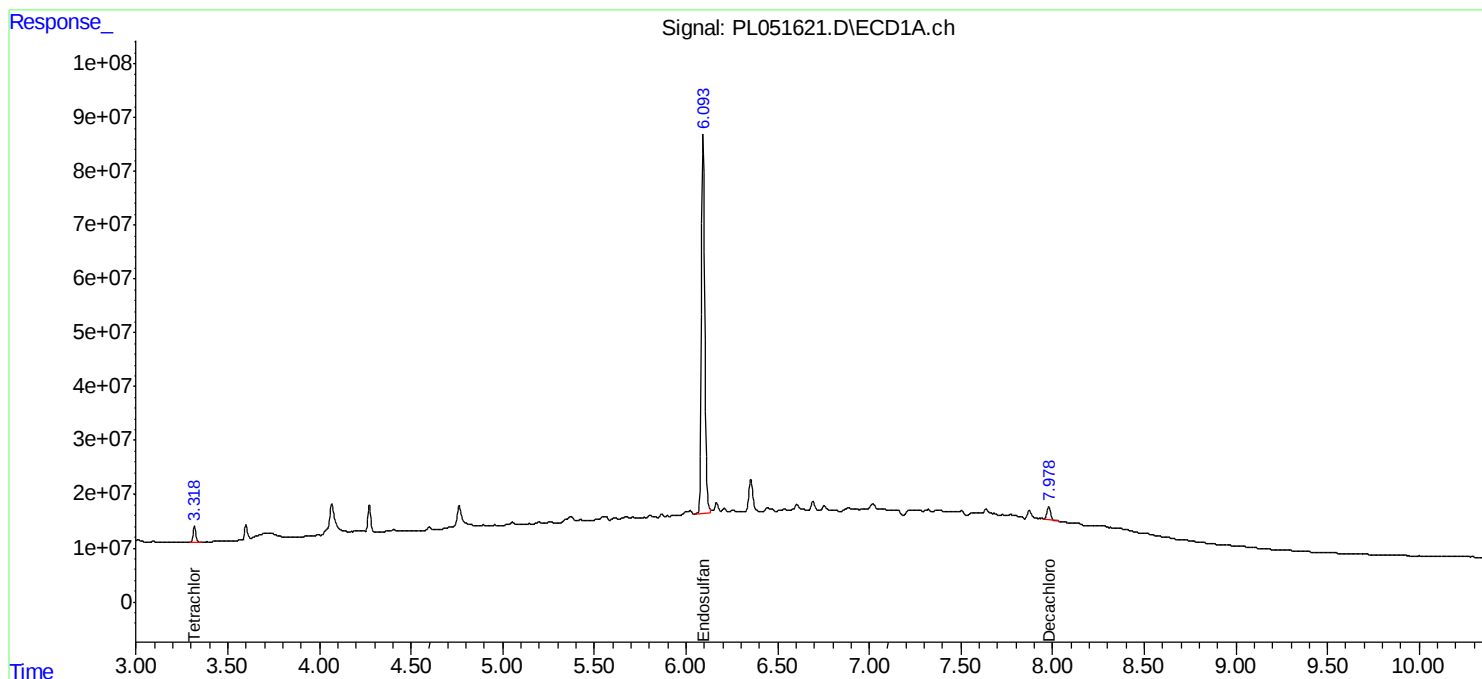


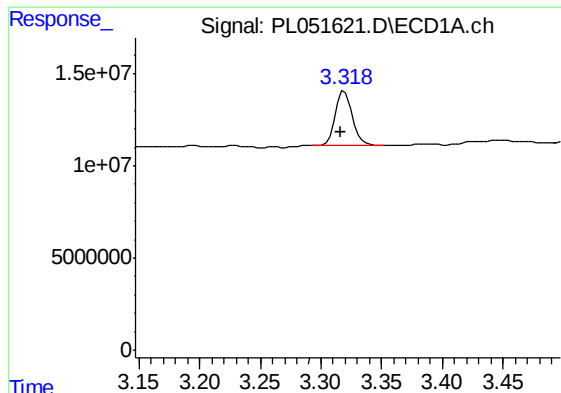

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: 0.004 min
Response: 28499006
Conc: 3.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-CONTAINMENT-S

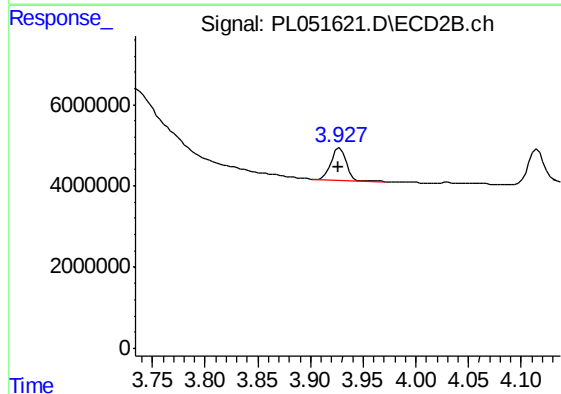


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.001 min
Response: 7617843
Conc: 3.49 ng/ml

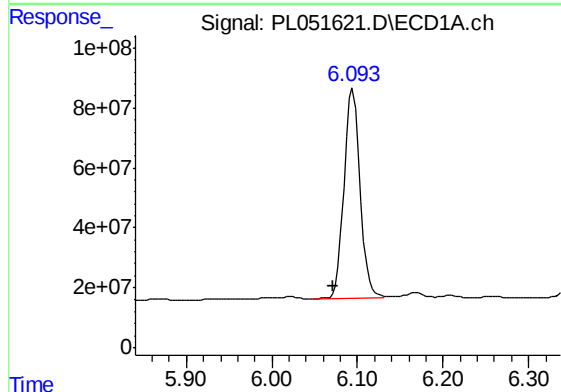


#15 Endosulfan II

R.T.: 6.095 min
Delta R.T.: 0.023 min
Response: 906111326
Conc: 65.12 ng/ml

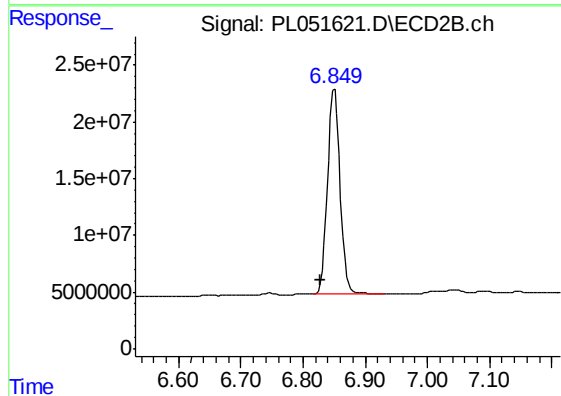

#15 Endosulfan II


R.T.: 6.850 min
Delta R.T.: 0.022 min
Response: 253386535
Conc: 76.88 ng/ml

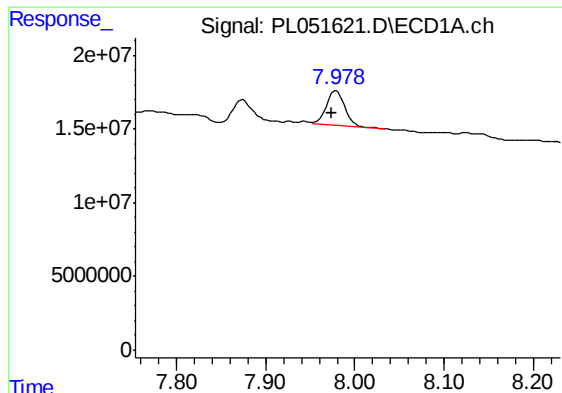

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: 0.005 min
Response: 32845353
Conc: 2.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-CONTAINMENT-S

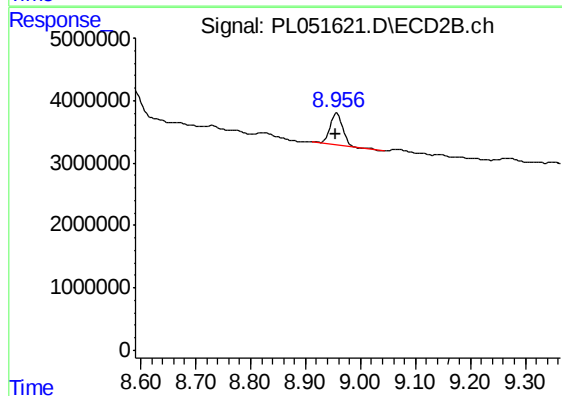

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: 0.003 min
Response: 8103774
Conc: 2.66 ng/ml