

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
 Data File : PL039493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2018 14:48
 Operator : AJ\SJ
 Sample : J4270-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 22:57:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.905	90146959	39280244	12.896	14.652
28)	SA Decachlor...	7.960	8.892	92410652	38254624	13.158	16.485 #
Target Compounds							
5)	MB Aldrin	4.518	0.000	5886114	0	0.588	N.D. #
10)	B gamma-Chl...	5.202	0.000	7457575	0	0.755	N.D. #
11)	B alpha-Chl...	5.202f	0.000	7457575	0	0.776	N.D. #
12)	B 4,4'-DDE	5.407	6.209	19463965	5996599	2.033	1.939
17)	MA 4,4'-DDT	6.152	0.000	5502785	0	0.726	N.D. #
23)	Chlordane-1	4.144	0.000	6633076	0	20.952	N.D. #
25)	Chlordane-3	5.202	0.000	7457575	0	6.828	N.D. #
26)	Chlordane-4	5.202	0.000	7457575	0	7.462	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
Data File : PL039493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2018 14:48
Operator : AJ\SJ
Sample : J4270-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 22:57:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

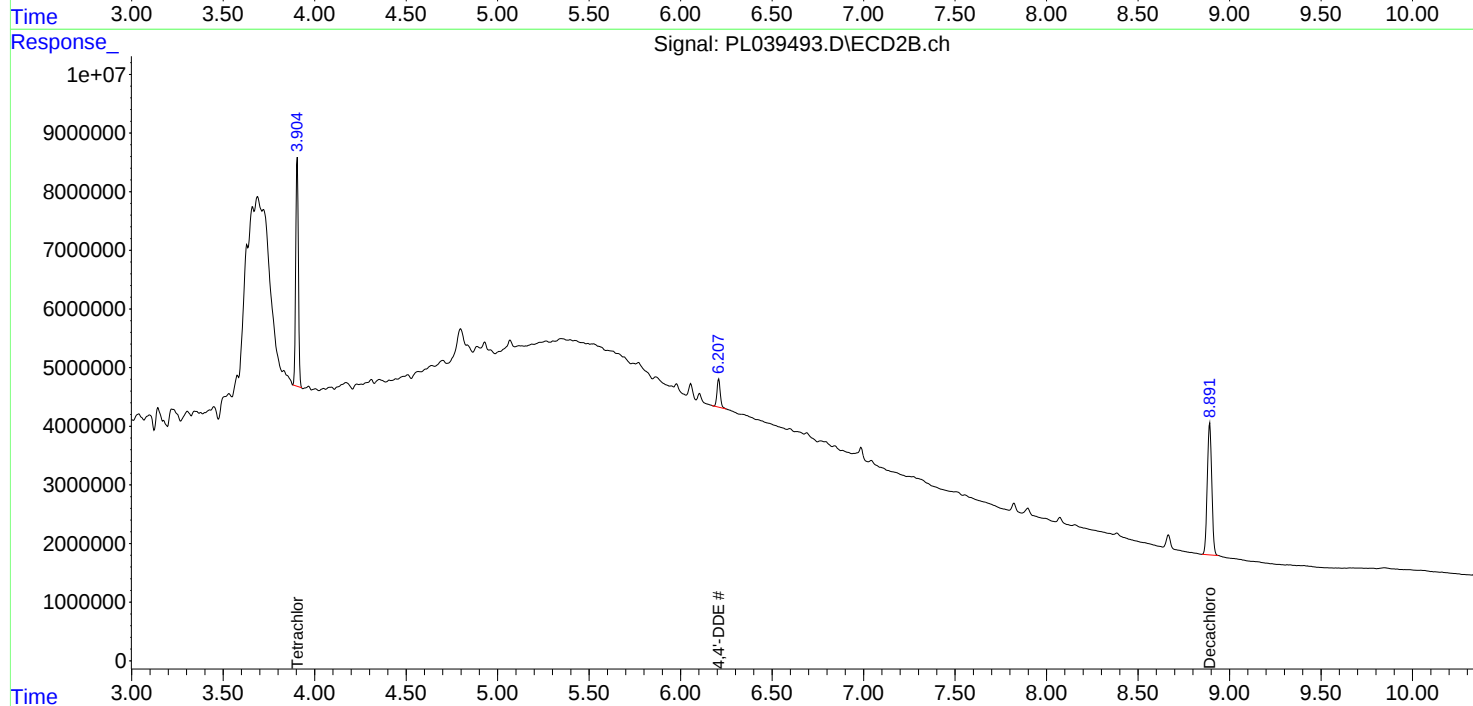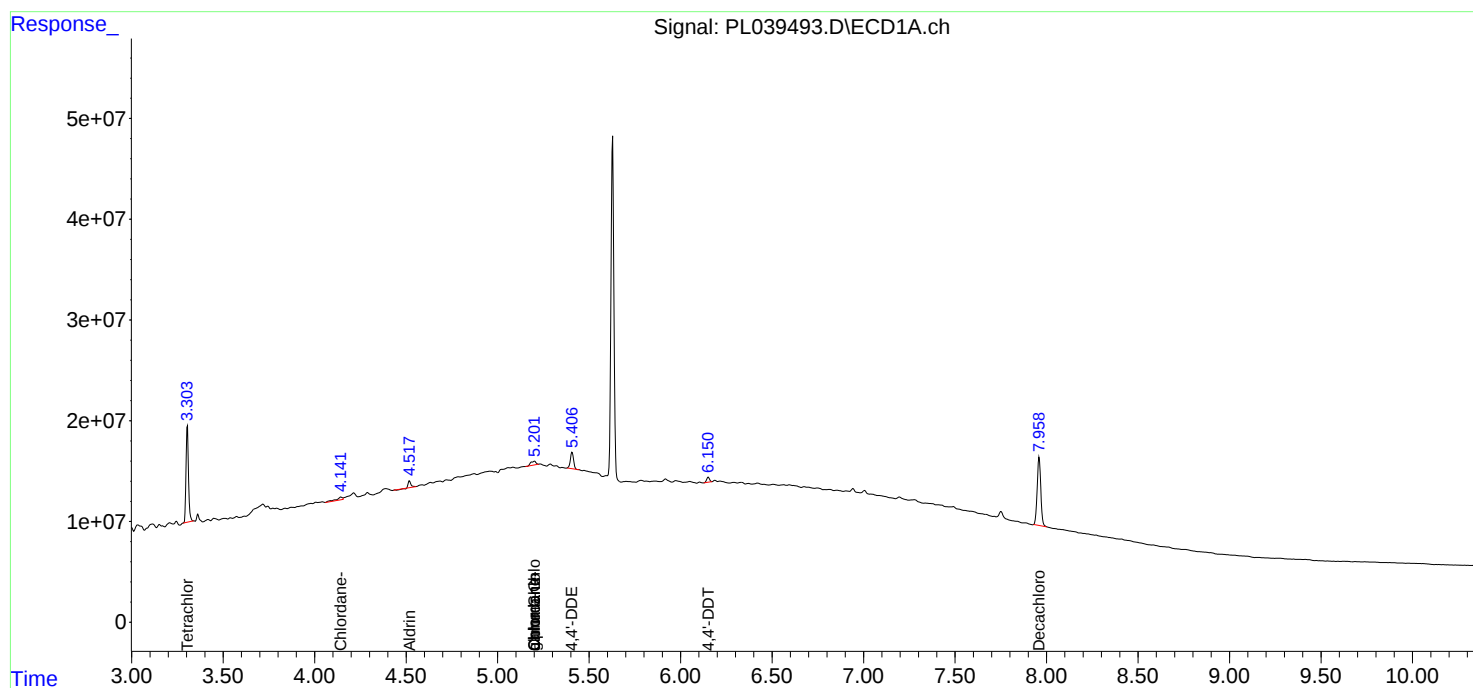


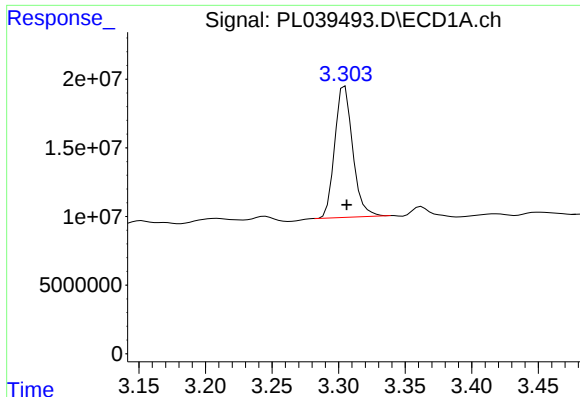

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 90146959
Conc: 12.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

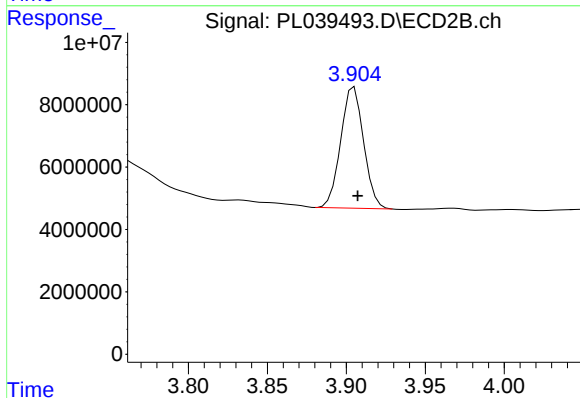


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 39280244
Conc: 14.65 ng/ml

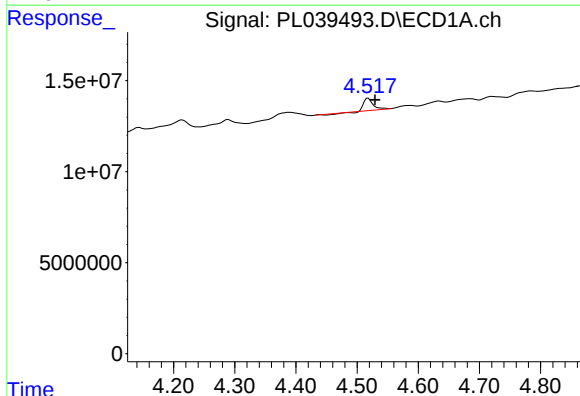


#5 Aldrin

R.T.: 4.518 min
Delta R.T.: -0.011 min
Response: 5886114
Conc: 0.59 ng/ml

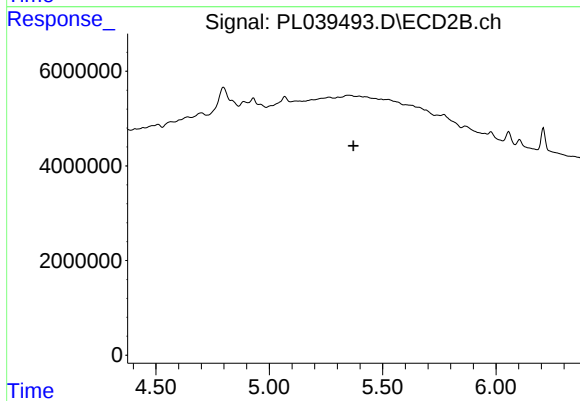

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.372 min
Response: 0
Conc: N.D.

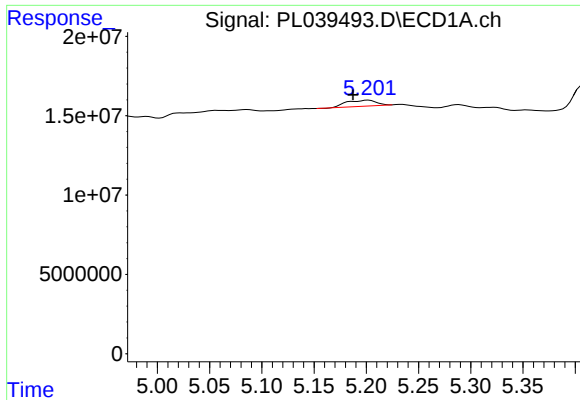

#10 gamma-Chlordane


R.T.: 5.202 min
Delta R.T.: 0.015 min
Response: 7457575
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

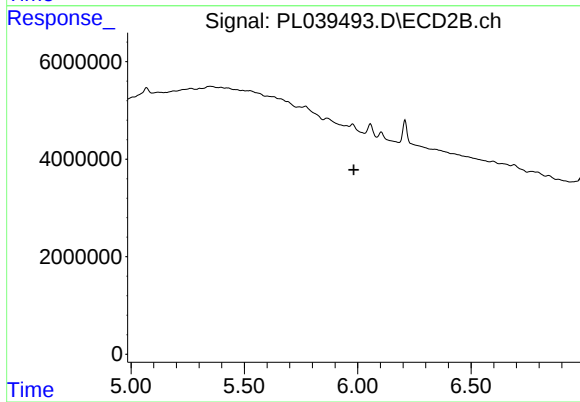


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

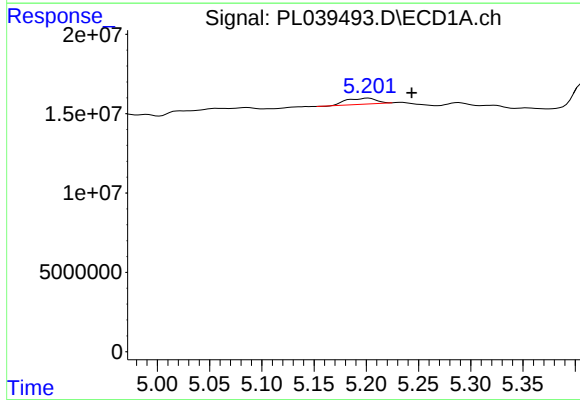


#11 alpha-Chlordane

R.T.: 5.202 min
Delta R.T.: -0.041 min
Response: 7457575
Conc: 0.78 ng/ml

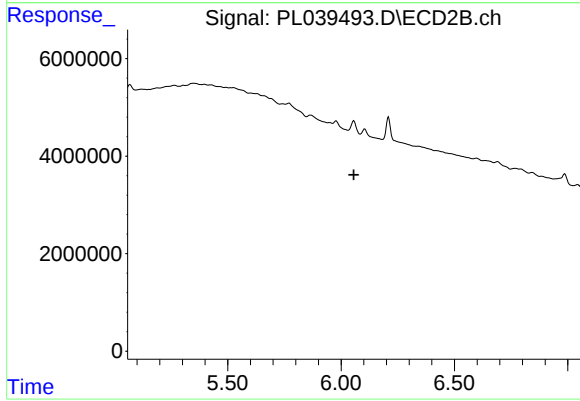

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

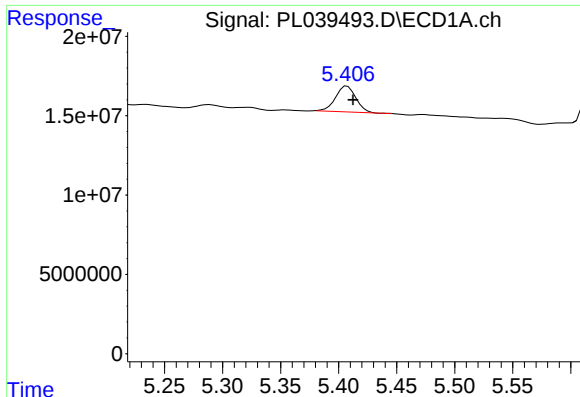

#12 4,4'-DDE


R.T.: 5.407 min
Delta R.T.: -0.005 min
Response: 19463965
Conc: 2.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

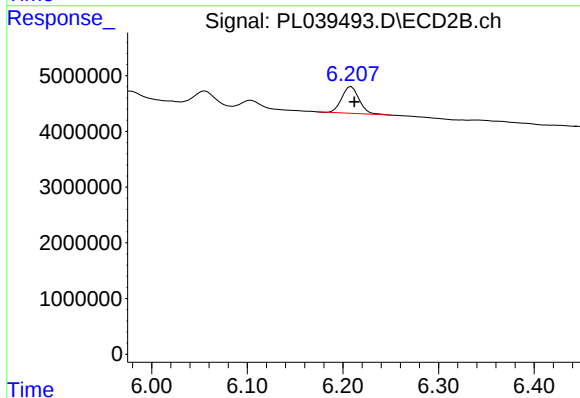


#12 4,4'-DDE

R.T.: 6.209 min
Delta R.T.: -0.003 min
Response: 5996599
Conc: 1.94 ng/ml

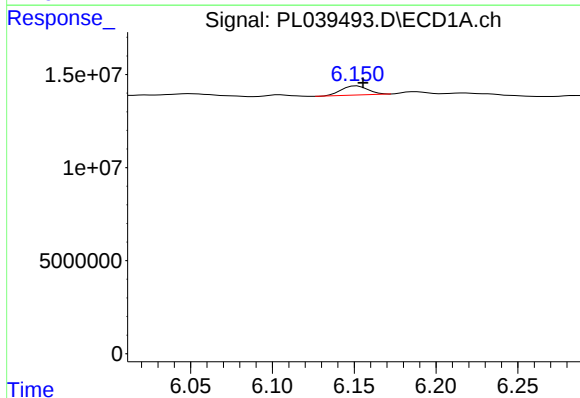


#17 4,4'-DDT

R.T.: 6.152 min
Delta R.T.: -0.004 min
Response: 5502785
Conc: 0.73 ng/ml

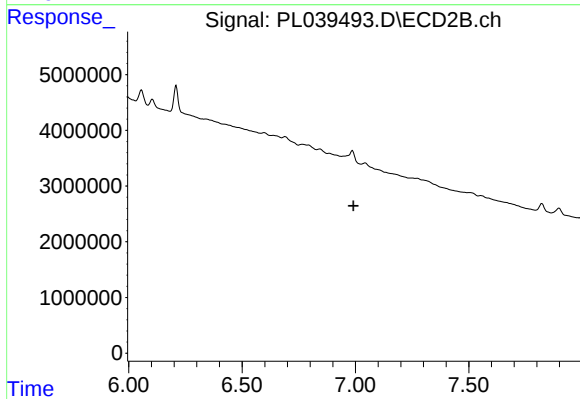

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.991 min
Response: 0
Conc: N.D.

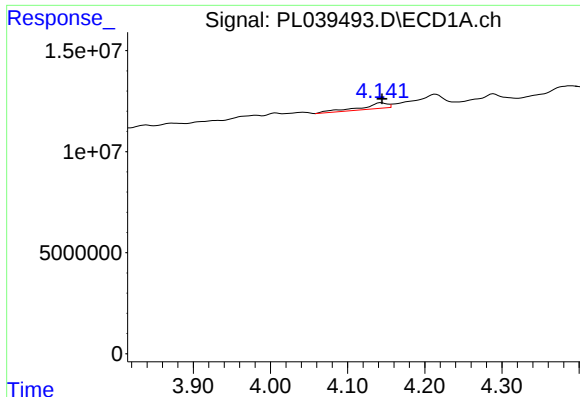

#23 Chlordane-1


R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 6633076
Conc: 20.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

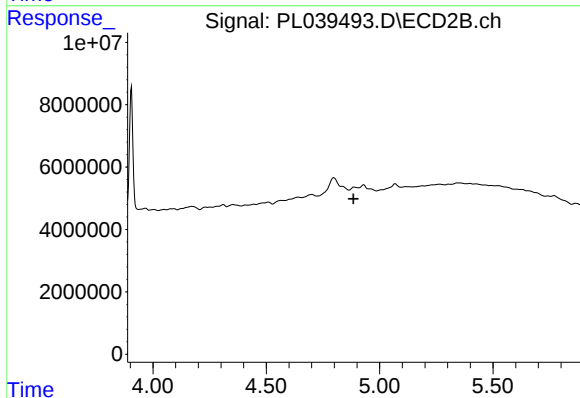


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

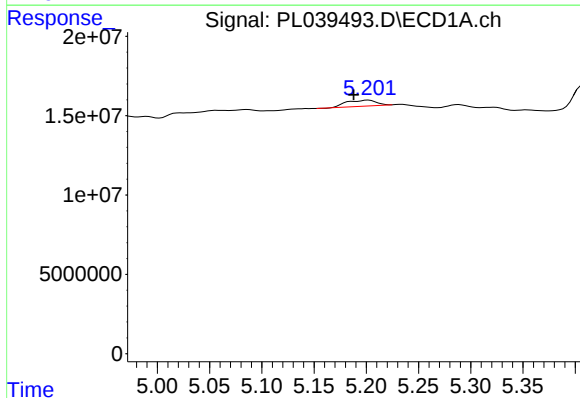


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.014 min
Response: 7457575
Conc: 6.83 ng/ml

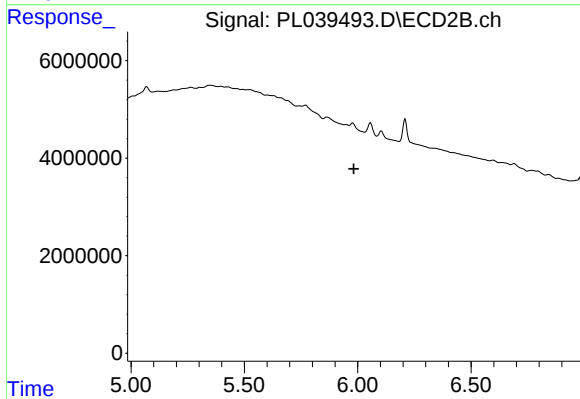

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

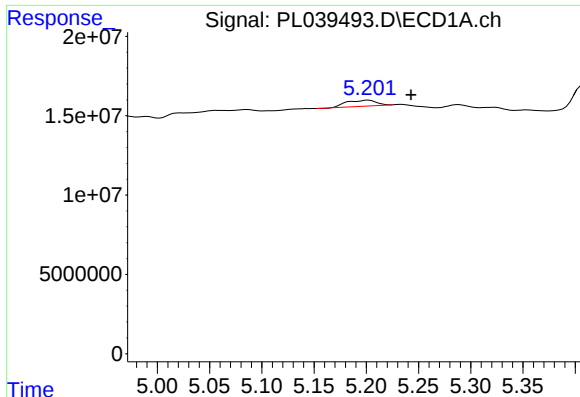

#26 Chlordane-4


R.T.: 5.202 min
Delta R.T.: -0.041 min
Response: 7457575
Conc: 7.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

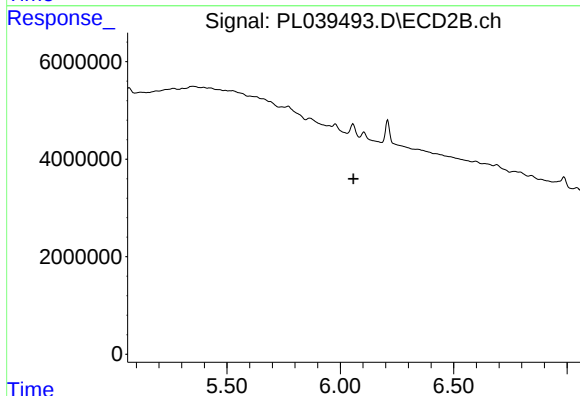


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.058 min
Response: 0
Conc: N.D.

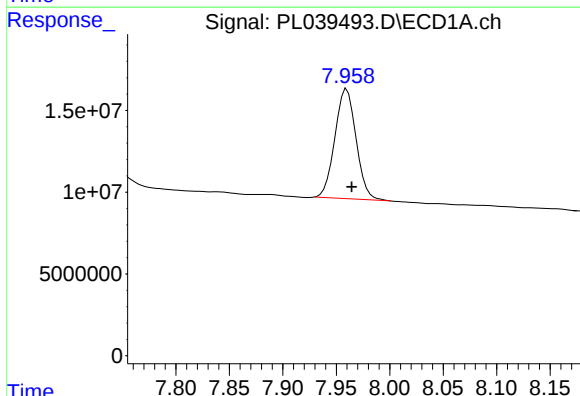

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 92410652
Conc: 13.16 ng/ml

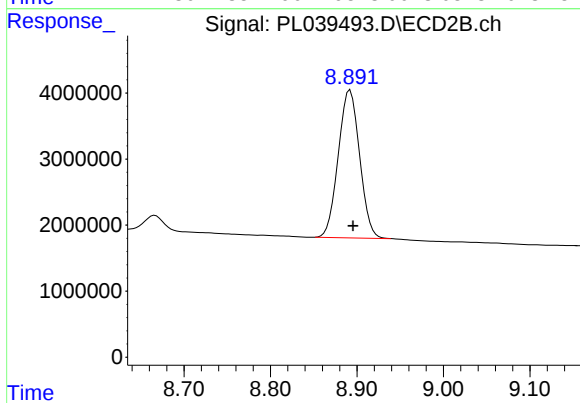

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.003 min
Response: 38254624
Conc: 16.48 ng/ml