

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
 Data File : PL039501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2018 16:41
 Operator : AJ\SJ
 Sample : J4636-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 23:00:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.905	70772999	30845209	10.124	11.506
28)	SA Decachlor...	7.957	8.891	81246516	33605600	11.568	14.481 #
Target Compounds							
2)	A alpha-BHC	3.686f	4.323f	44220337	19021608	3.741	4.517
9)	A Endosulfan I	5.237f	0.000	8766000	0	1.001	N.D. #
10)	B gamma-Chl...	5.201	0.000	10048336	0	1.017	N.D. #
11)	B alpha-Chl...	5.237	0.000	8766000	0	0.912	N.D. #
12)	B 4,4'-DDE	5.406	0.000	7328662	0	0.765	N.D. #
17)	MA 4,4'-DDT	6.146	0.000	4384855	0	0.578	N.D. #
23)	Chlordane-1	4.142	0.000	3102108	0	9.799	N.D. #
25)	Chlordane-3	5.201	0.000	10048336	0	9.200	N.D. #
26)	Chlordane-4	5.237	0.000	8766000	0	8.772	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
Data File : PL039501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2018 16:41
Operator : AJ\SJ
Sample : J4636-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 23:00:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

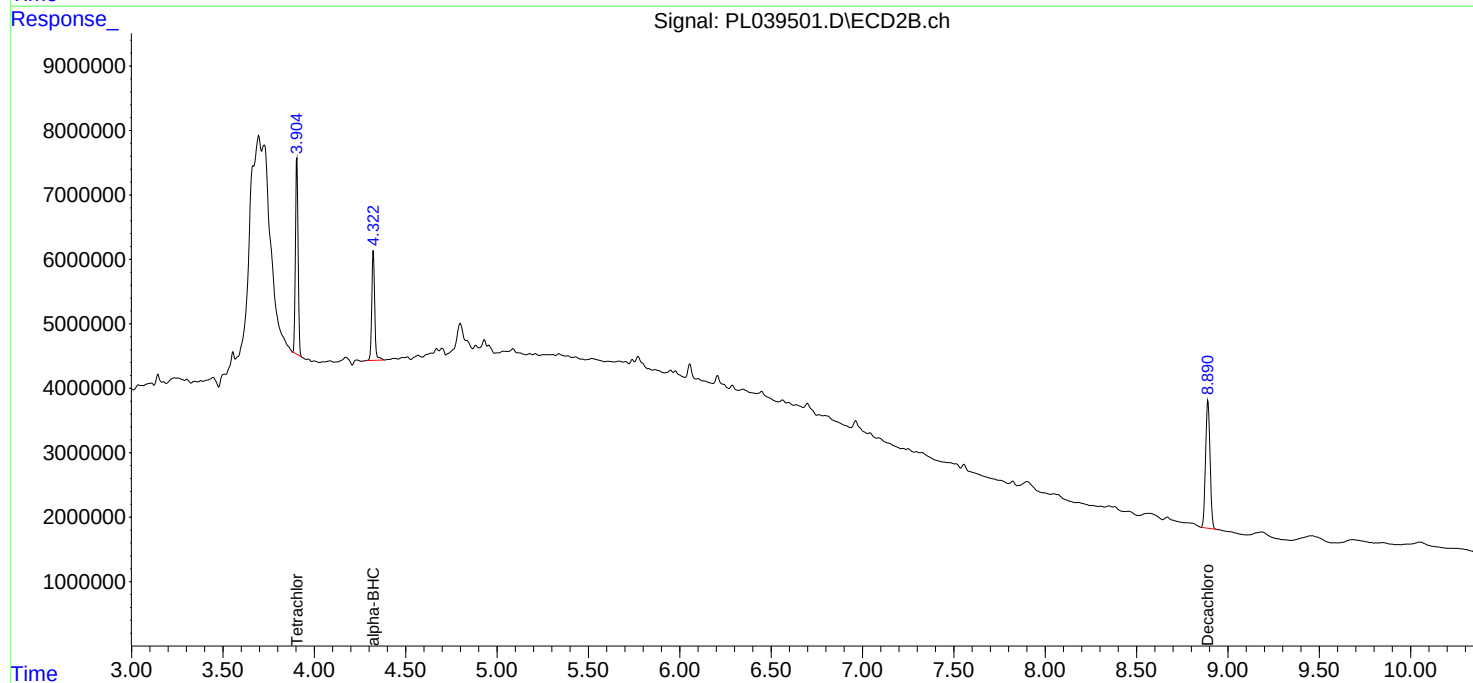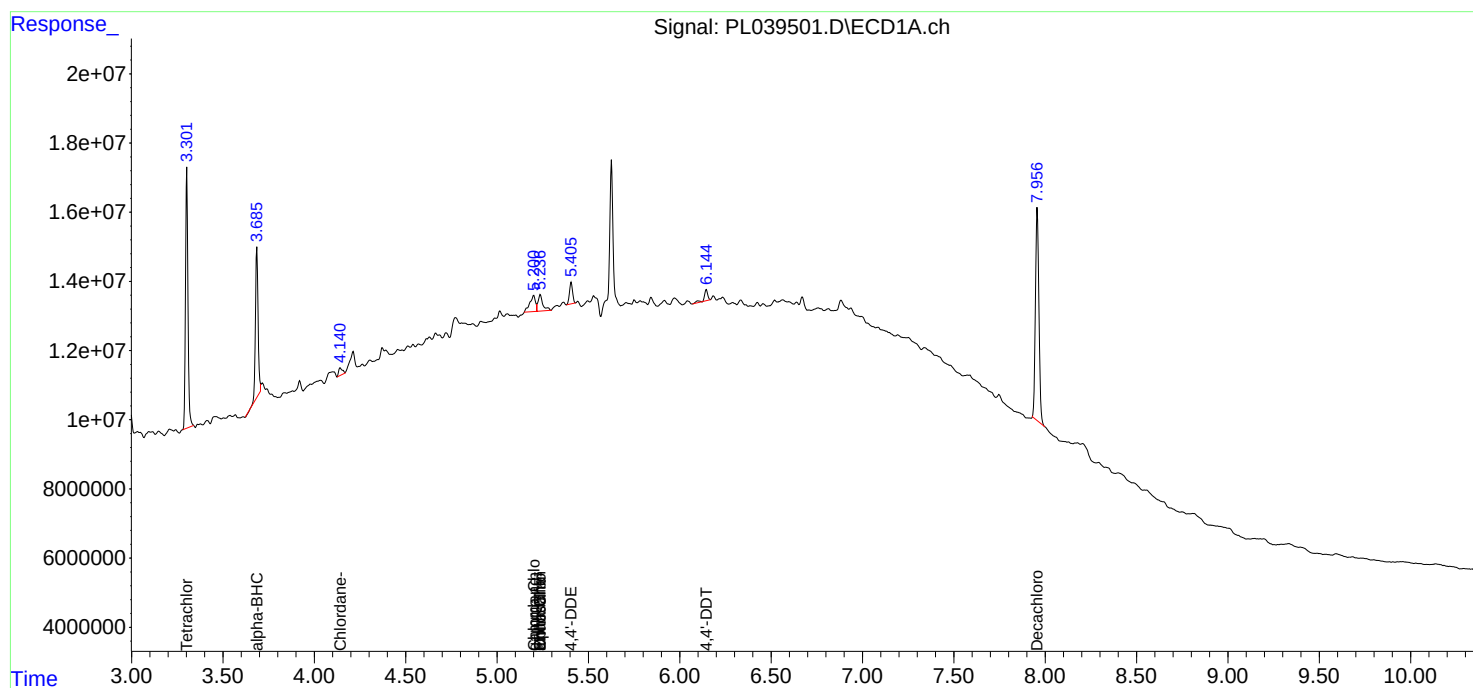


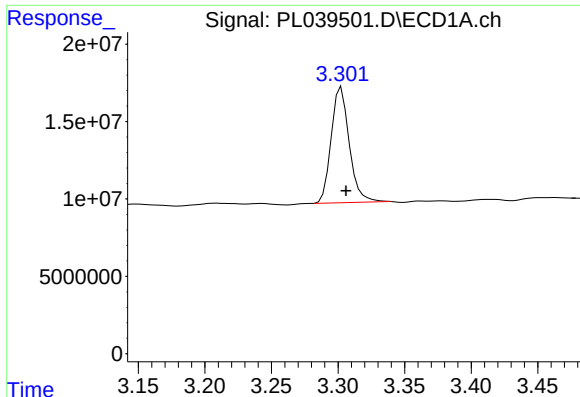

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 70772999
Conc: 10.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

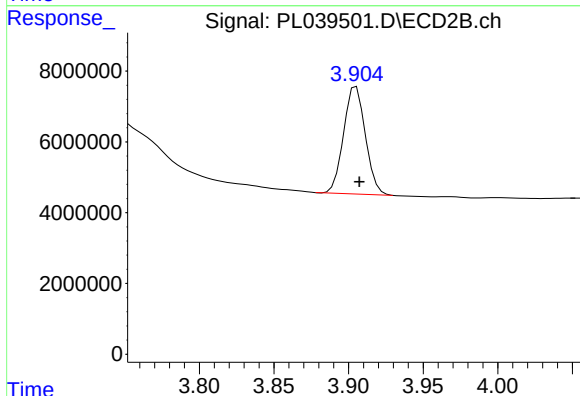


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 30845209
Conc: 11.51 ng/ml

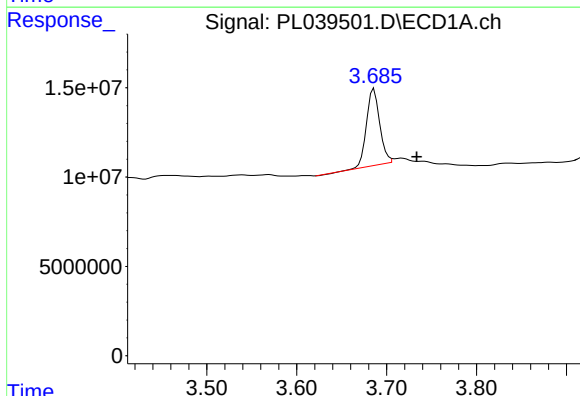


#2 alpha-BHC

R.T.: 3.686 min
Delta R.T.: -0.048 min
Response: 44220337
Conc: 3.74 ng/ml

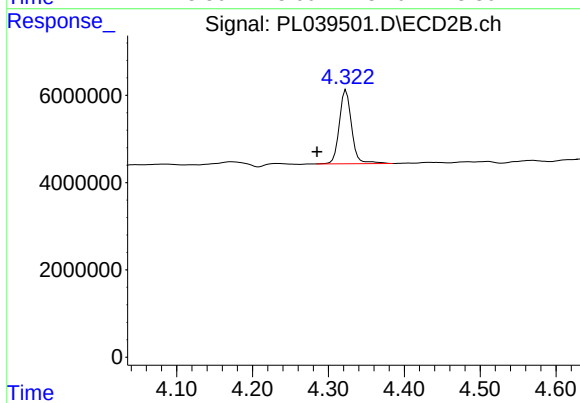

#2 alpha-BHC


R.T.: 4.323 min
Delta R.T.: 0.038 min
Response: 19021608
Conc: 4.52 ng/ml

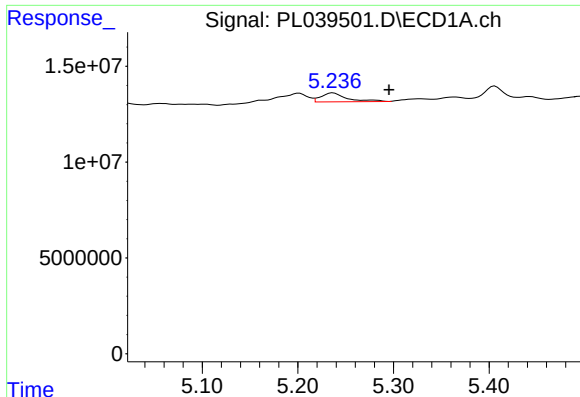

#9 Endosulfan I


R.T.: 5.237 min
Delta R.T.: -0.058 min
Response: 8766000
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

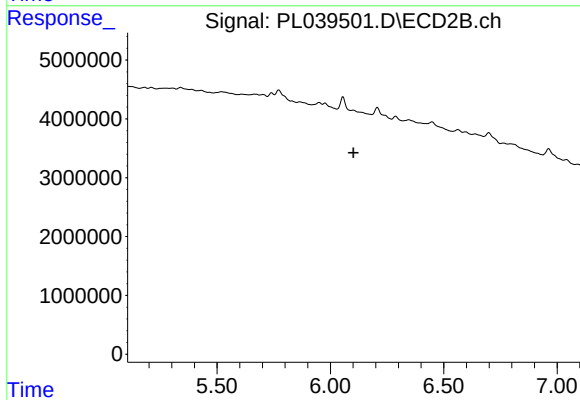


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

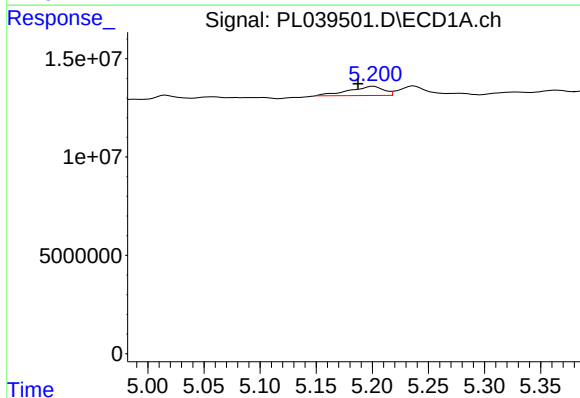


#10 gamma-Chlordane

R.T.: 5.201 min
Delta R.T.: 0.014 min
Response: 10048336
Conc: 1.02 ng/ml

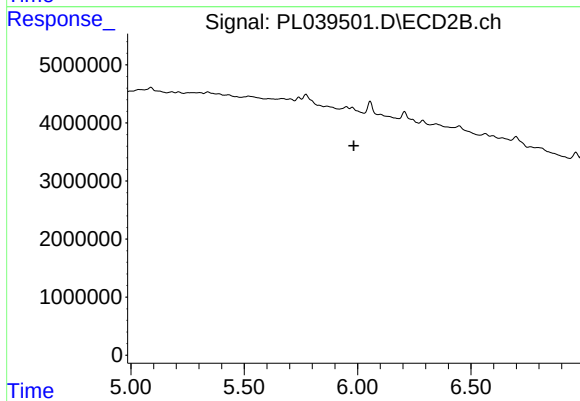

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

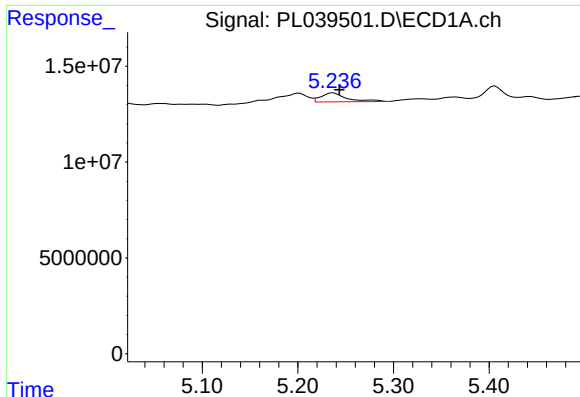

#11 alpha-Chlordane


R.T.: 5.237 min
Delta R.T.: -0.007 min
Response: 8766000
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

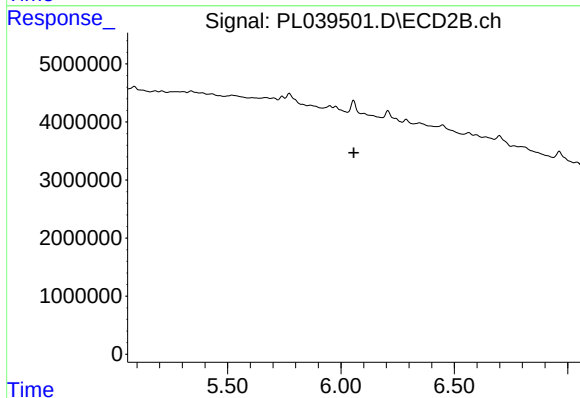


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

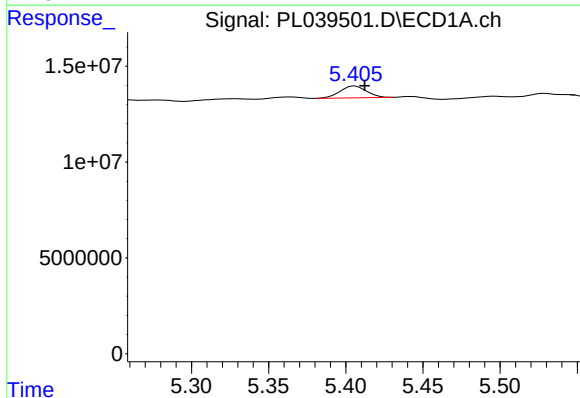


#12 4,4'-DDE

R.T.: 5.406 min
Delta R.T.: -0.006 min
Response: 7328662
Conc: 0.77 ng/ml

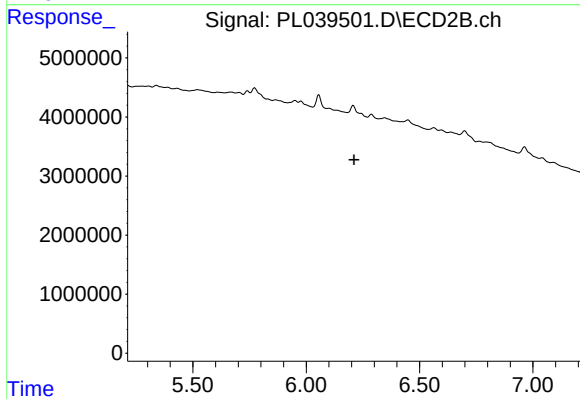

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

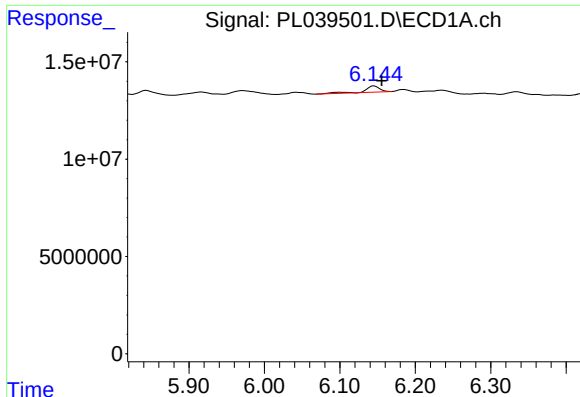

#17 4,4'-DDT


R.T.: 6.146 min
Delta R.T.: -0.010 min
Response: 4384855
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

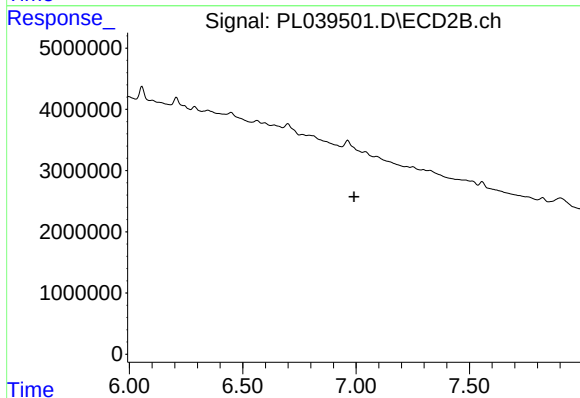


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

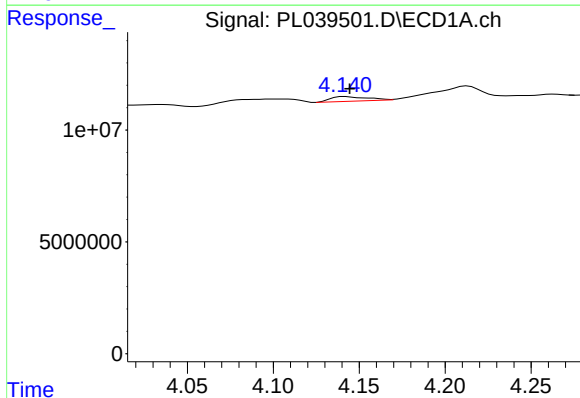


#23 Chlordane-1

R.T.: 4.142 min
Delta R.T.: -0.003 min
Response: 3102108
Conc: 9.80 ng/ml

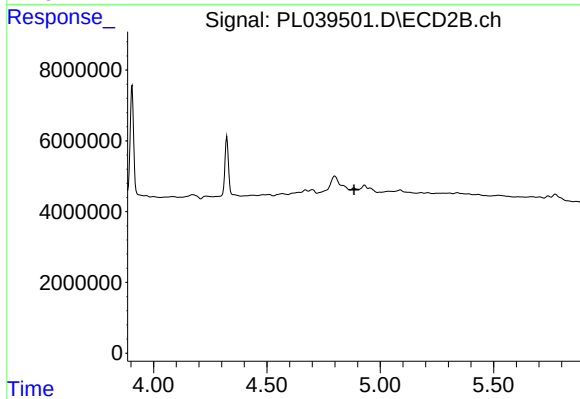

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

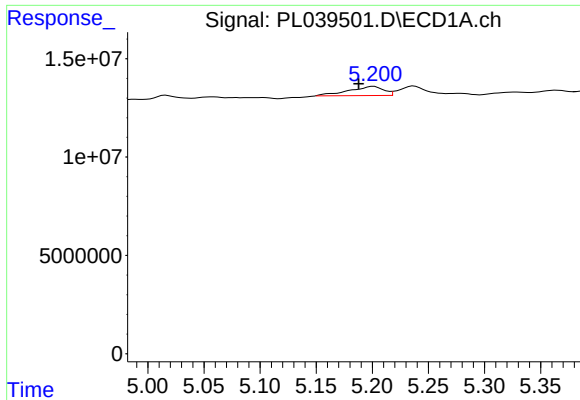

#25 Chlordane-3


R.T.: 5.201 min
Delta R.T.: 0.013 min
Response: 10048336
Conc: 9.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

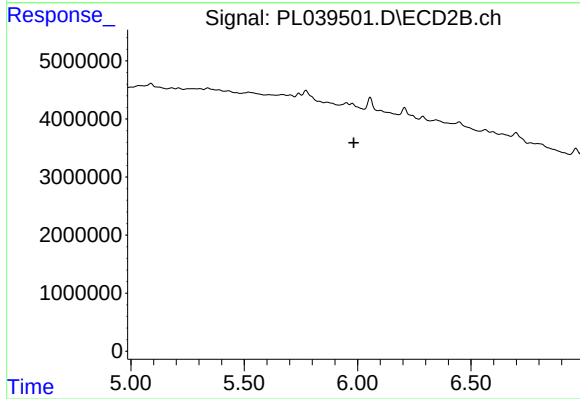


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

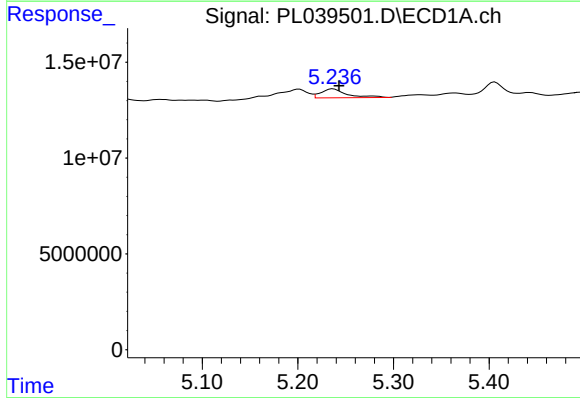


#26 Chlordane-4

R.T.: 5.237 min
Delta R.T.: -0.006 min
Response: 8766000
Conc: 8.77 ng/ml

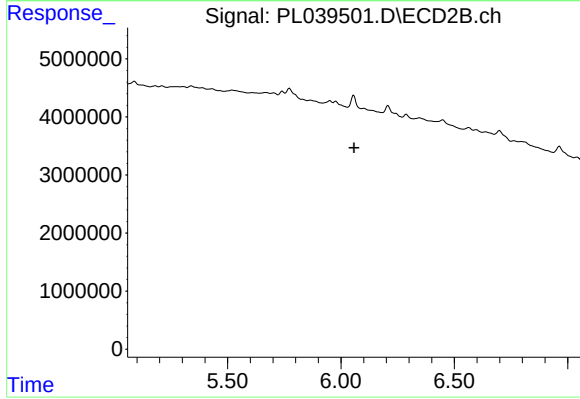

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

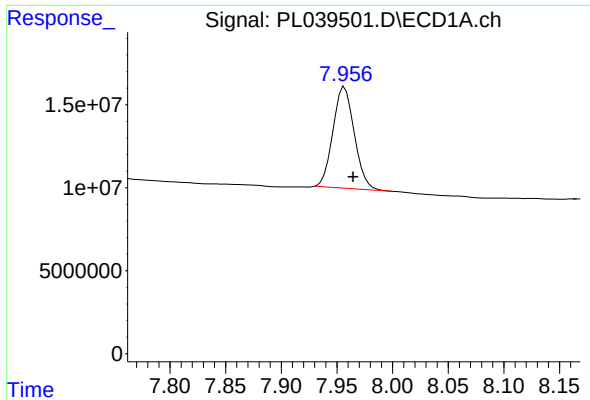

#28 Decachlorobiphenyl


R.T.: 7.957 min

Delta R.T.: -0.008 min

Response: 81246516

Conc: 11.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

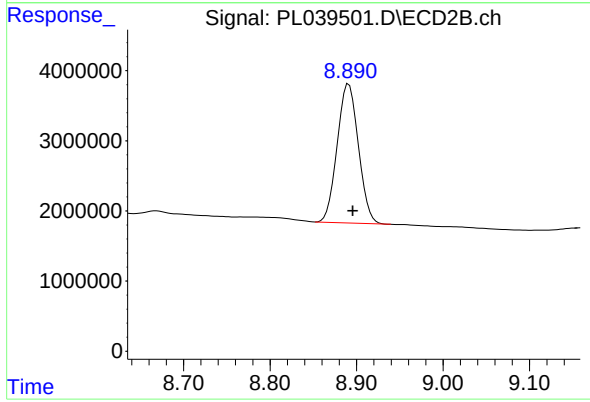

#28 Decachlorobiphenyl

R.T.: 8.891 min

Delta R.T.: -0.004 min

Response: 33605600

Conc: 14.48 ng/ml