

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
 Data File : PL039507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2018 18:06
 Operator : AJ\SJ
 Sample : PB112352BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 23:02:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	142.7E6	60467201	20.413	22.555
28)	SA Decachlor...	7.958	8.892	140.9E6	55613568	20.066	23.965
Target Compounds							
6)	B beta-BHC	4.214f	0.000	14033479	0	3.021	N.D. #
23)	Chlordane-1	4.078	0.000	17993975	0	56.837	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
Data File : PL039507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2018 18:06
Operator : AJ\SJ
Sample : PB112352BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 23:02:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

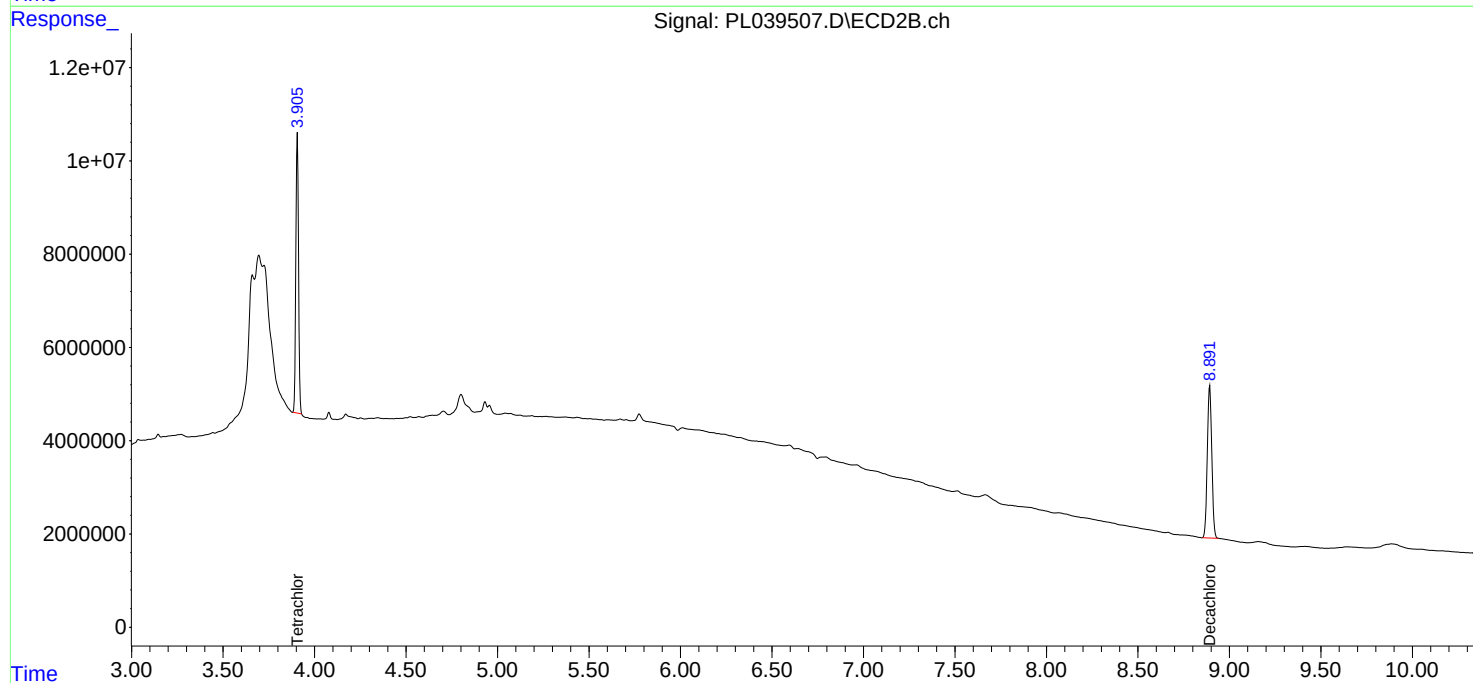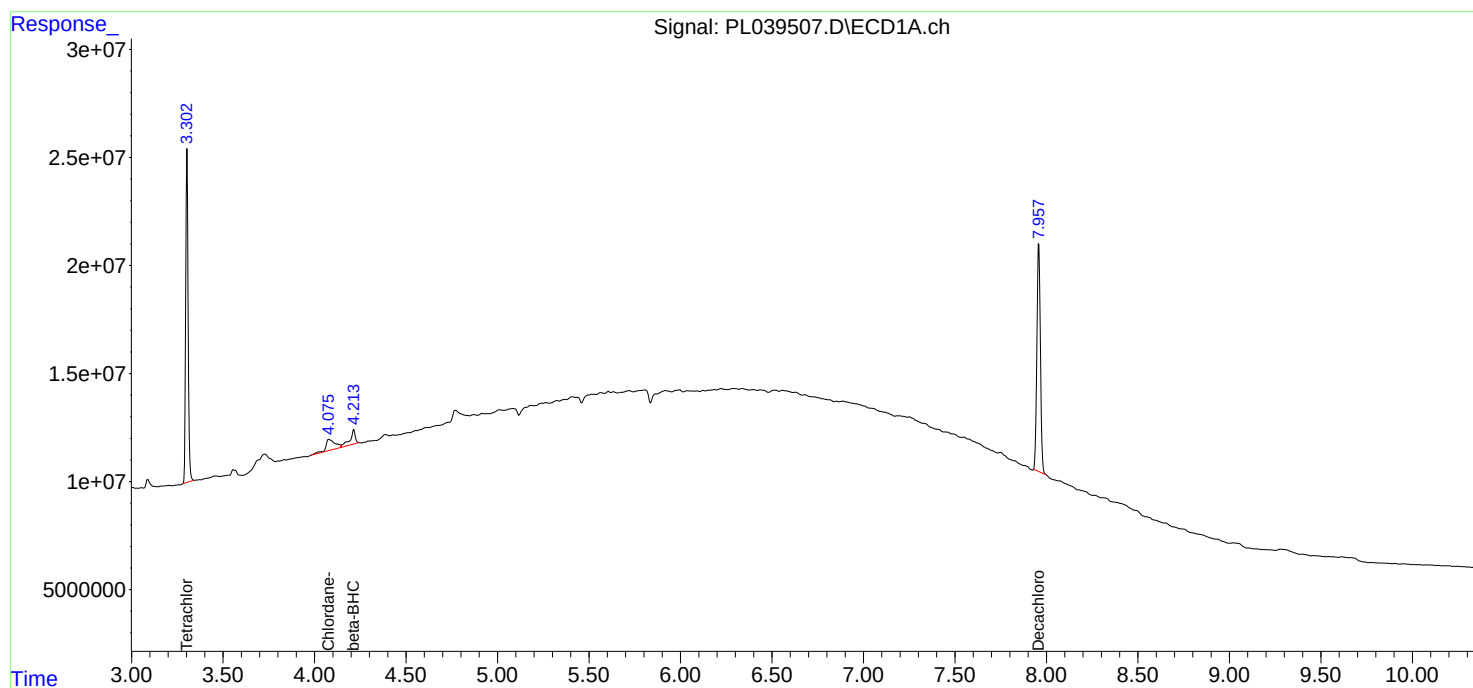


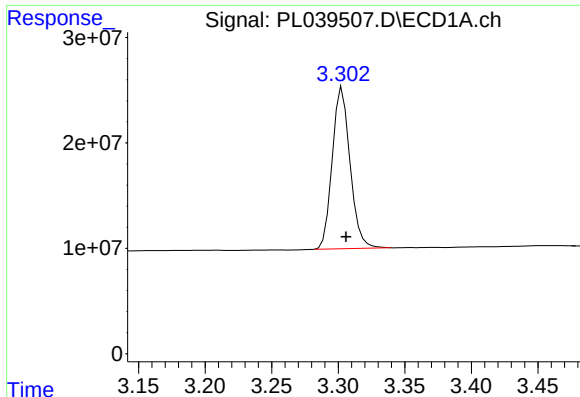

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 142693059
Conc: 20.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

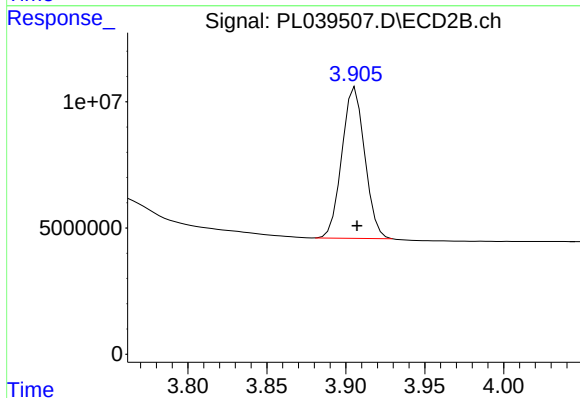


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 60467201
Conc: 22.55 ng/ml

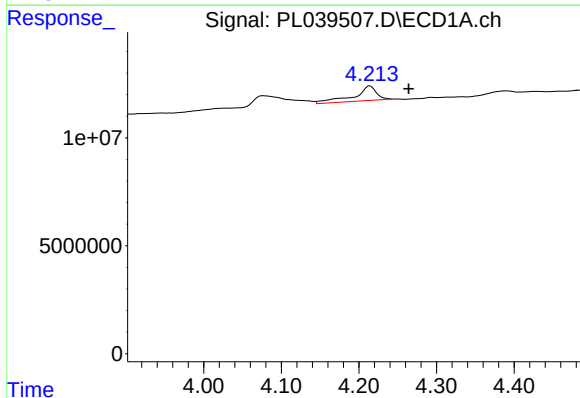


#6 beta-BHC

R.T.: 4.214 min
Delta R.T.: -0.050 min
Response: 14033479
Conc: 3.02 ng/ml

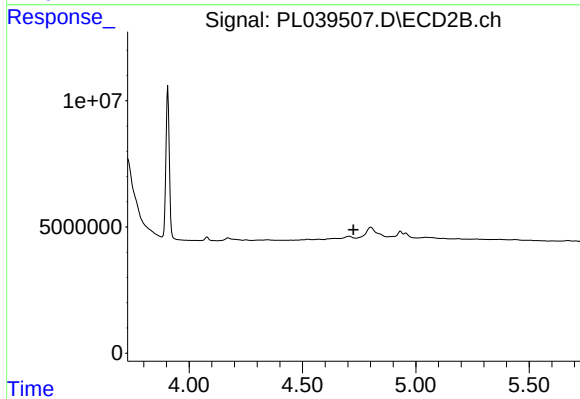

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.726 min
Response: 0
Conc: N.D.

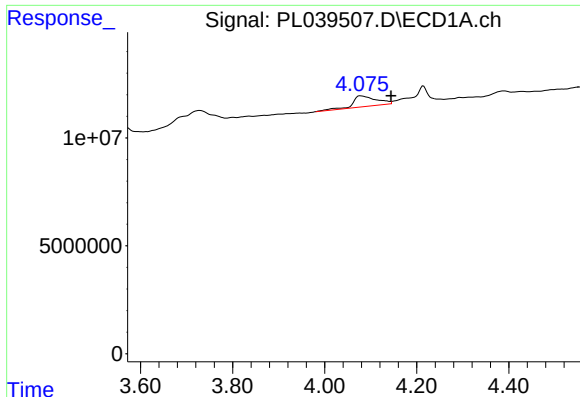

#23 Chlordane-1


R.T.: 4.078 min
Delta R.T.: -0.067 min
Response: 17993975
Conc: 56.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

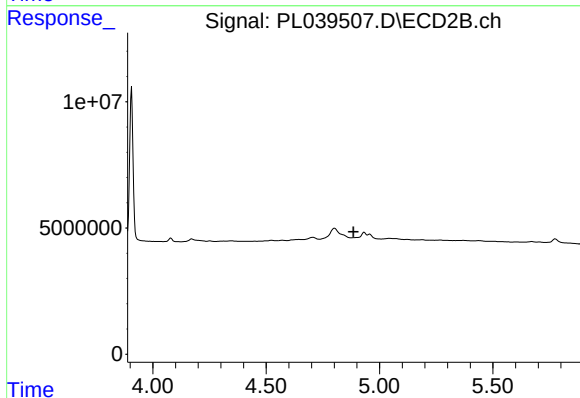


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

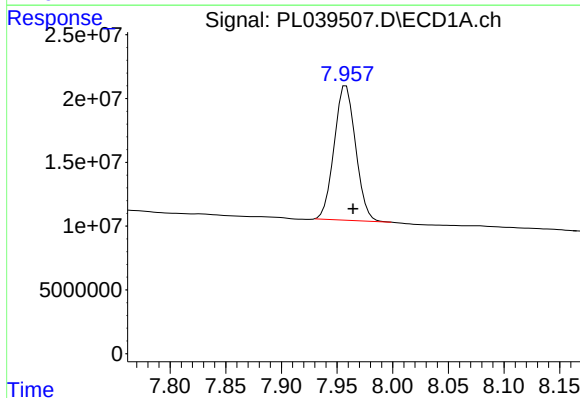

#28 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.006 min
Response: 140931253
Conc: 20.07 ng/ml

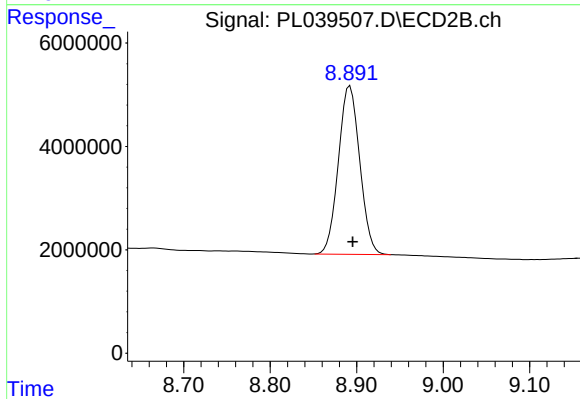

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.003 min
Response: 55613568
Conc: 23.97 ng/ml