

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
 Data File : PL039534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2018 00:28
 Operator : AJ\SJ
 Sample : J4270-04
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 02:02:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	154.9E6	66748552	22.152	24.898
28)	SA Decachlor...	7.957	8.892	149.6E6	59007434	21.296	25.428
Target Compounds							
6)	B beta-BHC	4.215f	0.000	13746911	0	2.959	N.D. #
8)	B Heptachlo...	4.961	0.000	3336302	0	0.349	N.D. #
9)	A Endosulfan I	5.276	6.077	11650220	14368119	1.331	4.898 #
10)	B gamma-Chl...	5.180	0.000	11374780	0	1.152	N.D. #
11)	B alpha-Chl...	5.238	6.077	6683989	14368119	0.696	4.441 #
14)	MA Endrin	5.838f	0.000	7592974	0	0.848	N.D. #
20)	A Methoxychlor	0.000	7.465	0	7844892	N.D.	6.334 #
21)	B Endrin ke...	6.865f	0.000	42352946	0	4.921	N.D. #
23)	Chlordane-1	4.188	0.000	3126052	0	9.874	N.D. #
24)	Chlordane-2	4.637	0.000	15760849	0	45.084	N.D. #
25)	Chlordane-3	5.180	0.000	11374780	0	10.414	N.D. #
26)	Chlordane-4	5.238	6.077	6683989	14368119	6.688	27.699 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082418\
Data File : PL039534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2018 00:28
Operator : AJ\SJ
Sample : J4270-04
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 02:02:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

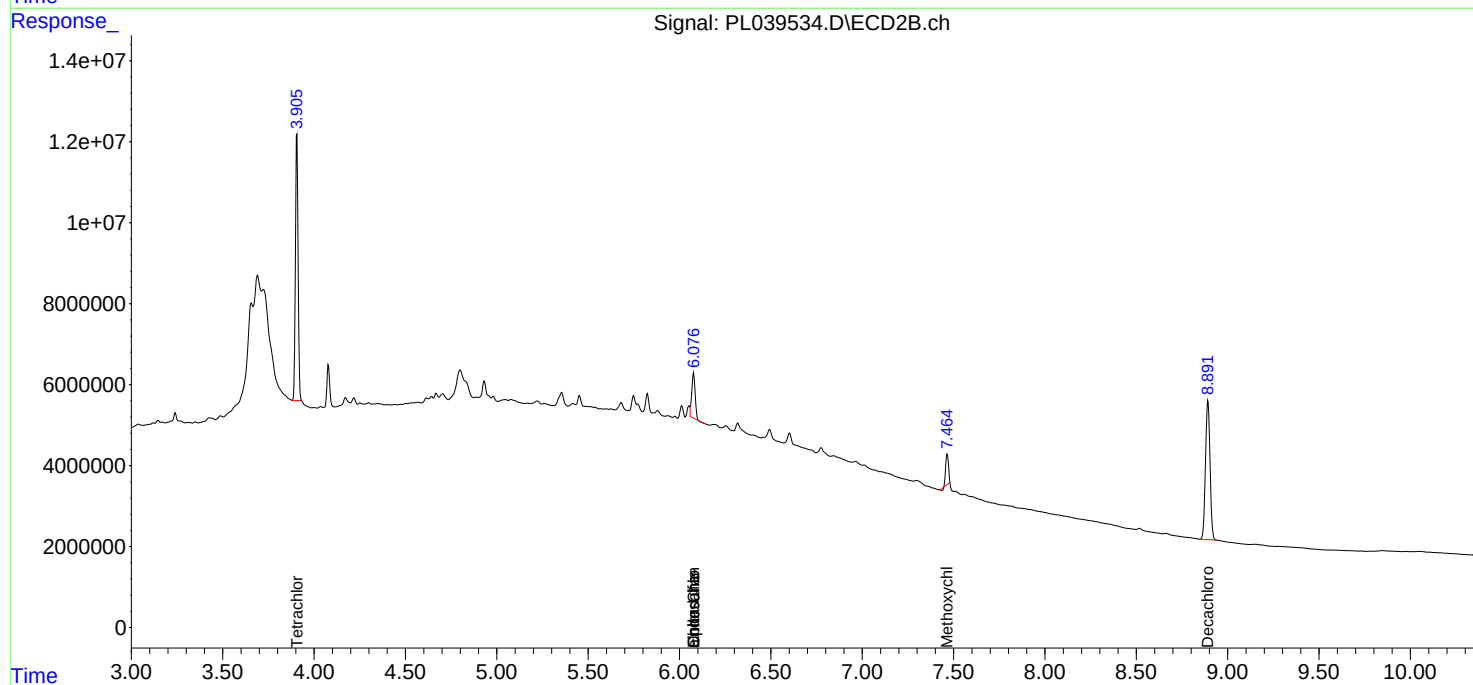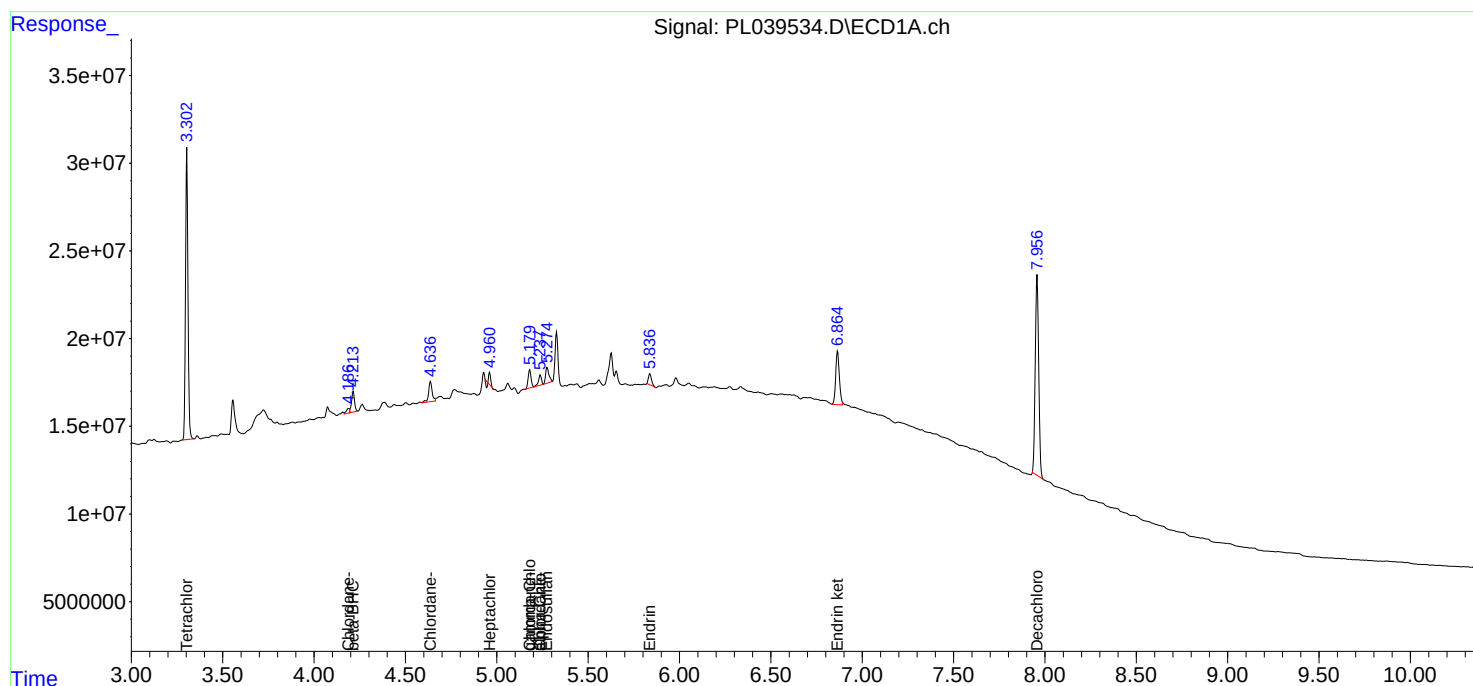


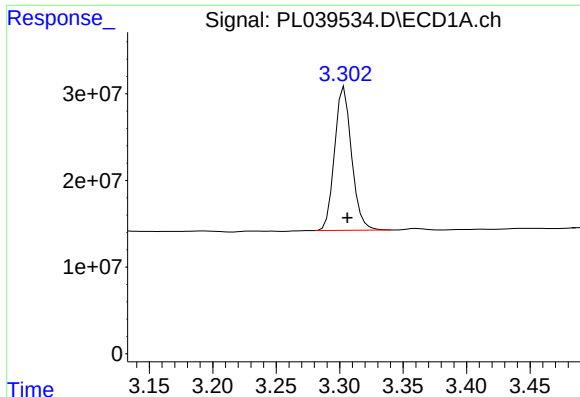

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 154850940
Conc: 22.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

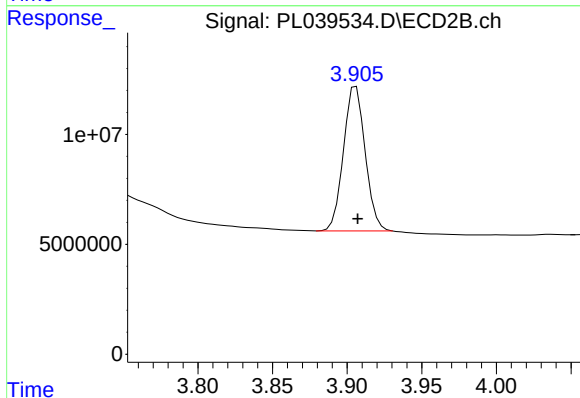


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 66748552
Conc: 24.90 ng/ml

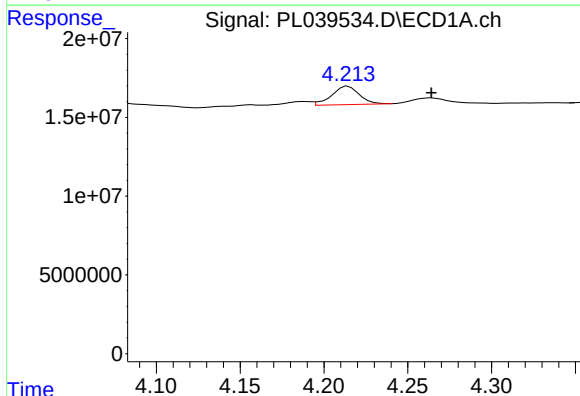


#6 beta-BHC

R.T.: 4.215 min
Delta R.T.: -0.050 min
Response: 13746911
Conc: 2.96 ng/ml

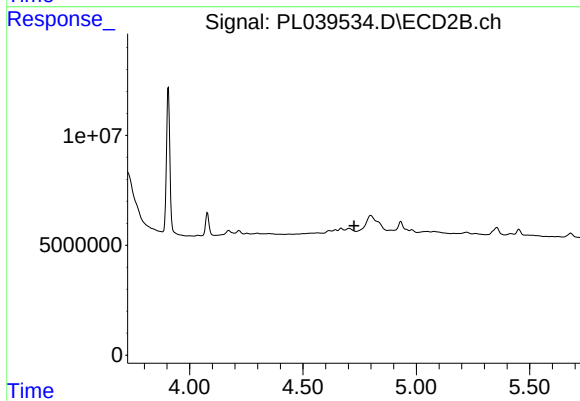

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

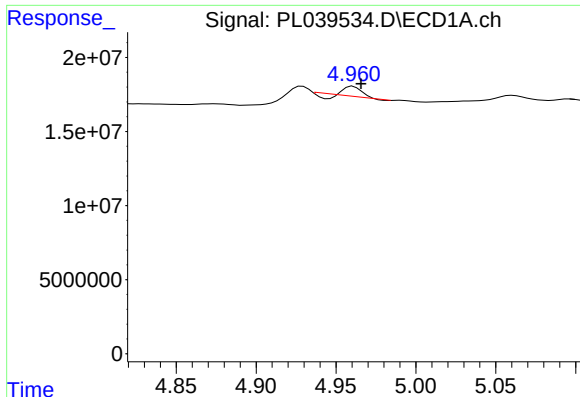

#8 Heptachlor epoxide


R.T.: 4.961 min
Delta R.T.: -0.005 min
Response: 3336302
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

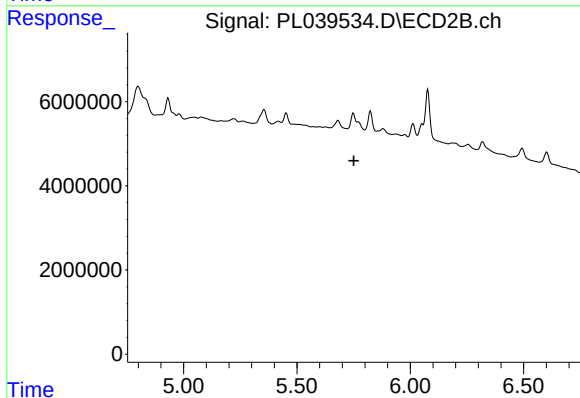


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

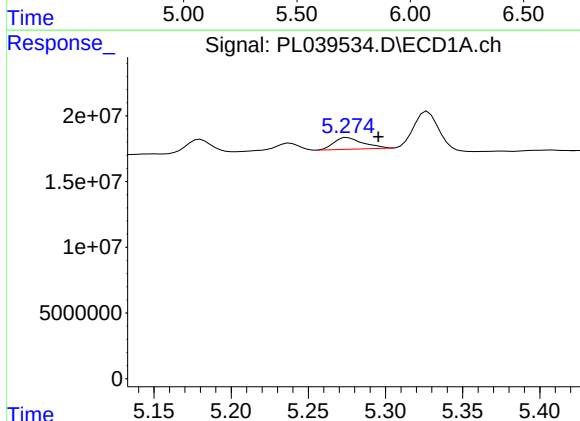


#9 Endosulfan I

R.T.: 5.276 min
Delta R.T.: -0.020 min
Response: 11650220
Conc: 1.33 ng/ml

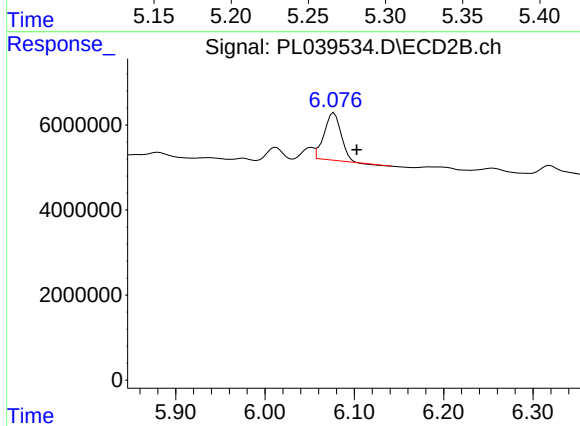

#9 Endosulfan I


R.T.: 6.077 min
Delta R.T.: -0.025 min
Response: 14368119
Conc: 4.90 ng/ml

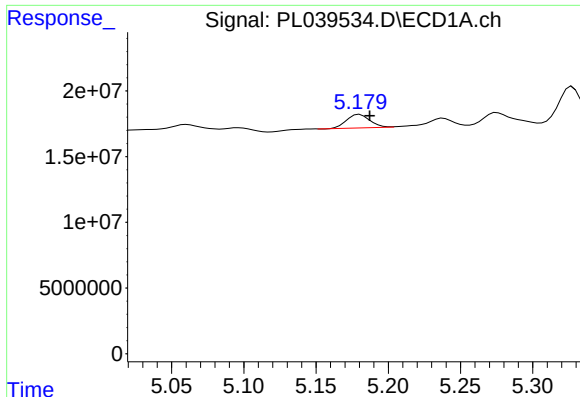

#10 gamma-Chlordane


R.T.: 5.180 min
Delta R.T.: -0.007 min
Response: 11374780
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

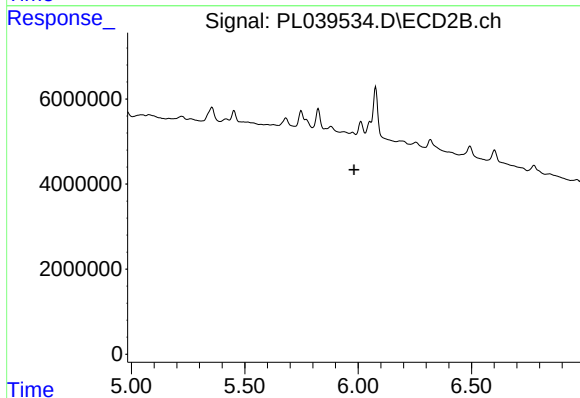


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

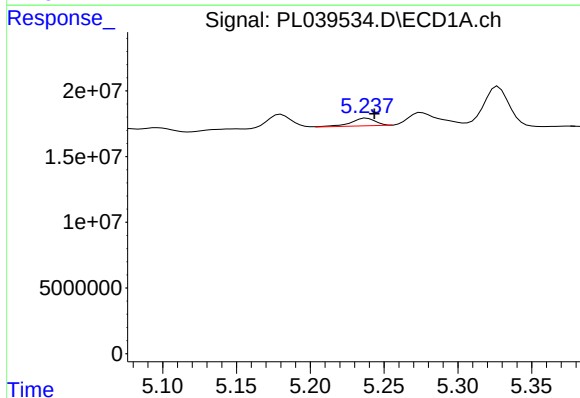


#11 alpha-Chlordane

R.T.: 5.238 min
Delta R.T.: -0.005 min
Response: 6683989
Conc: 0.70 ng/ml

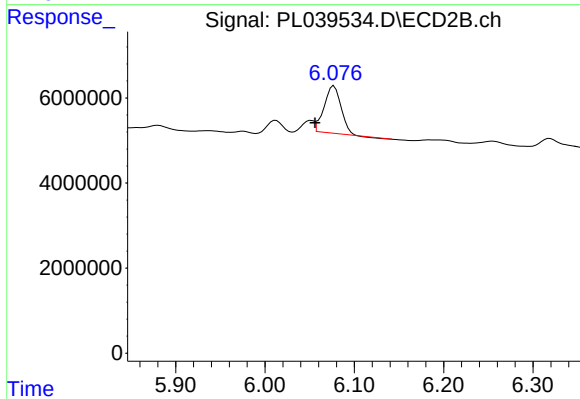

#11 alpha-Chlordane


R.T.: 6.077 min
Delta R.T.: 0.021 min
Response: 14368119
Conc: 4.44 ng/ml

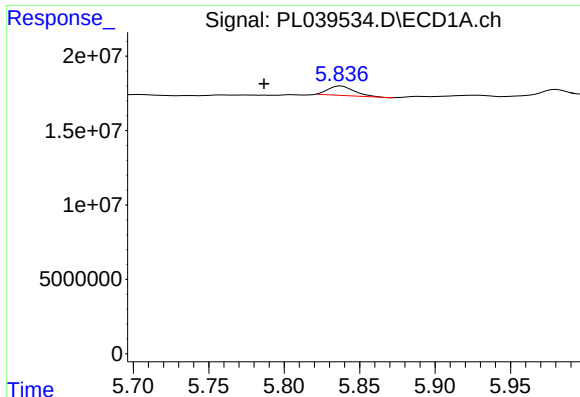

#14 Endrin


R.T.: 5.838 min
Delta R.T.: 0.051 min
Response: 7592974
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

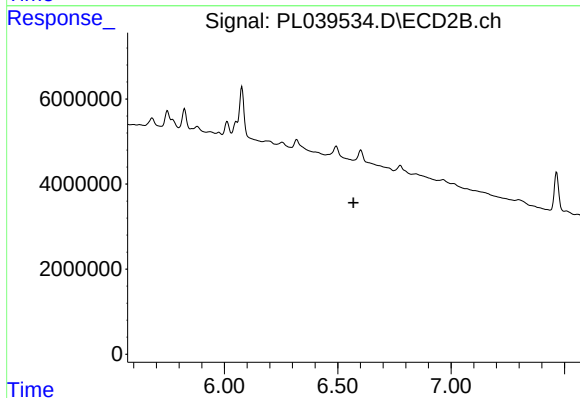


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

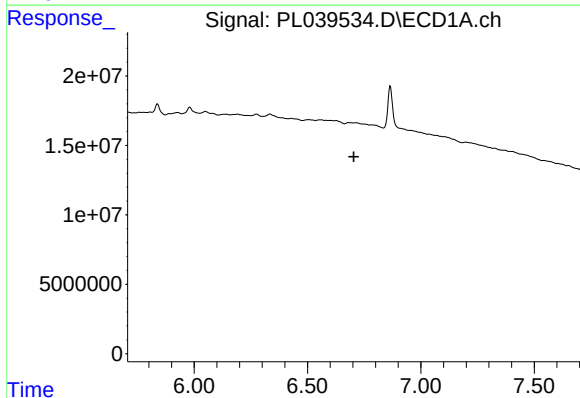


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.704 min
Response: 0
Conc: N.D.

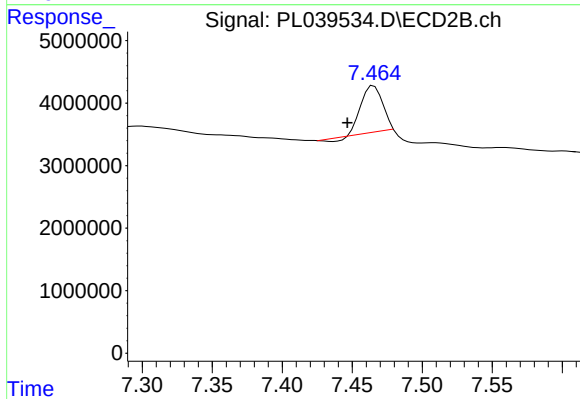

#20 Methoxychlor


R.T.: 7.465 min
Delta R.T.: 0.019 min
Response: 7844892
Conc: 6.33 ng/ml

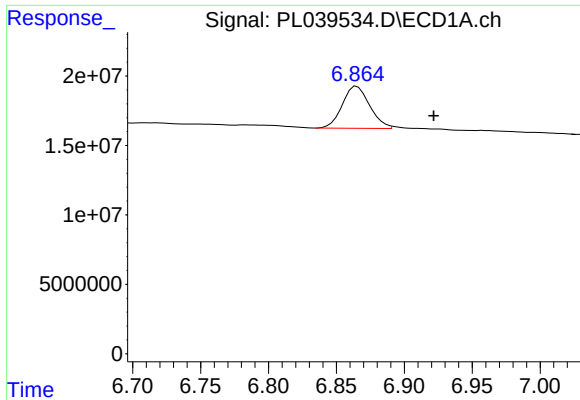

#21 Endrin ketone


R.T.: 6.865 min
Delta R.T.: -0.057 min
Response: 42352946
Conc: 4.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

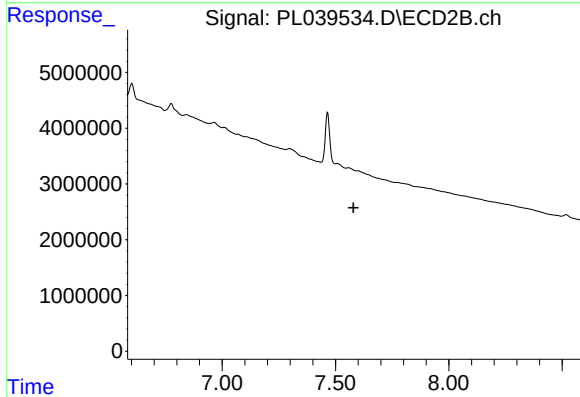


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.580 min
Response: 0
Conc: N.D.

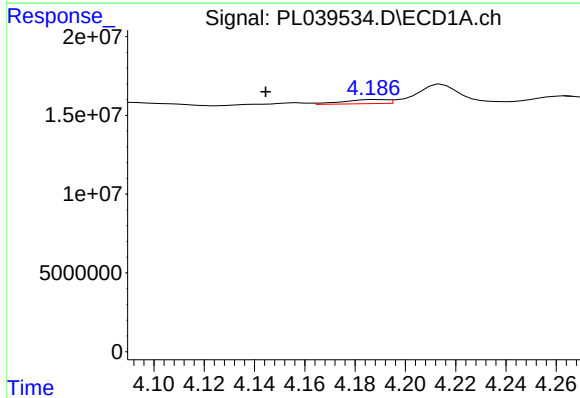


#23 Chlordane-1

R.T.: 4.188 min
Delta R.T.: 0.044 min
Response: 3126052
Conc: 9.87 ng/ml

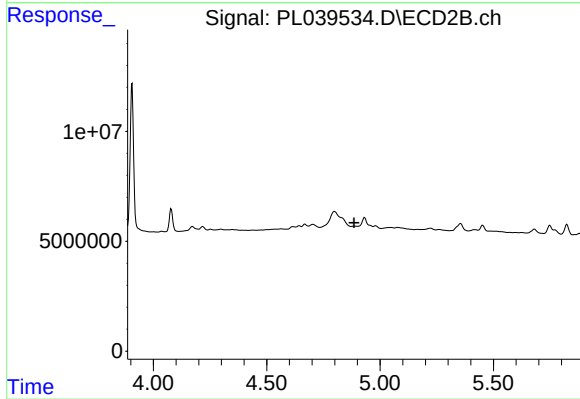

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

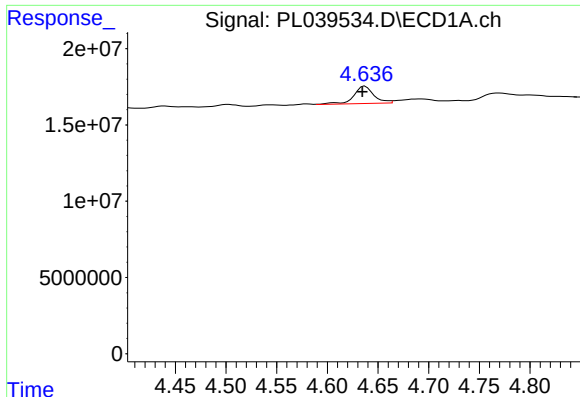

#24 Chlordane-2


R.T.: 4.637 min
Delta R.T.: 0.003 min
Response: 15760849
Conc: 45.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

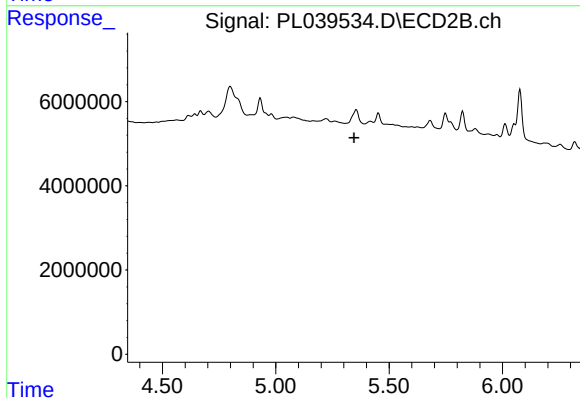


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

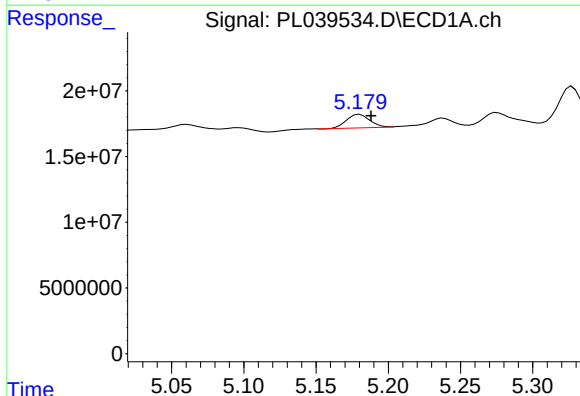


#25 Chlordane-3

R.T.: 5.180 min
Delta R.T.: -0.008 min
Response: 11374780
Conc: 10.41 ng/ml

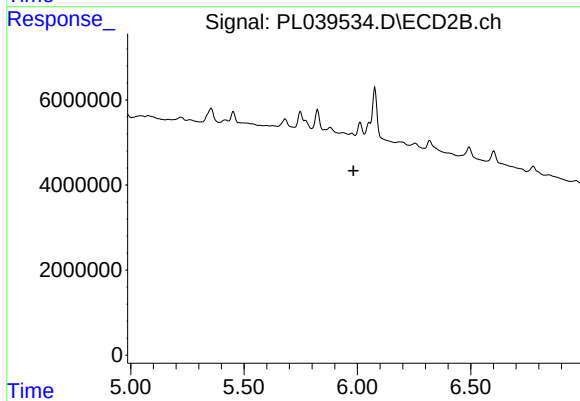

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

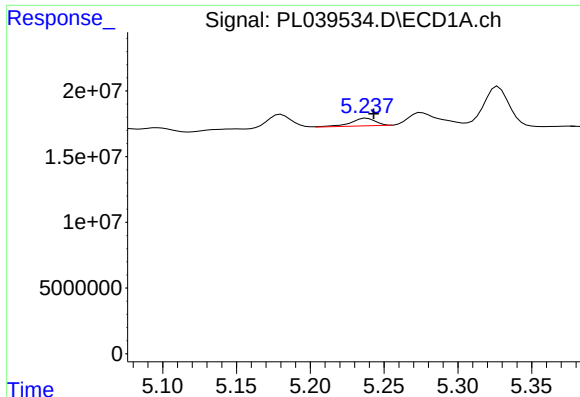

#26 Chlordane-4


R.T.: 5.238 min
Delta R.T.: -0.005 min
Response: 6683989
Conc: 6.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

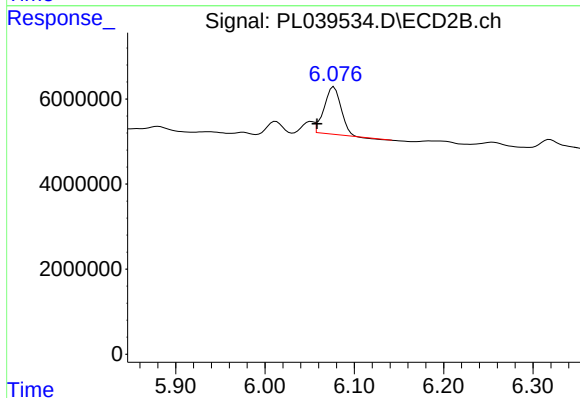


#26 Chlordane-4

R.T.: 6.077 min
Delta R.T.: 0.019 min
Response: 14368119
Conc: 27.70 ng/ml

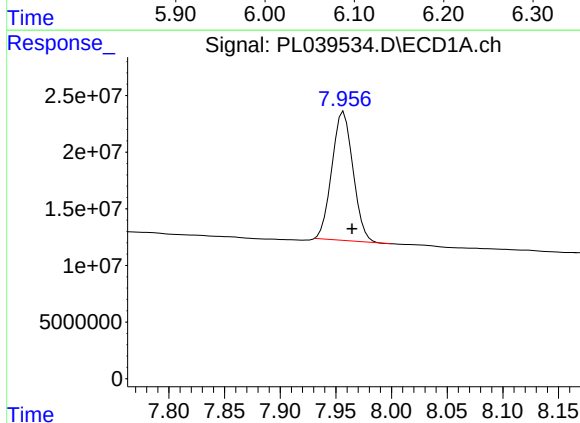

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.007 min
Response: 149570245
Conc: 21.30 ng/ml

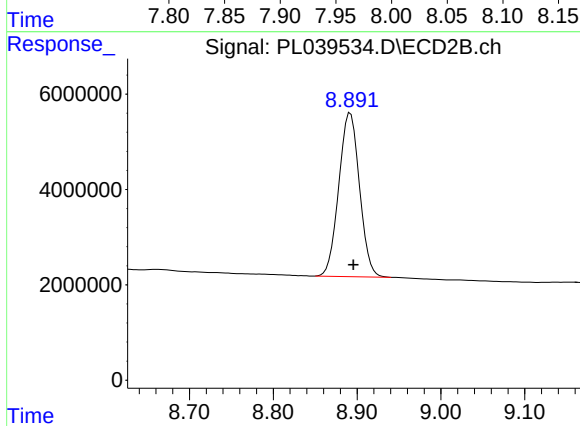

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.003 min
Response: 59007434
Conc: 25.43 ng/ml