

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082619\
 Data File : PL051796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2019 08:45
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 00:42:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) MA	gamma-BHC...	0.000	4.585	0	8132961	N.D. 2.583 #
9) A	Endosulfan I	5.298	0.000	64738533	0	4.816 N.D. #
10) B	gamma-Chl...	5.219f	0.000	16995026	0	1.138 N.D. #
11) B	alpha-Chl...	5.276f	0.000	44245647	0	3.057 N.D. #
13) MA	Dieldrin	5.540	0.000	8557642	0	0.563 N.D. #
16) A	4,4'-DDD	5.936	0.000	123.7E6	0	10.101 N.D. #
17) MA	4,4'-DDT	6.152	0.000	100.5E6	0	7.879 N.D. #
18) B	Endrin al...	6.229	0.000	55956224	0	4.810 N.D. #
20) A	Methoxychlor	6.722	0.000	34521923	0	5.092 N.D. #
21) B	Endrin ke...	6.938	0.000	69431843	0	4.908 N.D. #
25)	Chlordane-3	5.219f	0.000	16995026	0	13.090 N.D. #
26)	Chlordane-4	5.276f	0.000	44245647	0	36.286 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082619\
Data File : PL051796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2019 08:45
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 00:42:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

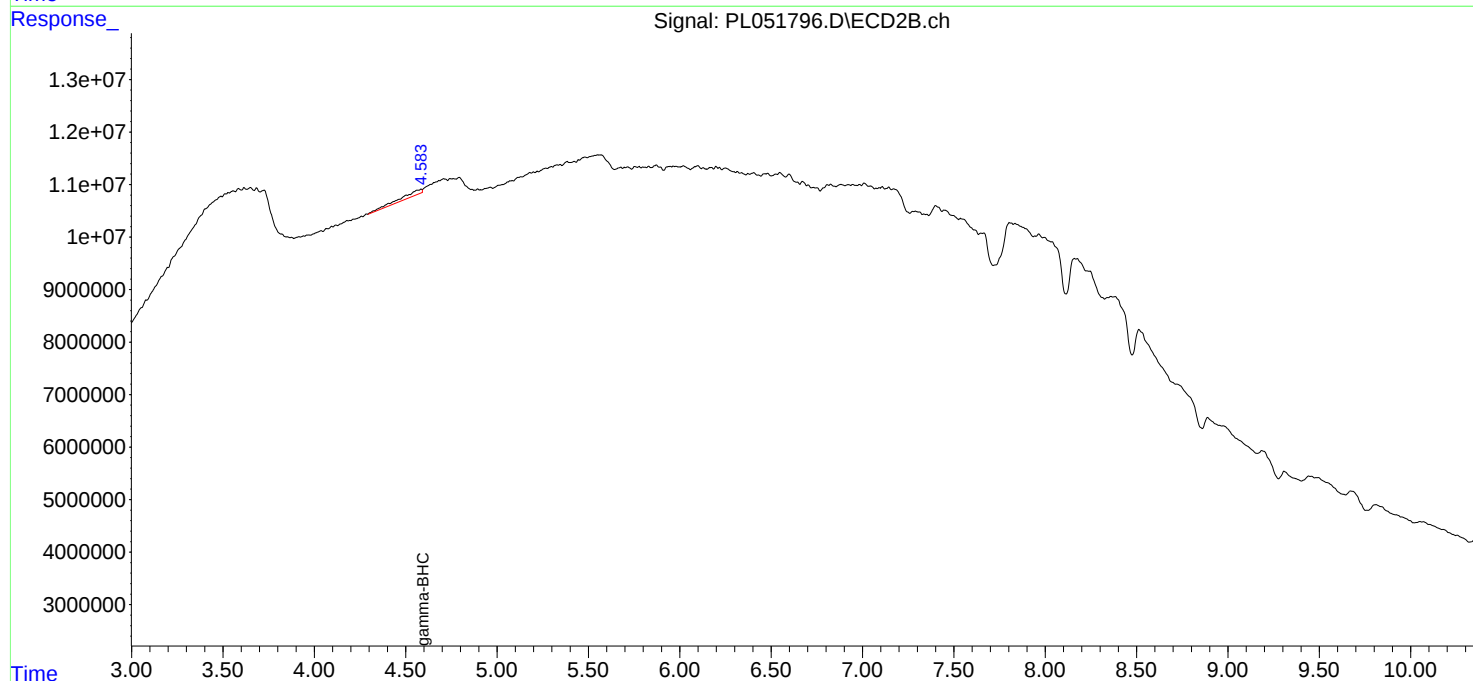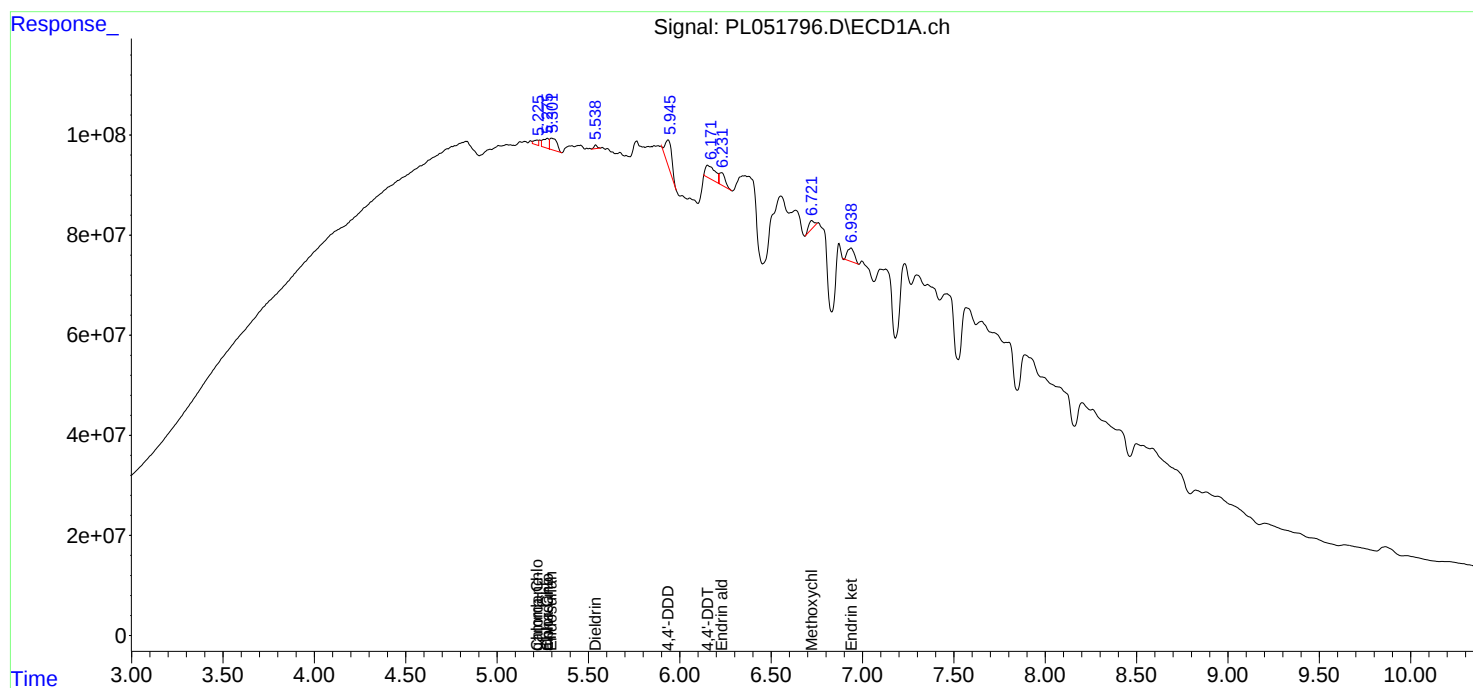


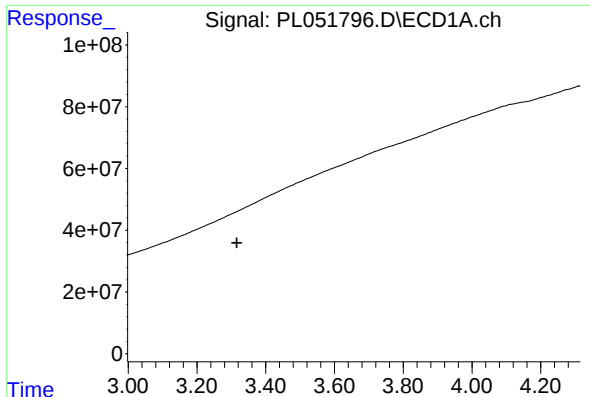

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

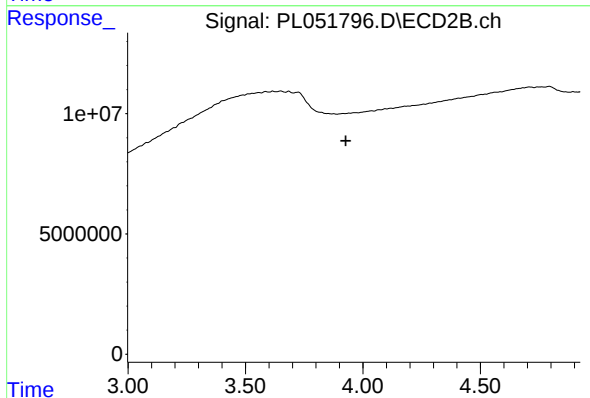


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.927 min
Response: 0
Conc: N.D.

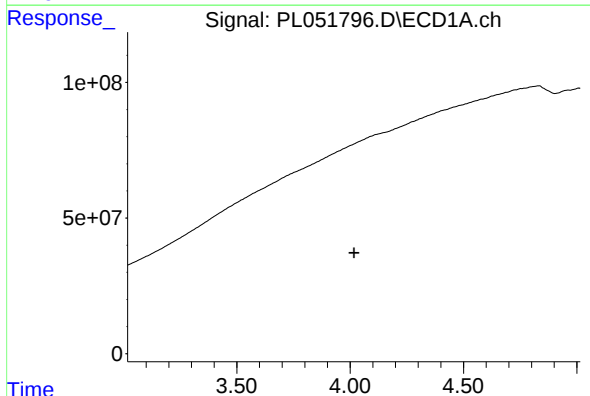


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.018 min
Response: 0
Conc: N.D.

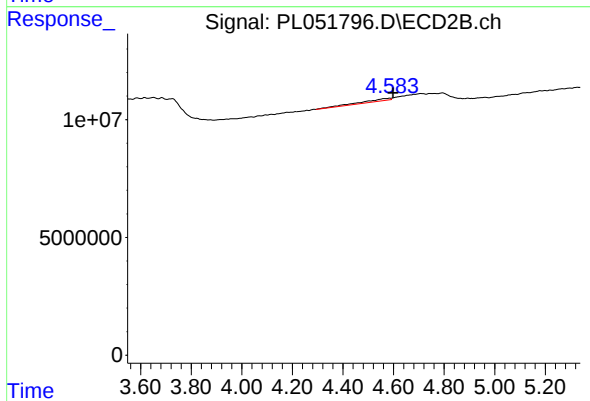

#3 gamma-BHC (Lindane)


R.T.: 4.585 min
Delta R.T.: -0.013 min
Response: 8132961
Conc: 2.58 ng/ml

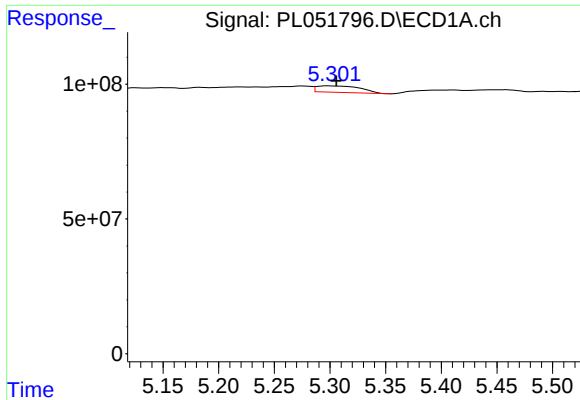

#9 Endosulfan I


R.T.: 5.298 min
Delta R.T.: -0.008 min
Response: 64738533
Conc: 4.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

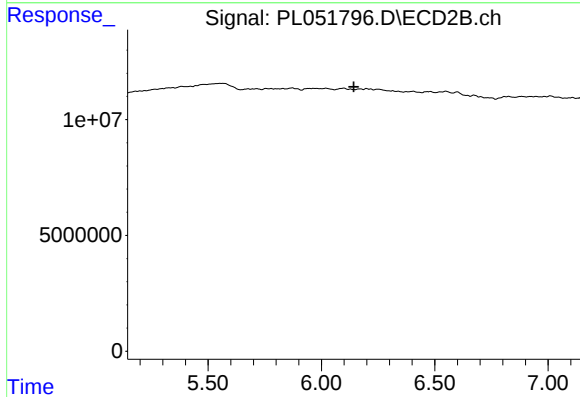


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

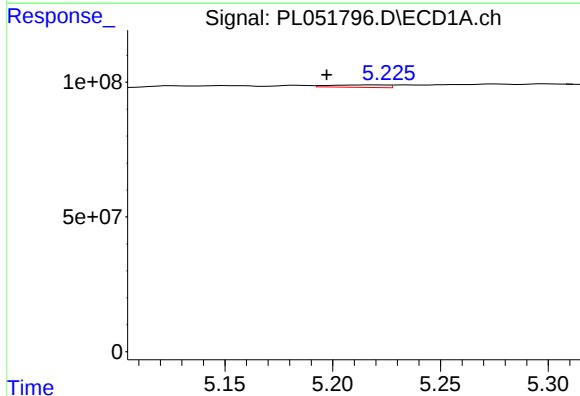


#10 gamma-Chlordane

R.T.: 5.219 min
Delta R.T.: 0.022 min
Response: 16995026
Conc: 1.14 ng/ml

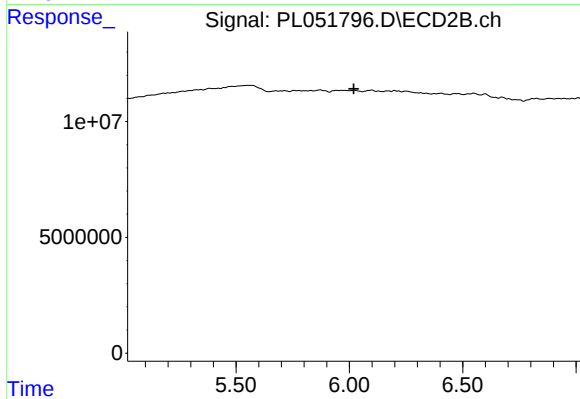

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

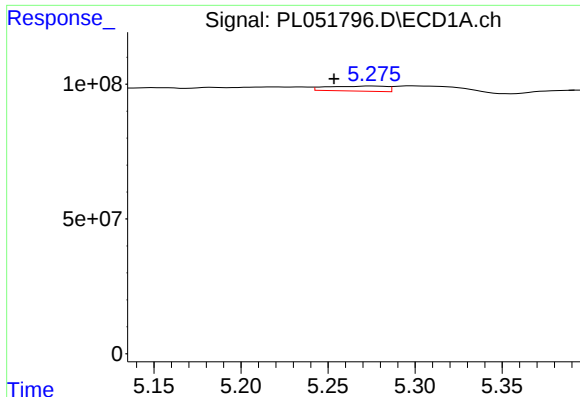

#11 alpha-Chlordane


R.T.: 5.276 min
Delta R.T.: 0.022 min
Response: 44245647
Conc: 3.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

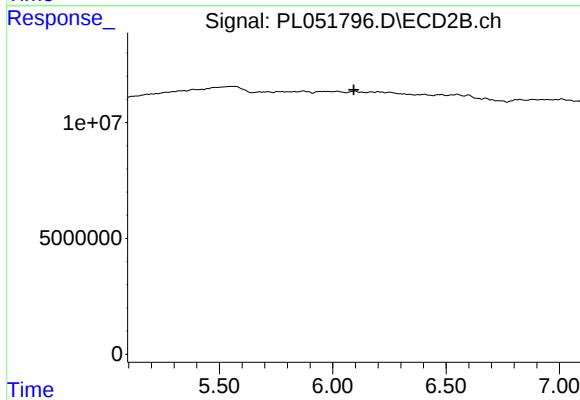


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

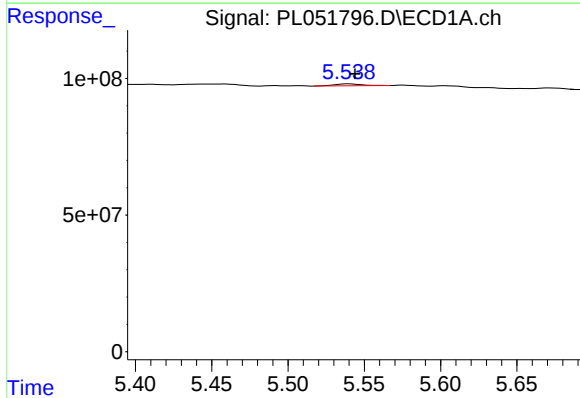


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: -0.004 min
Response: 8557642
Conc: 0.56 ng/ml

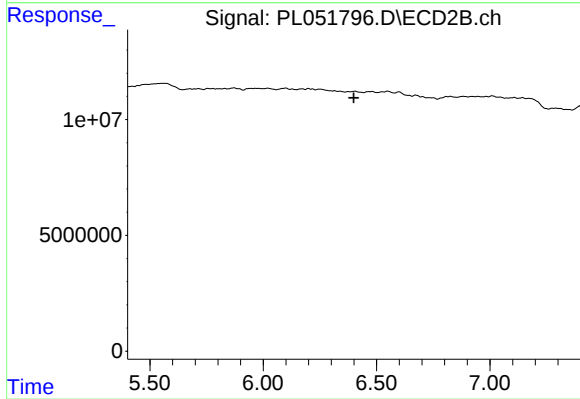

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

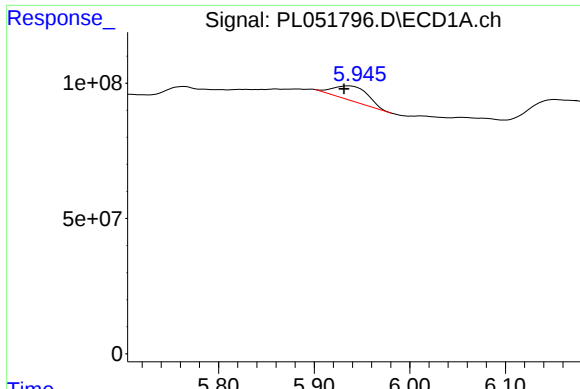

#16 4,4'-DDD


R.T.: 5.936 min
Delta R.T.: 0.005 min
Response: 123690433
Conc: 10.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

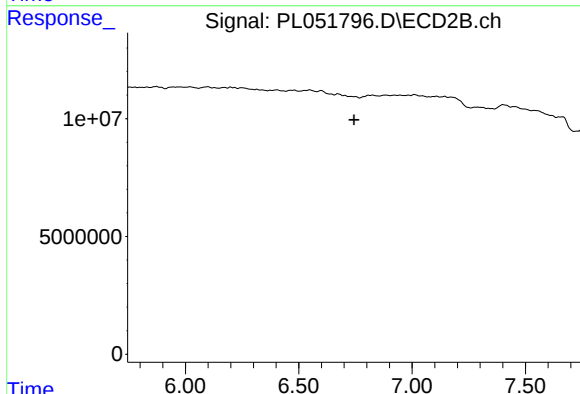


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.744 min
Response: 0
Conc: N.D.

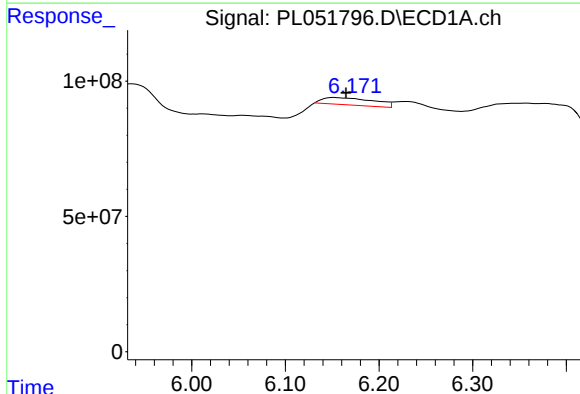


#17 4,4'-DDT

R.T.: 6.152 min
Delta R.T.: -0.013 min
Response: 100470440
Conc: 7.88 ng/ml

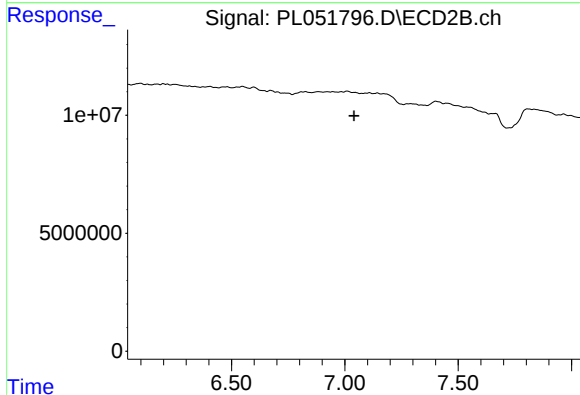

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

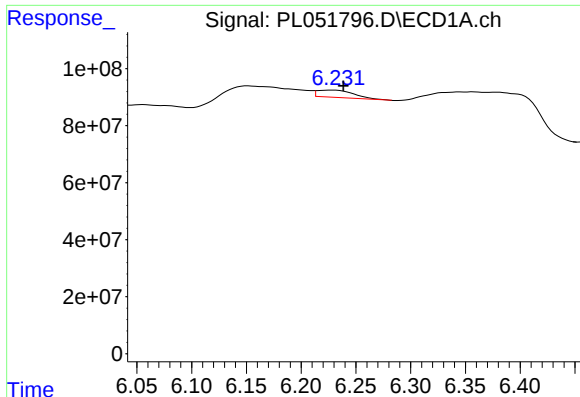

#18 Endrin aldehyde


R.T.: 6.229 min
Delta R.T.: -0.009 min
Response: 55956224
Conc: 4.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

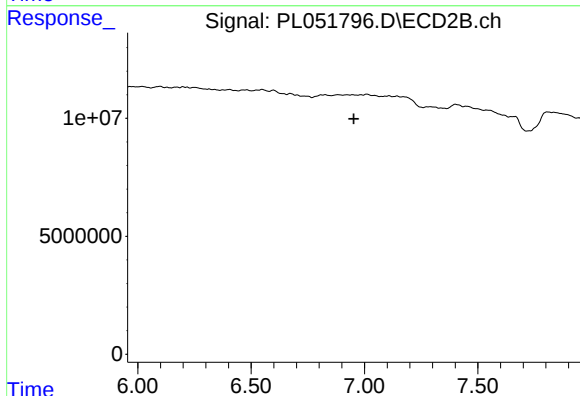


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.953 min
Response: 0
Conc: N.D.

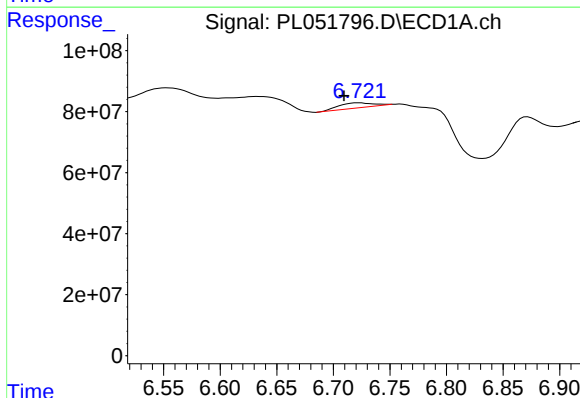


#20 Methoxychlor

R.T.: 6.722 min
Delta R.T.: 0.013 min
Response: 34521923
Conc: 5.09 ng/ml

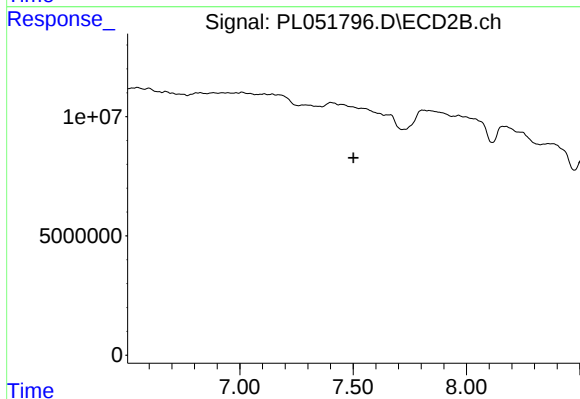

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.502 min
Response: 0
Conc: N.D.

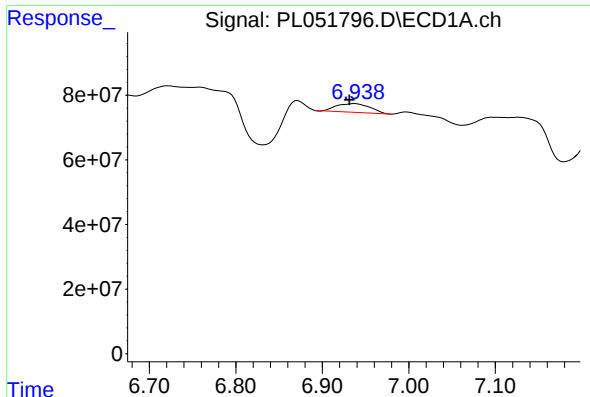

#21 Endrin ketone


R.T.: 6.938 min
Delta R.T.: 0.007 min
Response: 69431843
Conc: 4.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

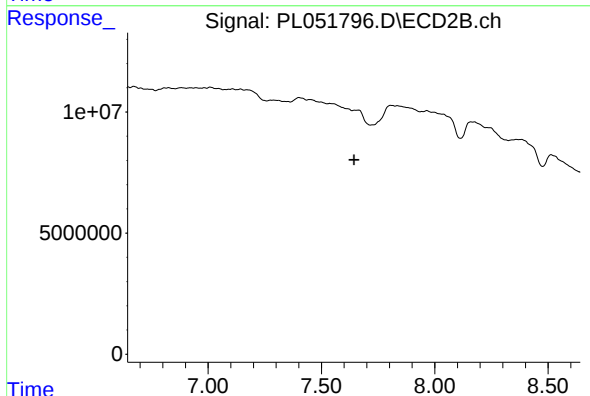


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.644 min
Response: 0
Conc: N.D.

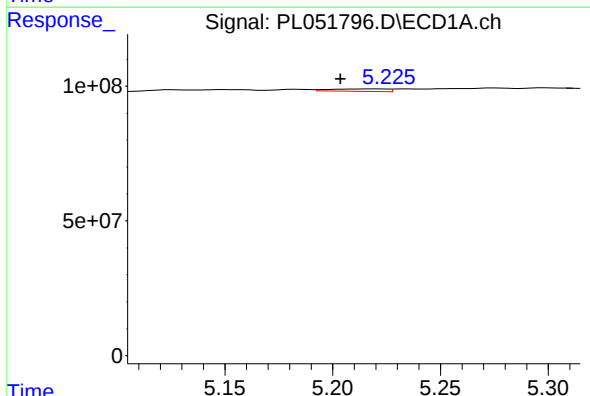


#25 Chlordane-3

R.T.: 5.219 min
Delta R.T.: 0.016 min
Response: 16995026
Conc: 13.09 ng/ml

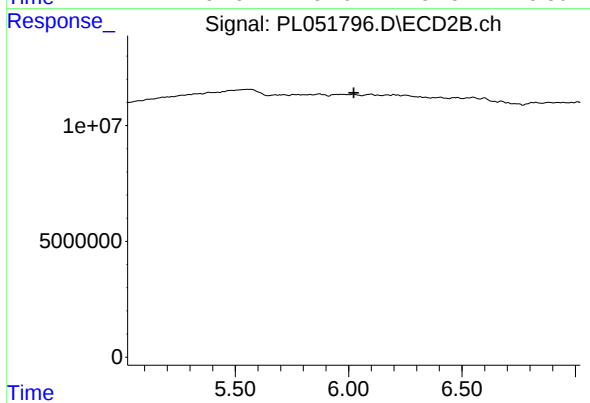

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

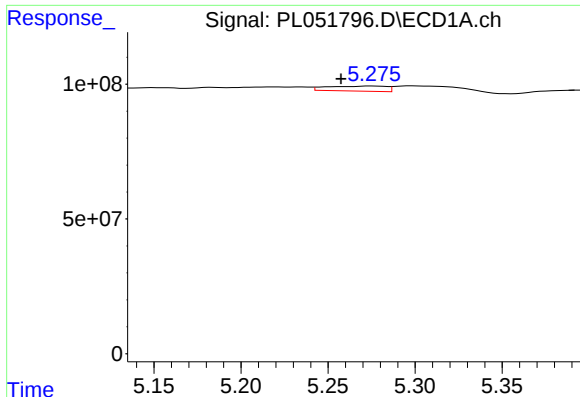

#26 Chlordane-4


R.T.: 5.276 min
Delta R.T.: 0.018 min
Response: 44245647
Conc: 36.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

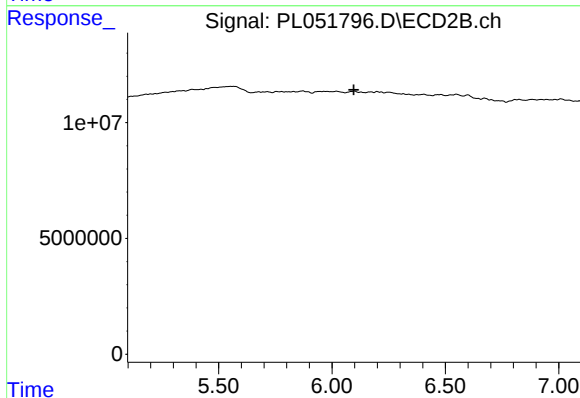


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

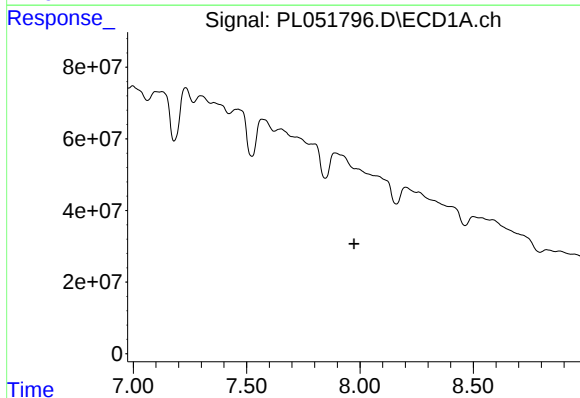

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.975 min
Response: 0
Conc: N.D.

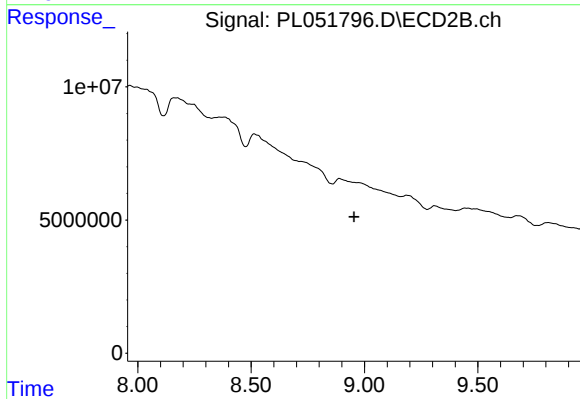

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.954 min
Response: 0
Conc: N.D.