

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082621\
 Data File : PD065322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 09:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 01:07:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:44:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.495	4.013	22857086	159.8E6	21.200	23.370
28) SA	Decachlor...	8.238	9.082	30572409	105.3E6	22.531	24.322
Target Compounds							
3) MA	gamma-BHC...	4.228	0.000	980533	0	0.646	N.D. #
15) B	Endosulfa...	0.000	6.947	0	1448010	N.D.	0.277 #
23)	Chlordane-1	4.393f	0.000	918019	0	23.388	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082621\
Data File : PD065322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 09:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 01:07:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:44:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

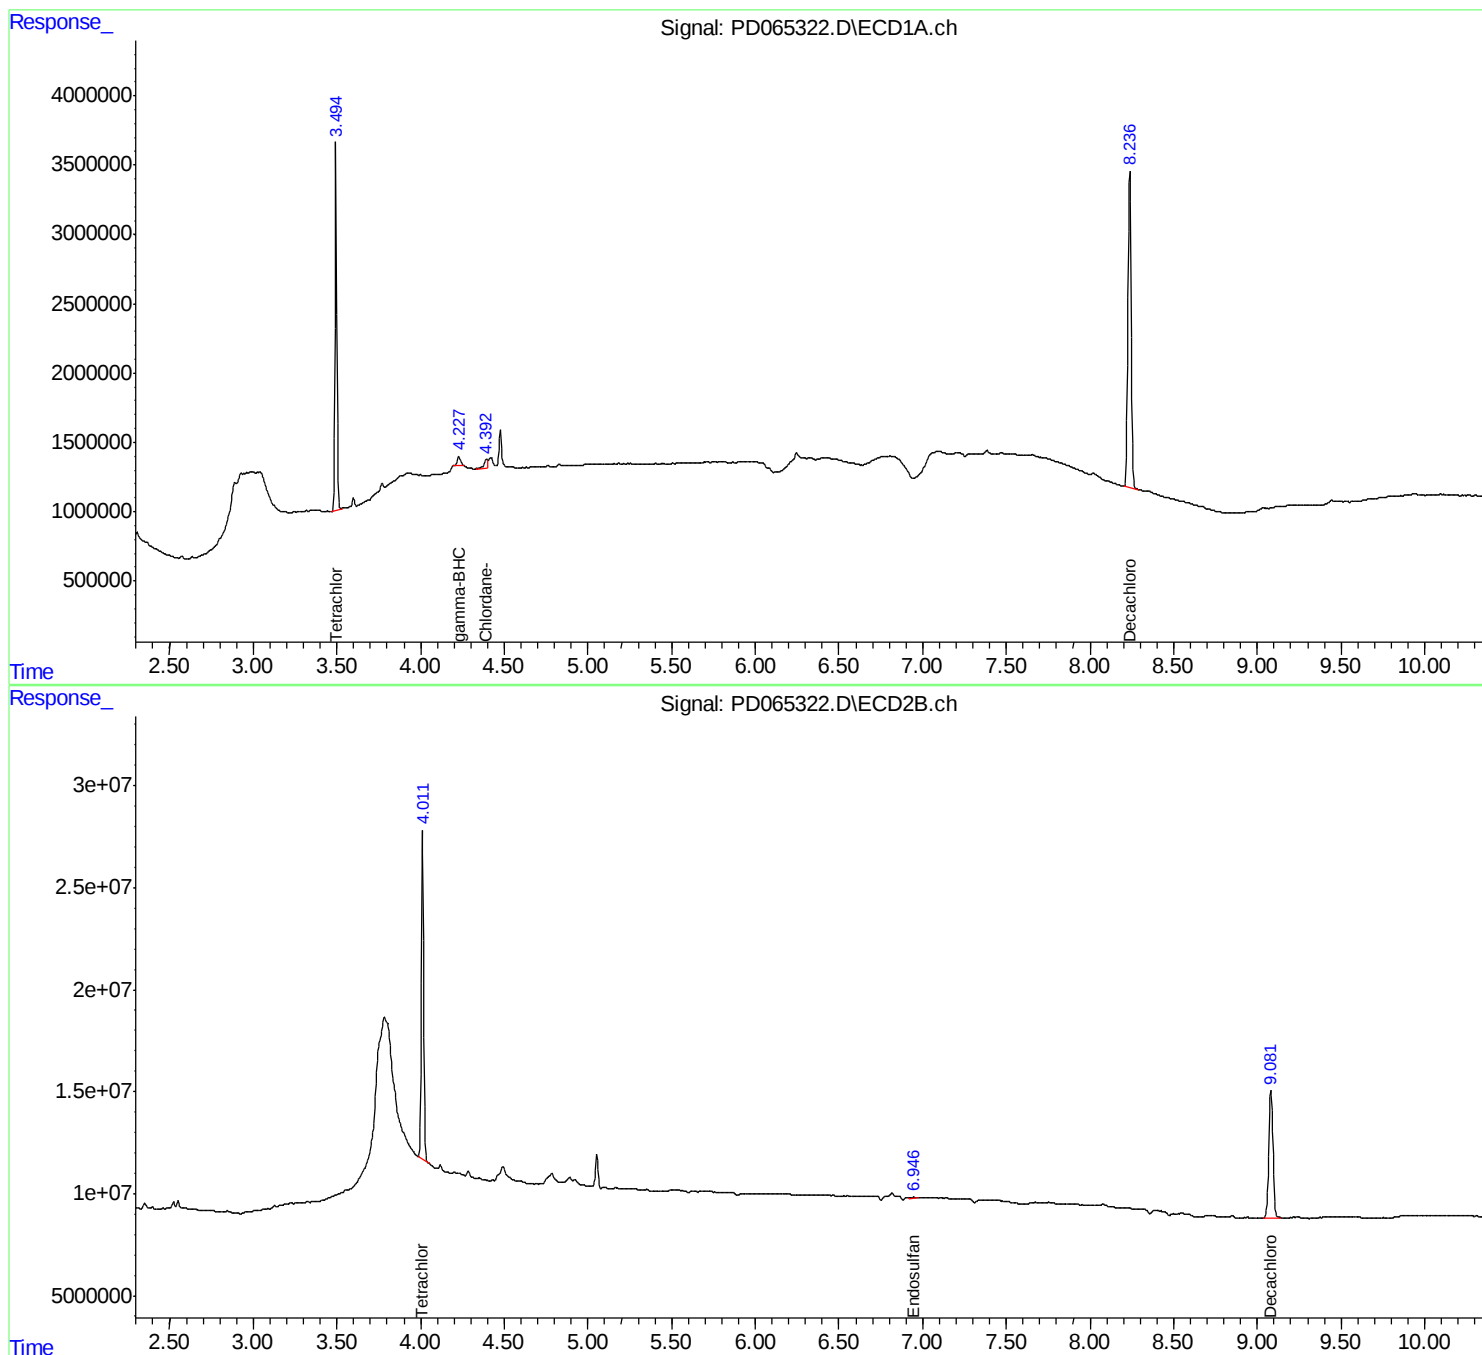


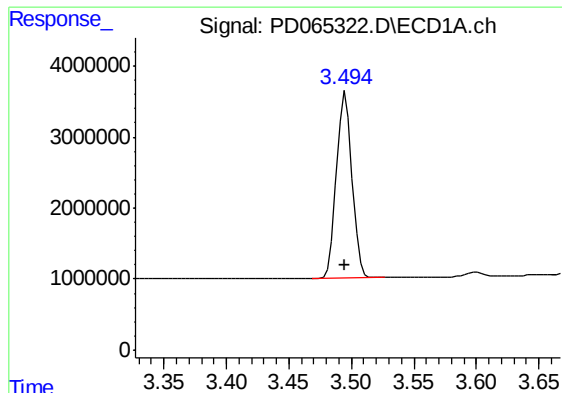

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 22857086
Conc: 21.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

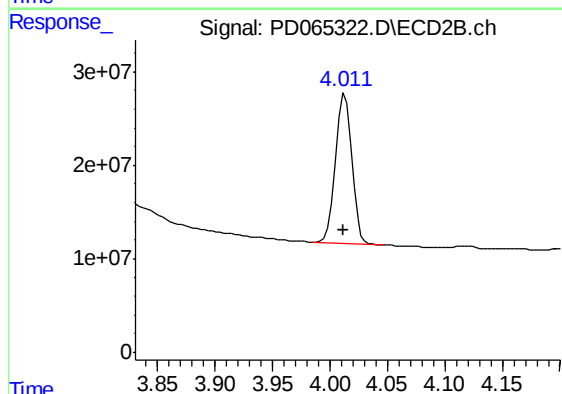


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 159789042
Conc: 23.37 ng/ml

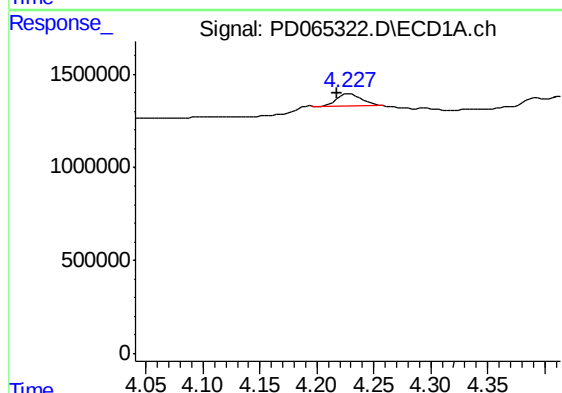


#3 gamma-BHC (Lindane)

R.T.: 4.228 min
Delta R.T.: 0.010 min
Response: 980533
Conc: 0.65 ng/ml

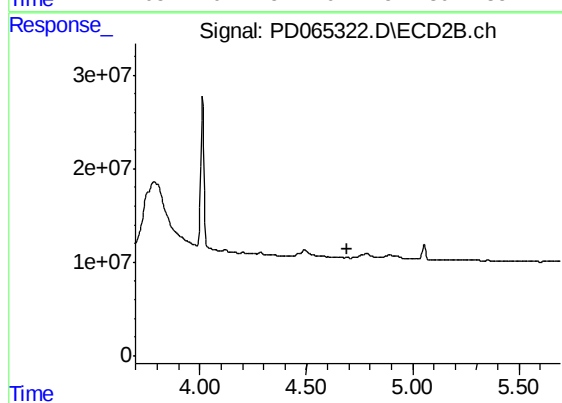

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.694 min
Response: 0
Conc: N.D.

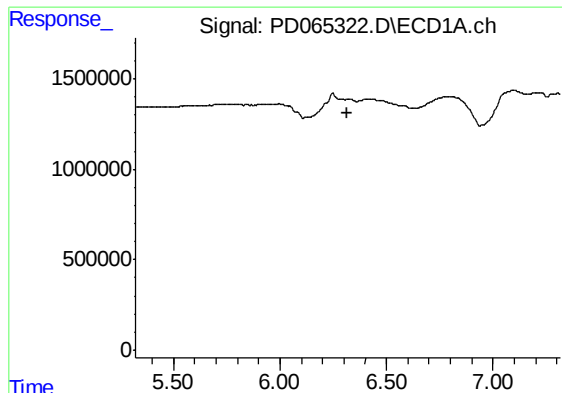

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

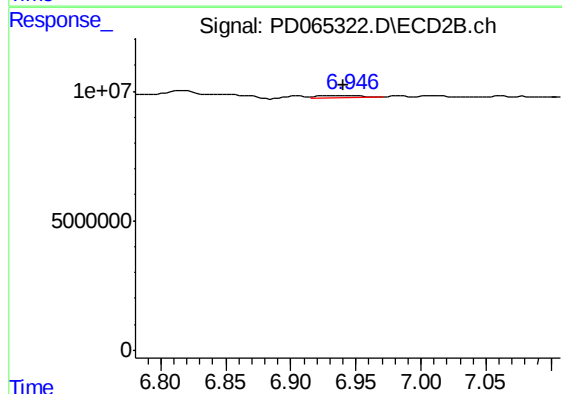


#15 Endosulfan II

R.T.: 6.947 min
Delta R.T.: 0.007 min
Response: 1448010
Conc: 0.28 ng/ml

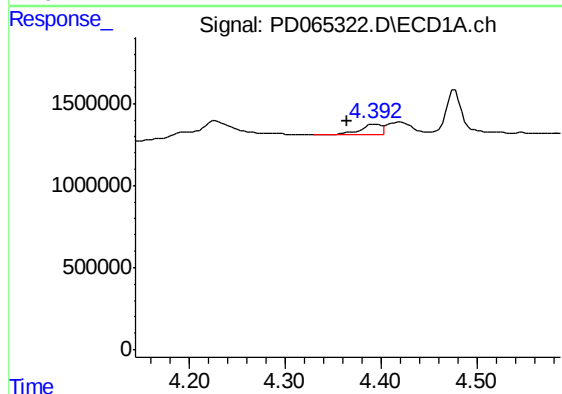


#23 Chlordane-1

R.T.: 4.393 min
Delta R.T.: 0.028 min
Response: 918019
Conc: 23.39 ng/ml

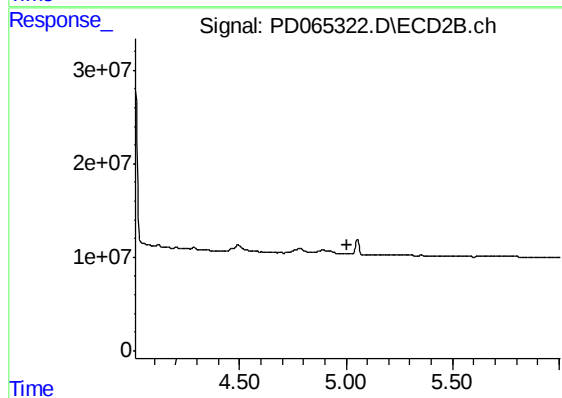

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

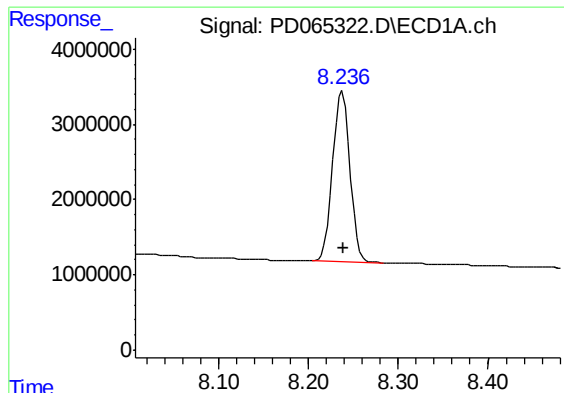

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: -0.001 min
Response: 30572409
Conc: 22.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

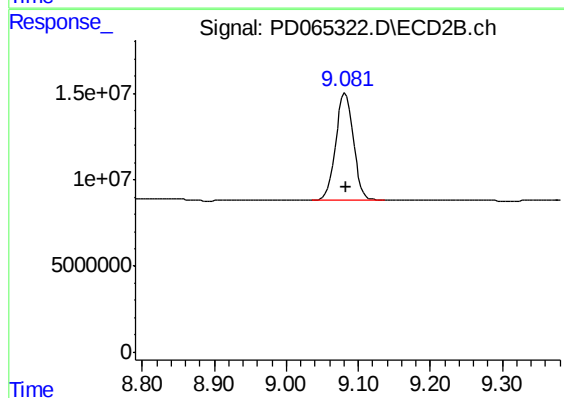

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 105327833
Conc: 24.32 ng/ml