

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082621\
 Data File : PD065327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 11:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 01:09:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:44:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.012	22834707	161.5E6	21.179	23.622
28)	SA Decachlor...	8.238	9.082	29529285	101.2E6	21.762	23.367
Target Compounds							
15)	B Endosulfa...	0.000	6.937	0	3221390	N.D.	0.617 #
20)	A Methoxychlor	0.000	7.604	0	2711976	N.D.	0.971 #
23)	Chlordane-1	4.393f	0.000	699823	0	17.829	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082621\
Data File : PD065327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 11:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 01:09:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:44:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

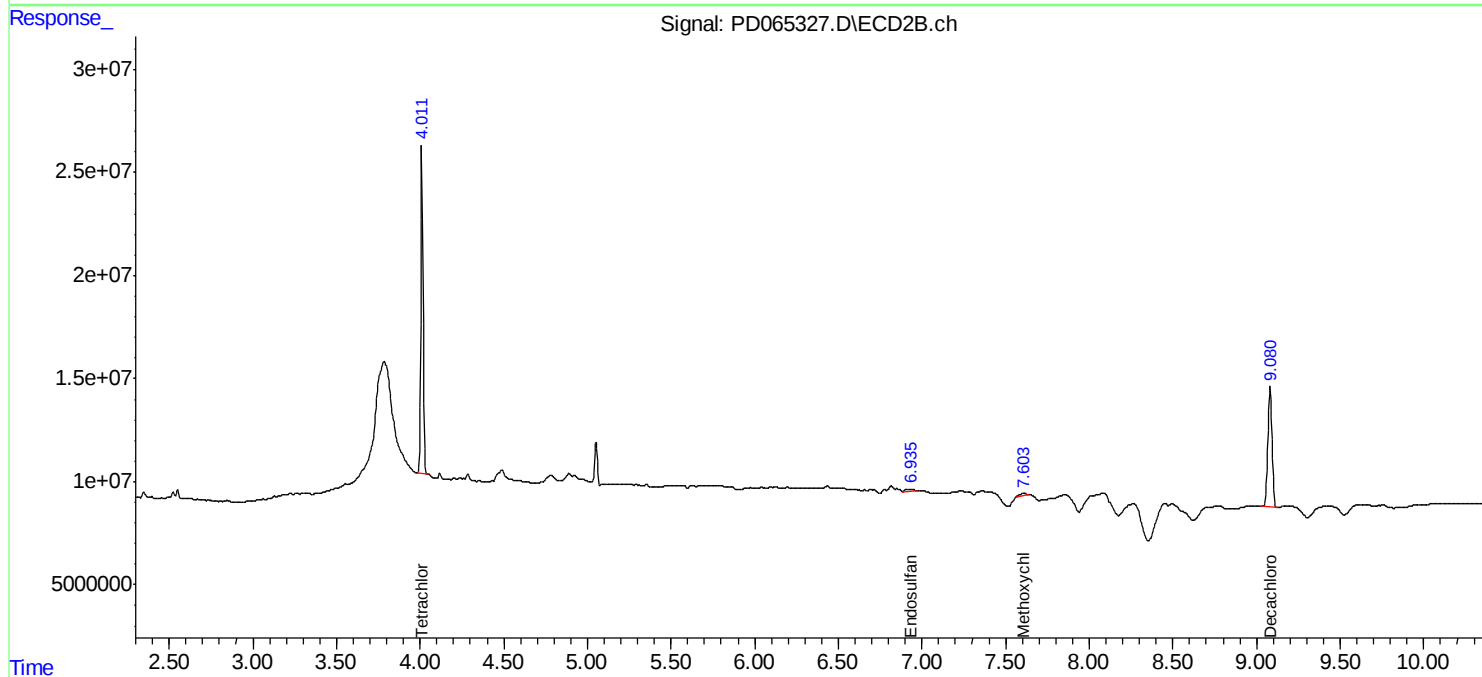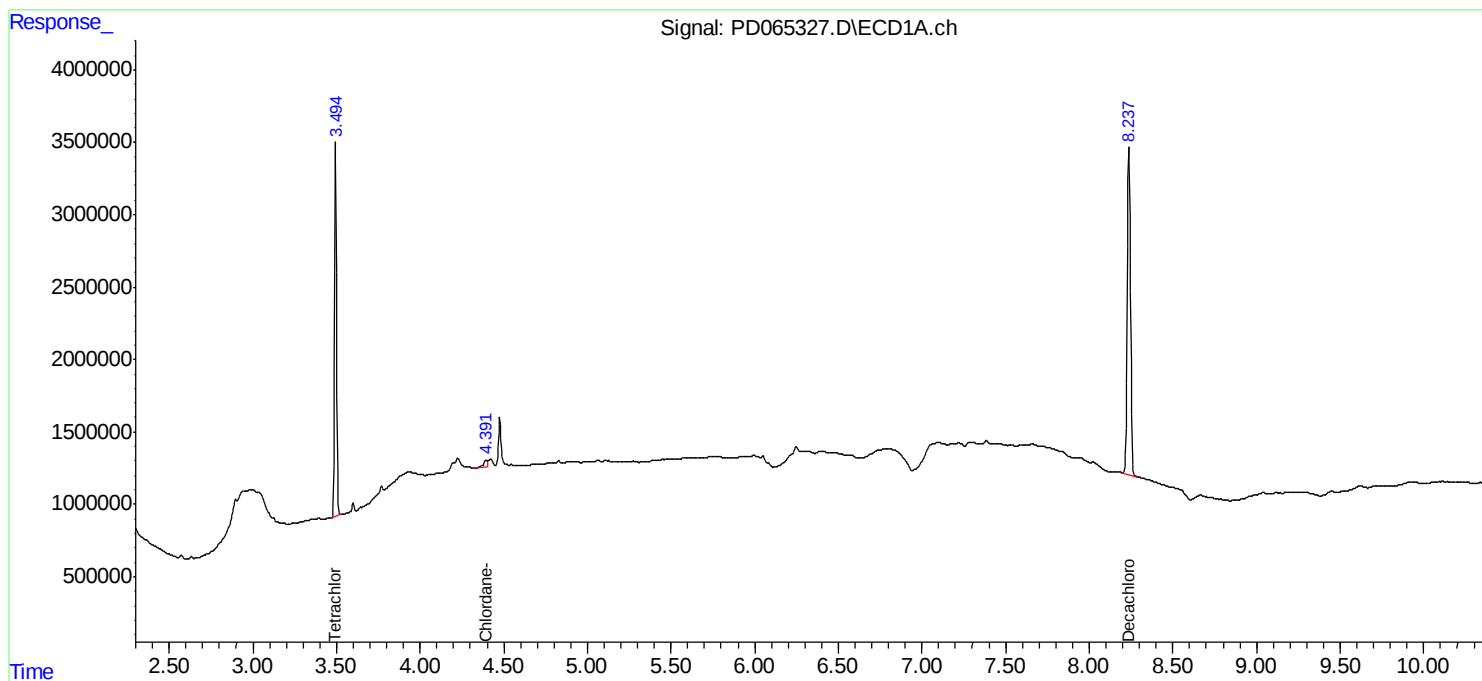


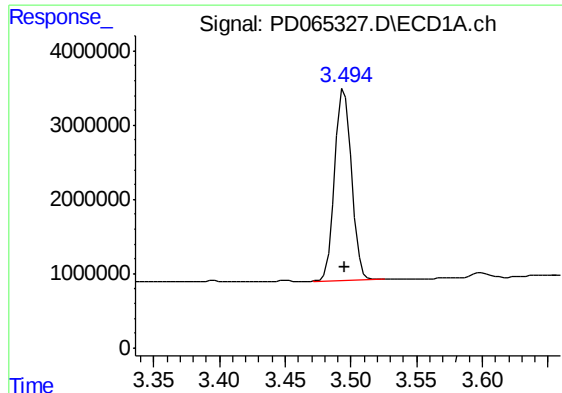

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 22834707
Conc: 21.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

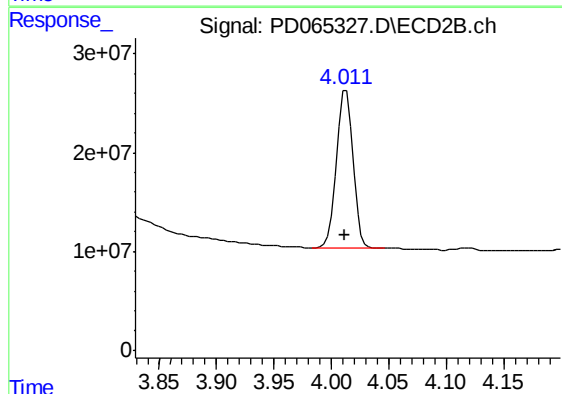


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 161511840
Conc: 23.62 ng/ml

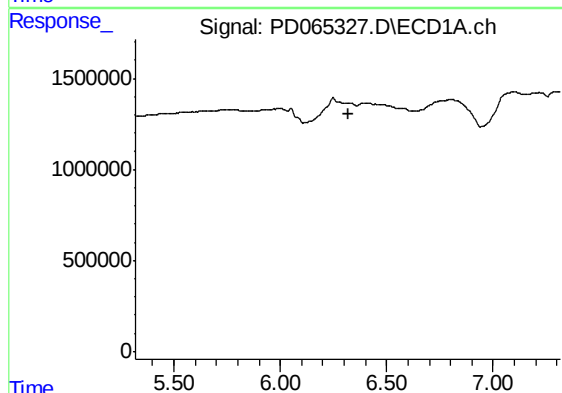


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.318 min
Response: 0
Conc: N.D.

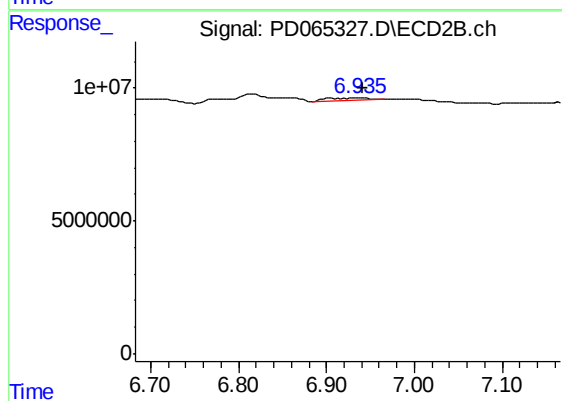

#15 Endosulfan II


R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 3221390
Conc: 0.62 ng/ml

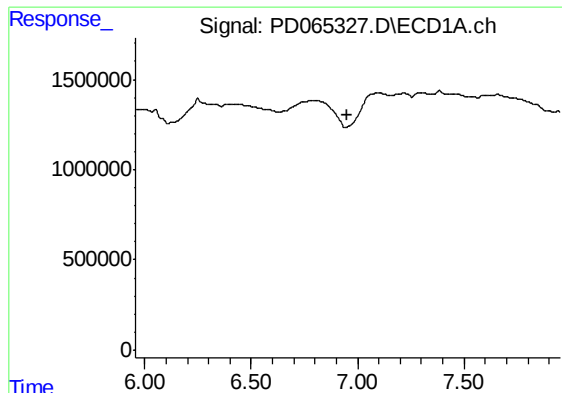

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

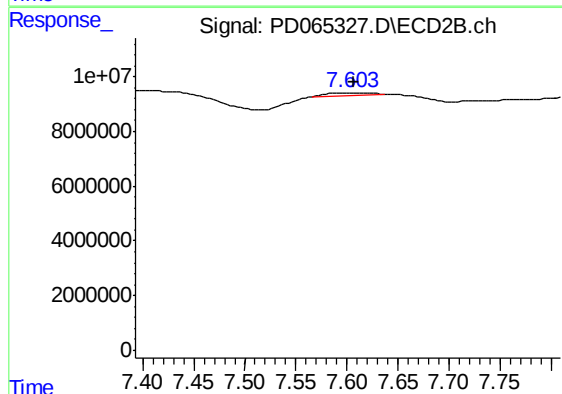


#20 Methoxychlor

R.T.: 7.604 min
Delta R.T.: -0.003 min
Response: 2711976
Conc: 0.97 ng/ml

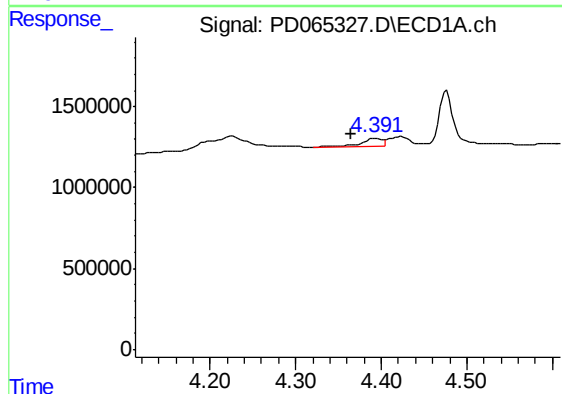


#23 Chlordane-1

R.T.: 4.393 min
Delta R.T.: 0.027 min
Response: 699823
Conc: 17.83 ng/ml

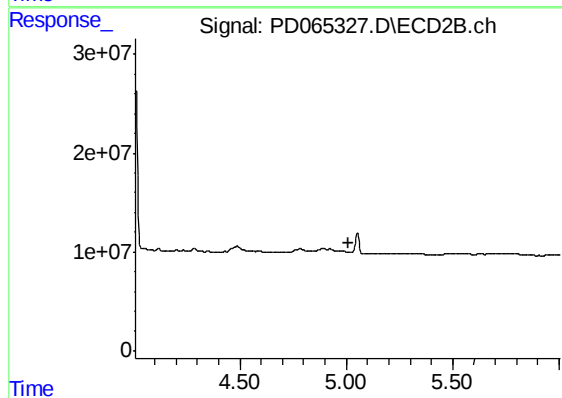

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

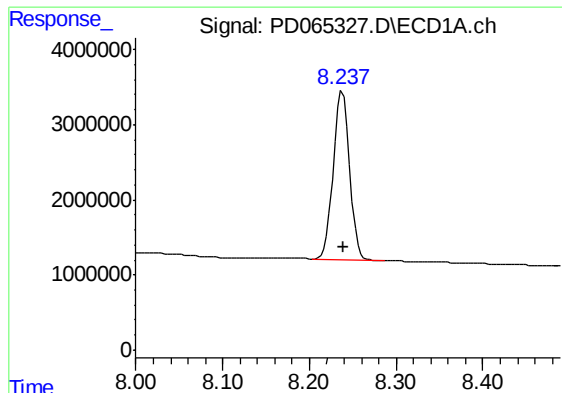

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 29529285
Conc: 21.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

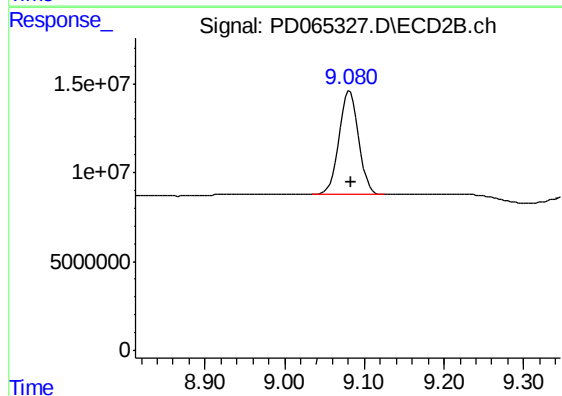

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.001 min
Response: 101195150
Conc: 23.37 ng/ml