

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
 Data File : PL069493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 16:39
 Operator : AR\AJ
 Sample : M3546-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TRP-7-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 04:43:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.566	7856508	26488869	17.029	18.492
28)	SA Decachlor...	10.399	11.486	10147997	20974289	15.035	17.114
Target Compounds							
16)	A 4,4'-DDD	0.000	9.106	0	1857247	N.D.	1.514 #
20)	A Methoxychlor	9.046f	0.000	739297	0	1.974	N.D. #
23)	Chlordane-1	0.000	6.973f	0	1664397	N.D.	29.400 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
Data File : PL069493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 16:39
Operator : AR\AJ
Sample : M3546-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TRP-7-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:43:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

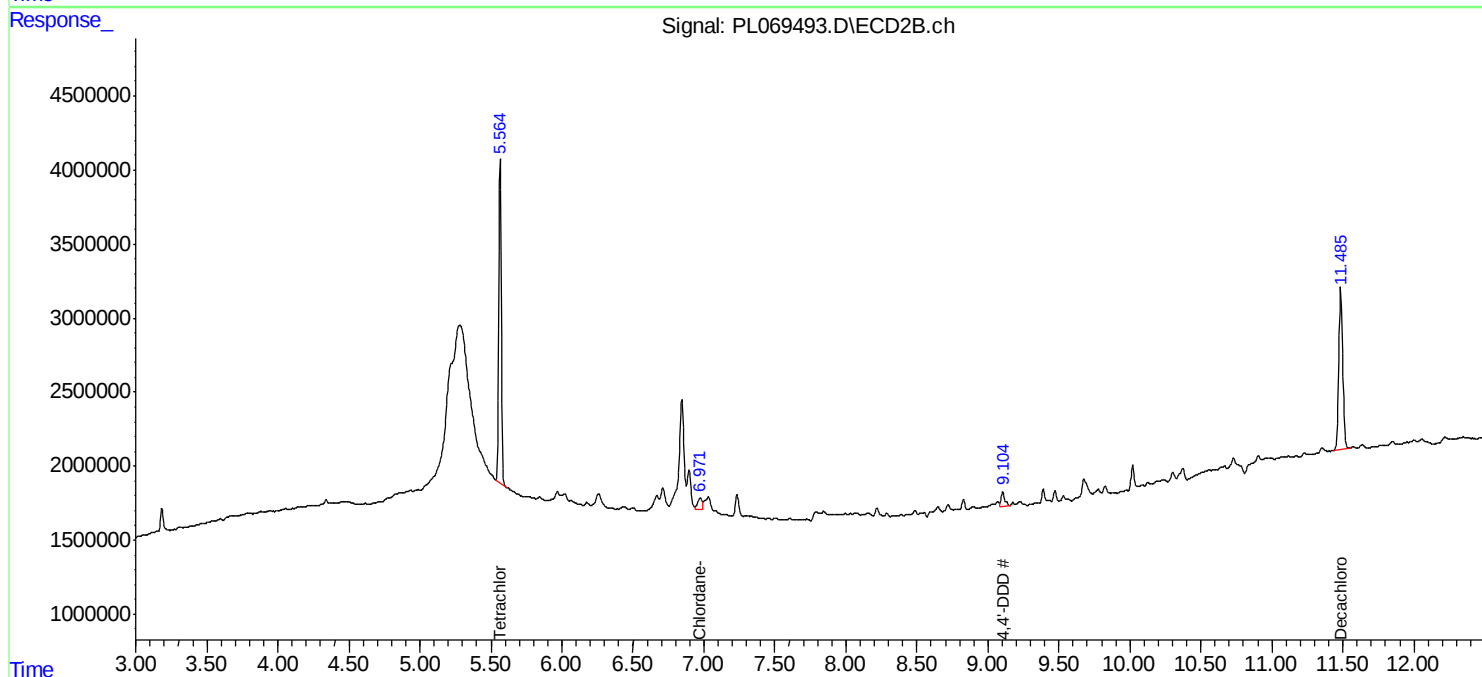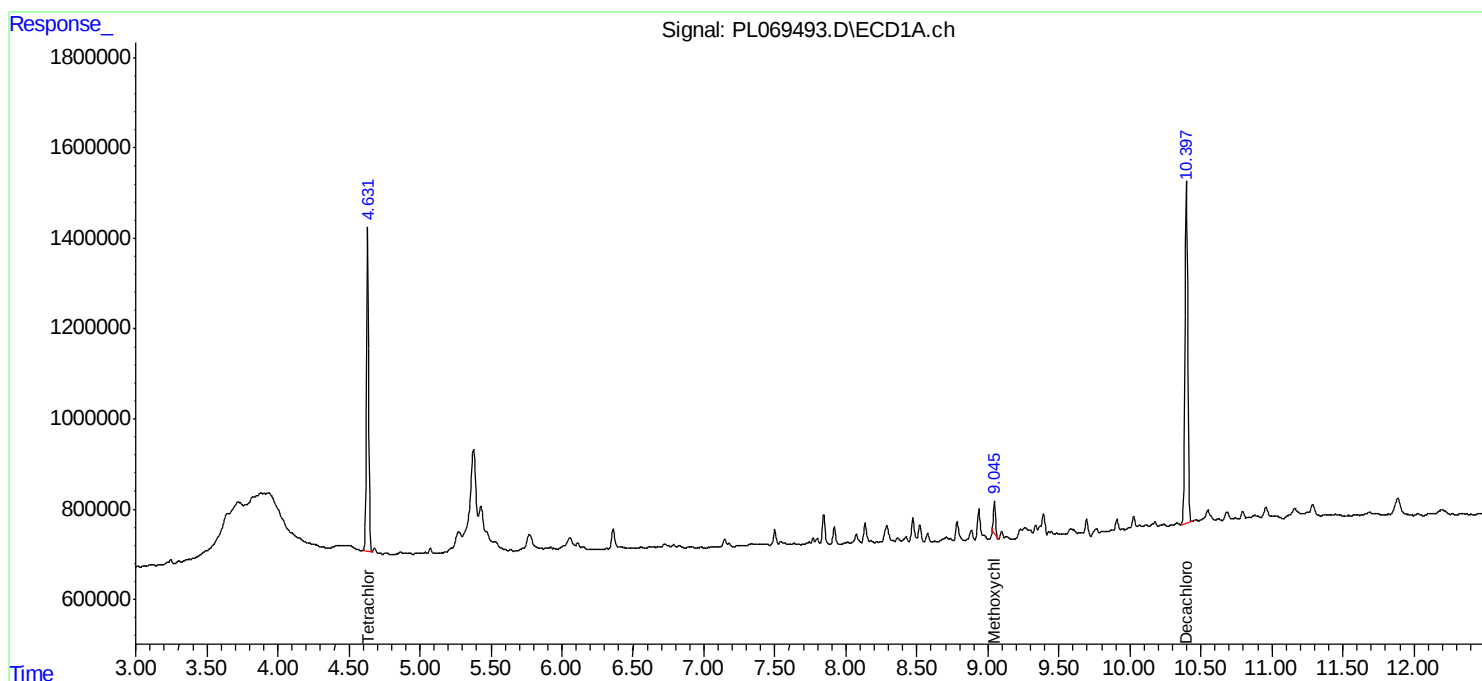


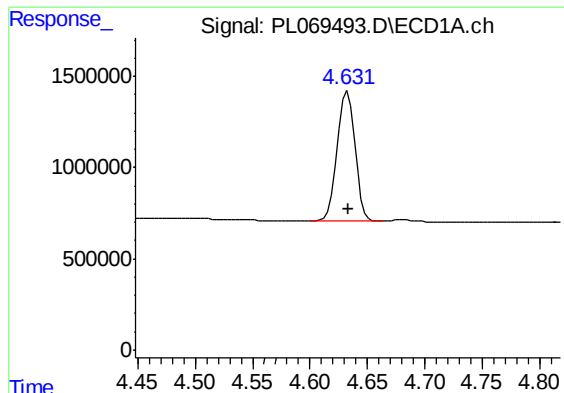

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 7856508
Conc: 17.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TRP-7-COMP

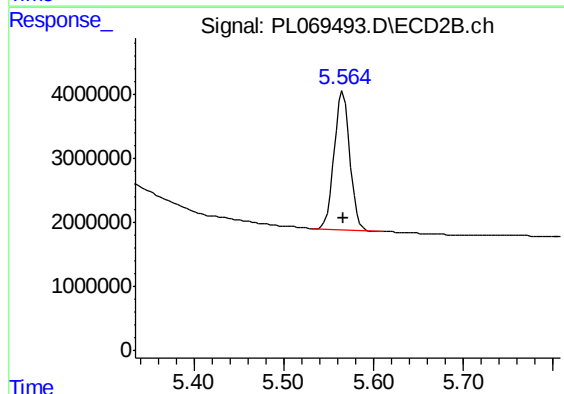


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 26488869
Conc: 18.49 ng/ml

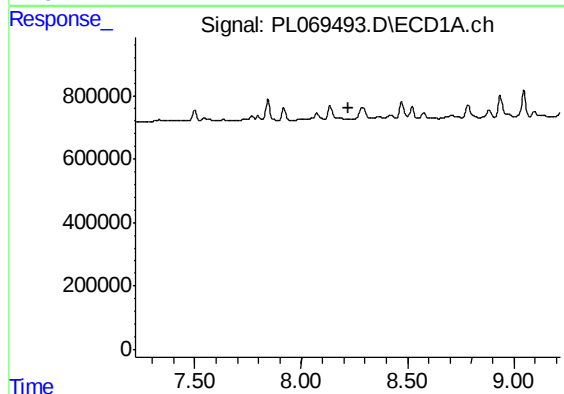


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.220 min
Response: 0
Conc: N.D.

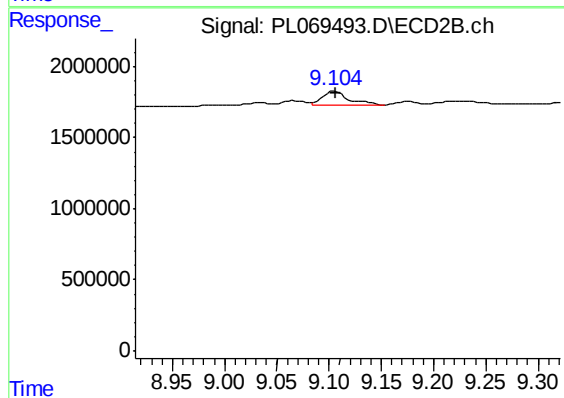

#16 4,4'-DDD


R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 1857247
Conc: 1.51 ng/ml

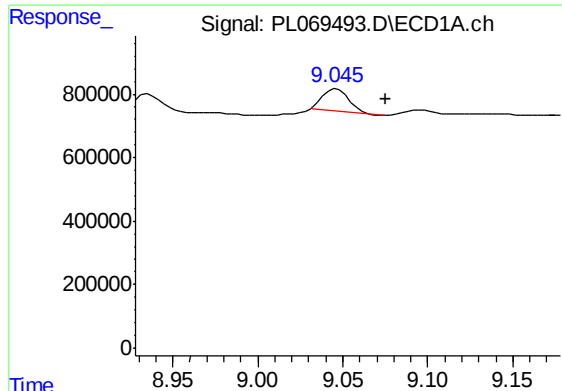

#20 Methoxychlor


R.T.: 9.046 min
Delta R.T.: -0.029 min
Response: 739297
Conc: 1.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TRP-7-COMP

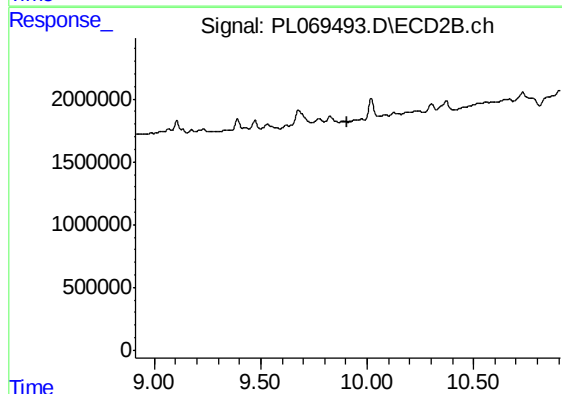


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.909 min
Response: 0
Conc: N.D.

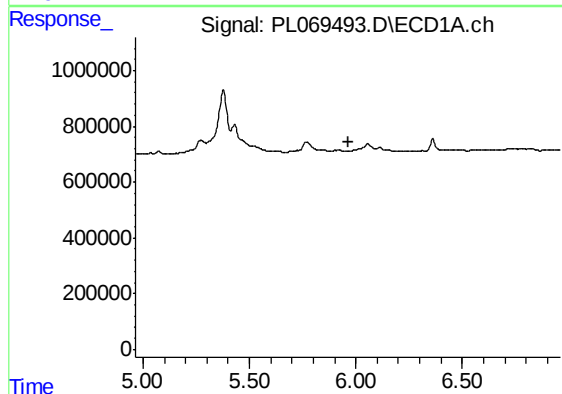


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.964 min
Response: 0
Conc: N.D.

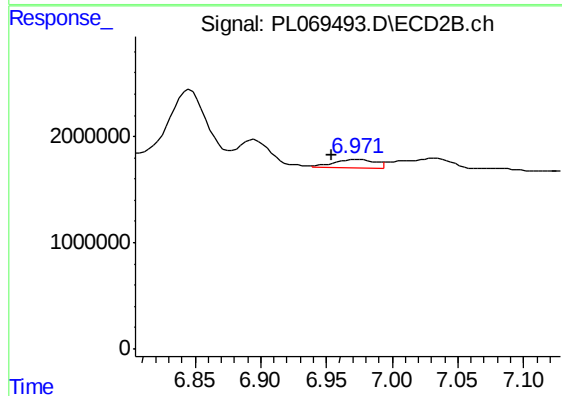

#23 Chlordane-1


R.T.: 6.973 min
Delta R.T.: 0.019 min
Response: 1664397
Conc: 29.40 ng/ml

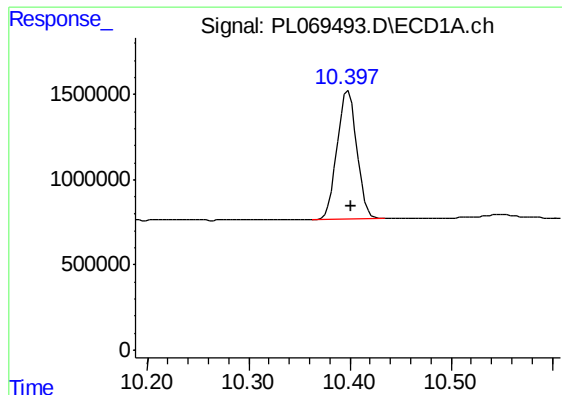

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.003 min
Response: 10147997
Conc: 15.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TRP-7-COMP

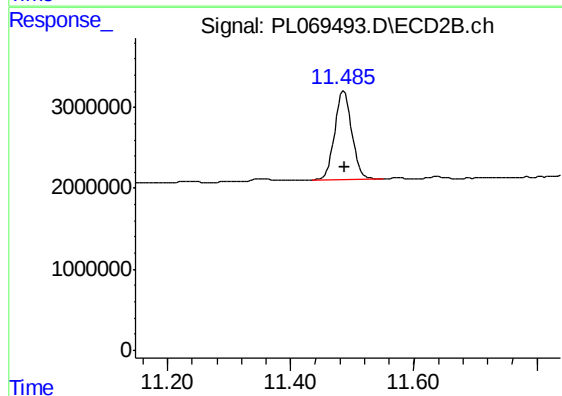

#28 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: -0.002 min
Response: 20974289
Conc: 17.11 ng/ml