

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
 Data File : PL069504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 19:59
 Operator : AR\AJ
 Sample : M3528-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-3-082421

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 04:47:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.565	7517405	26056048	16.294	18.189
28)	SA Decachlor...	10.397	11.485	8440081	16854222	12.505	13.752
Target Compounds							
7)	B delta-BHC	0.000	7.082f	0	1537982	N.D.	0.833 #
23)	Chlordane-1	0.000	6.979f	0	1370076	N.D.	24.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
Data File : PL069504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 19:59
Operator : AR\AJ
Sample : M3528-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PT-3-082421

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:47:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

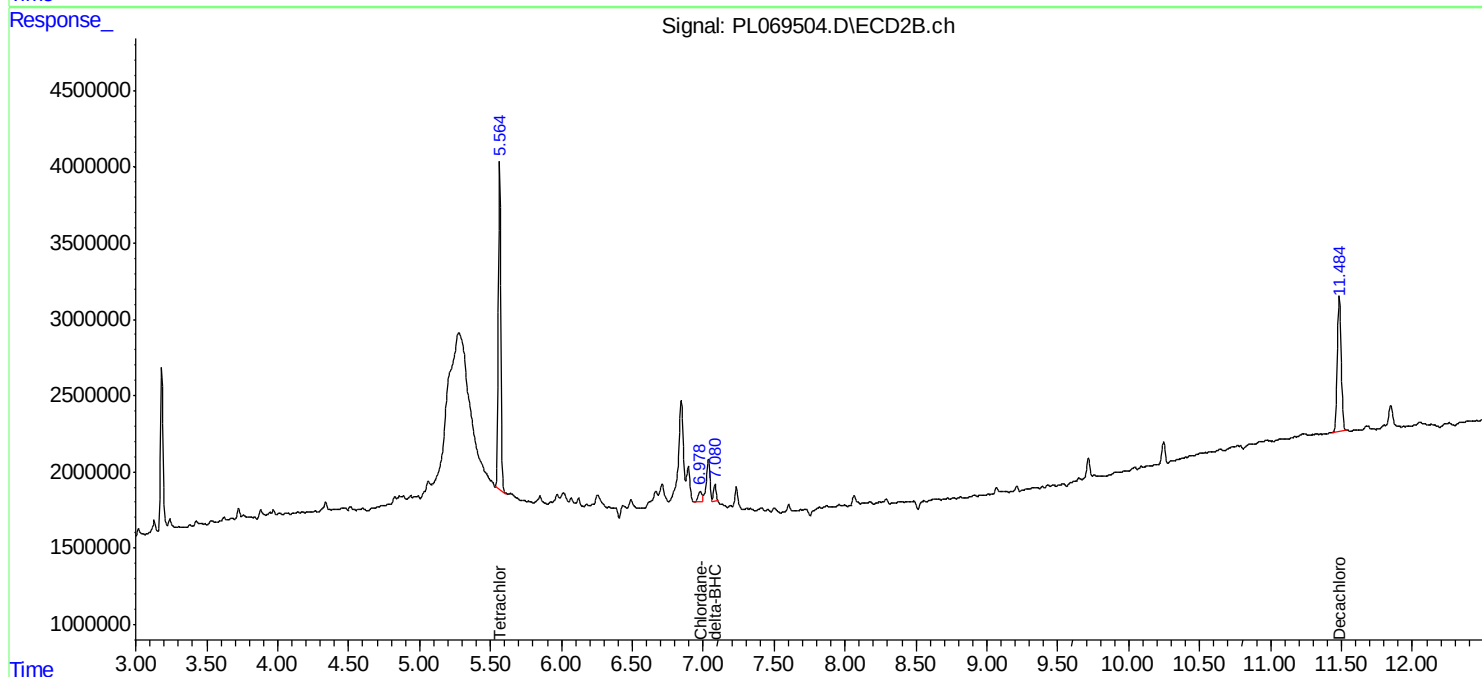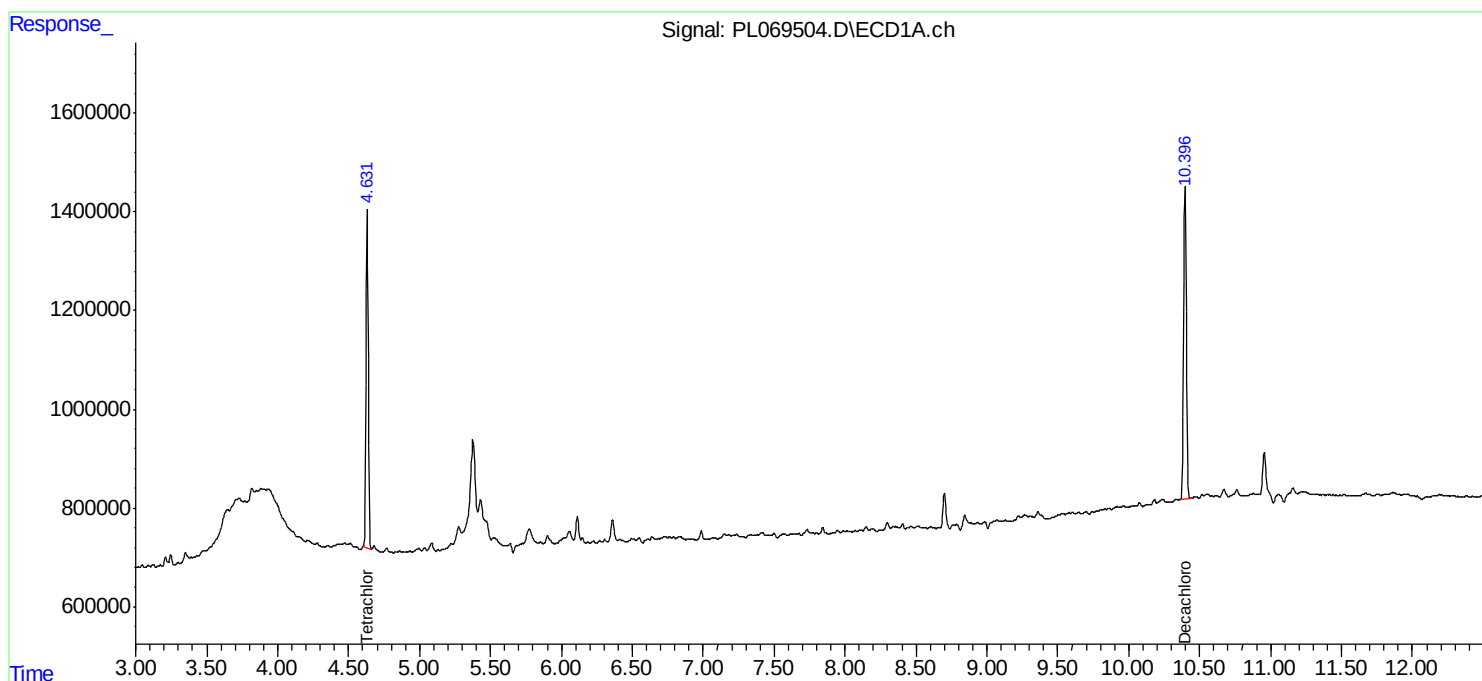


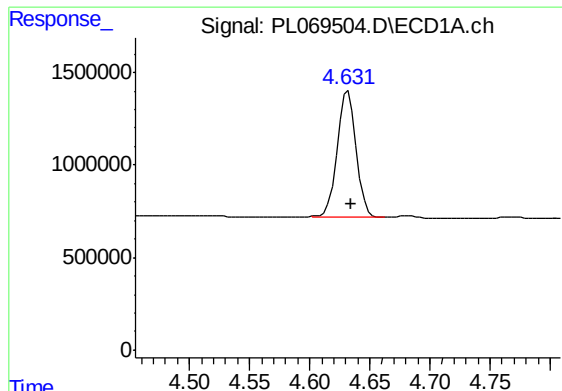

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 7517405
Conc: 16.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-3-082421

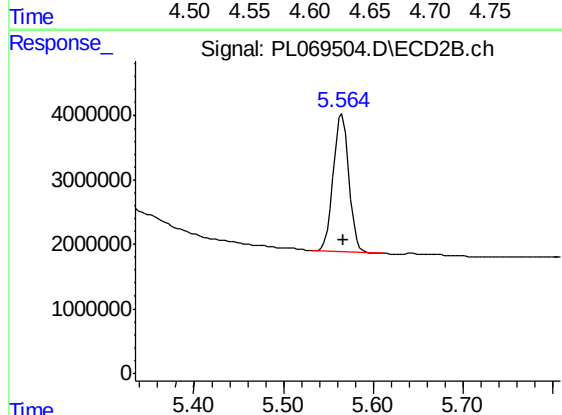


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: -0.001 min
Response: 26056048
Conc: 18.19 ng/ml

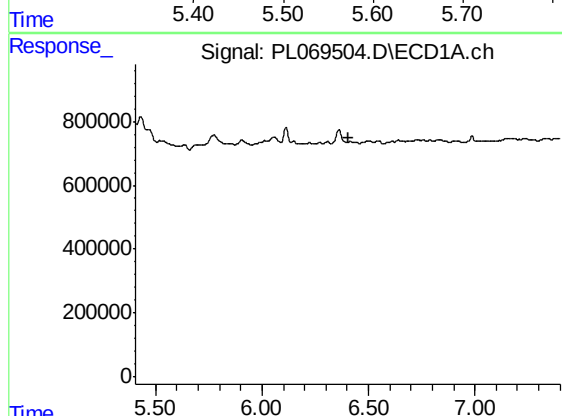


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

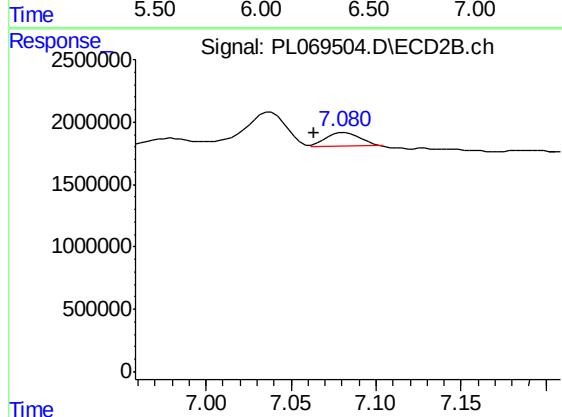

#7 delta-BHC


R.T.: 7.082 min
Delta R.T.: 0.018 min
Response: 1537982
Conc: 0.83 ng/ml

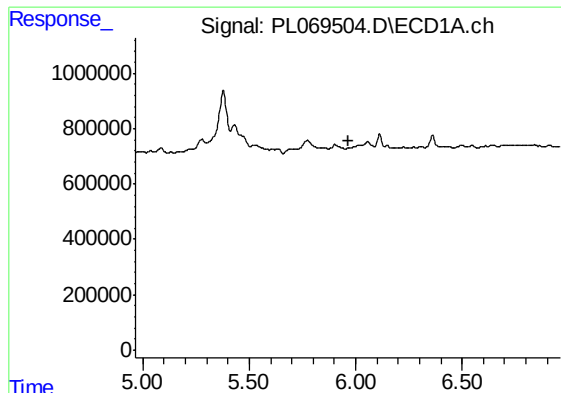

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-3-082421

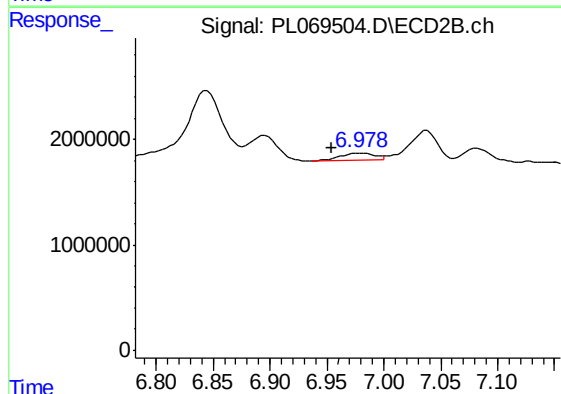


#23 Chlordane-1

R.T.: 6.979 min
Delta R.T.: 0.025 min
Response: 1370076
Conc: 24.20 ng/ml

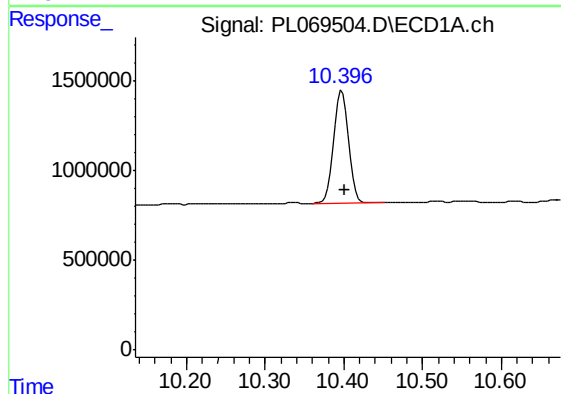

#28 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: -0.004 min
Response: 8440081
Conc: 12.50 ng/ml

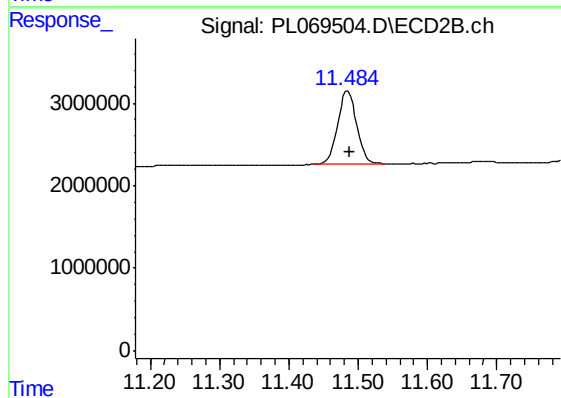

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.003 min
Response: 16854222
Conc: 13.75 ng/ml