

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
 Data File : PL069490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 15:49
 Operator : AR\AJ
 Sample : M3545-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NCS-COMP-1

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:04:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 04:42:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.566	6174912	20297189	13.384	14.169
28)	SA Decachlor...	10.398	11.486	7599722	15642262	11.260	12.763
Target Compounds							
12)	B 4,4'-DDE	7.633	8.563	2554876	12648391	4.517	9.042m#
16)	A 4,4'-DDD	8.216	9.106	2733237	14093015	5.374m	11.490 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
Data File : PL069490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 15:49
Operator : AR\AJ
Sample : M3545-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
NCS-COMP-1


Manual Integrations
APPROVED

mohammad
8/27/2021 5:04:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:42:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

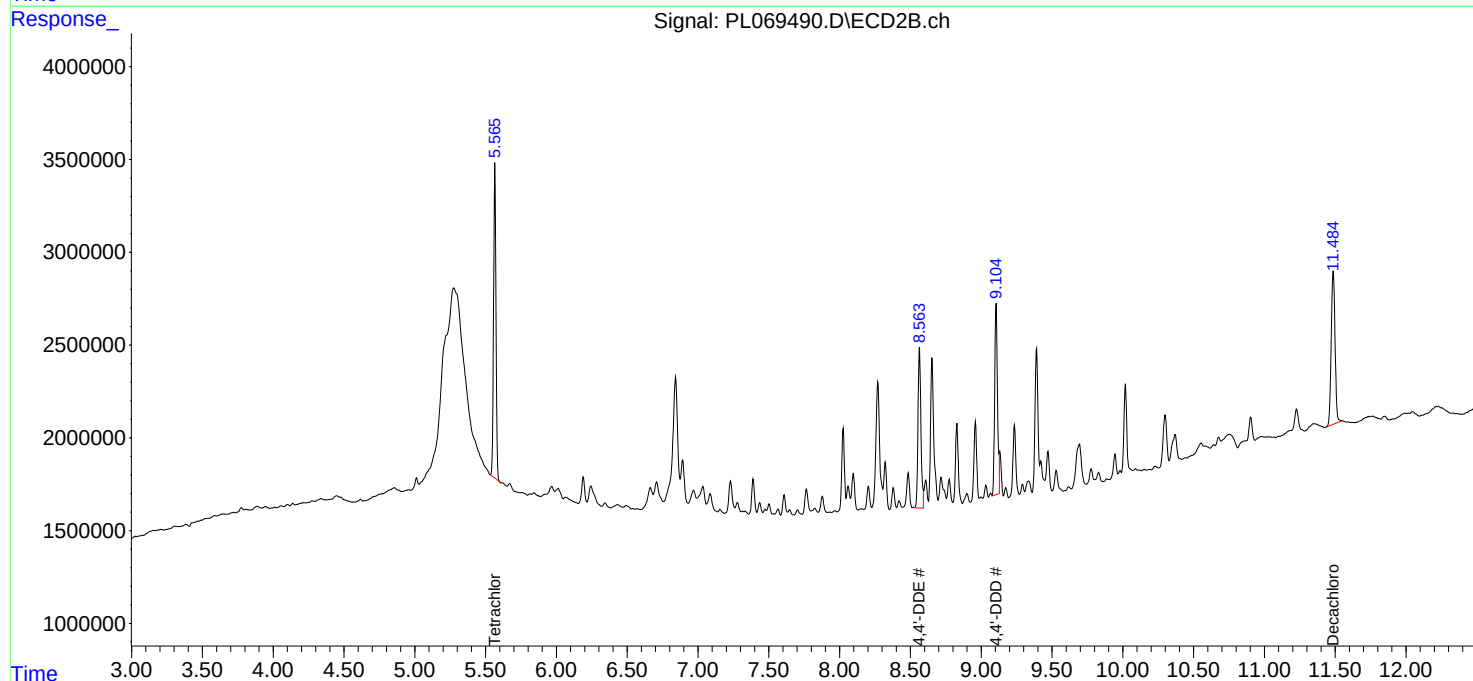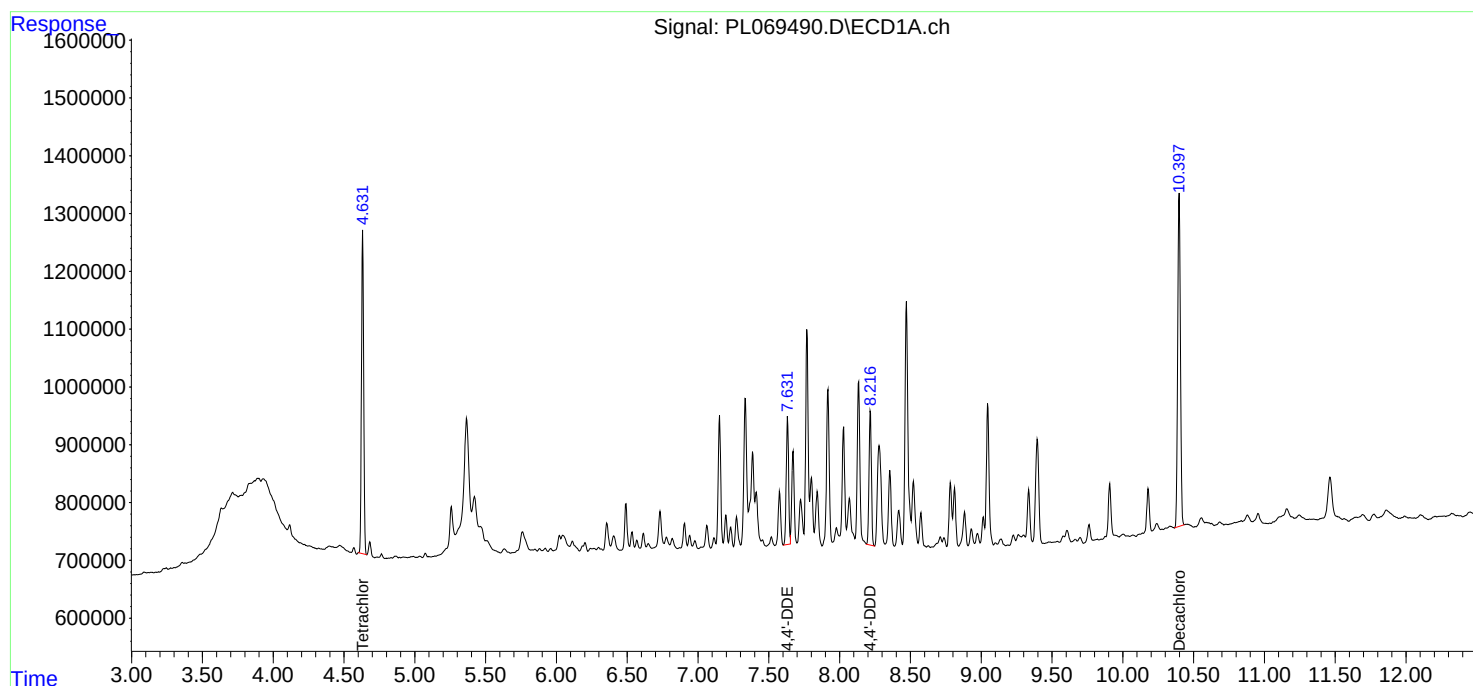

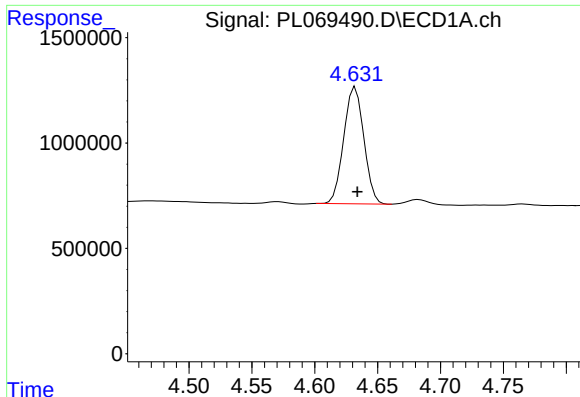


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 6174912
Conc: 13.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
NCS-COMP-1


Manual Integrations
APPROVED

mohammad
8/27/2021 5:04:23 PM

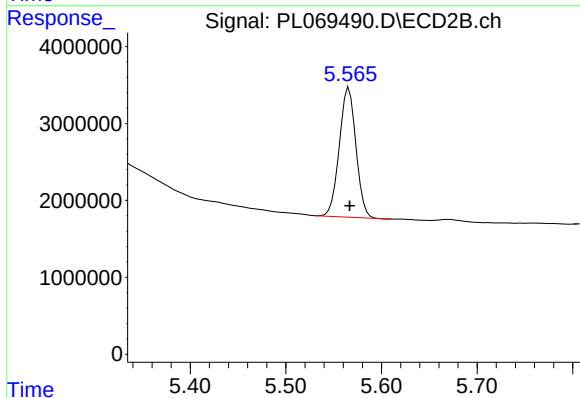


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 20297189
Conc: 14.17 ng/ml

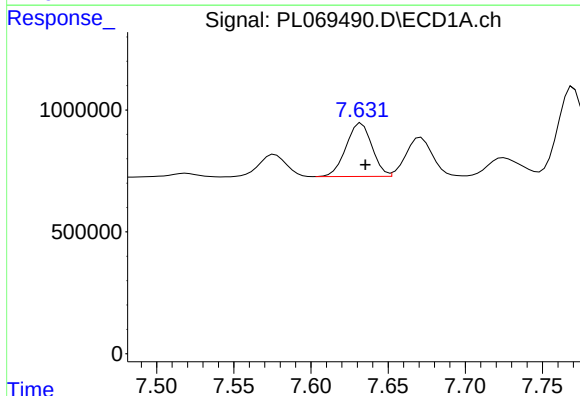


#12 4,4'-DDE

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 2554876
Conc: 4.52 ng/ml

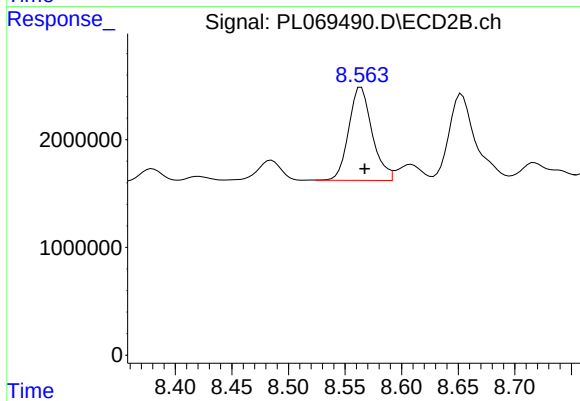

#12 4,4'-DDE

R.T.: 8.563 min
Delta R.T.: -0.005 min
Response: 12648391
Conc: 9.04 ng/ml m

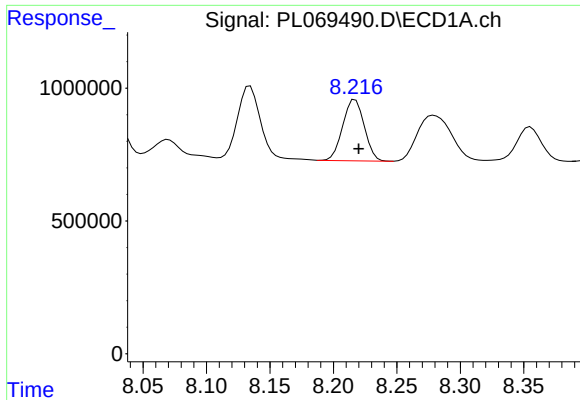


#16 4,4'-DDD

R.T.: 8.216 min
Delta R.T.: -0.004 min
Response: 2733237
Conc: 5.37 ng/ml m

Instrument :
ECD_L
ClientSampleId :
NCS-COMP-1


Manual Integrations
APPROVED

mohammad
8/27/2021 5:04:23 PM

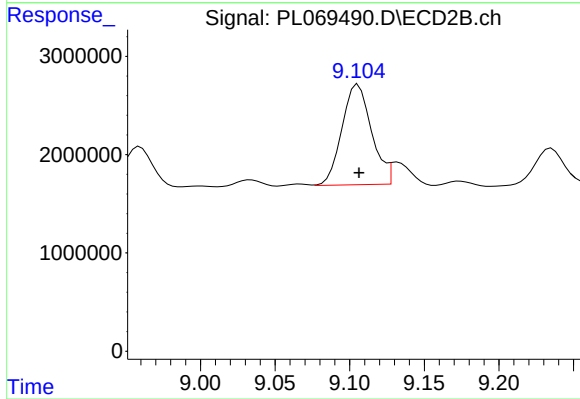


#16 4,4'-DDD

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 14093015
Conc: 11.49 ng/ml

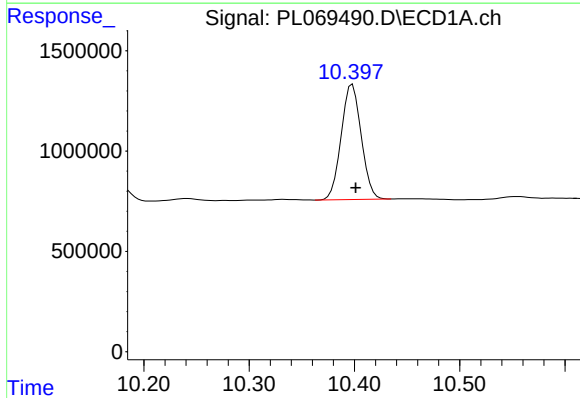

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.003 min
Response: 7599722
Conc: 11.26 ng/ml

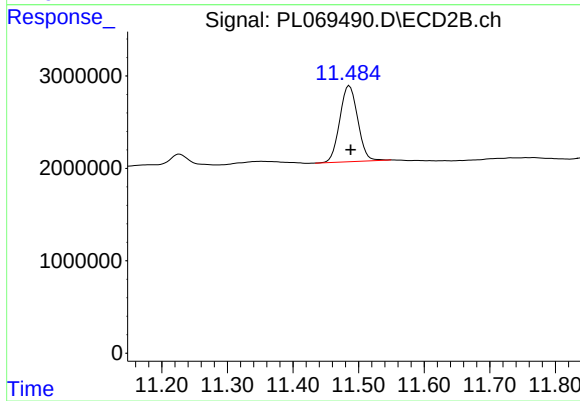

#28 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: -0.002 min
Response: 15642262
Conc: 12.76 ng/ml