

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
 Data File : PL069491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 16:05
 Operator : AR\AJ
 Sample : M3545-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NCS-COMP-2

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:04:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 04:43:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.566	5705133	18627167	12.366	13.003
28)	SA Decachlor...	10.398	11.485	6960722	13576703	10.313	11.078
Target Compounds							
12)	B 4,4'-DDE	7.633	8.564	2178230	9372530	3.851	6.700 #
16)	A 4,4'-DDD	8.217	9.104	2134542	12519604	4.197	10.207m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082621\
Data File : PL069491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 16:05
Operator : AR\AJ
Sample : M3545-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
NCS-COMP-2


Manual Integrations
APPROVED

mohammad
8/27/2021 5:04:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:43:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

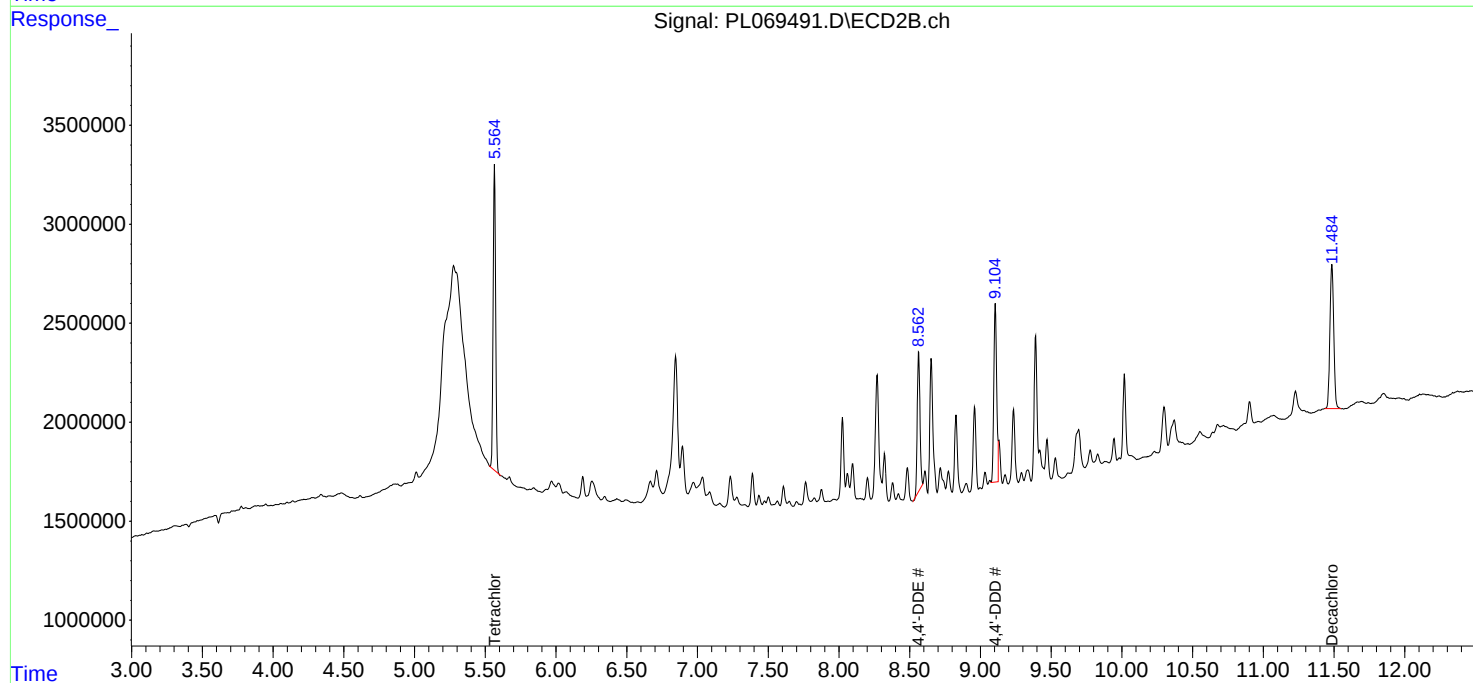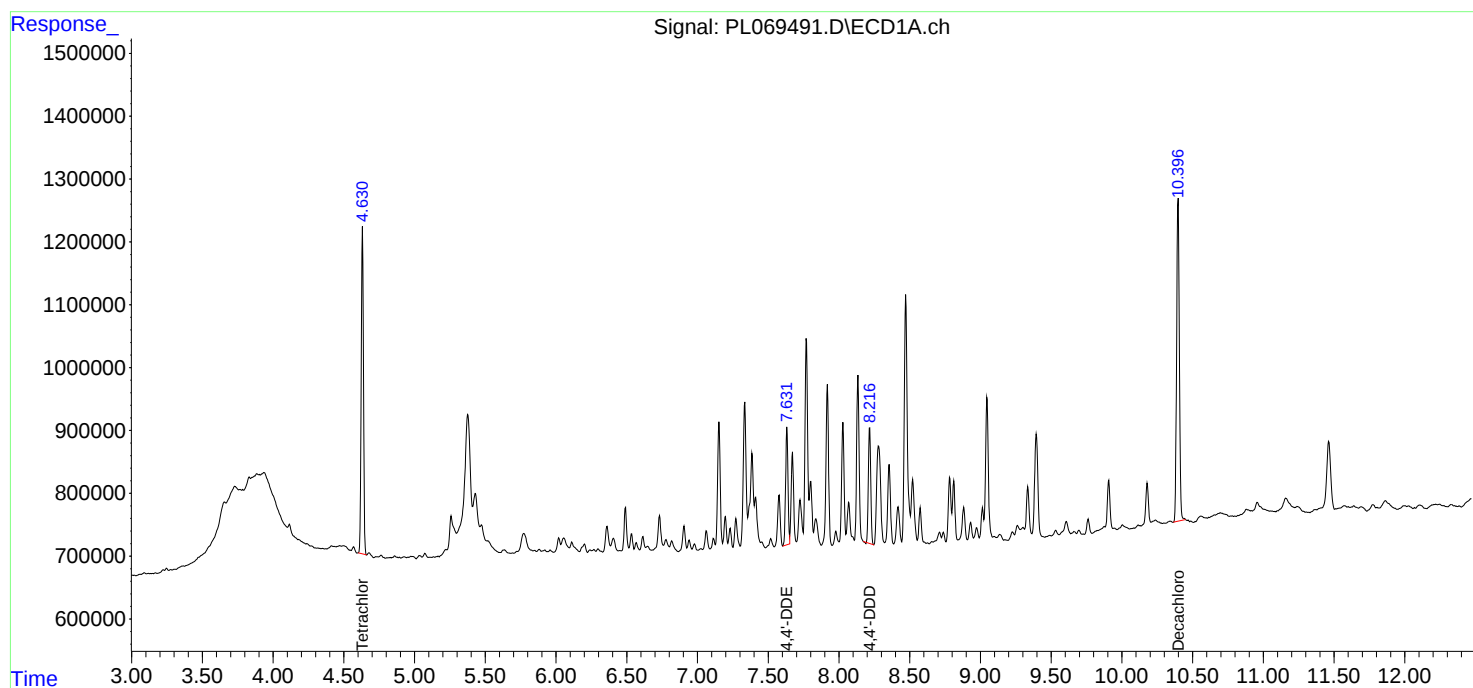

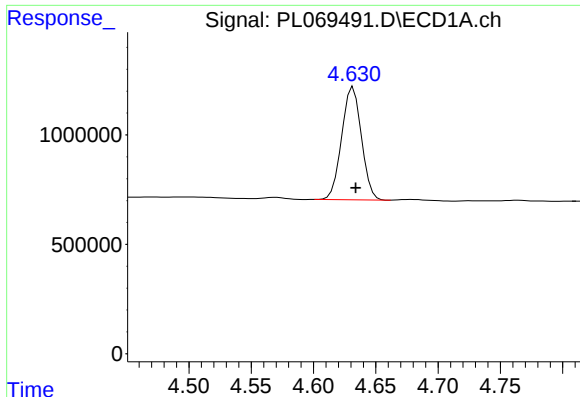


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 5705133
Conc: 12.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
NCS-COMP-2


Manual Integrations
APPROVED

mohammad
8/27/2021 5:04:25 PM

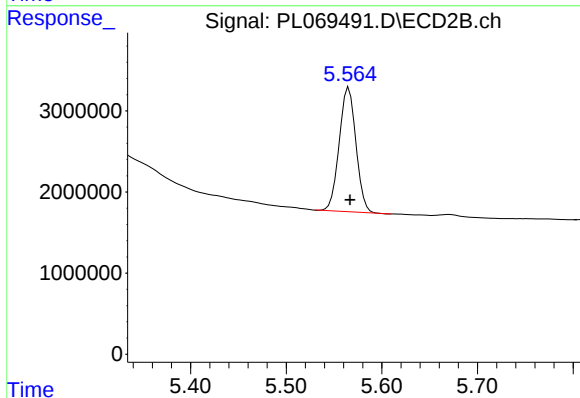


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.001 min
Response: 18627167
Conc: 13.00 ng/ml

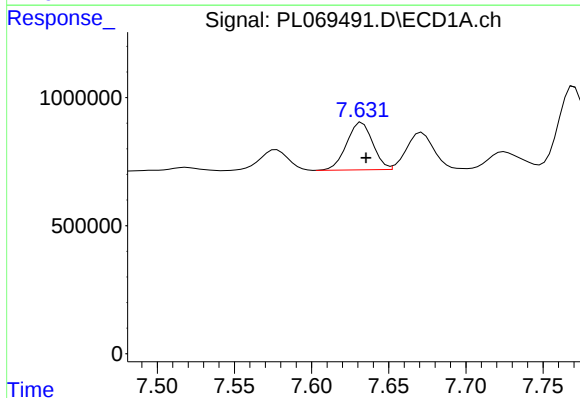


#12 4,4'-DDE

R.T.: 7.633 min
Delta R.T.: -0.003 min
Response: 2178230
Conc: 3.85 ng/ml

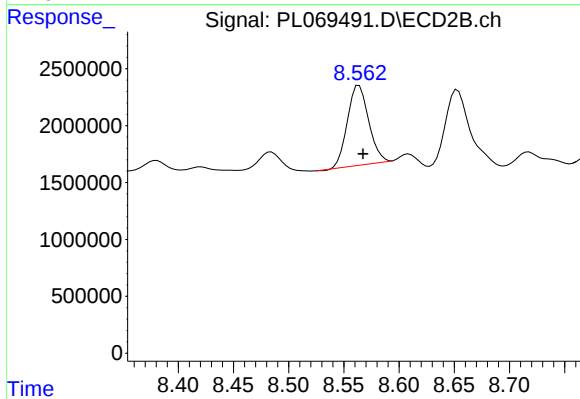

#12 4,4'-DDE

R.T.: 8.564 min
Delta R.T.: -0.004 min
Response: 9372530
Conc: 6.70 ng/ml

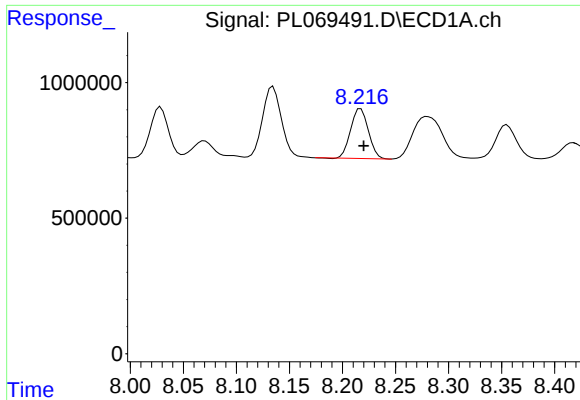


#16 4,4'-DDD

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 2134542
Conc: 4.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
NCS-COMP-2


Manual Integrations
APPROVED

mohammad
8/27/2021 5:04:25 PM

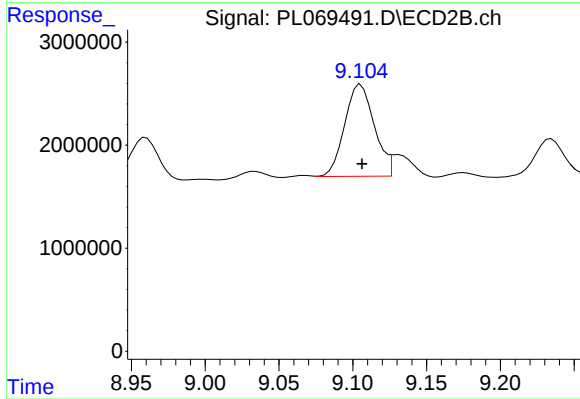


#16 4,4'-DDD

R.T.: 9.104 min
Delta R.T.: -0.002 min
Response: 12519604
Conc: 10.21 ng/ml m

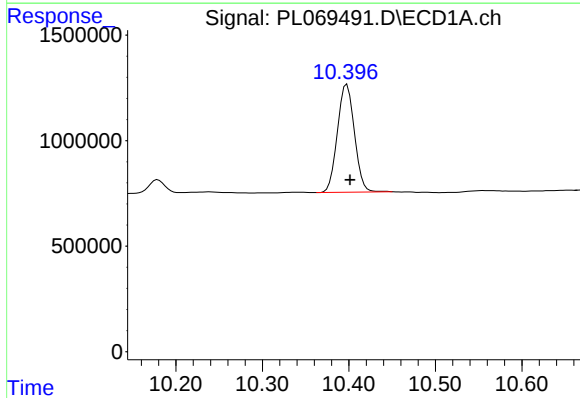

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.004 min
Response: 6960722
Conc: 10.31 ng/ml

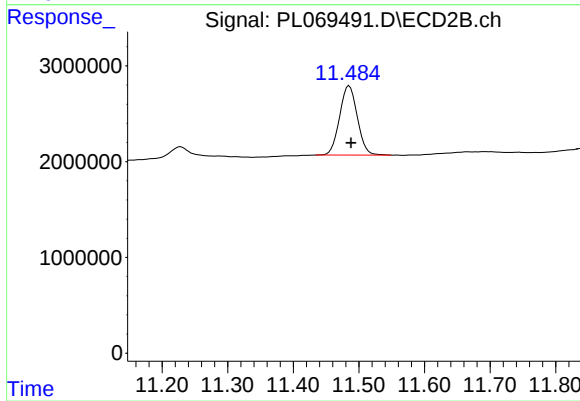

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.003 min
Response: 13576703
Conc: 11.08 ng/ml