

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082721\
 Data File : PL069524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2021 14:56
 Operator : AR\AJ
 Sample : M3463-23RE
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 23:46:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.568	7709479	24784776	16.710	17.302
28)	SA Decachlor...	10.402	11.492	9022972	18620248	13.368	15.193
Target Compounds							
7)	B delta-BHC	0.000	7.042f	0	2451881	N.D.	1.328 #
10)	B gamma-Chl...	0.000	8.301	0	790553	N.D.	0.514 #
11)	B alpha-Chl...	0.000	8.384	0	1466238	N.D.	0.981 #
17)	MA 4,4'-DDT	0.000	9.395f	0	639973	N.D.	0.522 #
25)	Chlordane-3	0.000	8.301	0	790553	N.D.	3.692 #
26)	Chlordane-4	0.000	8.384	0	1466238	N.D.	5.697 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082721\
Data File : PL069524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 14:56
Operator : AR\AJ
Sample : M3463-23RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 23:46:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

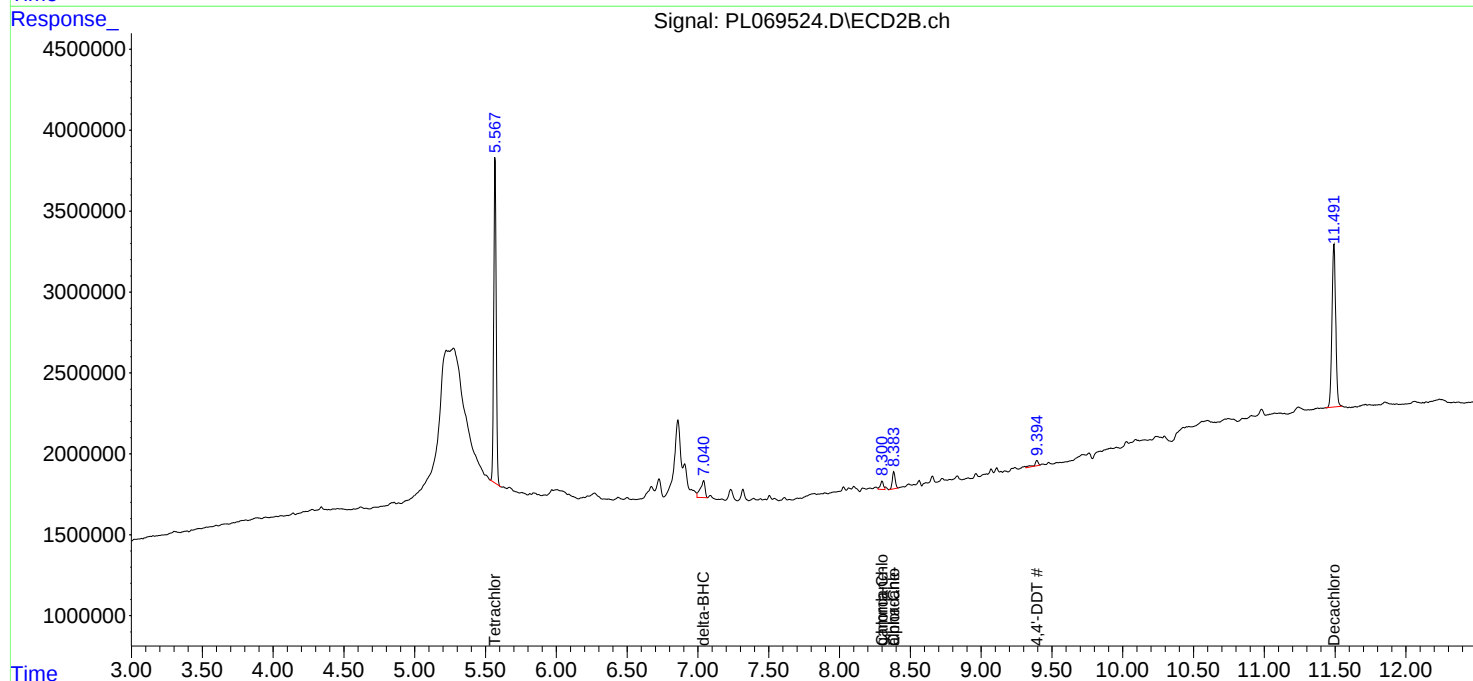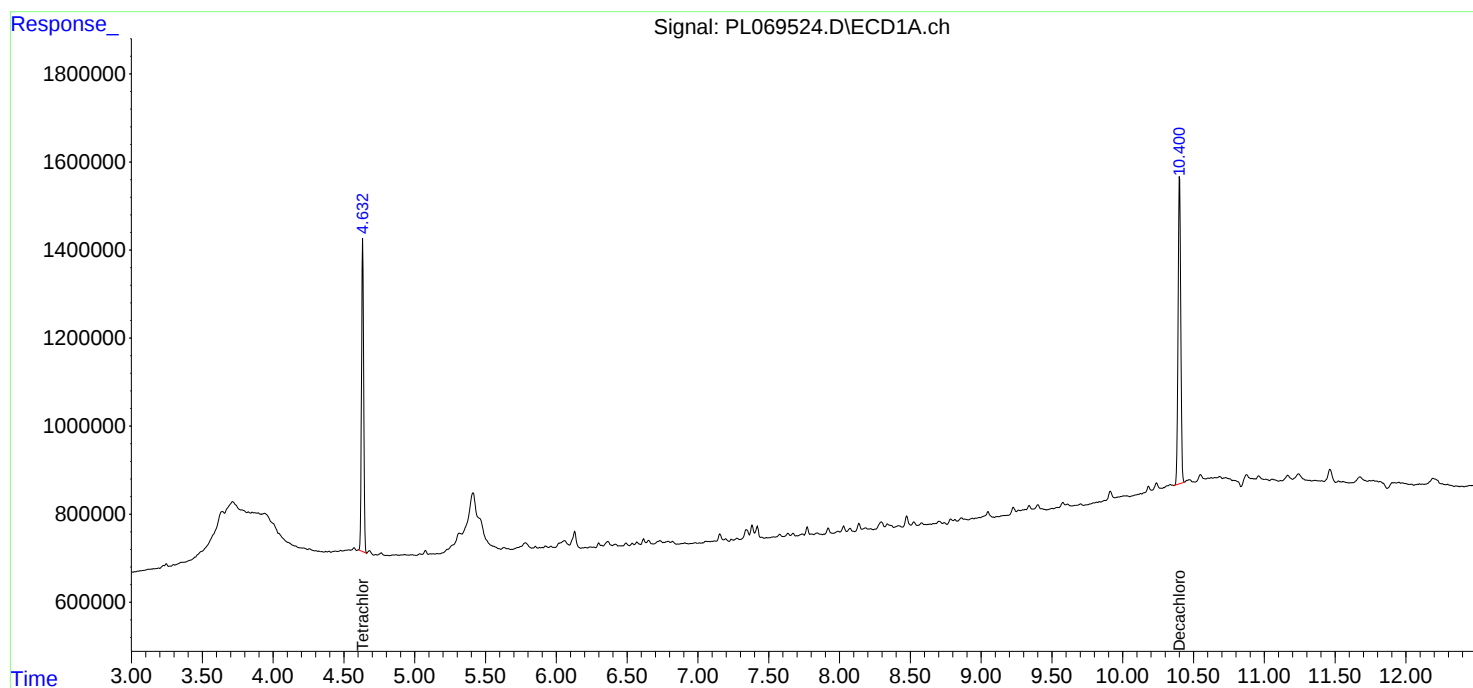


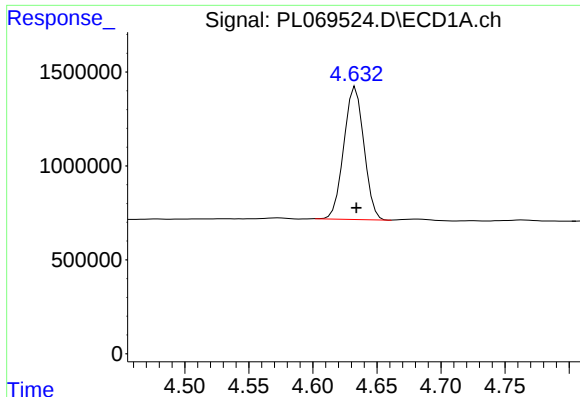

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 7709479
Conc: 16.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

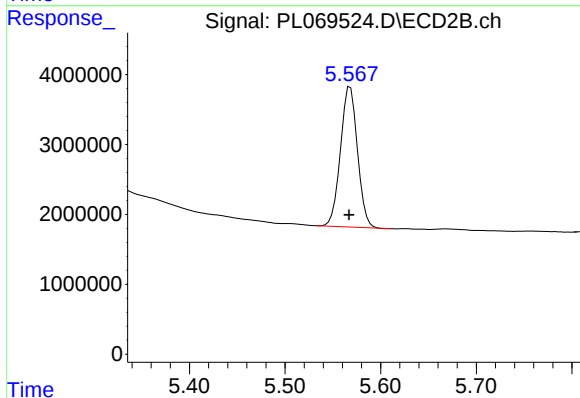


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: 0.001 min
Response: 24784776
Conc: 17.30 ng/ml

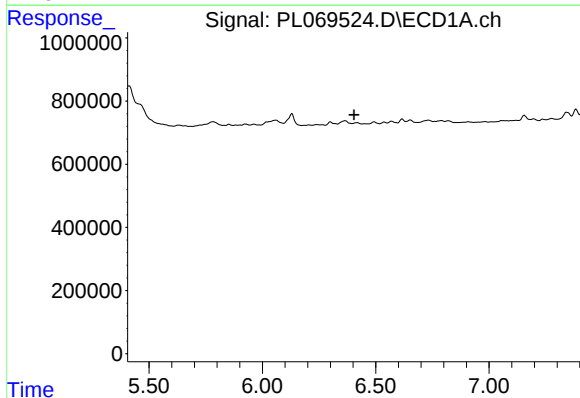


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

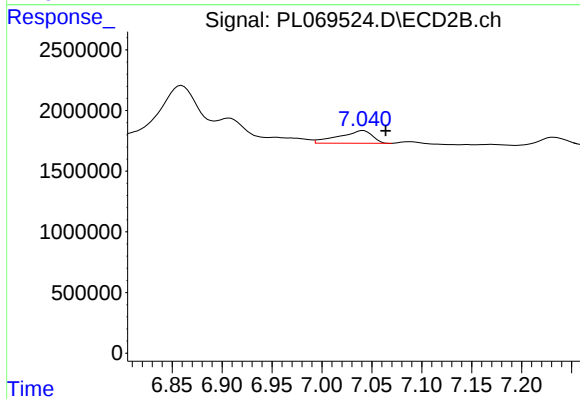

#7 delta-BHC


R.T.: 7.042 min
Delta R.T.: -0.022 min
Response: 2451881
Conc: 1.33 ng/ml

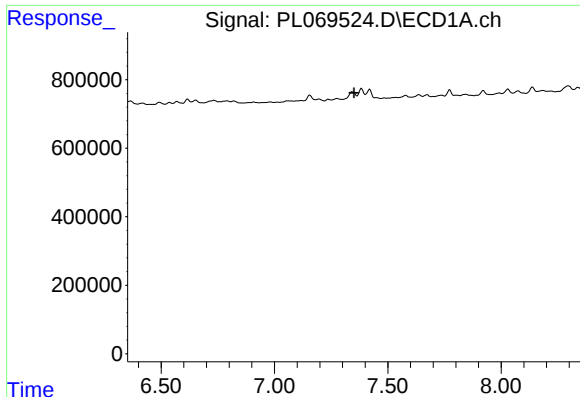

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

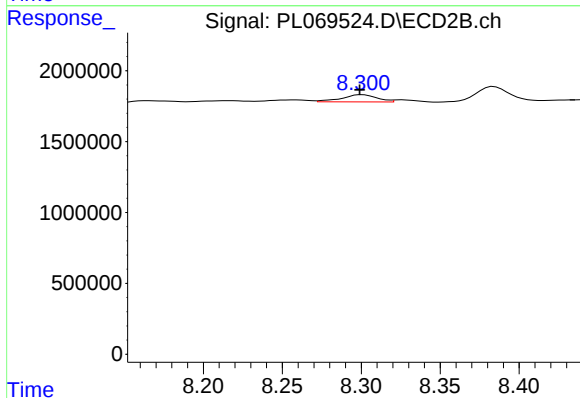


#10 gamma-Chlordane

R.T.: 8.301 min
Delta R.T.: 0.002 min
Response: 790553
Conc: 0.51 ng/ml

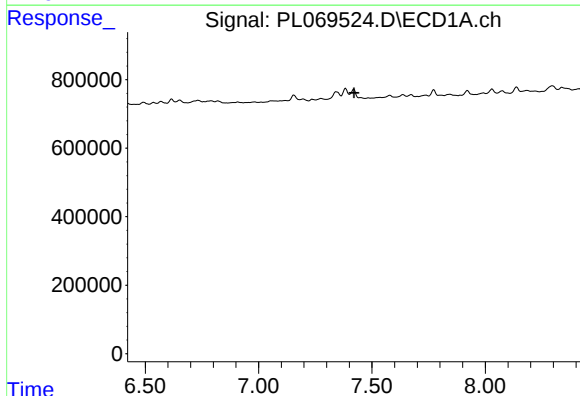


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.422 min
Response: 0
Conc: N.D.

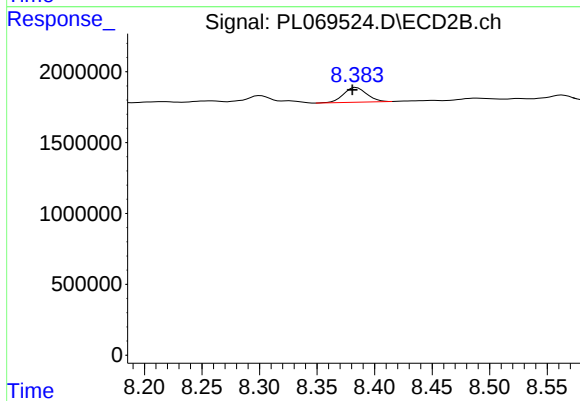

#11 alpha-Chlordane


R.T.: 8.384 min
Delta R.T.: 0.003 min
Response: 1466238
Conc: 0.98 ng/ml

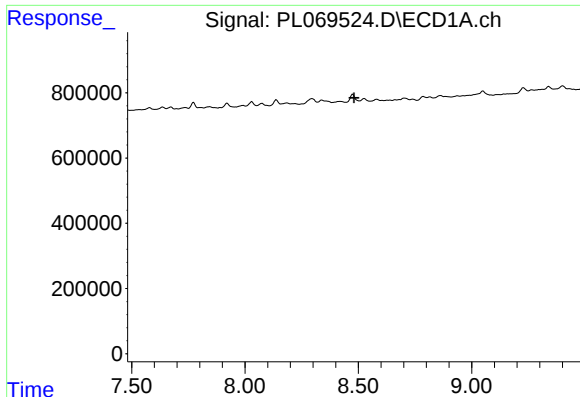

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

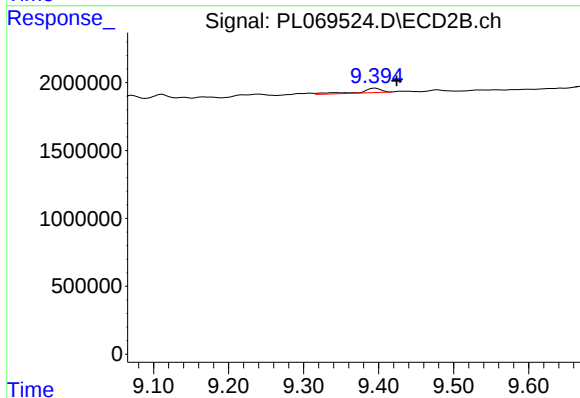


#17 4,4'-DDT

R.T.: 9.395 min
Delta R.T.: -0.029 min
Response: 639973
Conc: 0.52 ng/ml

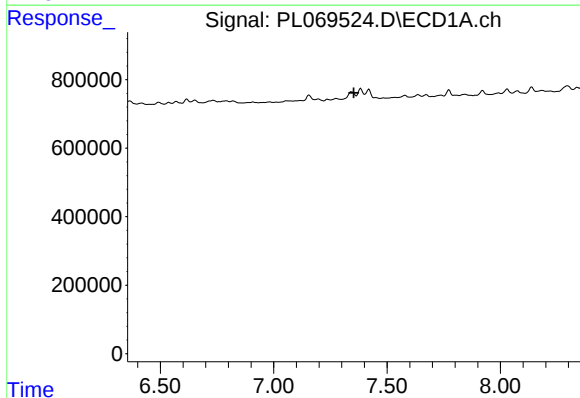


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

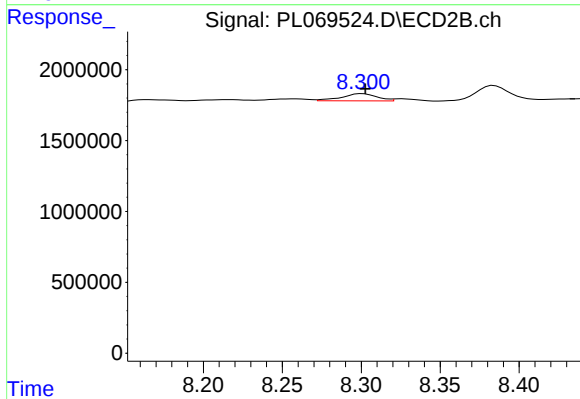

#25 Chlordane-3


R.T.: 8.301 min
Delta R.T.: -0.002 min
Response: 790553
Conc: 3.69 ng/ml

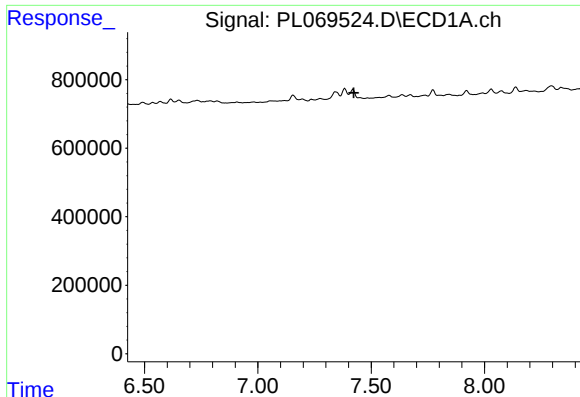

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

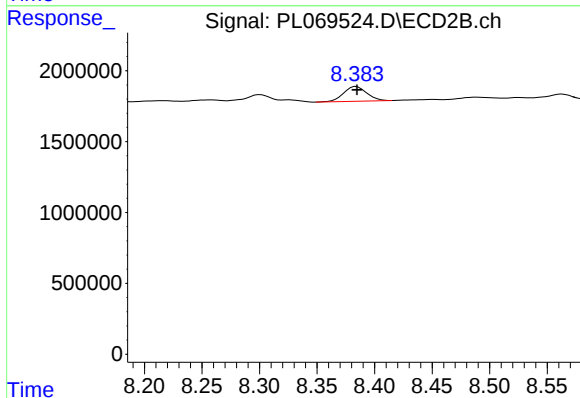


#26 Chlordane-4

R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 1466238
Conc: 5.70 ng/ml

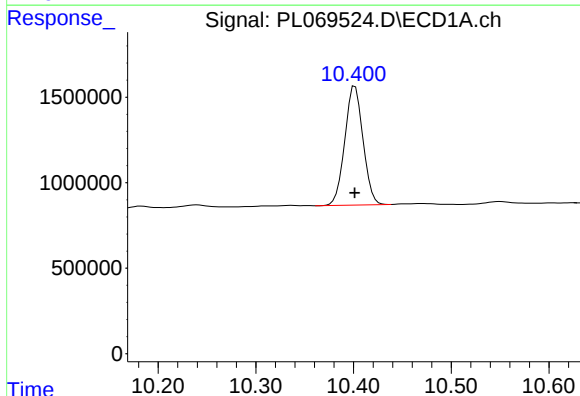

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 9022972
Conc: 13.37 ng/ml

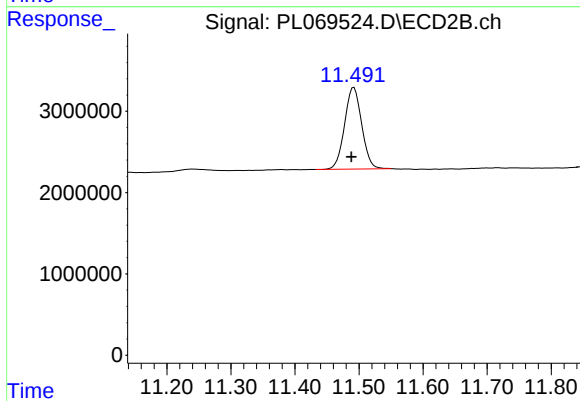

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.004 min
Response: 18620248
Conc: 15.19 ng/ml