

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082721\
 Data File : PL069534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2021 17:59
 Operator : AR\AJ
 Sample : M3493-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20211008-MANASQUAN-WATER

Manual Integrations
 APPROVED

mohammad
 8/30/2021 2:52:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:49:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.631	5.584f	6671186	22455502	14.459	15.676m
28)	SA Decachlor...	10.397	11.504f	9992324	18485947	14.805	15.084

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082721\
Data File : PL069534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 17:59
Operator : AR\AJ
Sample : M3493-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20211008-MANASQUAN-WATER


Manual Integrations
APPROVED

mohammad
8/30/2021 2:52:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:49:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

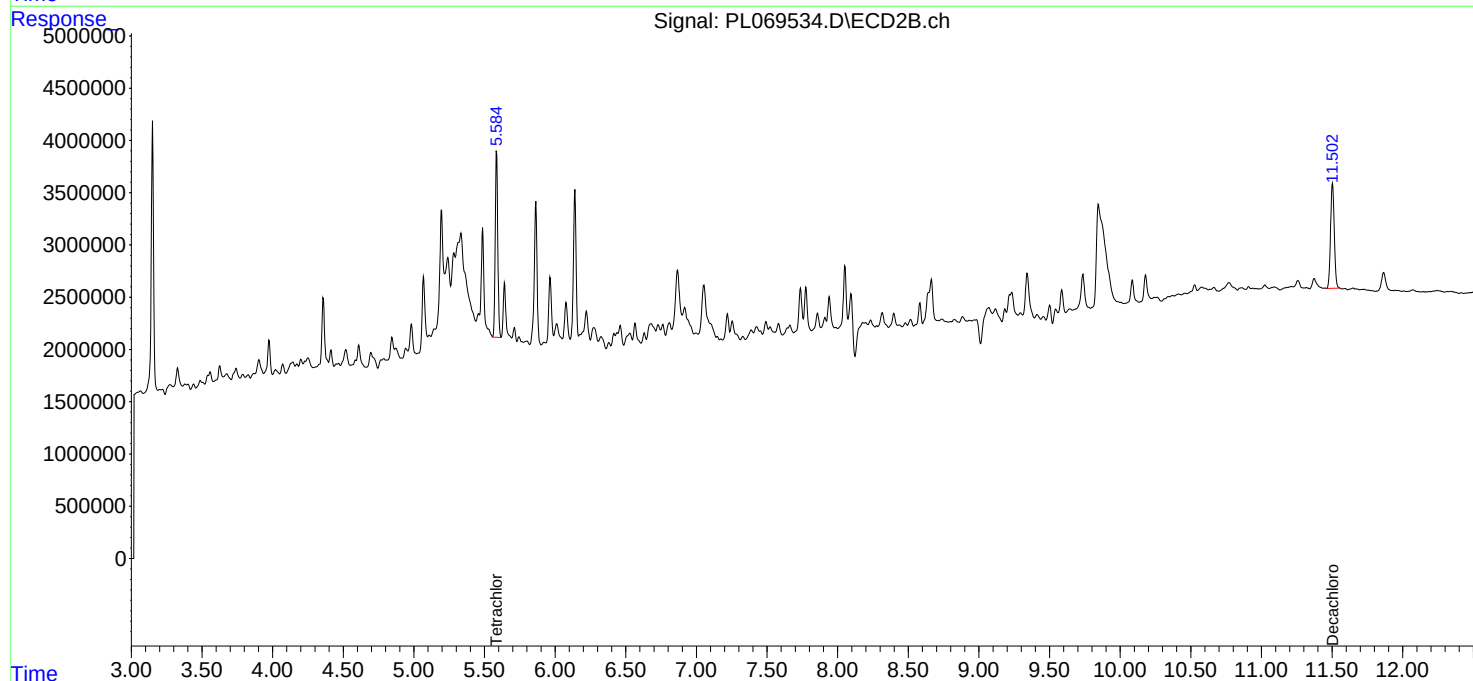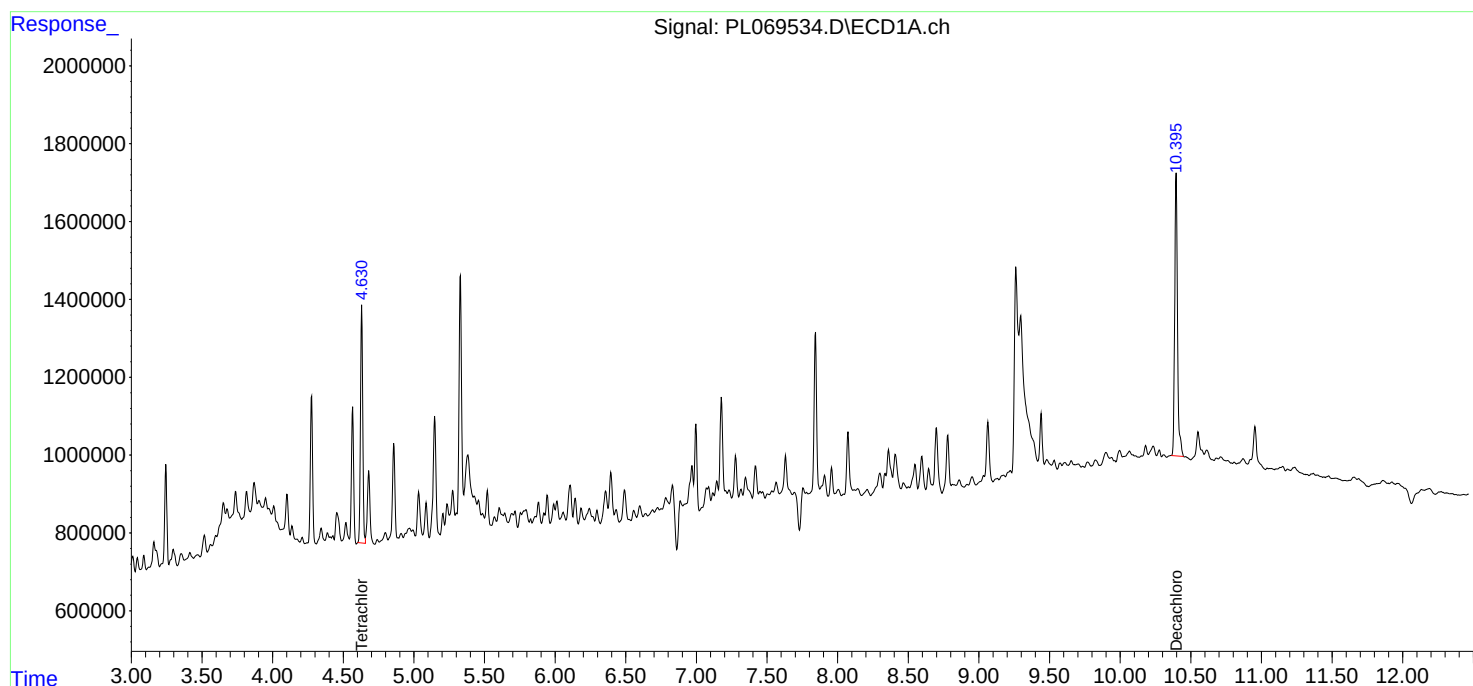

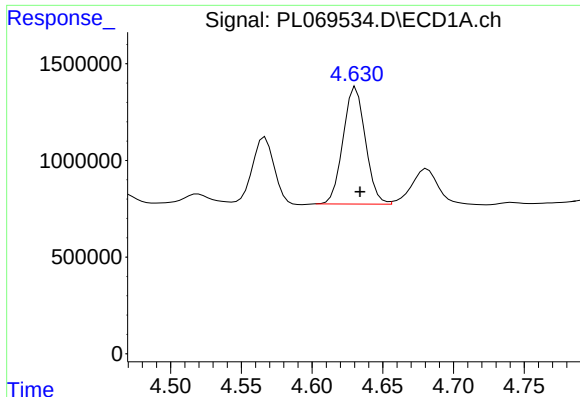


#1 Tetrachloro-m-xylene

R.T.: 4.631 min
Delta R.T.: -0.003 min
Response: 6671186
Conc: 14.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
20211008-MANASQUAN-WATER


Manual Integrations
APPROVED

mohammad
8/30/2021 2:52:51 PM

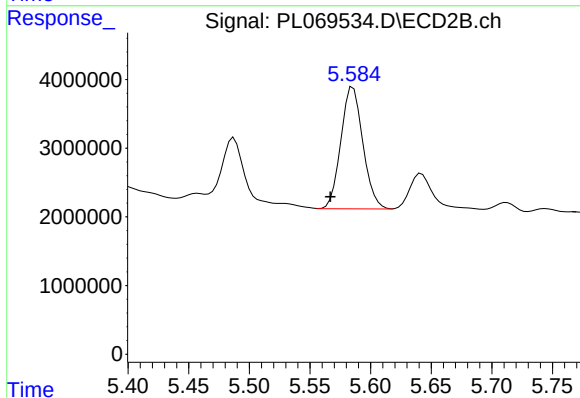


#1 Tetrachloro-m-xylene

R.T.: 5.584 min
Delta R.T.: 0.017 min
Response: 22455502
Conc: 15.68 ng/ml m

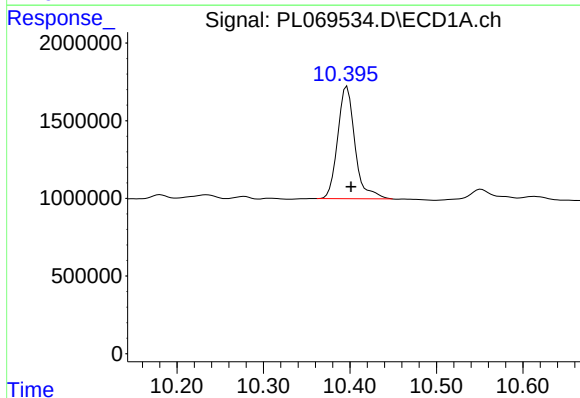

#28 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: -0.005 min
Response: 9992324
Conc: 14.80 ng/ml

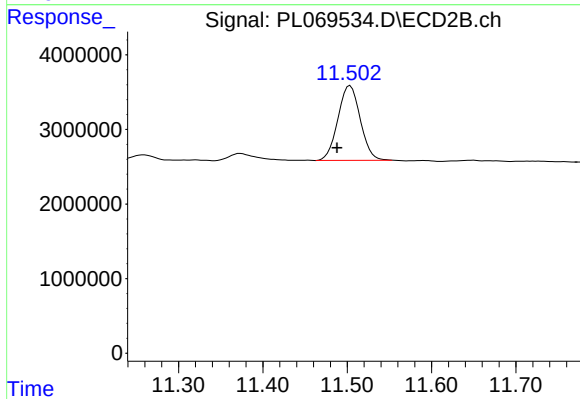

#28 Decachlorobiphenyl

R.T.: 11.504 min
Delta R.T.: 0.015 min
Response: 18485947
Conc: 15.08 ng/ml