

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
 Data File : PL052167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2019 09:05
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 18:07:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.923	213.3E6	52688896	24.919	24.116
28)	SA Decachlor...	7.971	8.947	130.5E6	54011017	10.752	17.744 #
Target Compounds							
2)	A alpha-BHC	3.738	0.000	14996289	0	1.035	N.D. #
3)	MA gamma-BHC...	0.000	4.592	0	101435	N.D.	0.032 #
6)	B beta-BHC	0.000	4.802f	0	701231	N.D.	0.481 #
9)	A Endosulfan I	5.323f	6.138	10612720	704318	0.789	0.218 #
13)	MA Dieldrin	0.000	6.410	0	584537	N.D.	0.171 #
17)	MA 4,4'-DDT	0.000	7.055	0	1345365	N.D.	0.460 #
18)	B Endrin al...	6.239	0.000	3292036	0	0.283	N.D. #
20)	A Methoxychlor	0.000	7.477f	0	2266565	N.D.	1.351 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
Data File : PL052167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2019 09:05
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 18:07:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

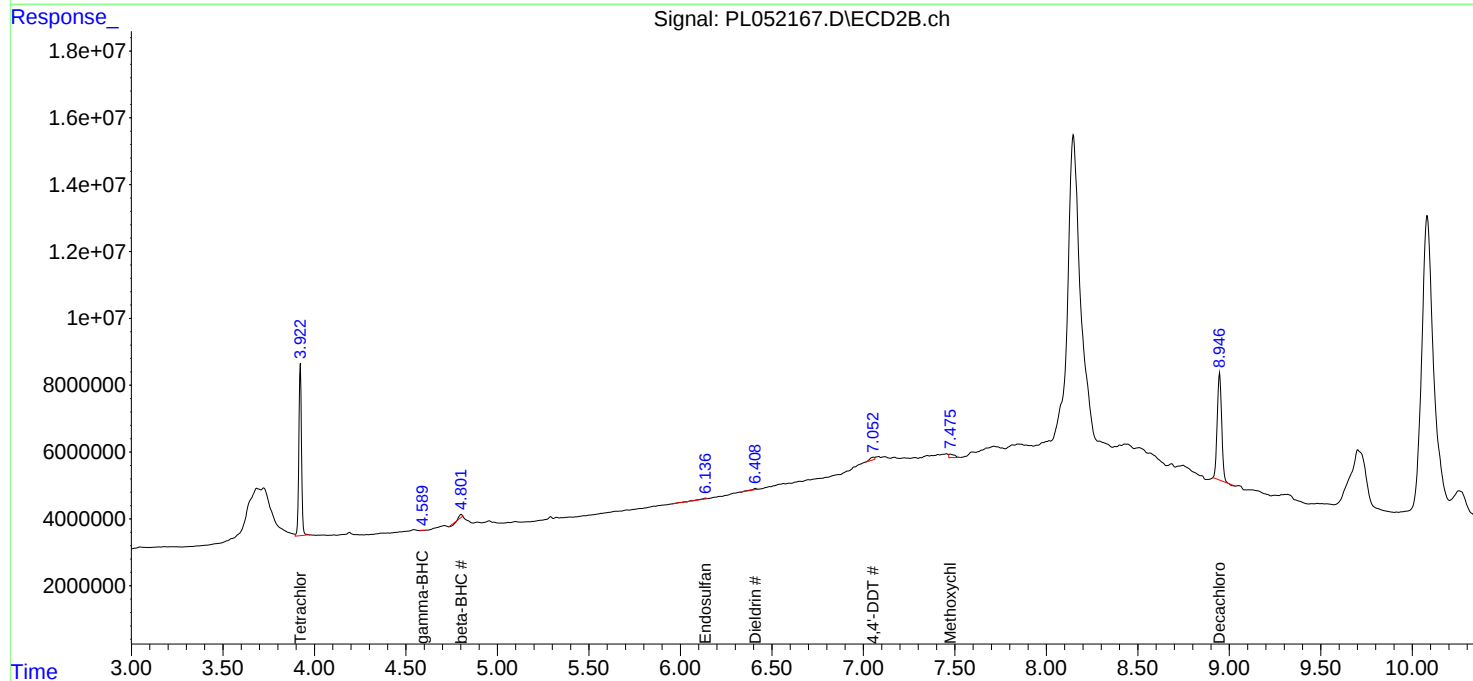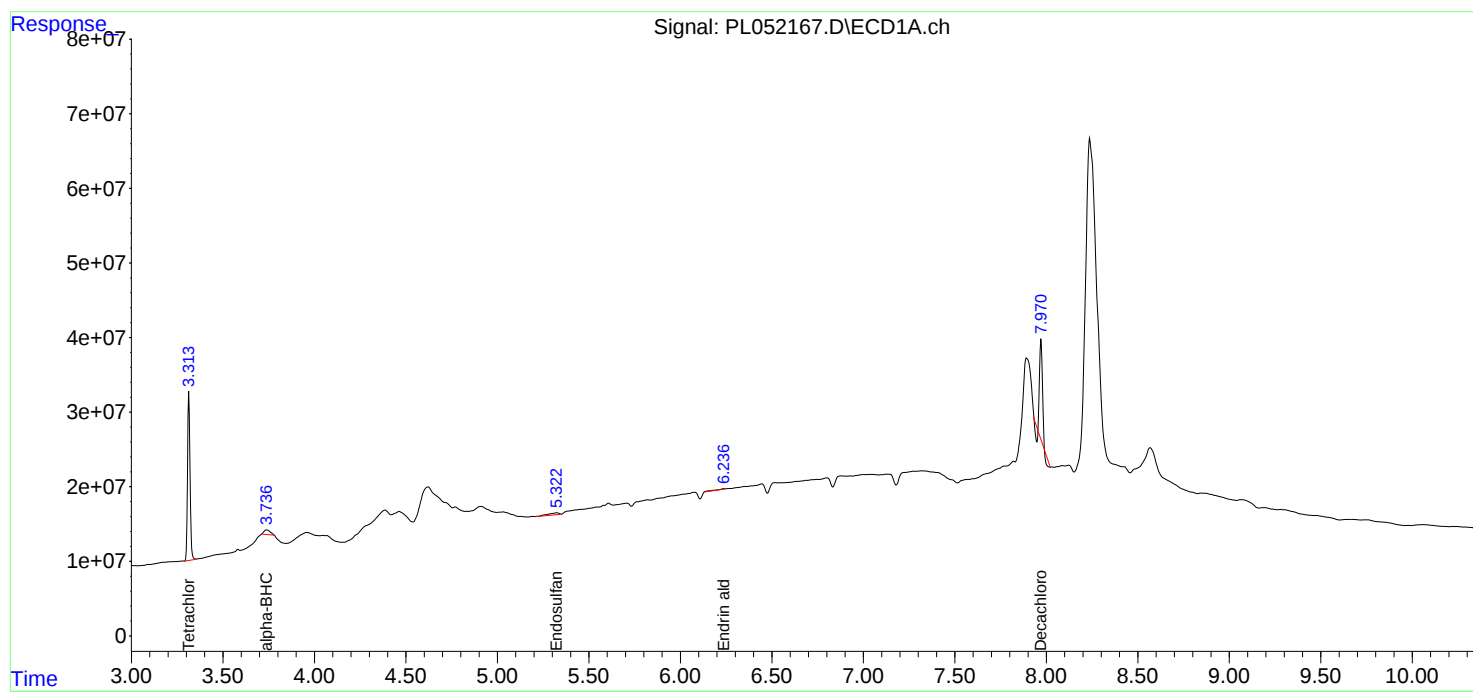


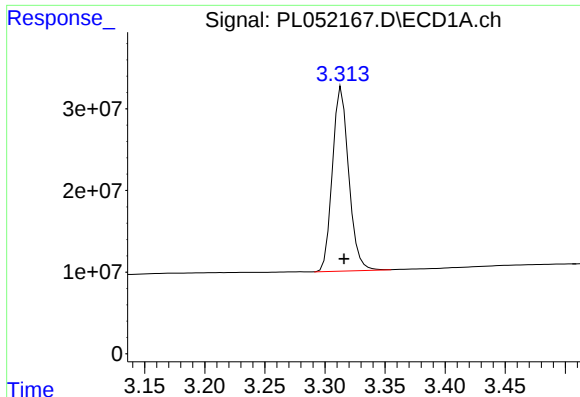

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 213274729
Conc: 24.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

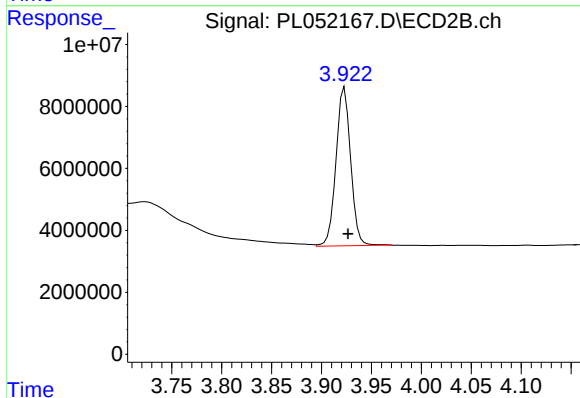


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 52688896
Conc: 24.12 ng/ml

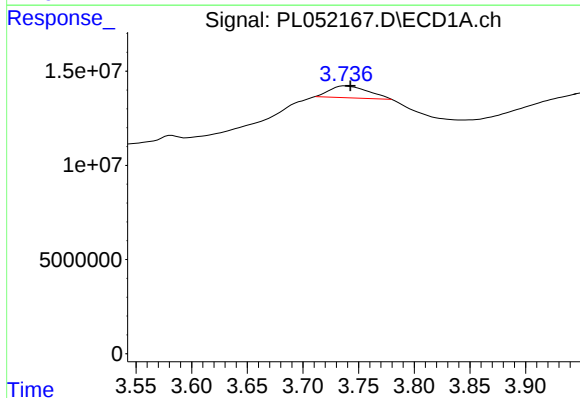


#2 alpha-BHC

R.T.: 3.738 min
Delta R.T.: -0.005 min
Response: 14996289
Conc: 1.03 ng/ml

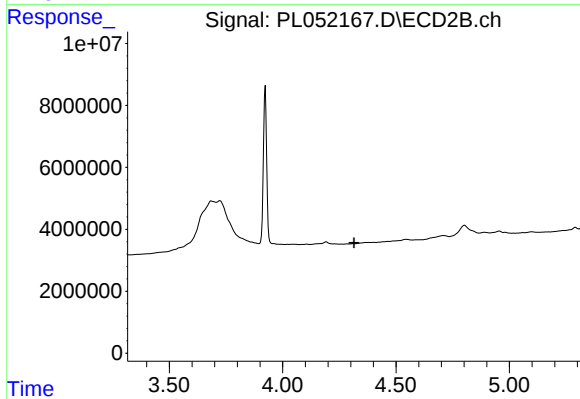

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.315 min
Response: 0
Conc: N.D.

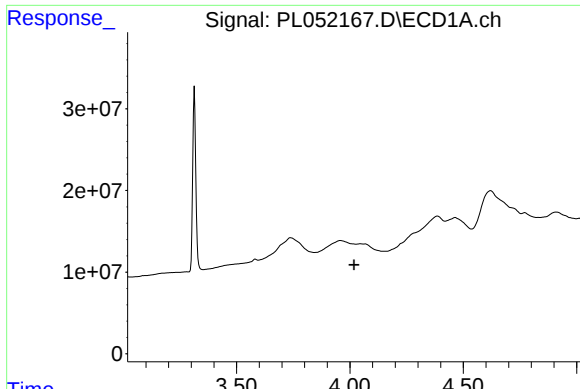

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.018 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

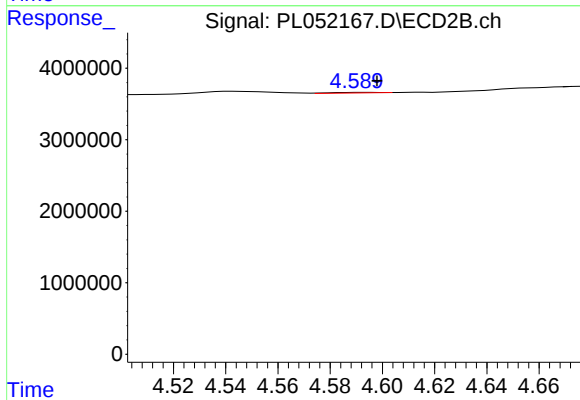


#3 gamma-BHC (Lindane)

R.T.: 4.592 min
Delta R.T.: -0.006 min
Response: 101435
Conc: 0.03 ng/ml

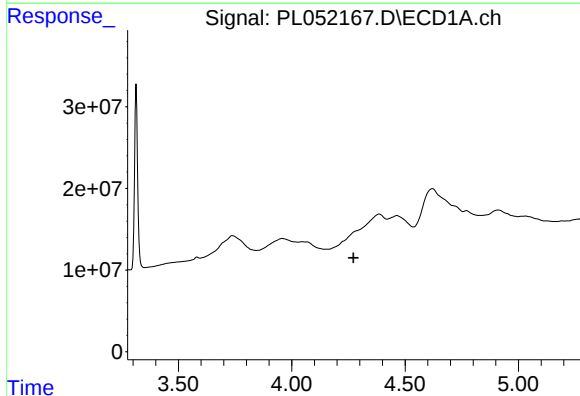


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

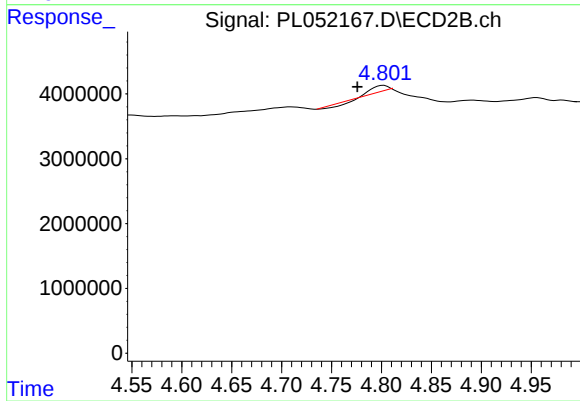

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 701231
Conc: 0.48 ng/ml

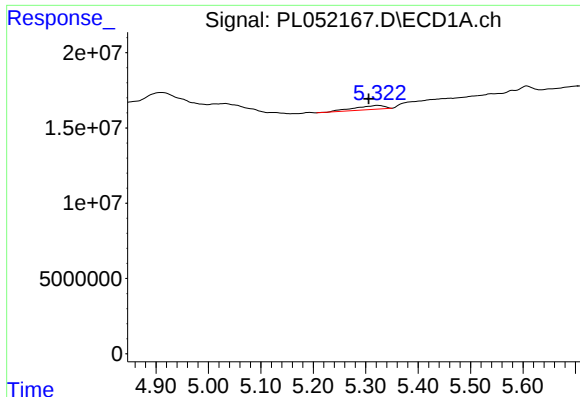

#9 Endosulfan I


R.T.: 5.323 min
Delta R.T.: 0.017 min
Response: 10612720
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

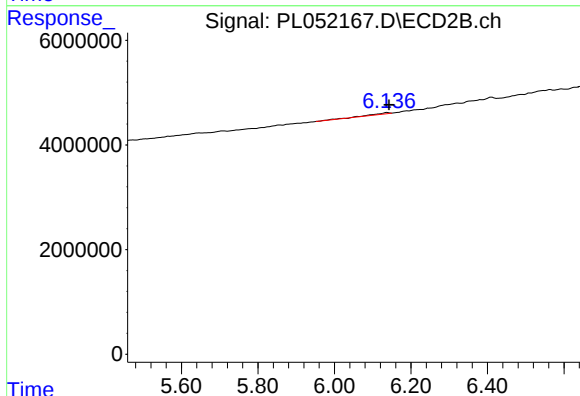


#9 Endosulfan I

R.T.: 6.138 min
Delta R.T.: -0.005 min
Response: 704318
Conc: 0.22 ng/ml

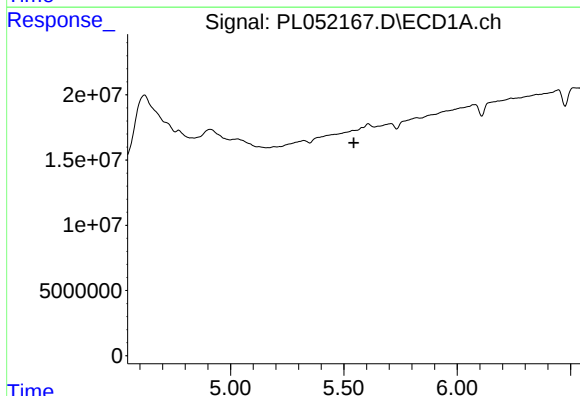


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.544 min
Response: 0
Conc: N.D.

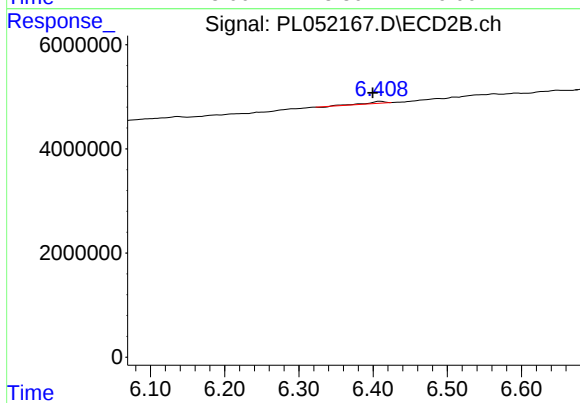

#13 Dieldrin


R.T.: 6.410 min
Delta R.T.: 0.011 min
Response: 584537
Conc: 0.17 ng/ml

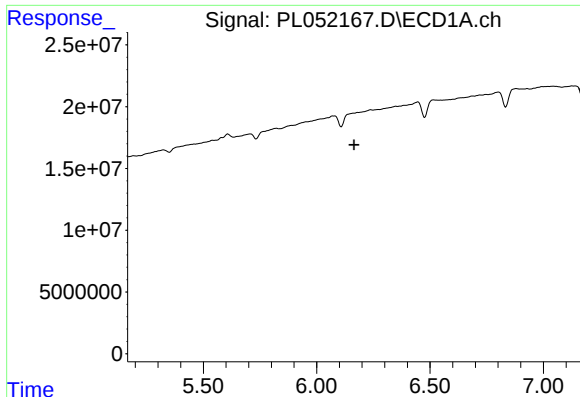

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

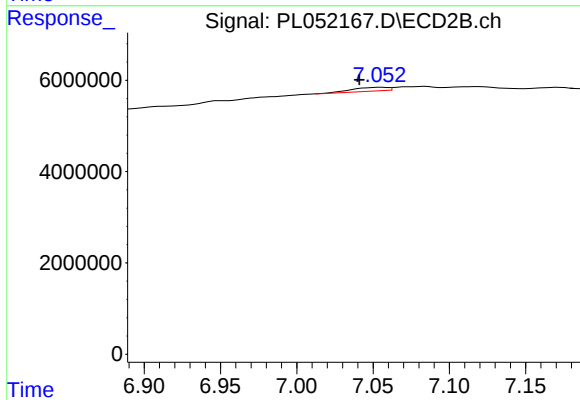


#17 4,4'-DDT

R.T.: 7.055 min
Delta R.T.: 0.014 min
Response: 1345365
Conc: 0.46 ng/ml

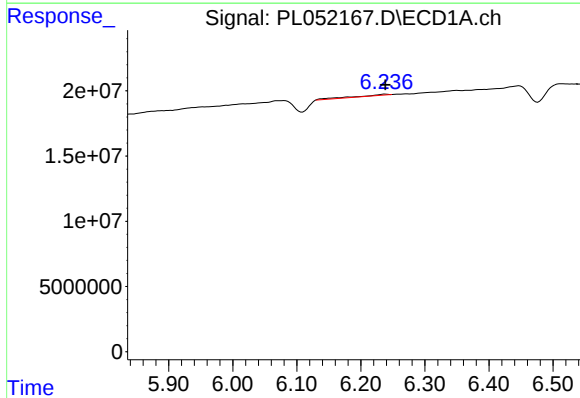


#18 Endrin aldehyde

R.T.: 6.239 min
Delta R.T.: 0.000 min
Response: 3292036
Conc: 0.28 ng/ml

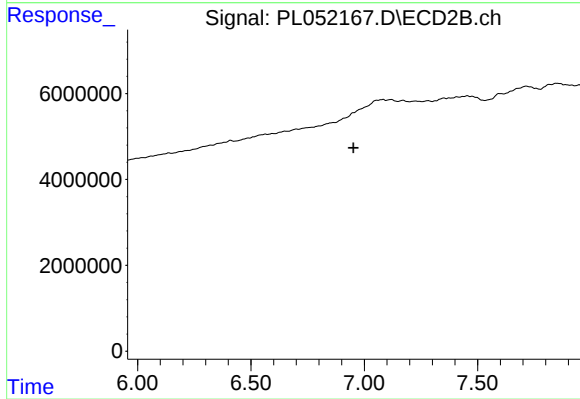

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.953 min
Response: 0
Conc: N.D.

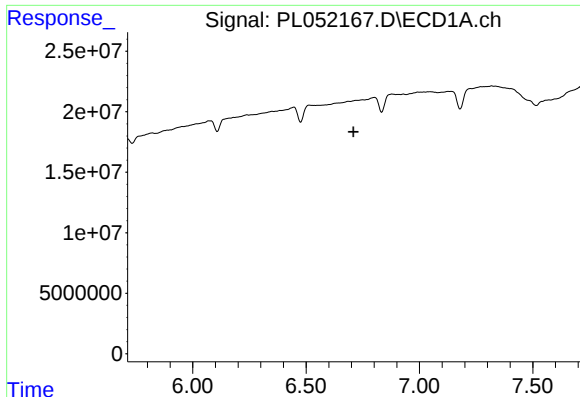

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

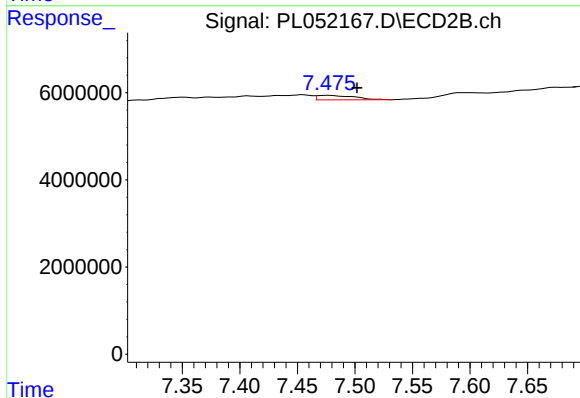


#20 Methoxychlor

R.T.: 7.477 min
Delta R.T.: -0.025 min
Response: 2266565
Conc: 1.35 ng/ml

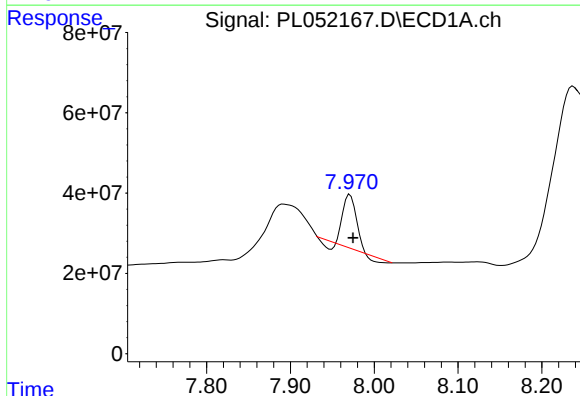

#28 Decachlorobiphenyl

R.T.: 7.971 min
Delta R.T.: -0.004 min
Response: 130507998
Conc: 10.75 ng/ml

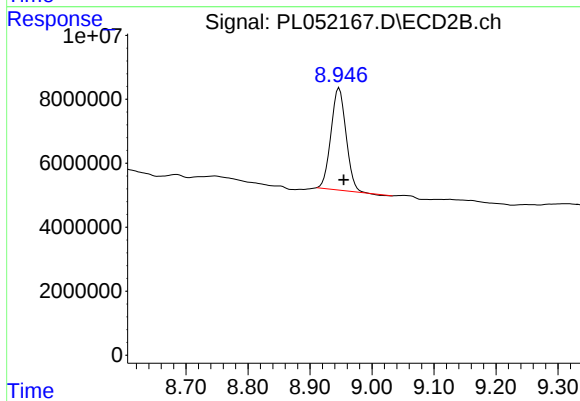

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.007 min
Response: 54011017
Conc: 17.74 ng/ml