

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
 Data File : PL052172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2019 11:53
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 18:08:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.923	213.2E6	53168303	24.906	24.335
28)	SA Decachlor...	7.971	8.948	242.3E6	56774993	19.965	18.652
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	533931	N.D.	0.366 #
8)	B Heptachlo...	0.000	5.784	0	6480084	N.D.	1.920 #
9)	A Endosulfan I	5.327f	0.000	5974256	0	0.444	N.D. #
11)	B alpha-Chl...	5.265	6.069f	16670885	448866	1.152	0.130 #
13)	MA Dieldrin	0.000	6.410	0	302413	N.D.	0.088 #
15)	B Endosulfa...	6.081	0.000	9664135	0	0.695	N.D. #
26)	Chlordane-4	5.265	6.069f	16670885	448866	13.672	0.826 #
27)	Chlordane-5	6.081	0.000	9664135	0	19.694	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
Data File : PL052172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2019 11:53
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 18:08:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

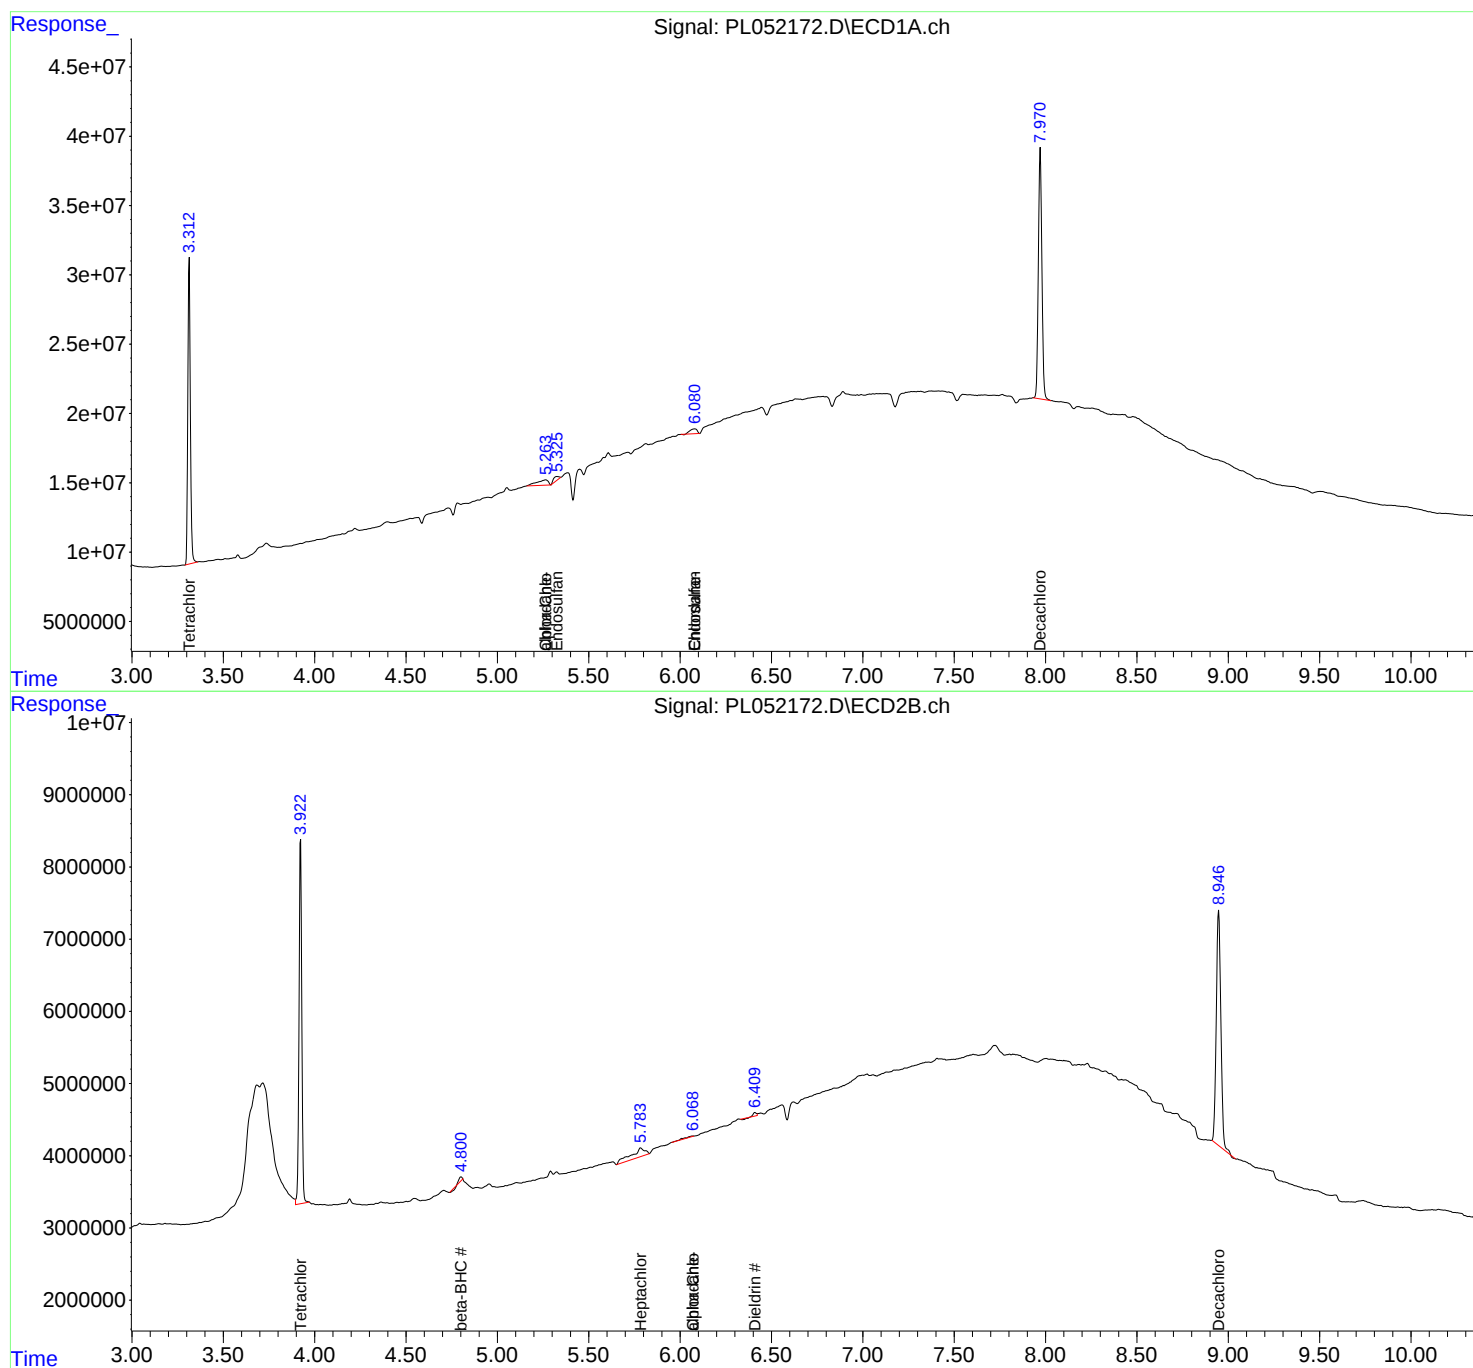


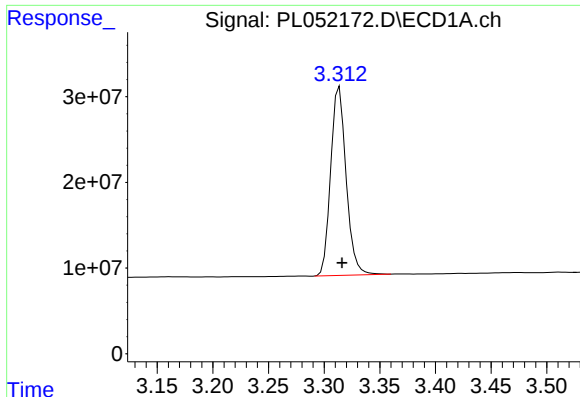

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 213157587
Conc: 24.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

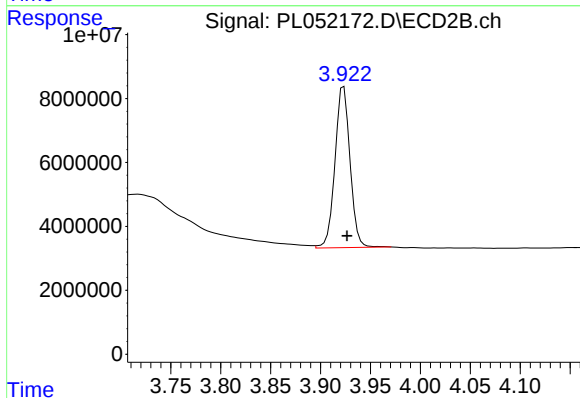


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.003 min
Response: 53168303
Conc: 24.34 ng/ml

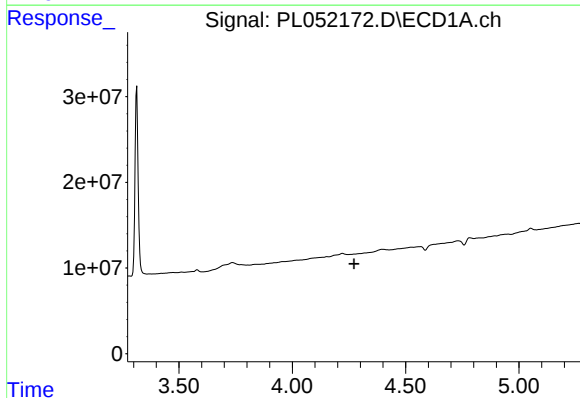


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

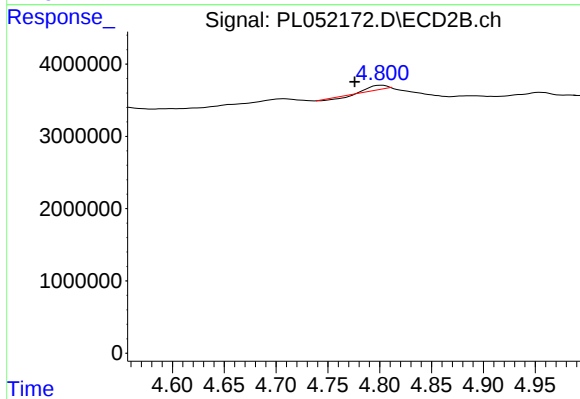

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 533931
Conc: 0.37 ng/ml

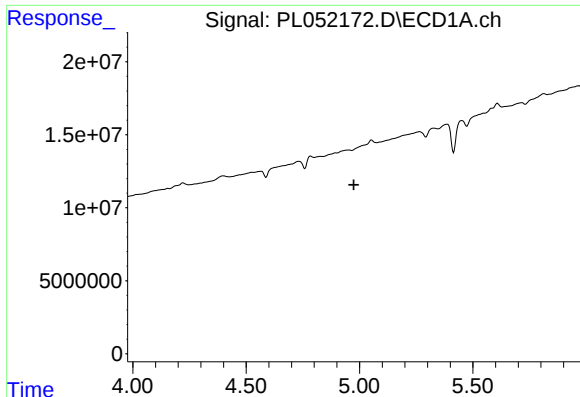

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

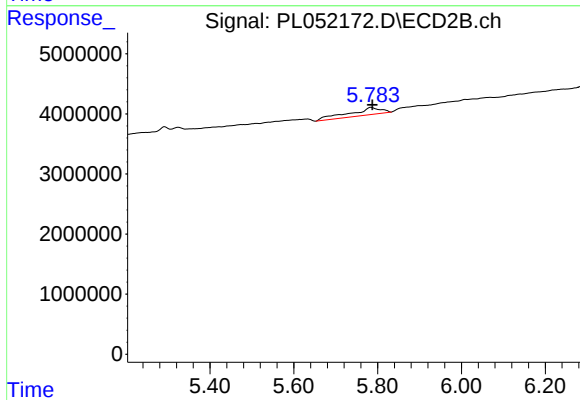


#8 Heptachlor epoxide

R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 6480084
Conc: 1.92 ng/ml

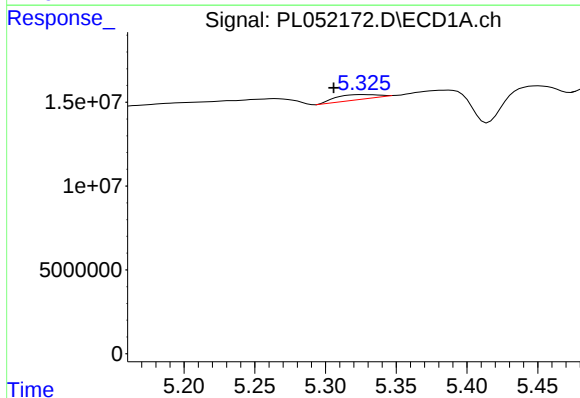


#9 Endosulfan I

R.T.: 5.327 min
Delta R.T.: 0.021 min
Response: 5974256
Conc: 0.44 ng/ml

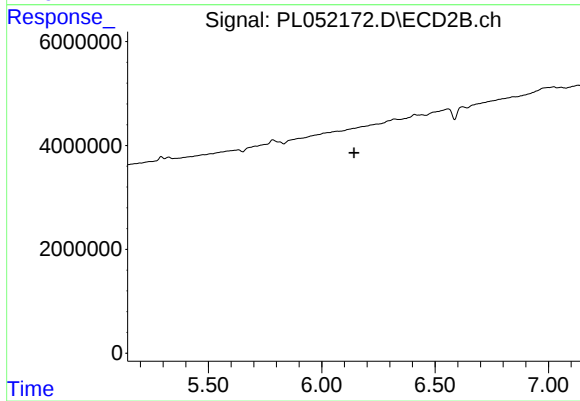

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

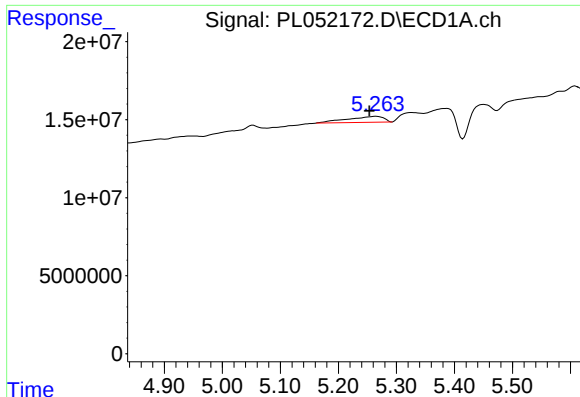

#11 alpha-Chlordane


R.T.: 5.265 min
Delta R.T.: 0.011 min
Response: 16670885
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

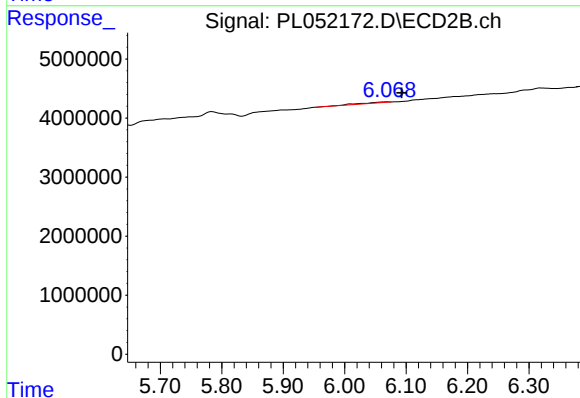


#11 alpha-Chlordane

R.T.: 6.069 min
Delta R.T.: -0.024 min
Response: 448866
Conc: 0.13 ng/ml

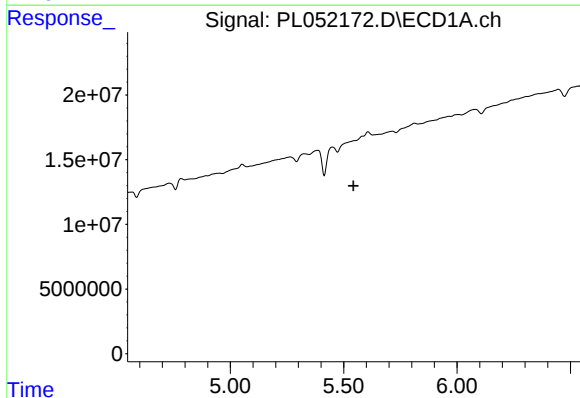


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.544 min
Response: 0
Conc: N.D.

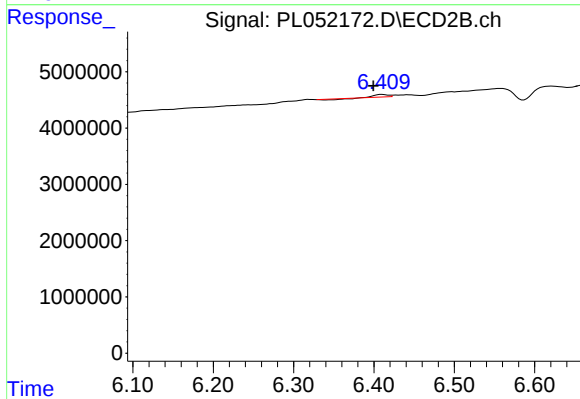

#13 Dieldrin


R.T.: 6.410 min
Delta R.T.: 0.011 min
Response: 302413
Conc: 0.09 ng/ml

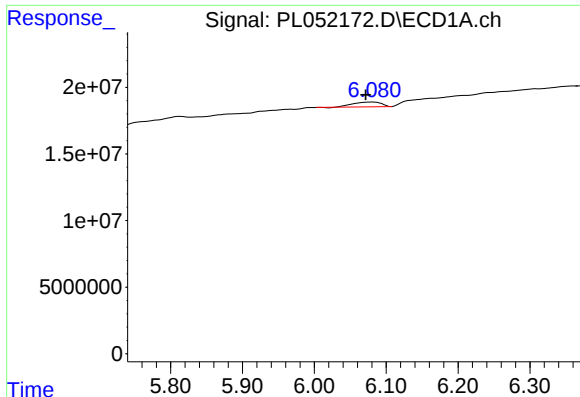

#15 Endosulfan II


R.T.: 6.081 min
Delta R.T.: 0.010 min
Response: 9664135
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

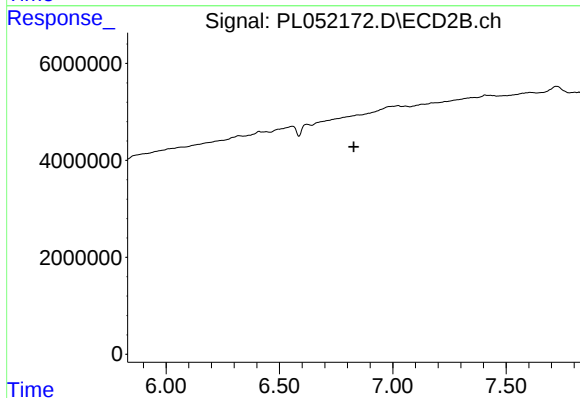


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.829 min
Response: 0
Conc: N.D.

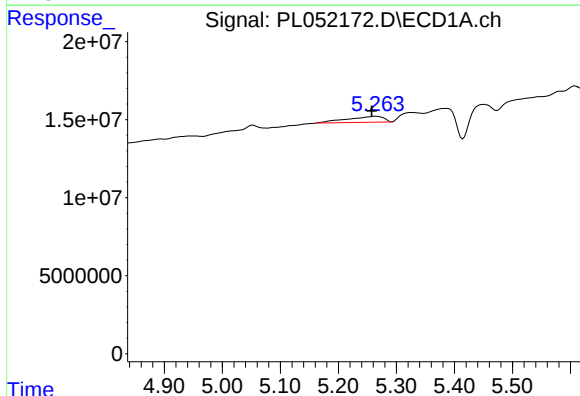


#26 Chlordane-4

R.T.: 5.265 min
Delta R.T.: 0.007 min
Response: 16670885
Conc: 13.67 ng/ml

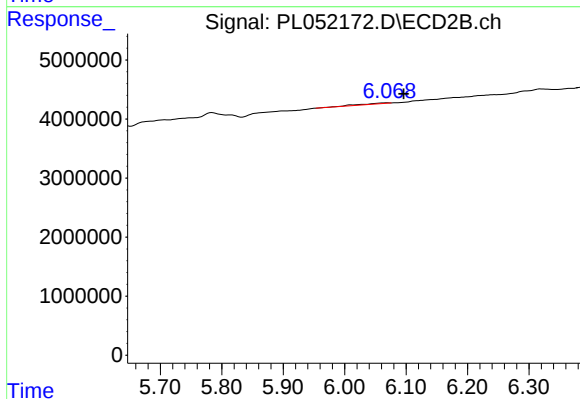

#26 Chlordane-4


R.T.: 6.069 min
Delta R.T.: -0.027 min
Response: 448866
Conc: 0.83 ng/ml

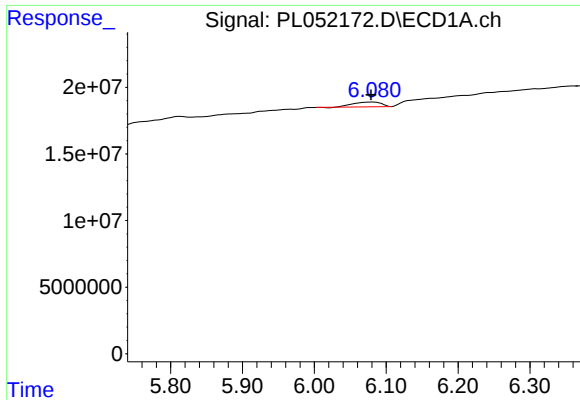

#27 Chlordane-5


R.T.: 6.081 min
Delta R.T.: 0.002 min
Response: 9664135
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

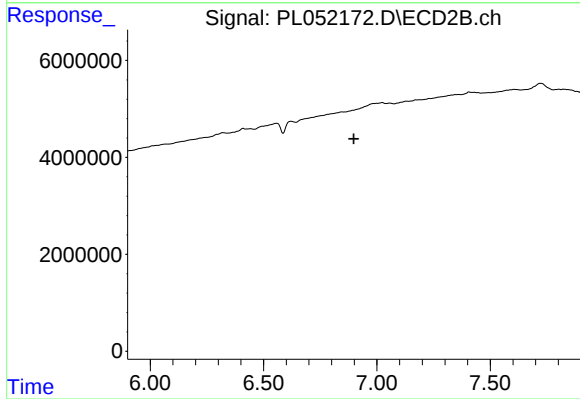


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.898 min
Response: 0
Conc: N.D.

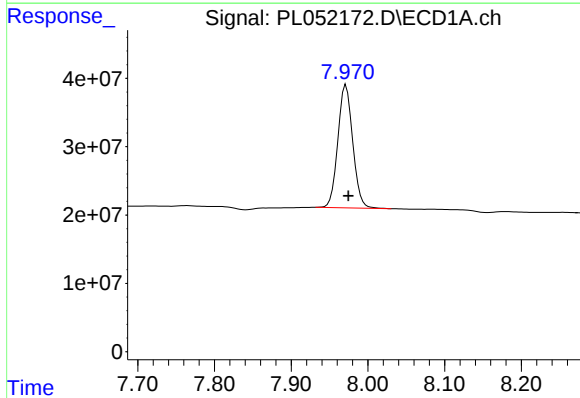

#28 Decachlorobiphenyl

R.T.: 7.971 min
Delta R.T.: -0.003 min
Response: 242325902
Conc: 19.96 ng/ml

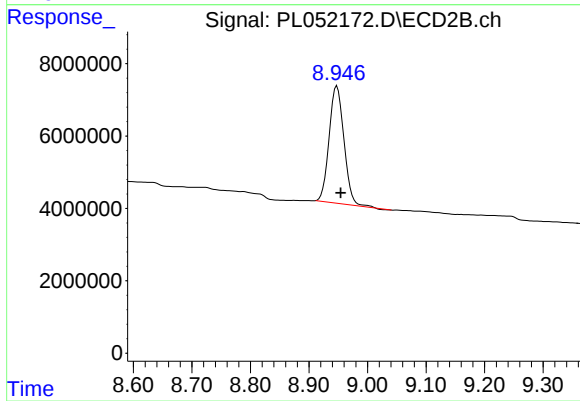

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.006 min
Response: 56774993
Conc: 18.65 ng/ml