

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
 Data File : PL052185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2019 16:08
 Operator : SG\AJ
 Sample : K4622-39
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 18:11:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.924	195.0E6	50878051	22.787	23.287
28)	SA Decachlor...	7.971	8.948	255.5E6	59420129	21.052	19.521
Target Compounds							
2)	A alpha-BHC	0.000	4.287f	0	694177	N.D.	0.215 #
5)	MB Aldrin	4.566f	0.000	2846484	0	0.197	N.D. #
6)	B beta-BHC	0.000	4.801f	0	848706	N.D.	0.582 #
8)	B Heptachlo...	0.000	5.808f	0	1409816	N.D.	0.418 #
9)	A Endosulfan I	0.000	6.167f	0	1185085	N.D.	0.367 #
15)	B Endosulfa...	0.000	6.843	0	4257051	N.D.	1.292 #
18)	B Endrin al...	0.000	6.947	0	358756	N.D.	0.127 #
27)	Chlordane-5	0.000	6.917f	0	2312418	N.D.	23.456 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
Data File : PL052185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2019 16:08
Operator : SG\AJ
Sample : K4622-39
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 18:11:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

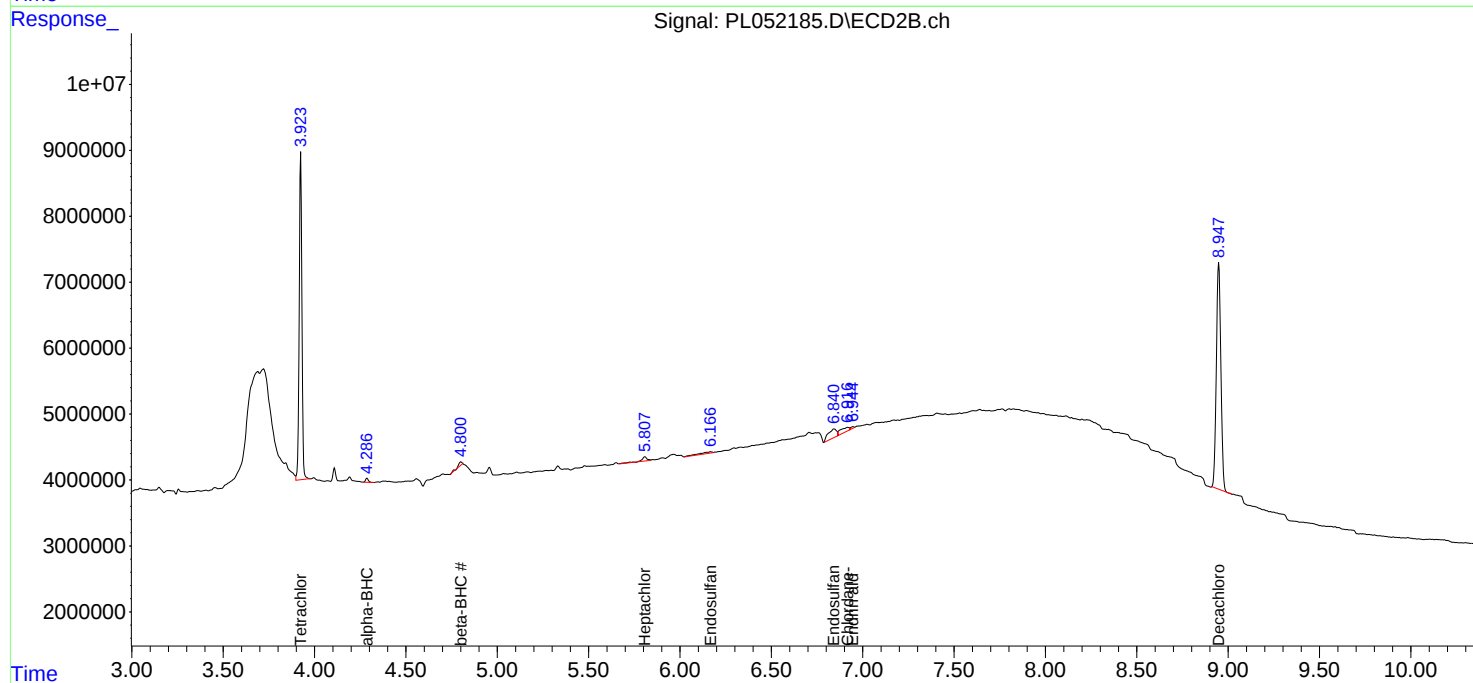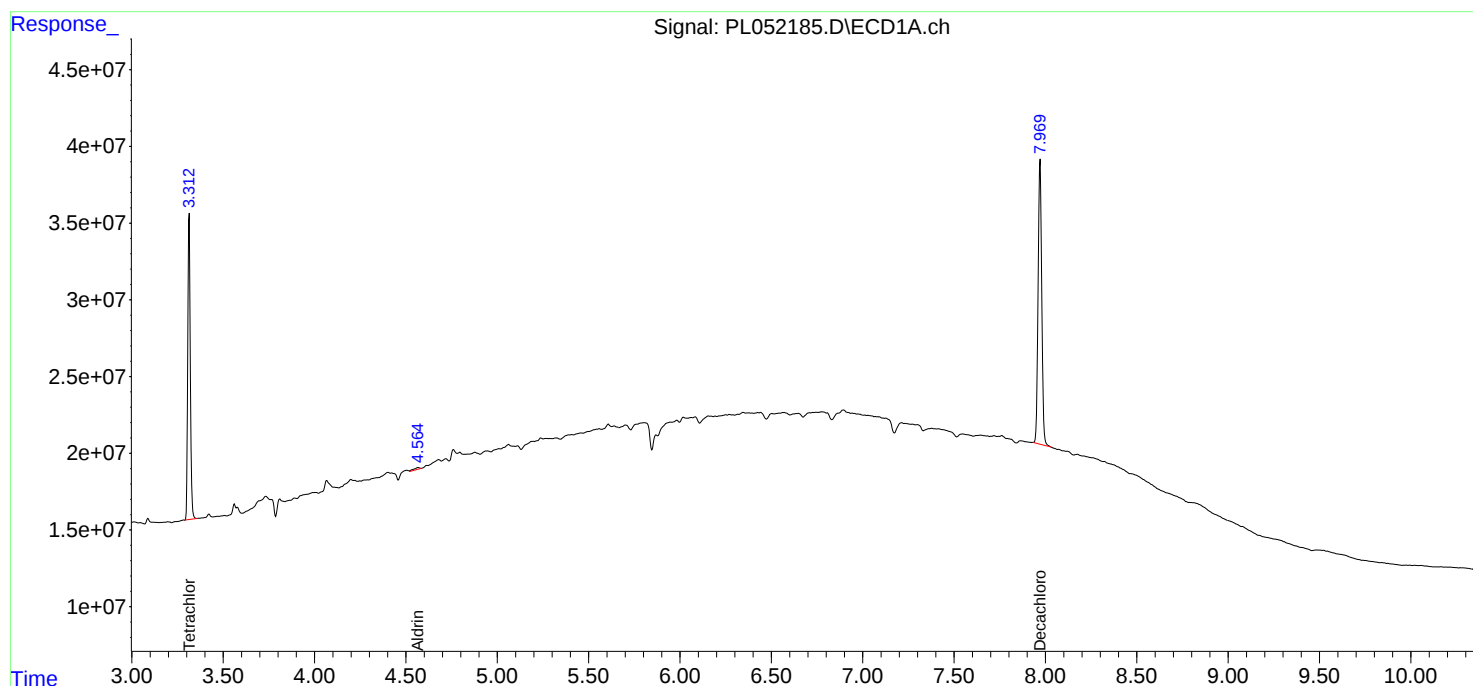


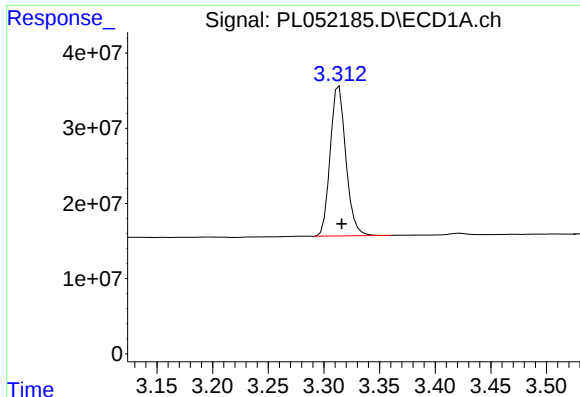

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 195026737
Conc: 22.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

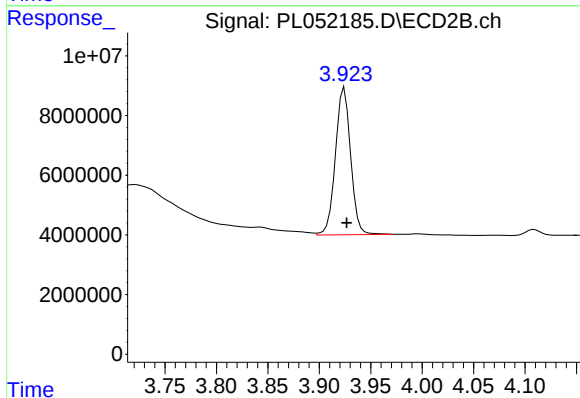


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 50878051
Conc: 23.29 ng/ml

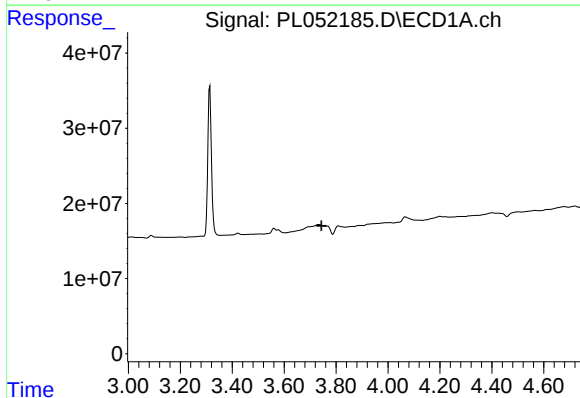


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.743 min
Response: 0
Conc: N.D.

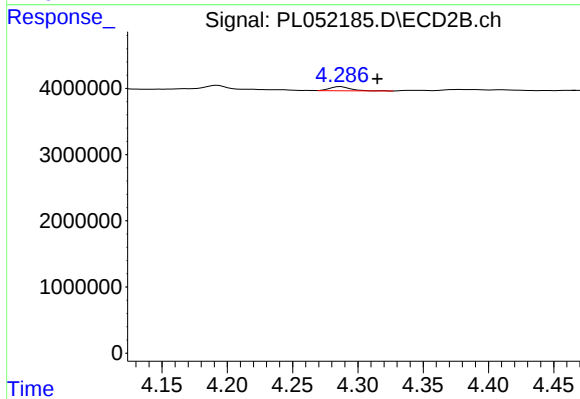

#2 alpha-BHC


R.T.: 4.287 min
Delta R.T.: -0.028 min
Response: 694177
Conc: 0.22 ng/ml

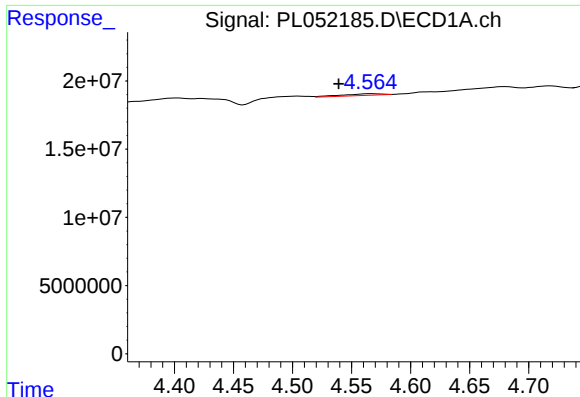

#5 Aldrin


R.T.: 4.566 min
Delta R.T.: 0.027 min
Response: 2846484
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

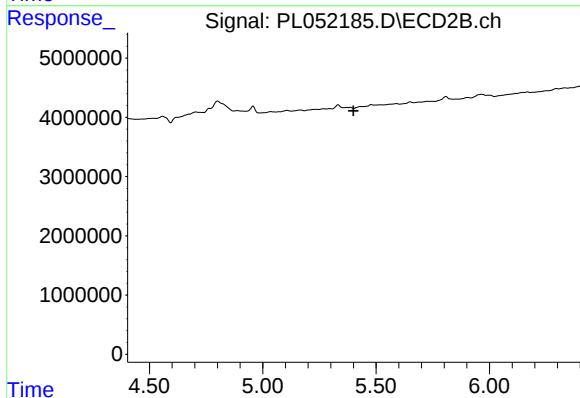


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.401 min
Response: 0
Conc: N.D.

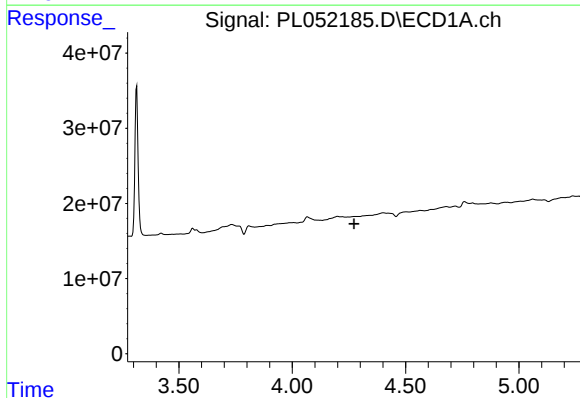


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

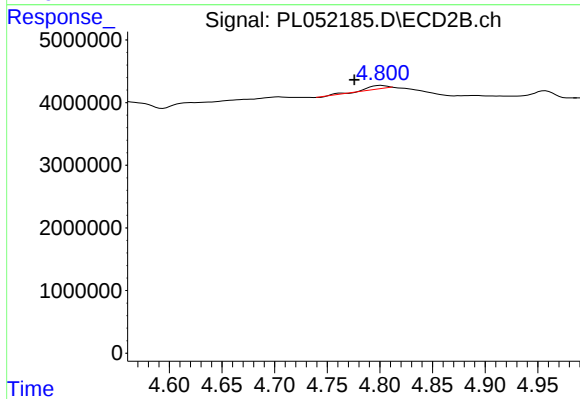

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.025 min
Response: 848706
Conc: 0.58 ng/ml

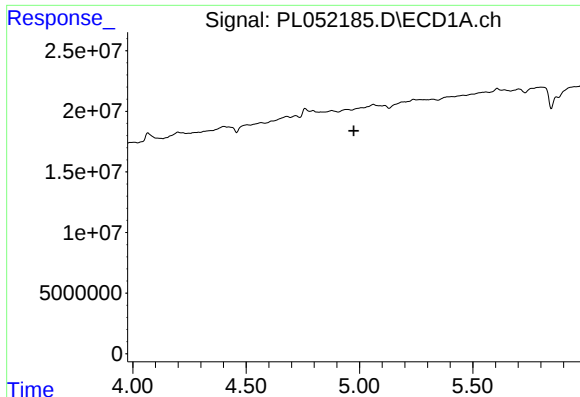

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

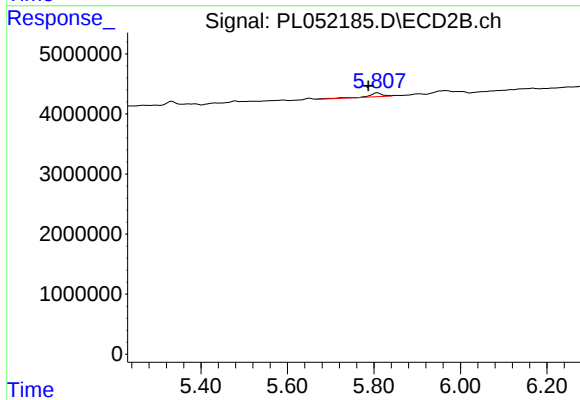


#8 Heptachlor epoxide

R.T.: 5.808 min
Delta R.T.: 0.021 min
Response: 1409816
Conc: 0.42 ng/ml

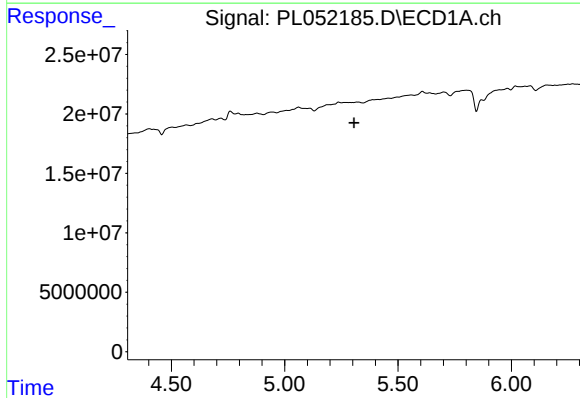


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

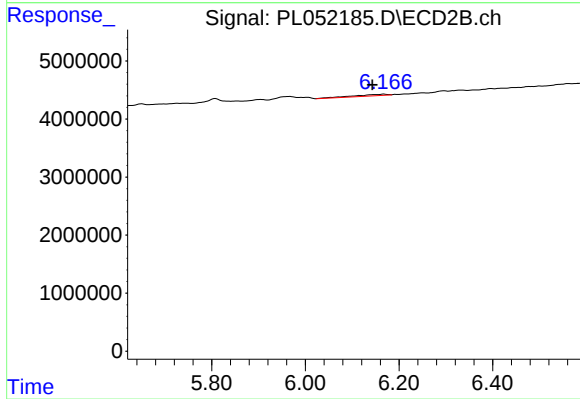

#9 Endosulfan I


R.T.: 6.167 min
Delta R.T.: 0.024 min
Response: 1185085
Conc: 0.37 ng/ml

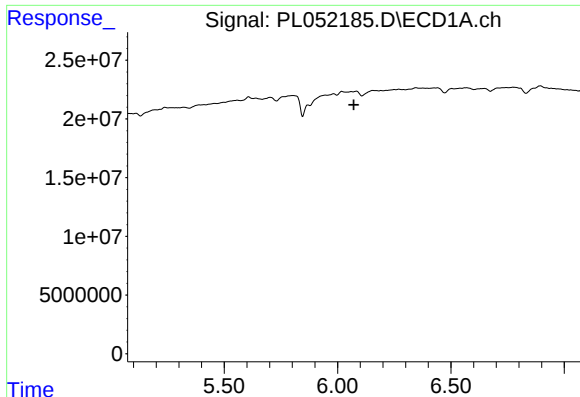

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

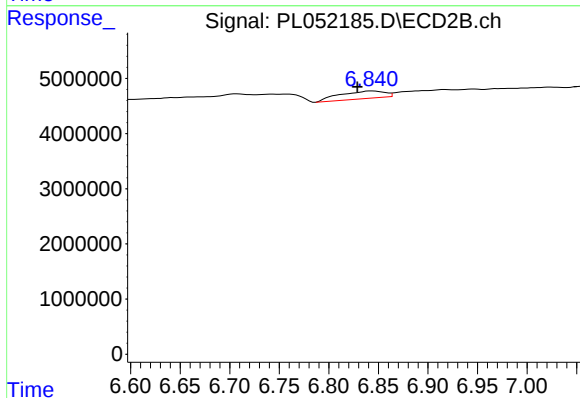


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.014 min
Response: 4257051
Conc: 1.29 ng/ml

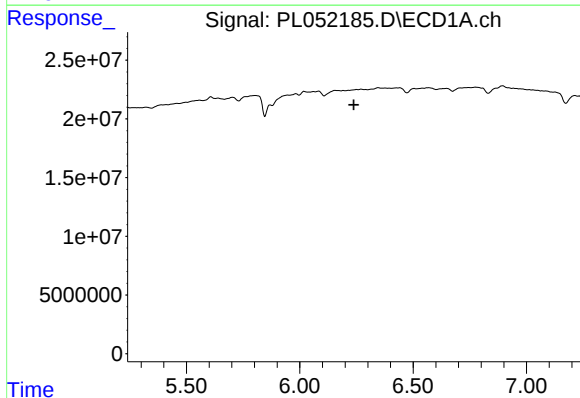


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

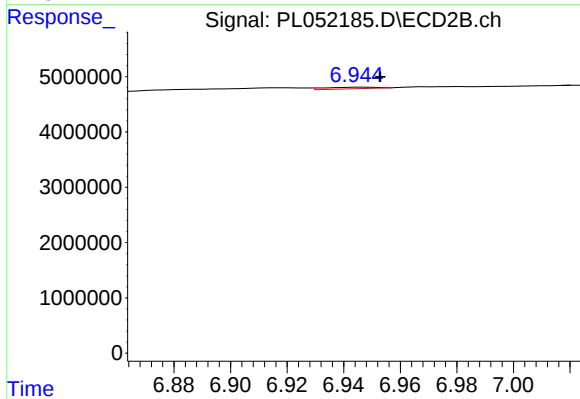

#18 Endrin aldehyde


R.T.: 6.947 min
Delta R.T.: -0.006 min
Response: 358756
Conc: 0.13 ng/ml

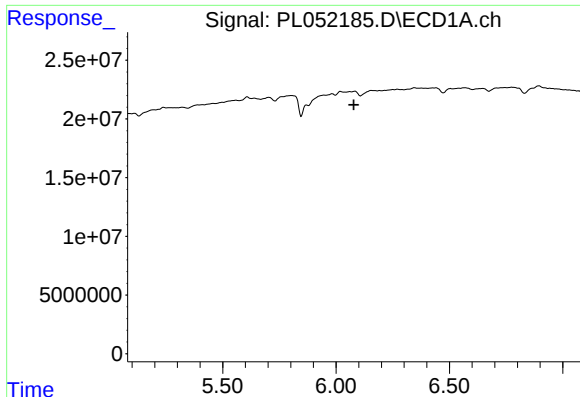

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

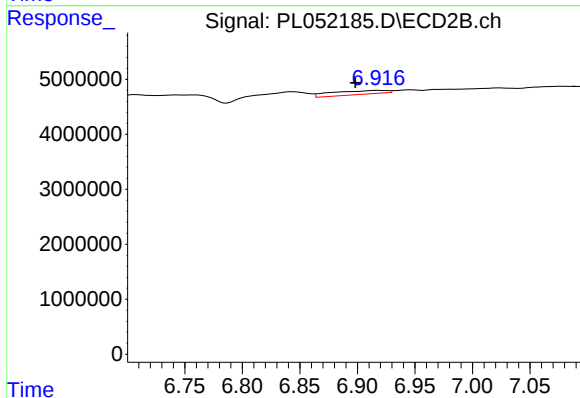


#27 Chlorodane-5

R.T.: 6.917 min
Delta R.T.: 0.019 min
Response: 2312418
Conc: 23.46 ng/ml

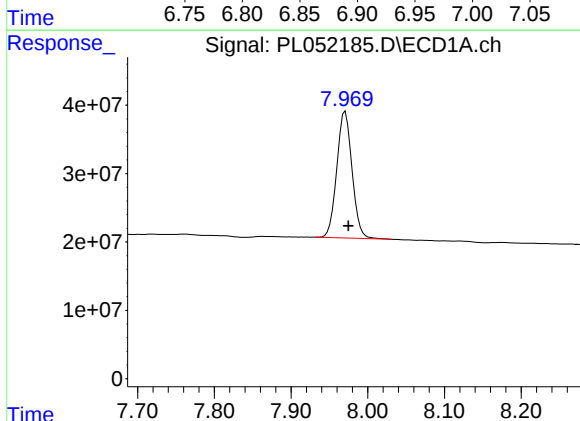

#28 Decachlorobiphenyl

R.T.: 7.971 min
Delta R.T.: -0.004 min
Response: 255526040
Conc: 21.05 ng/ml

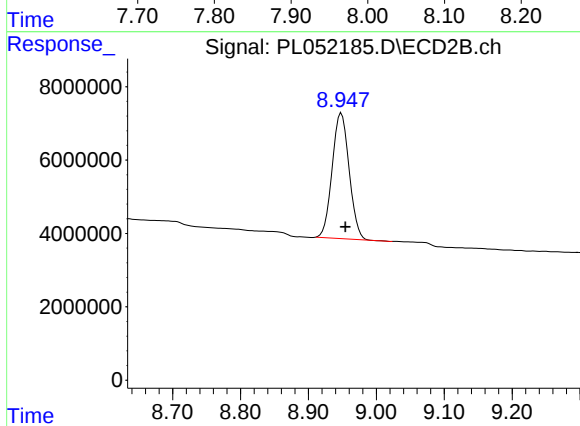

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.006 min
Response: 59420129
Conc: 19.52 ng/ml