

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
 Data File : PL052195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2019 18:30
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 00:45:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.924	211.3E6	53191222	24.694	24.346
28)	SA Decachlor...	7.970	8.948	265.6E6	59931348	21.882	19.689
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	690950	N.D.	0.474 #
8)	B Heptachlo...	0.000	5.783	0	3377838	N.D.	1.001 #
9)	A Endosulfan I	5.330f	6.161f	6285049	203289	0.468	0.063 #
13)	MA Dieldrin	0.000	6.409	0	443846	N.D.	0.130 #
15)	B Endosulfa...	0.000	6.849f	0	226899	N.D.	0.069 #
27)	Chlordane-5	0.000	6.907	0	91384	N.D.	0.927 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090319\
Data File : PL052195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2019 18:30
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 00:45:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

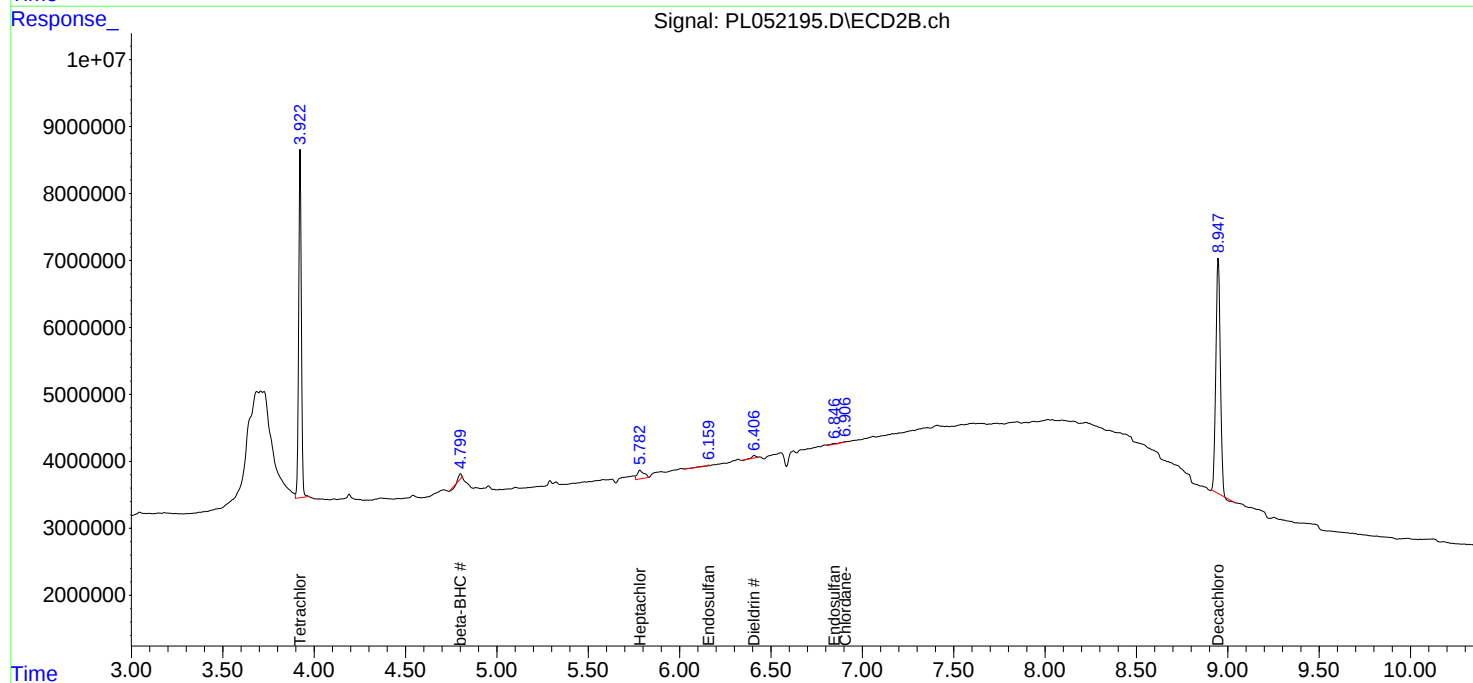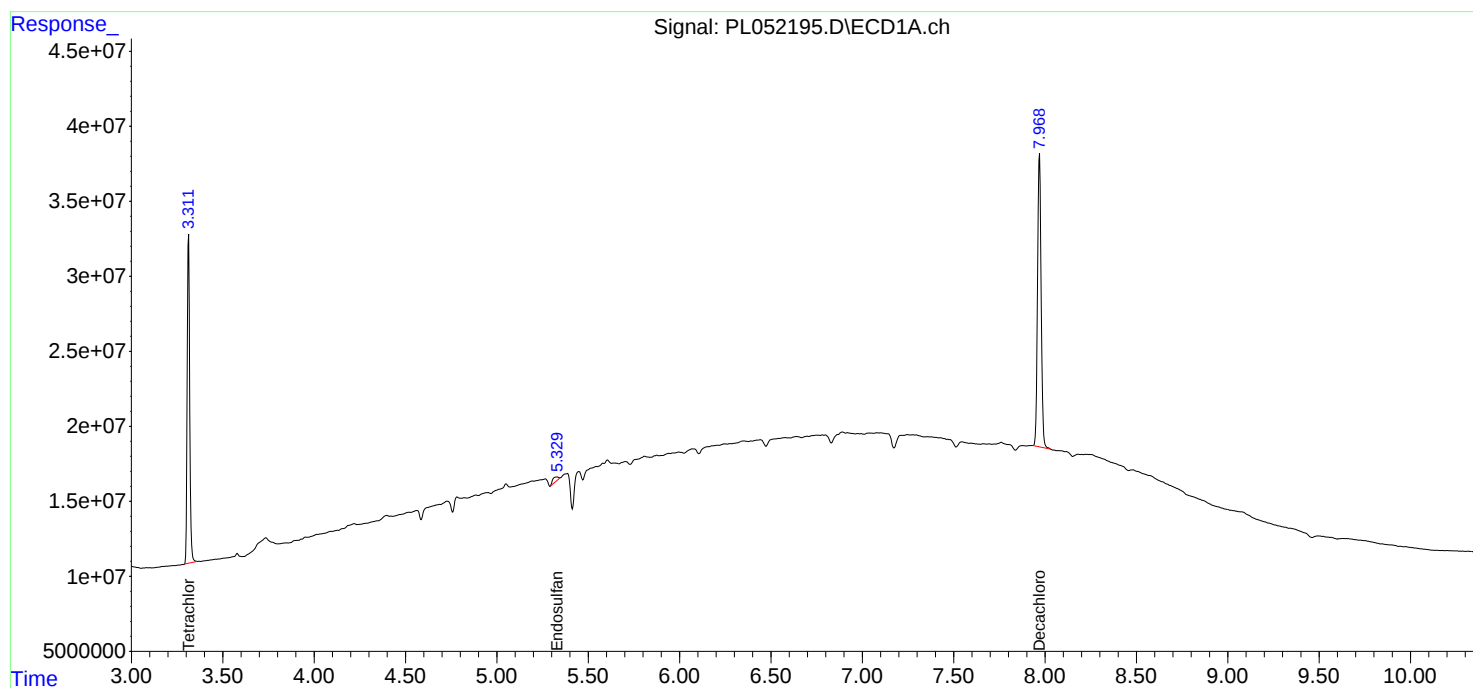


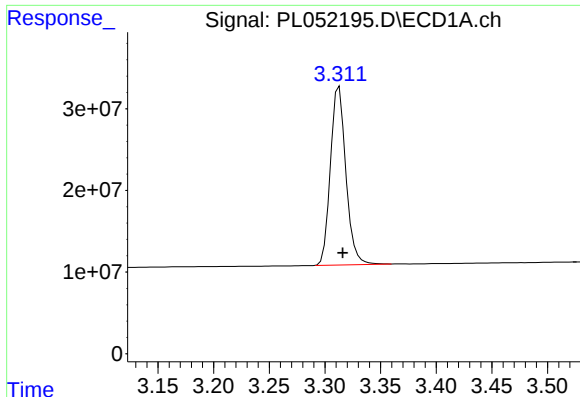

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: -0.003 min
Response: 211344964
Conc: 24.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

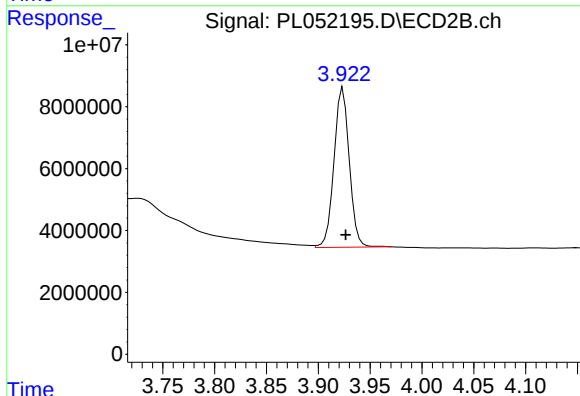


#1 Tetrachloro-m-xylene

R.T.: 3.924 min
Delta R.T.: -0.003 min
Response: 53191222
Conc: 24.35 ng/ml

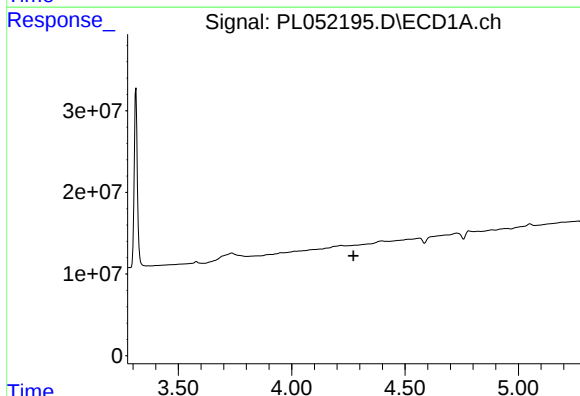


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

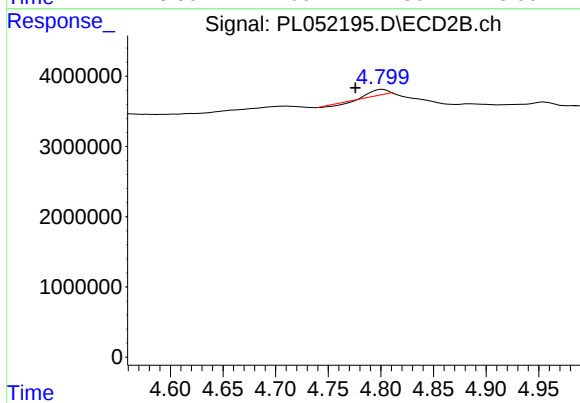

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 690950
Conc: 0.47 ng/ml

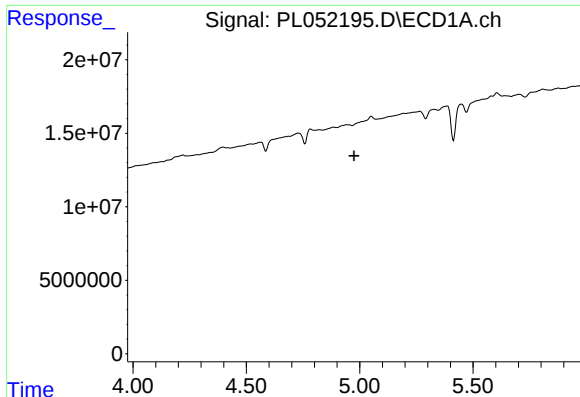

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

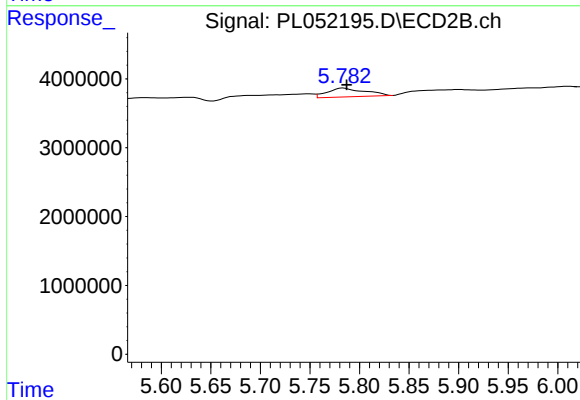


#8 Heptachlor epoxide

R.T.: 5.783 min
Delta R.T.: -0.004 min
Response: 3377838
Conc: 1.00 ng/ml

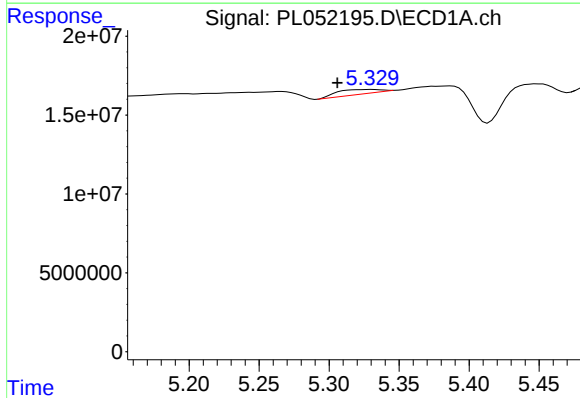


#9 Endosulfan I

R.T.: 5.330 min
Delta R.T.: 0.025 min
Response: 6285049
Conc: 0.47 ng/ml

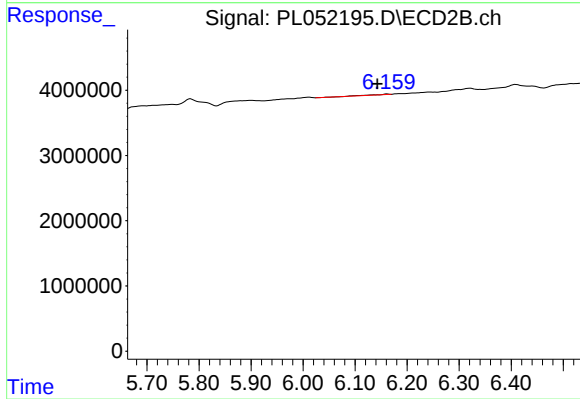

#9 Endosulfan I


R.T.: 6.161 min
Delta R.T.: 0.018 min
Response: 203289
Conc: 0.06 ng/ml

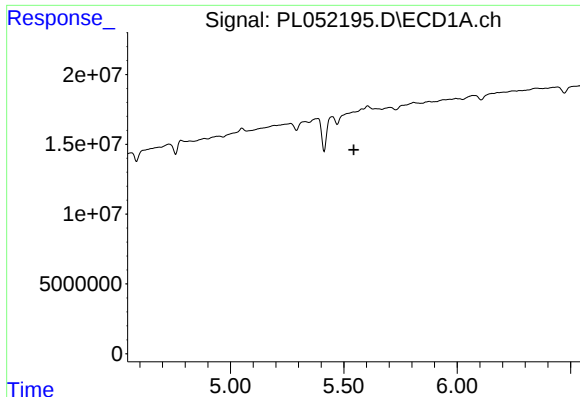

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

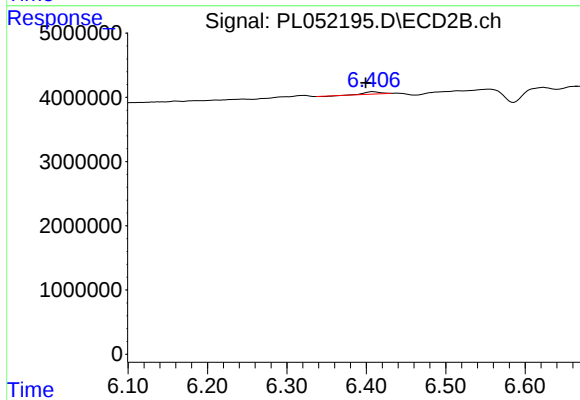


#13 Dieldrin

R.T.: 6.409 min
Delta R.T.: 0.010 min
Response: 443846
Conc: 0.13 ng/ml

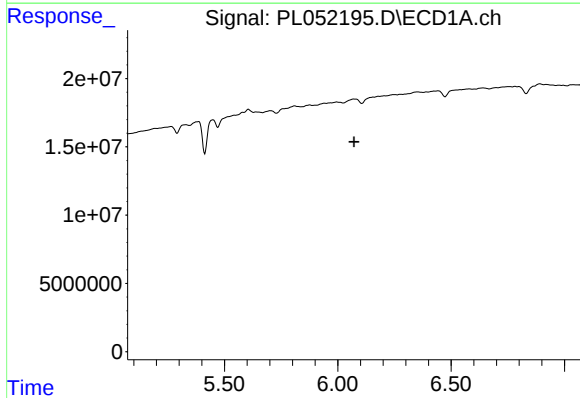


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

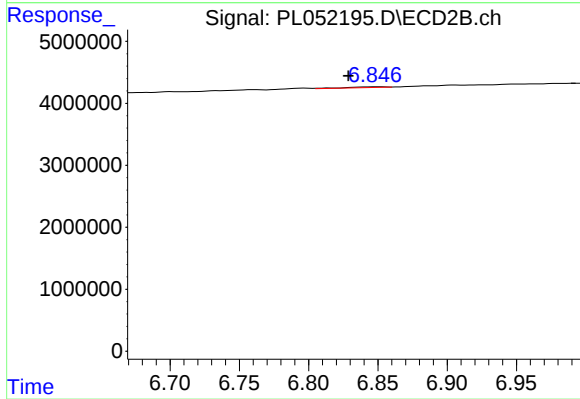

#15 Endosulfan II


R.T.: 6.849 min
Delta R.T.: 0.020 min
Response: 226899
Conc: 0.07 ng/ml

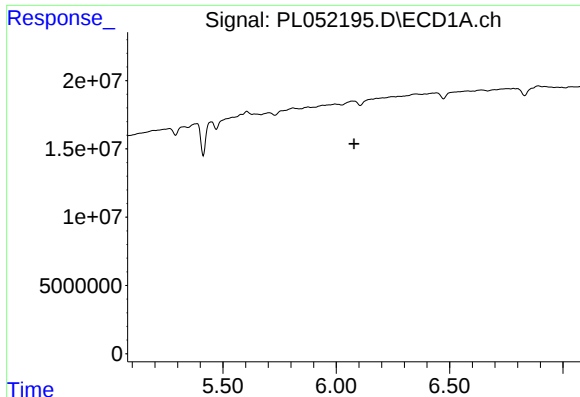

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

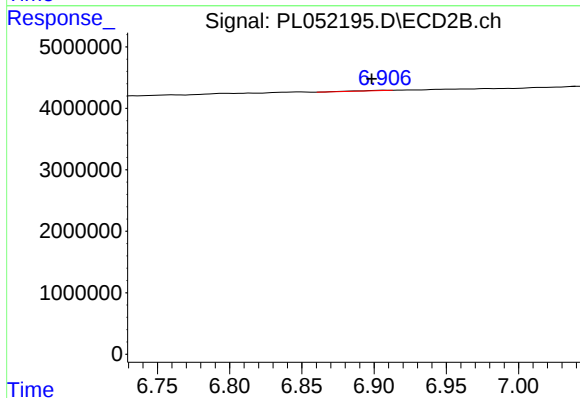


#27 Chlordane-5

R.T.: 6.907 min
Delta R.T.: 0.009 min
Response: 91384
Conc: 0.93 ng/ml

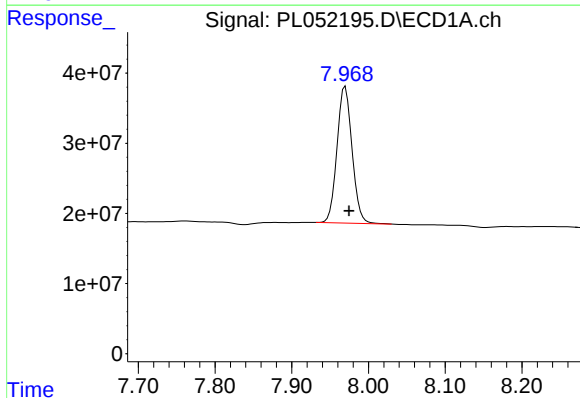

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.005 min
Response: 265603572
Conc: 21.88 ng/ml

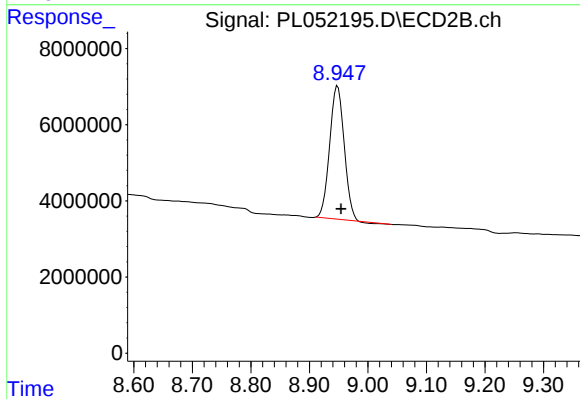

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.006 min
Response: 59931348
Conc: 19.69 ng/ml