

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
 Data File : PL052323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 21:53
 Operator : SG\AJ
 Sample : K4663-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-090519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 03:51:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.922	205.6E6	51750590	24.018	23.686
28)	SA Decachlor...	7.967	8.946	226.1E6	50896247	18.628	16.721
Target Compounds							
5)	MB Aldrin	4.555f	5.416f	2709376	354691	0.187	0.108 #
6)	B beta-BHC	0.000	4.763	0	280719	N.D.	0.193 #
8)	B Heptachlo...	0.000	5.774	0	957304	N.D.	0.284 #
15)	B Endosulfa...	0.000	6.838	0	6984486	N.D.	2.119 #
18)	B Endrin al...	0.000	6.948	0	869999	N.D.	0.308 #
22)	Mirex	0.000	8.068f	0	2539497	N.D.	1.044 #
24)	Chlordane-2	4.677f	0.000	8458204	0	20.695	N.D. #
27)	Chlordane-5	0.000	6.923f	0	4757331	N.D.	48.257 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
Data File : PL052323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 21:53
Operator : SG\AJ
Sample : K4663-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-03-090519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 03:51:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

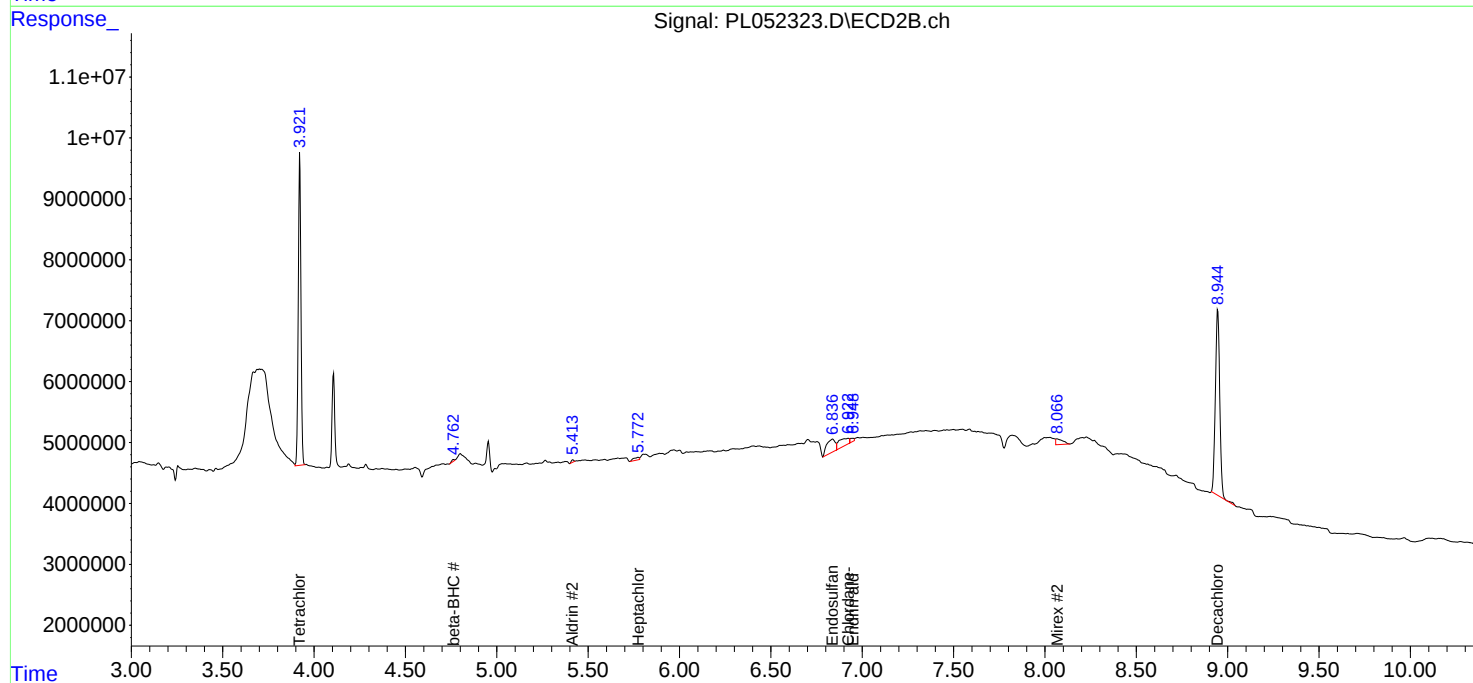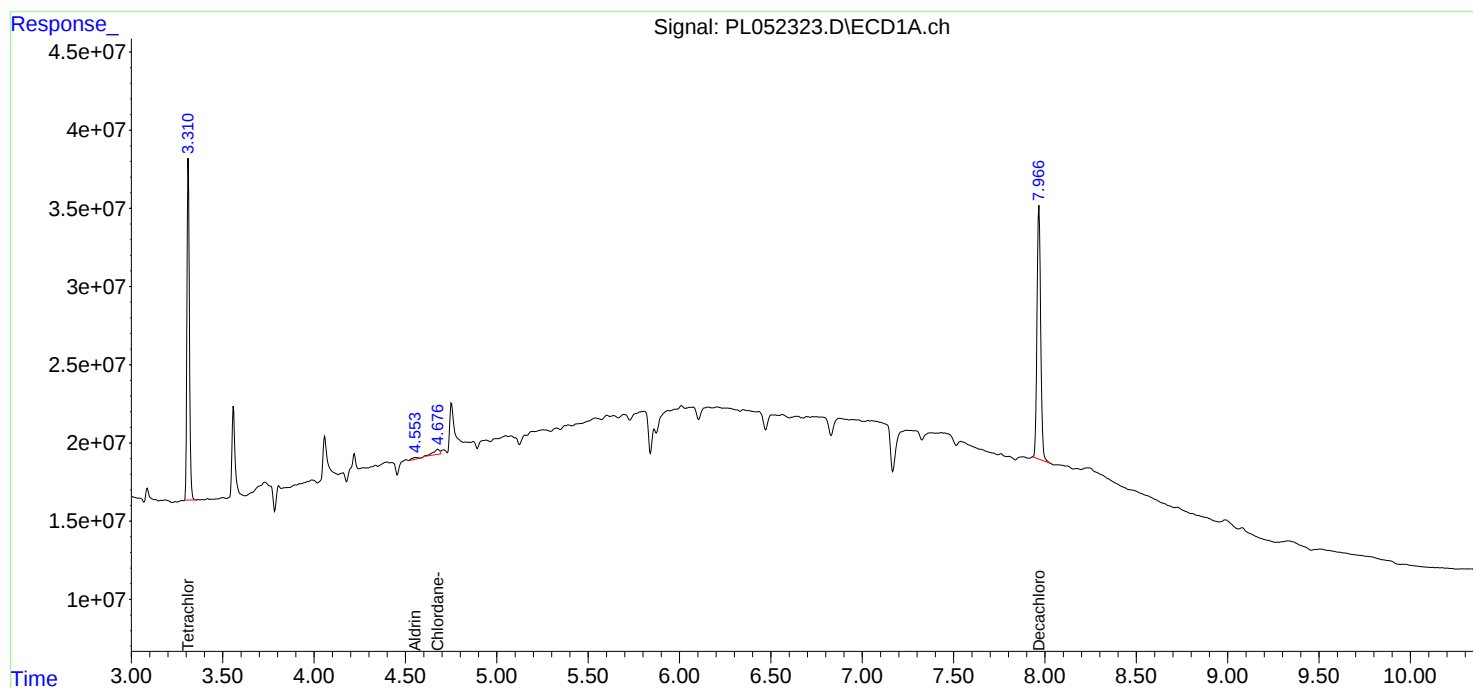


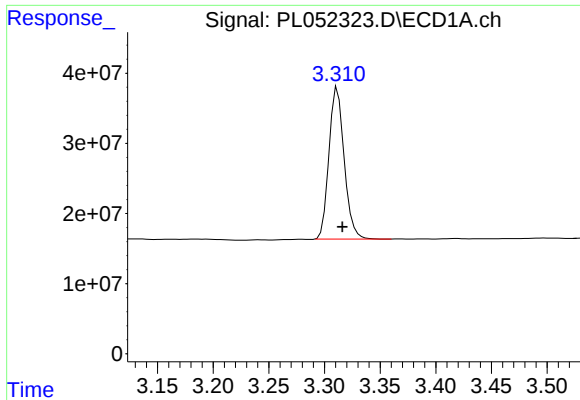

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 205560435
Conc: 24.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-090519

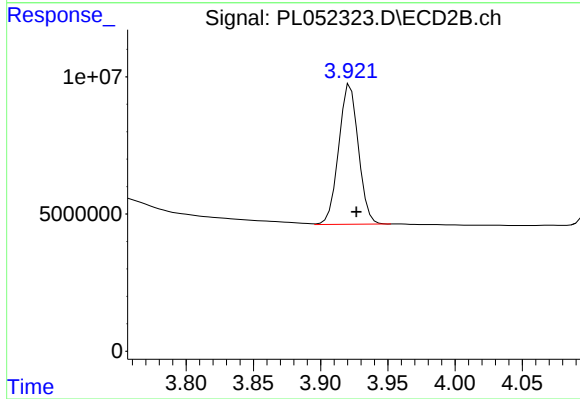


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.005 min
Response: 51750590
Conc: 23.69 ng/ml

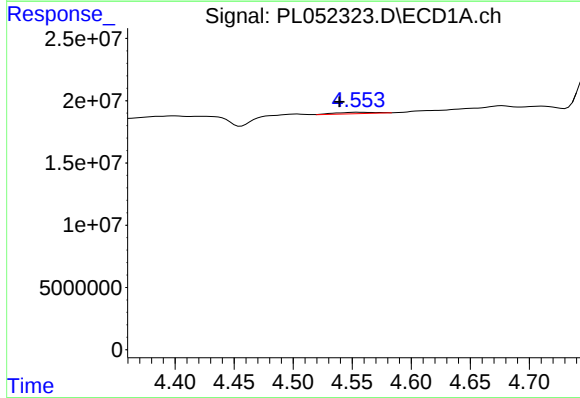


#5 Aldrin

R.T.: 4.555 min
Delta R.T.: 0.016 min
Response: 2709376
Conc: 0.19 ng/ml

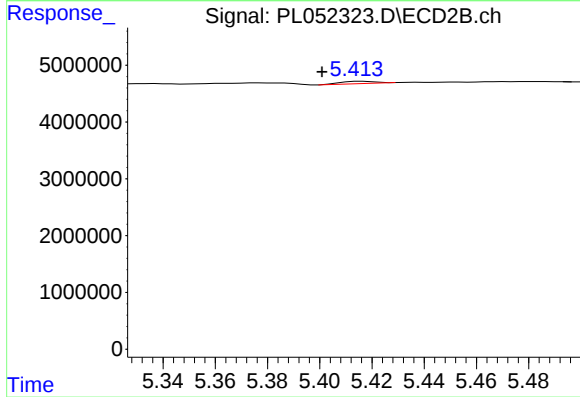

#5 Aldrin


R.T.: 5.416 min
Delta R.T.: 0.015 min
Response: 354691
Conc: 0.11 ng/ml

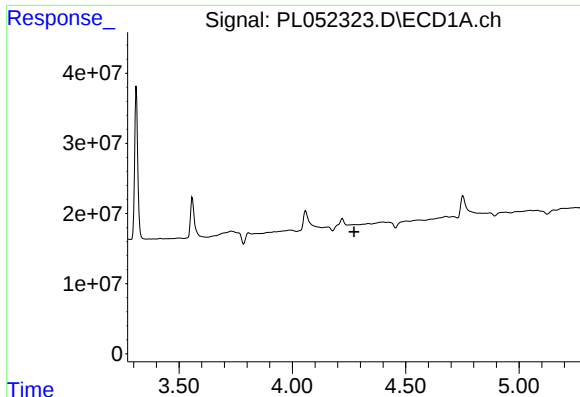

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-03-090519

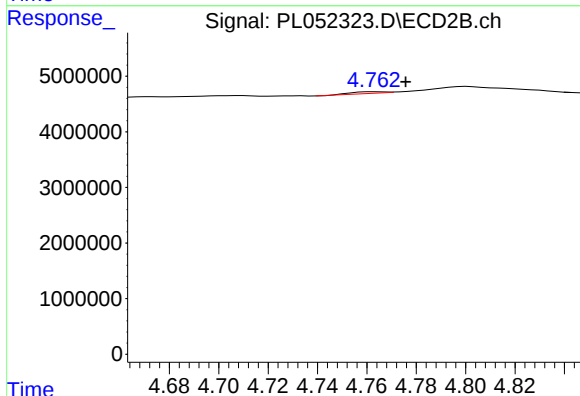


#6 beta-BHC

R.T.: 4.763 min
Delta R.T.: -0.013 min
Response: 280719
Conc: 0.19 ng/ml

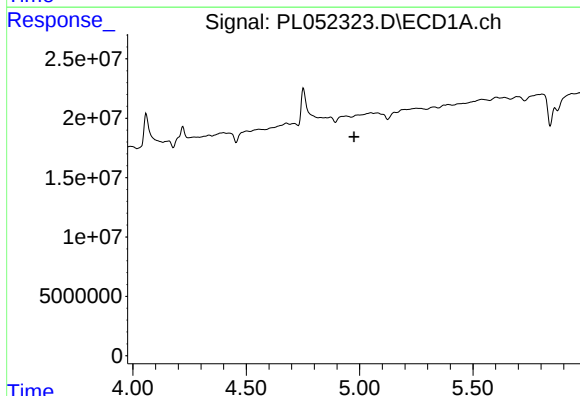


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

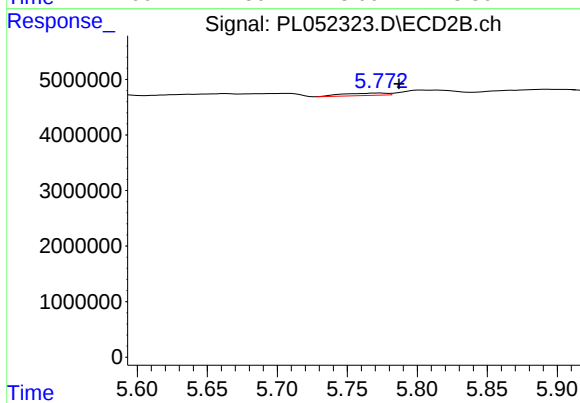

#8 Heptachlor epoxide


R.T.: 5.774 min
Delta R.T.: -0.013 min
Response: 957304
Conc: 0.28 ng/ml

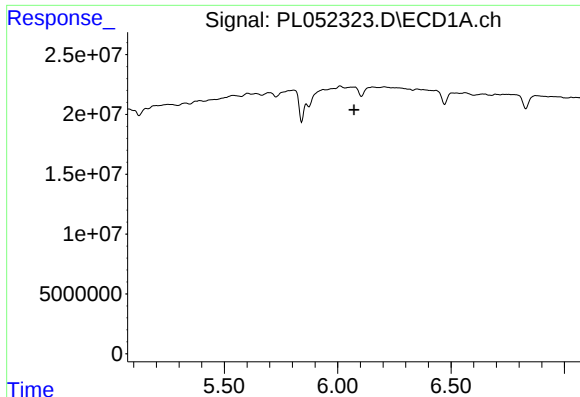

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-03-090519

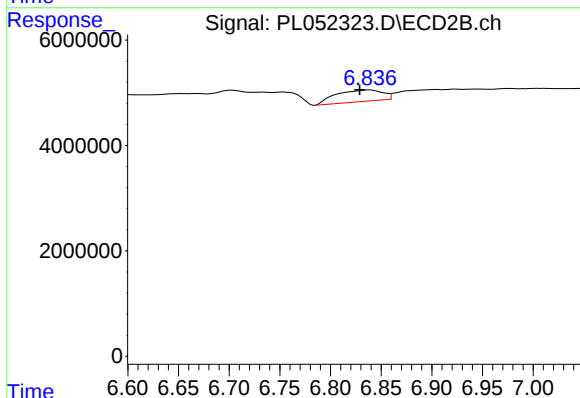


#15 Endosulfan II

R.T.: 6.838 min
Delta R.T.: 0.010 min
Response: 6984486
Conc: 2.12 ng/ml

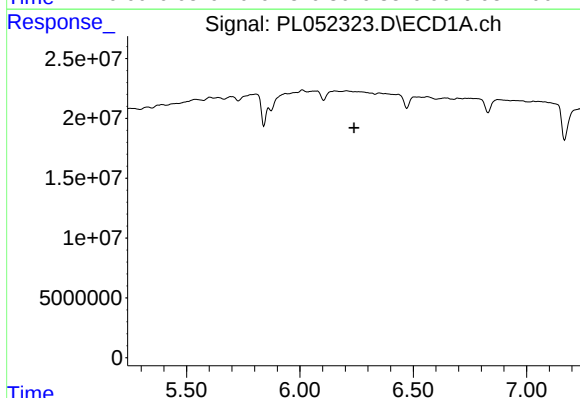


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

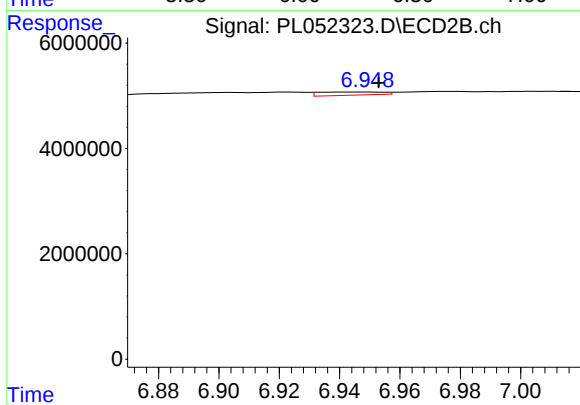

#18 Endrin aldehyde


R.T.: 6.948 min
Delta R.T.: -0.005 min
Response: 869999
Conc: 0.31 ng/ml

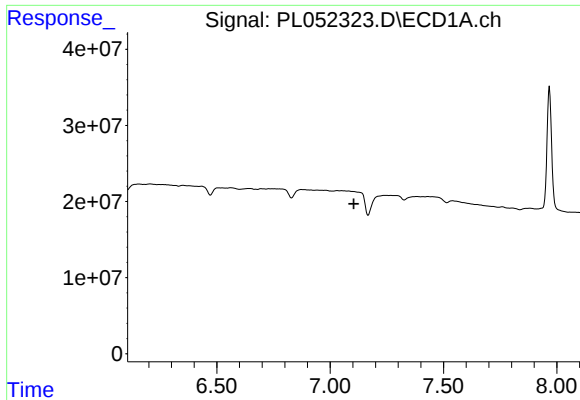

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-03-090519

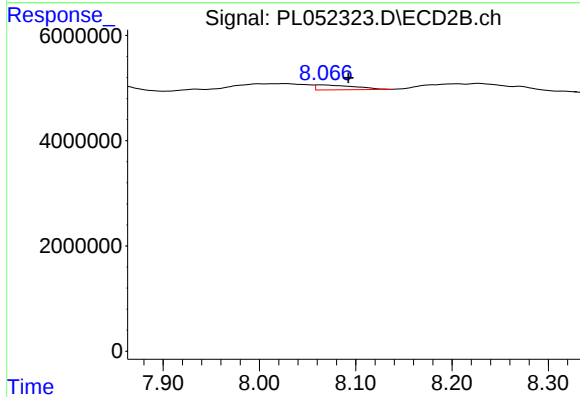


#22 Mirex

R.T.: 8.068 min
Delta R.T.: -0.025 min
Response: 2539497
Conc: 1.04 ng/ml

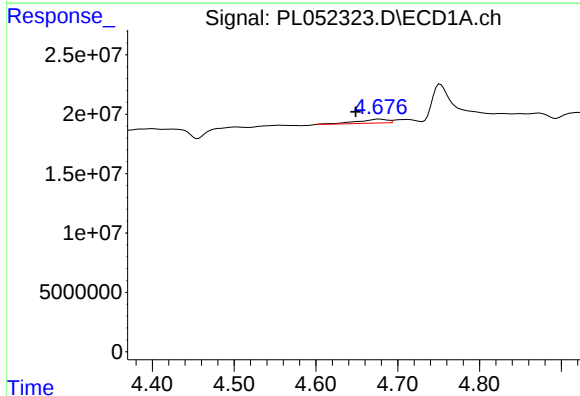


#24 Chlordane-2

R.T.: 4.677 min
Delta R.T.: 0.029 min
Response: 8458204
Conc: 20.69 ng/ml

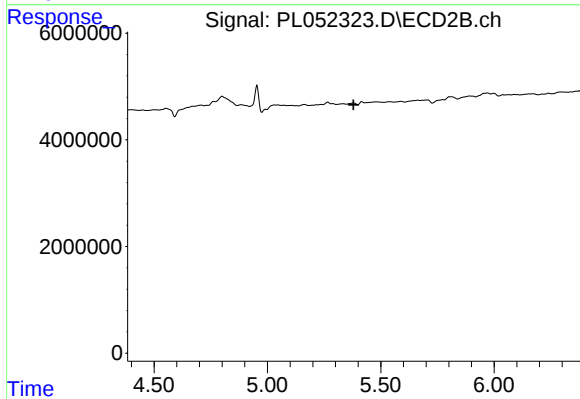

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

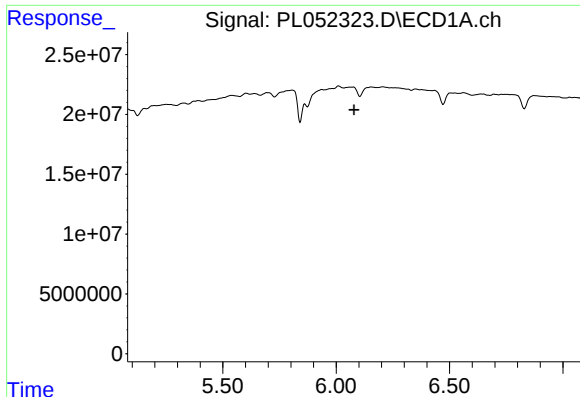

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-03-090519

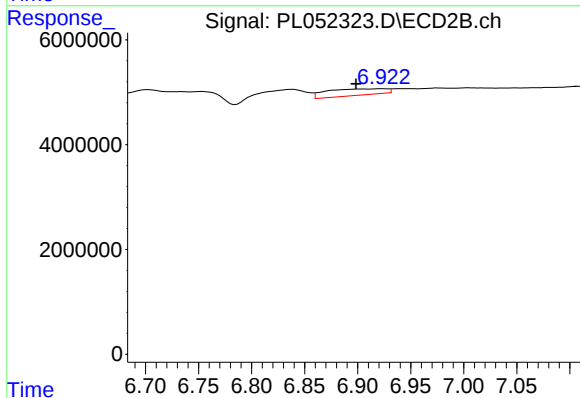


#27 Chlordane-5

R.T.: 6.923 min
Delta R.T.: 0.025 min
Response: 4757331
Conc: 48.26 ng/ml

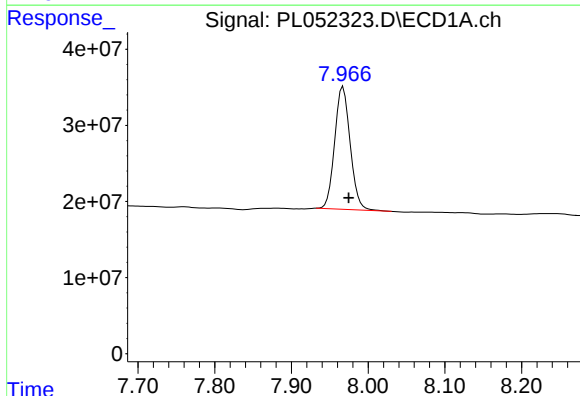

#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.007 min
Response: 226102099
Conc: 18.63 ng/ml

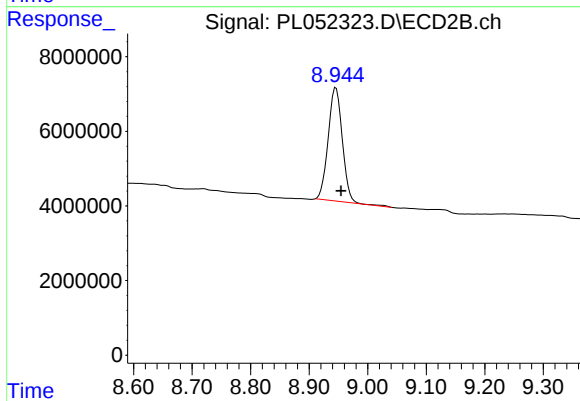

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.008 min
Response: 50896247
Conc: 16.72 ng/ml