

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
 Data File : PL052326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 22:36
 Operator : SG\AJ
 Sample : K4719-17
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T4-1-4-(0-1.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 03:52:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.922	194.7E6	50597932	22.746	23.159
28)	SA Decachlor...	7.967	8.944	229.8E6	52104449	18.934	17.118
Target Compounds							
6)	B beta-BHC	0.000	4.799f	0	701768	N.D.	0.482 #
8)	B Heptachlo...	0.000	5.806f	0	1730903	N.D.	0.513 #
11)	B alpha-Chl...	0.000	6.103	0	376635	N.D.	0.109 #
13)	MA Dieldrin	5.531	0.000	8172950	0	0.538	N.D. #
15)	B Endosulfa...	0.000	6.838	0	5800345	N.D.	1.760 #
18)	B Endrin al...	0.000	6.932f	0	1093316	N.D.	0.387 #
26)	Chlordane-4	0.000	6.103	0	376635	N.D.	0.693 #
27)	Chlordane-5	0.000	6.916f	0	3387001	N.D.	34.357 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
Data File : PL052326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 22:36
Operator : SG\AJ
Sample : K4719-17
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 03:52:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

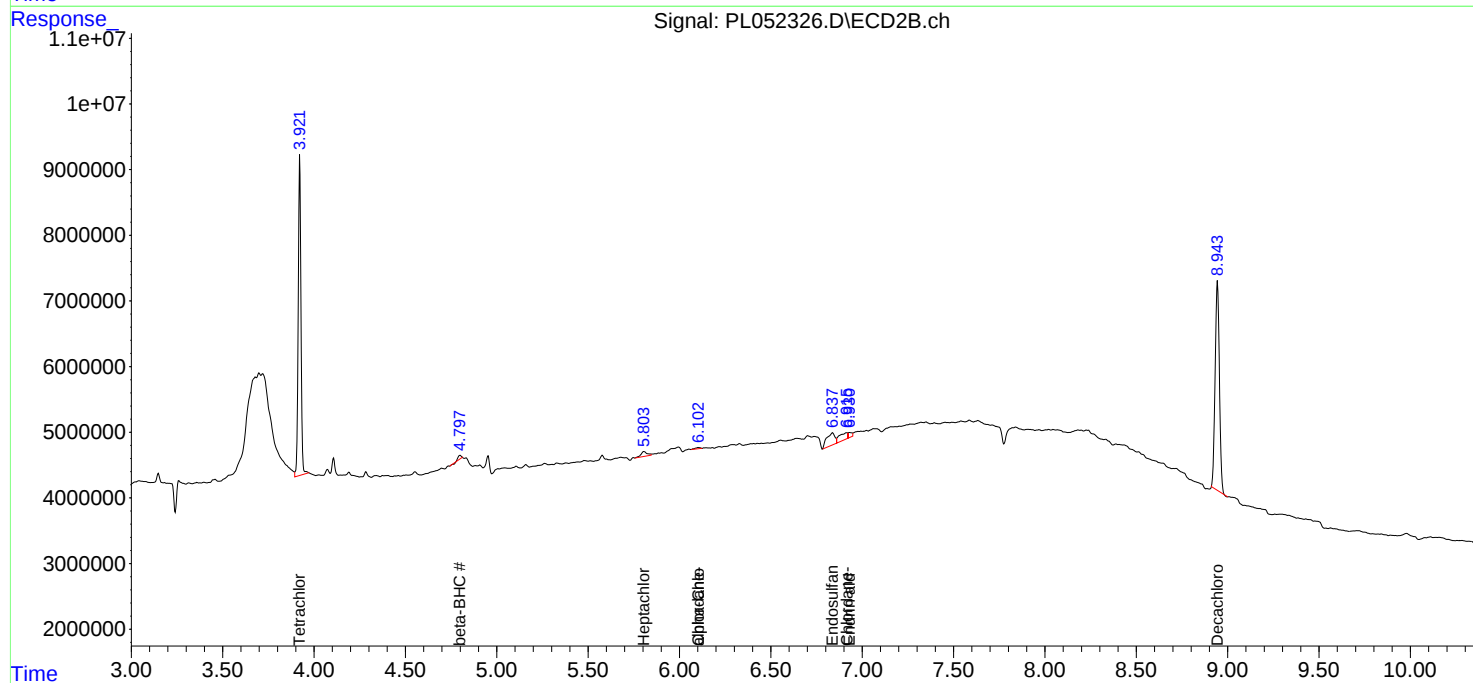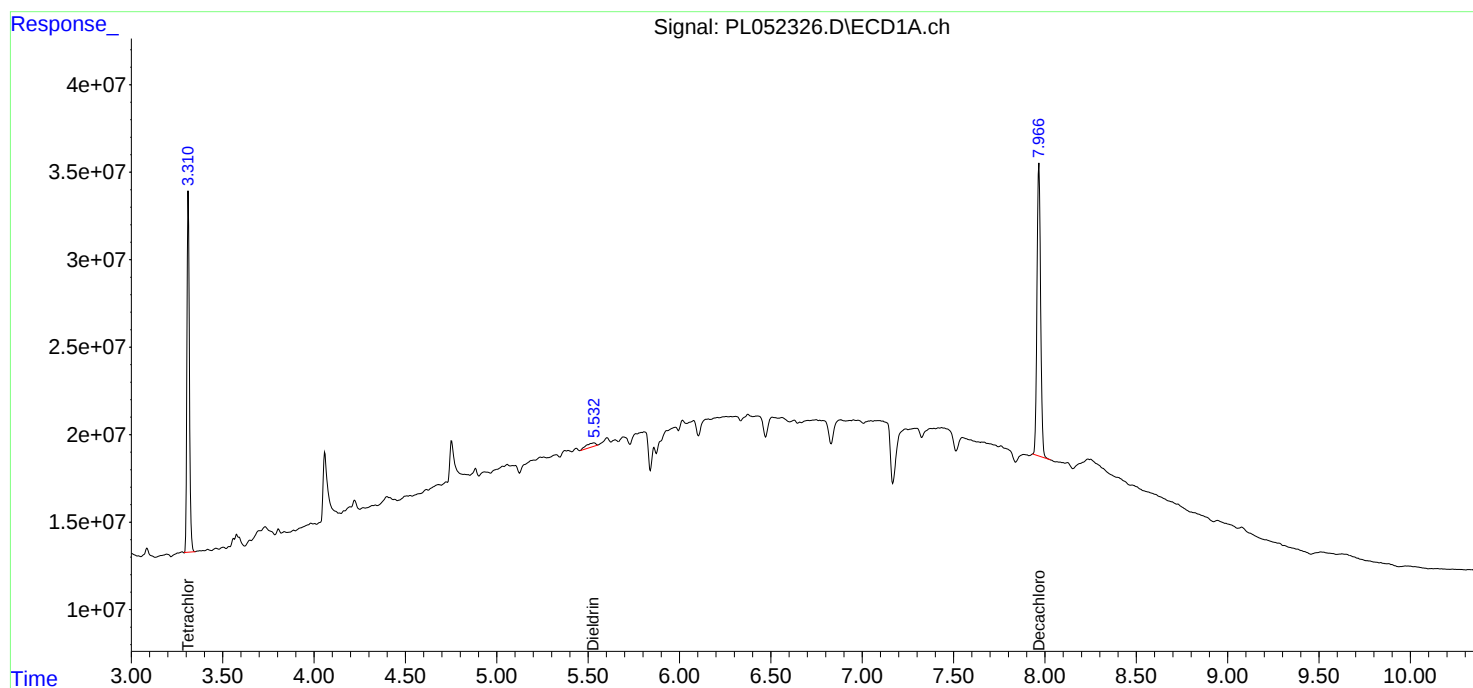


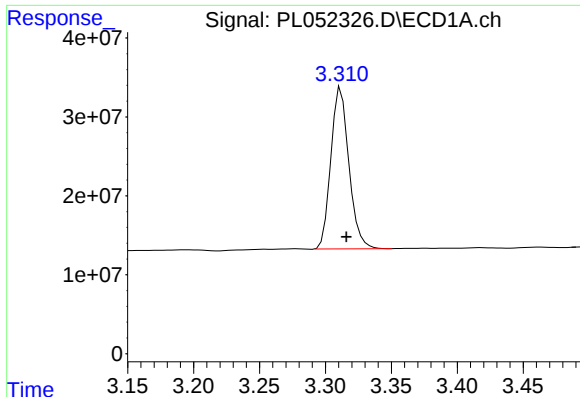

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 194678038
Conc: 22.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)

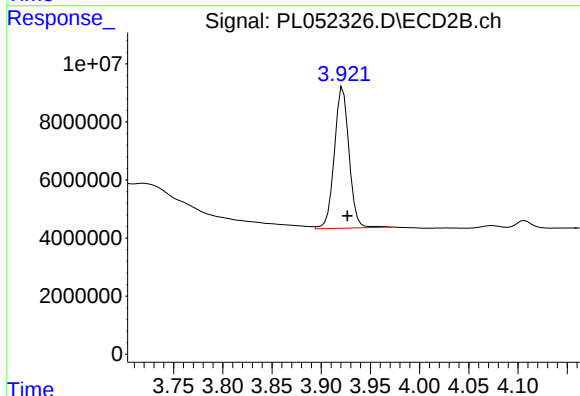


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.004 min
Response: 50597932
Conc: 23.16 ng/ml

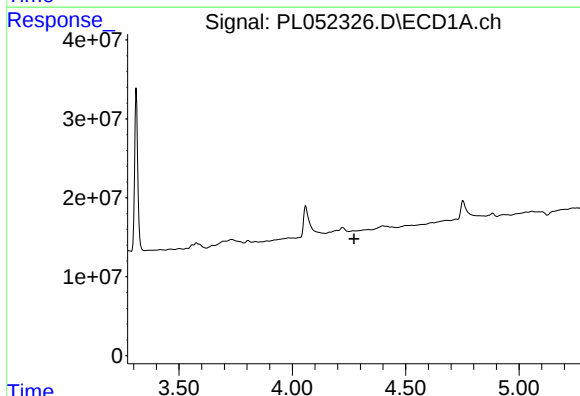


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

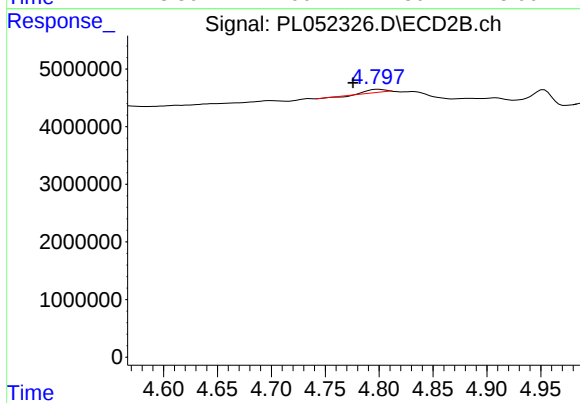

#6 beta-BHC


R.T.: 4.799 min
Delta R.T.: 0.023 min
Response: 701768
Conc: 0.48 ng/ml

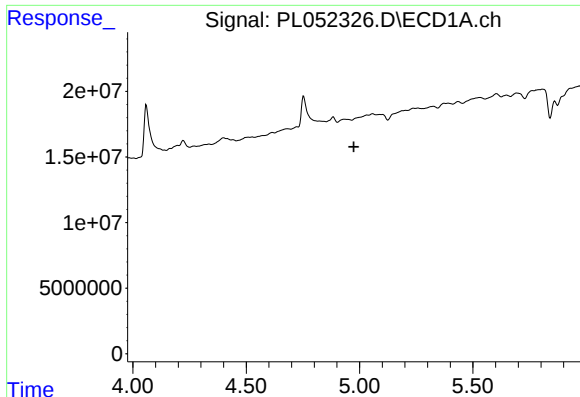

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)

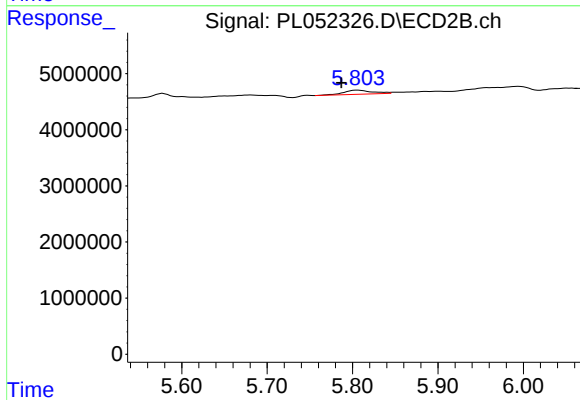


#8 Heptachlor epoxide

R.T.: 5.806 min
Delta R.T.: 0.018 min
Response: 1730903
Conc: 0.51 ng/ml

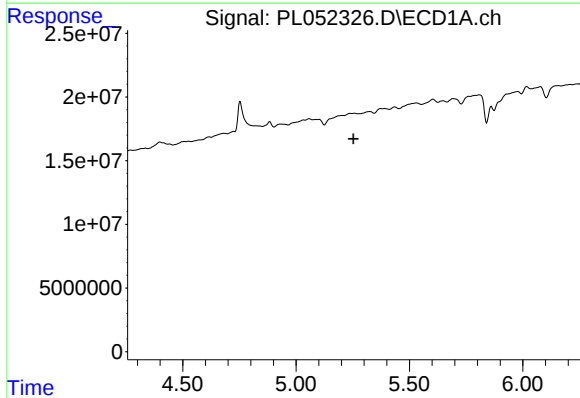


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

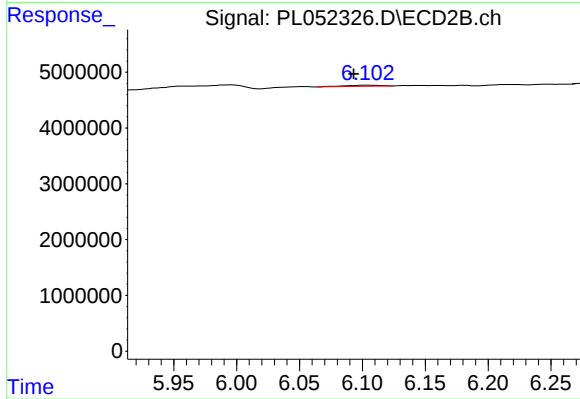

#11 alpha-Chlordane


R.T.: 6.103 min
Delta R.T.: 0.010 min
Response: 376635
Conc: 0.11 ng/ml

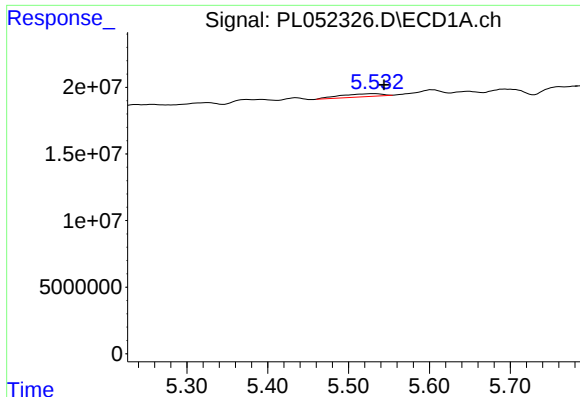

#13 Dieldrin


R.T.: 5.531 min
Delta R.T.: -0.013 min
Response: 8172950
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)

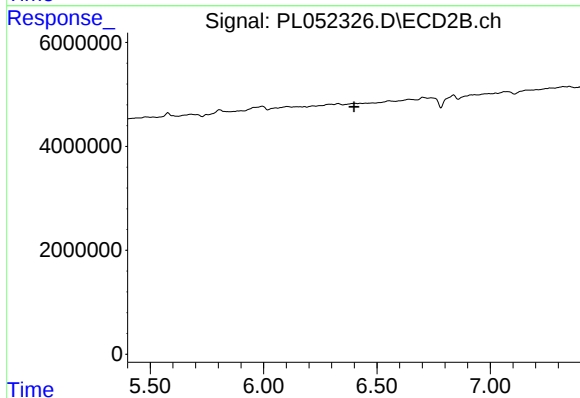


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

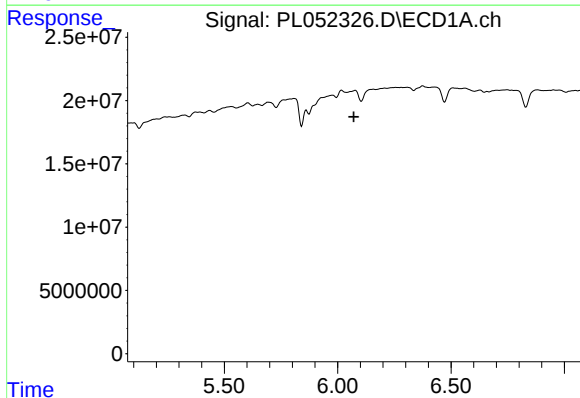


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

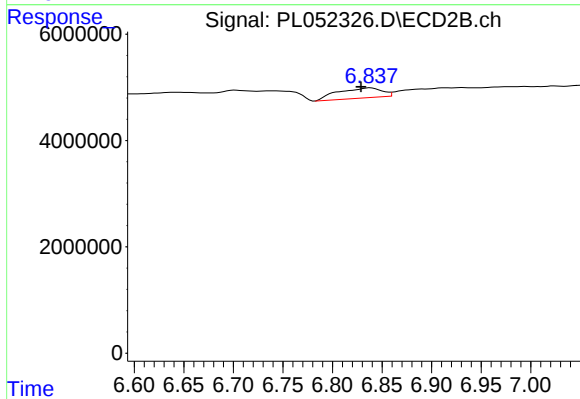

#15 Endosulfan II


R.T.: 6.838 min
Delta R.T.: 0.009 min
Response: 5800345
Conc: 1.76 ng/ml

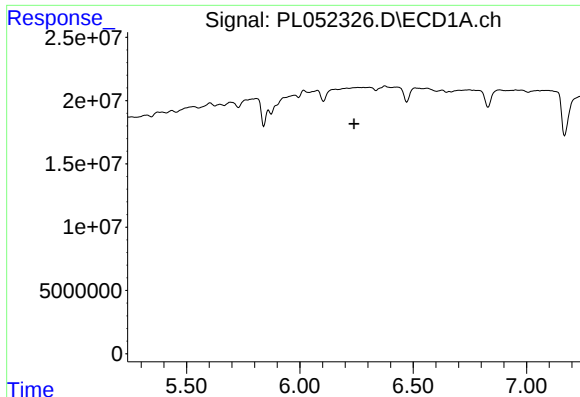

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)

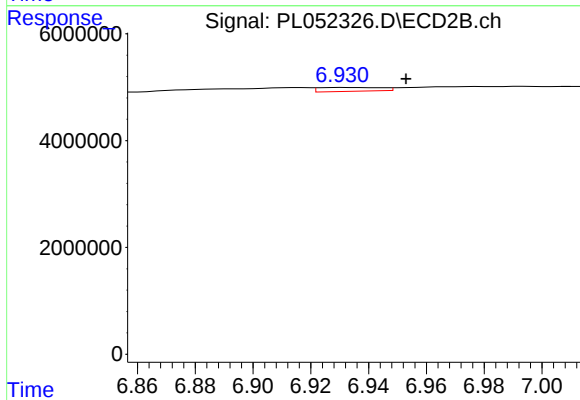


#18 Endrin aldehyde

R.T.: 6.932 min
Delta R.T.: -0.021 min
Response: 1093316
Conc: 0.39 ng/ml

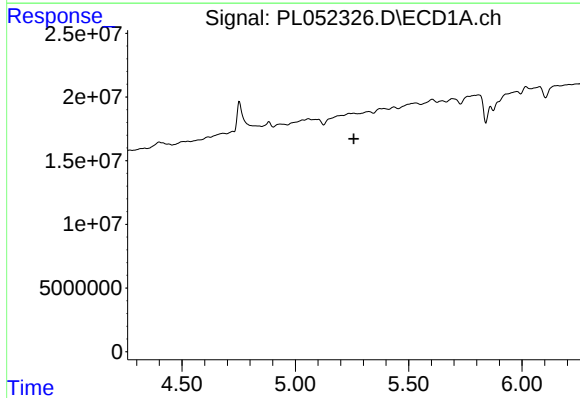


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

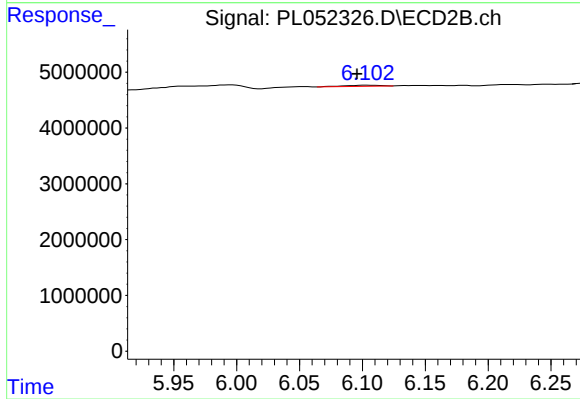

#26 Chlordane-4


R.T.: 6.103 min
Delta R.T.: 0.007 min
Response: 376635
Conc: 0.69 ng/ml

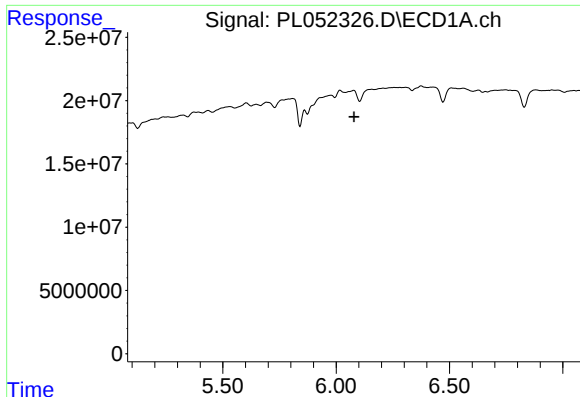

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)

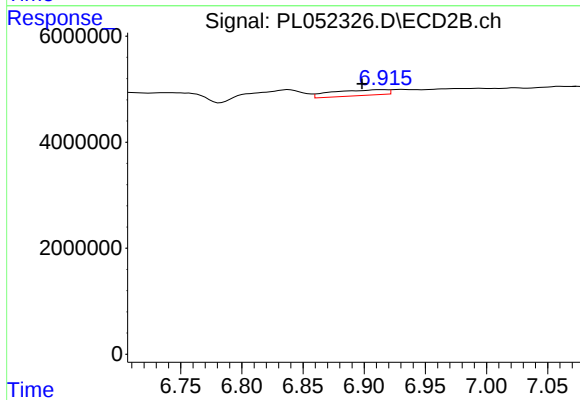


#27 Chlordane-5

R.T.: 6.916 min
Delta R.T.: 0.018 min
Response: 3387001
Conc: 34.36 ng/ml

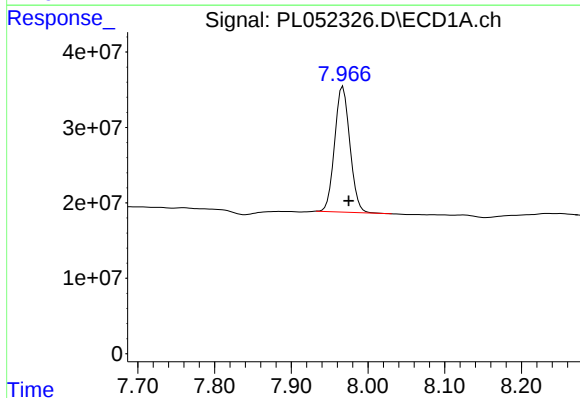

#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.007 min
Response: 229820807
Conc: 18.93 ng/ml

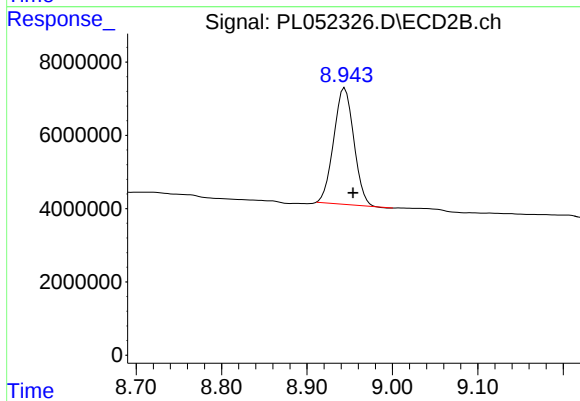

#28 Decachlorobiphenyl

R.T.: 8.944 min
Delta R.T.: -0.010 min
Response: 52104449
Conc: 17.12 ng/ml