

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
 Data File : PL052302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 16:58
 Operator : SG\AJ
 Sample : K4719-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T4-1-4-(0-1.5)

Manual Integrations
 APPROVED

Ankita
 9/10/2019 11:15:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 04:41:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.312	3.922	119.5E6	33143325	13.968	15.170
28) SA Decachlor...	7.968	8.945	150.8E6	34635655	12.420	11.379
Target Compounds						
14) MA Endrin	5.794	6.604	13074197	1577512	0.896m	0.522 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
Data File : PL052302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 16:58
Operator : SG\AJ
Sample : K4719-10
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)


Manual Integrations
APPROVED

Ankita
9/10/2019 11:15:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 04:41:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

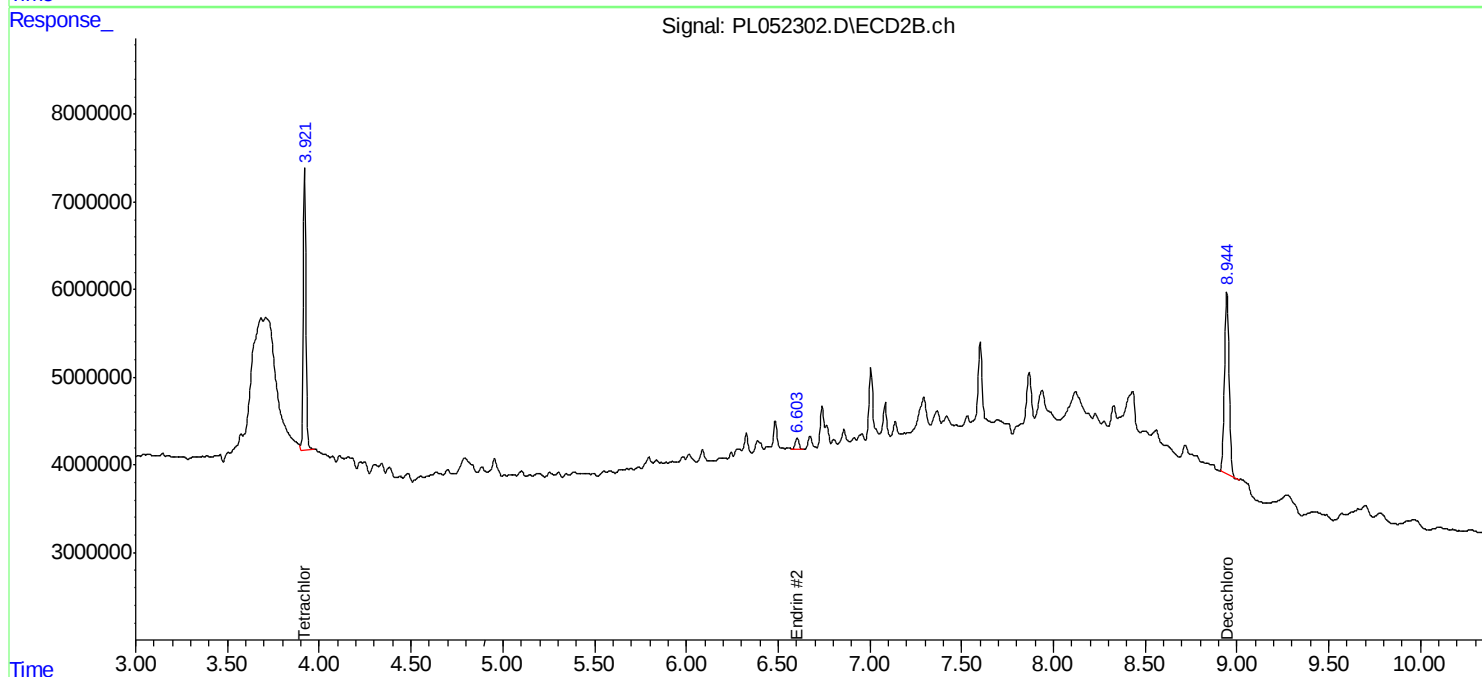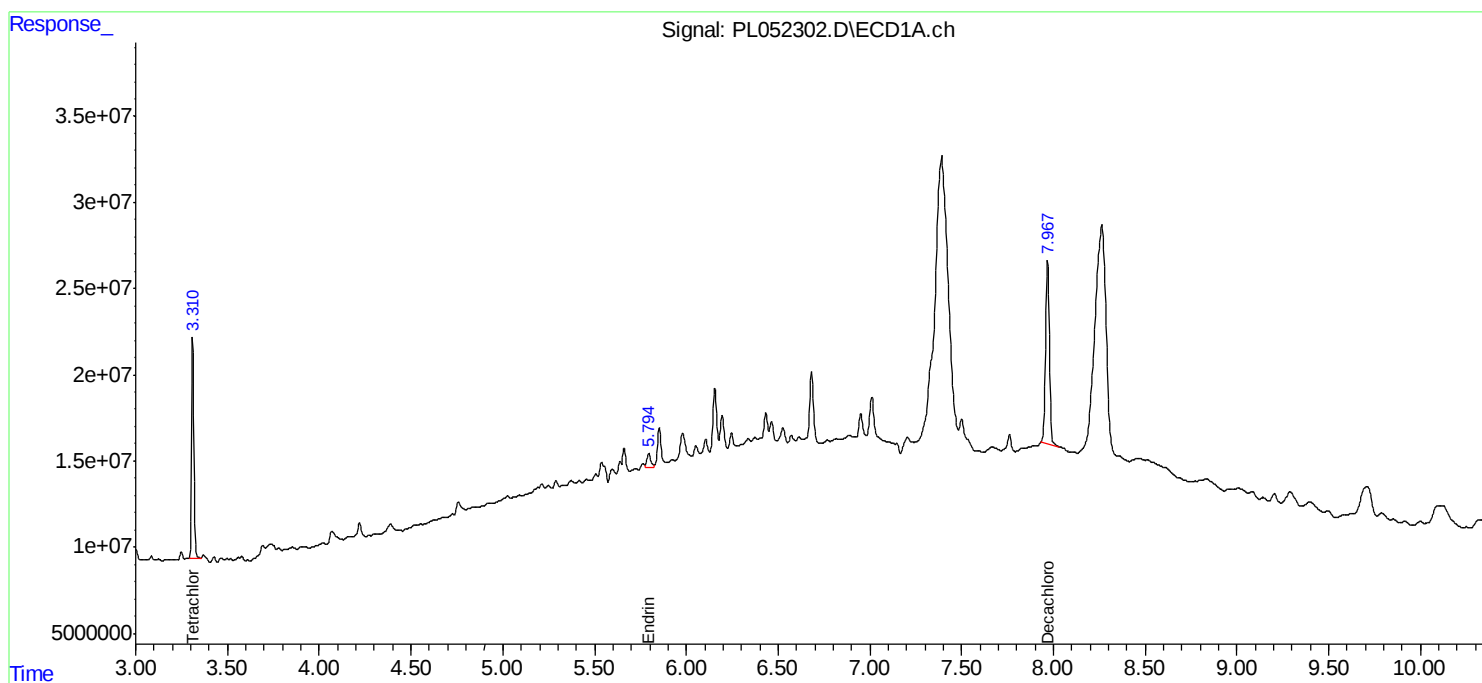

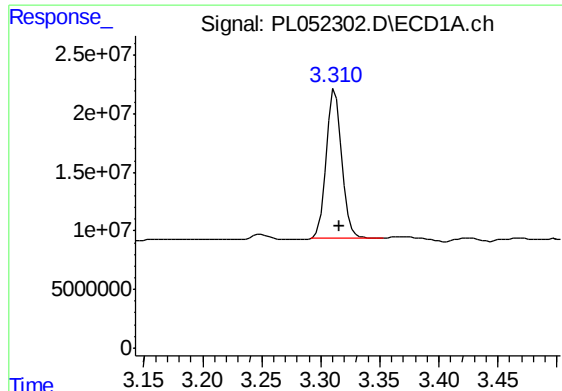


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 119543151
Conc: 13.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)


Manual Integrations
APPROVED

Ankita
9/10/2019 11:15:33 AM

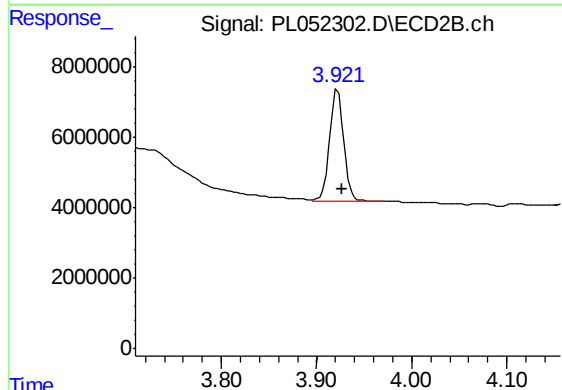


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.005 min
Response: 33143325
Conc: 15.17 ng/ml

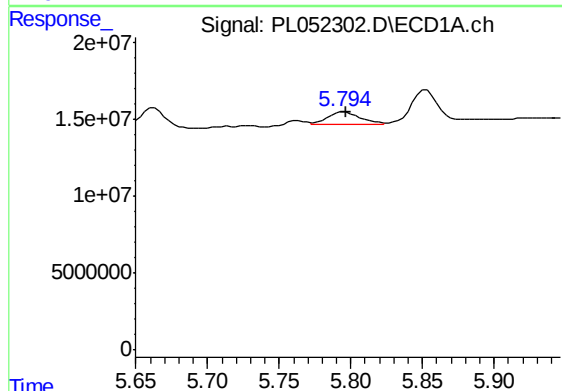


#14 Endrin

R.T.: 5.794 min
Delta R.T.: -0.002 min
Response: 13074197
Conc: 0.90 ng/ml m

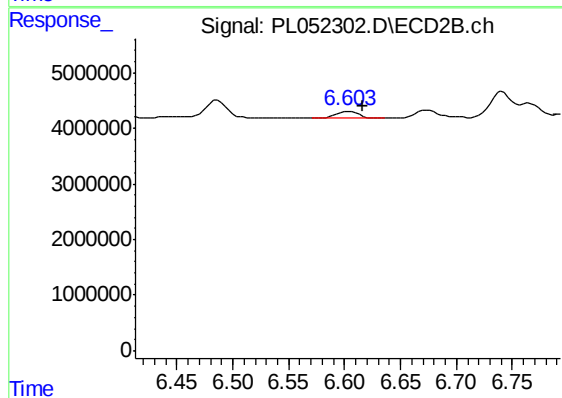

#14 Endrin

R.T.: 6.604 min
Delta R.T.: -0.012 min
Response: 1577512
Conc: 0.52 ng/ml

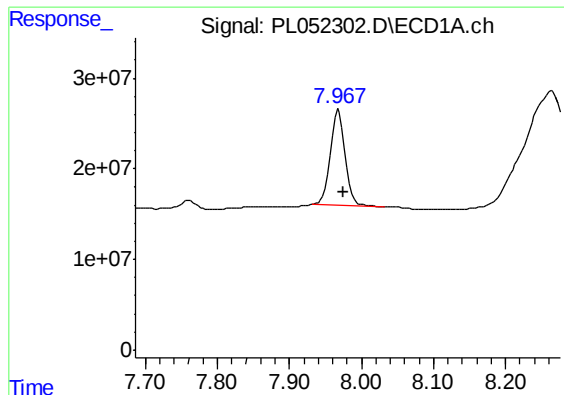


#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.006 min
Response: 150750594
Conc: 12.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-1-4-(0-1.5)

Manual Integrations
APPROVED

Ankita
9/10/2019 11:15:33 AM

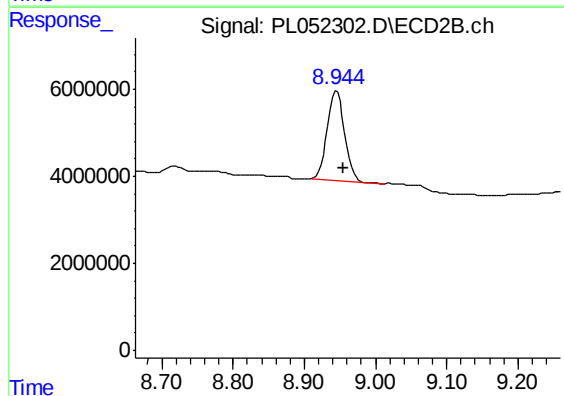

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.009 min
Response: 34635655
Conc: 11.38 ng/ml