

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
 Data File : PL052306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 17:54
 Operator : SG\AJ
 Sample : K4745-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-058

Manual Integrations
 APPROVED

Ankita
 9/11/2019 8:56:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 03:45:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.922	105.9E6	26581351	12.375	12.166
28)	SA Decachlor...	7.968	8.945	94790464	21617220	7.810	7.102
Target Compounds							
10)	B gamma-Chl...	5.197	6.014	4127845	1240064	0.276m	0.340m
11)	B alpha-Chl...	5.247	6.087	8052576	3857573	0.556	1.118m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
Data File : PL052306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 17:54
Operator : SG\AJ
Sample : K4745-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-PS-01-058


Manual Integrations
APPROVED

Ankita
9/11/2019 8:56:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 03:45:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

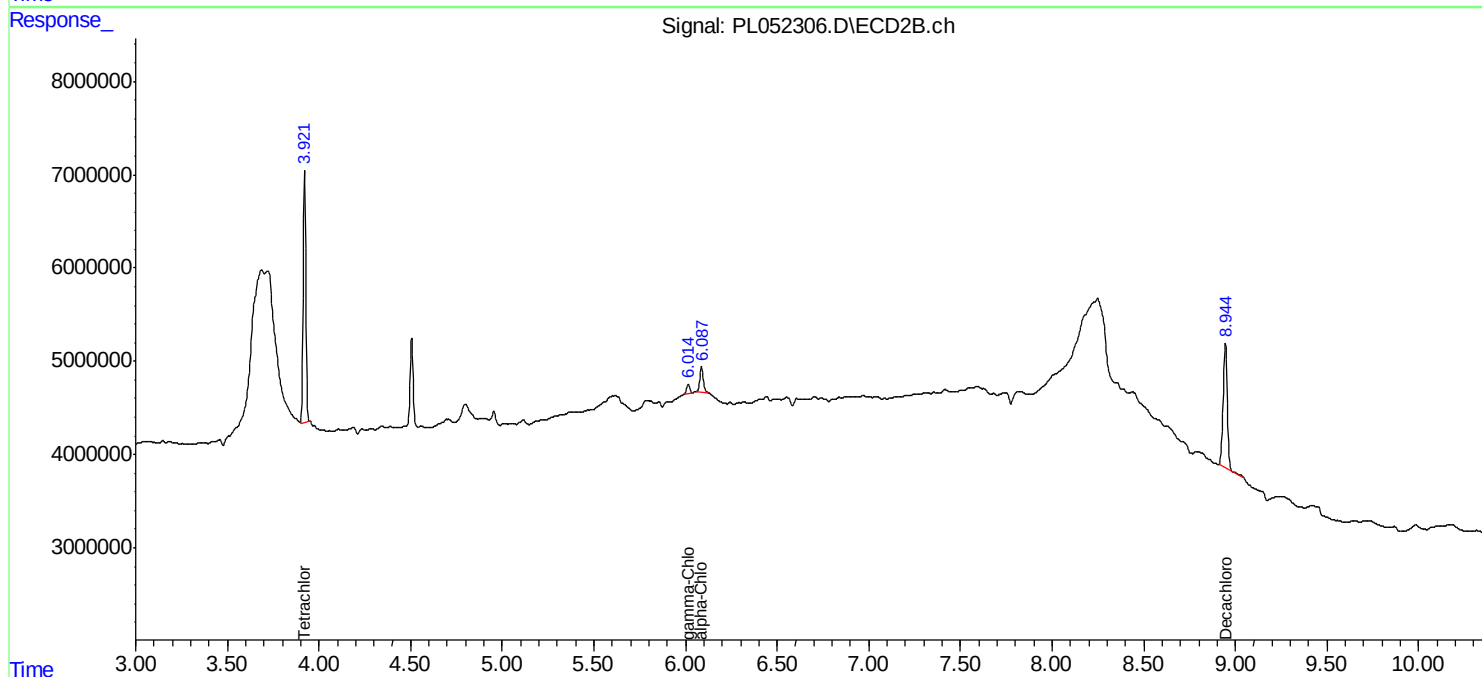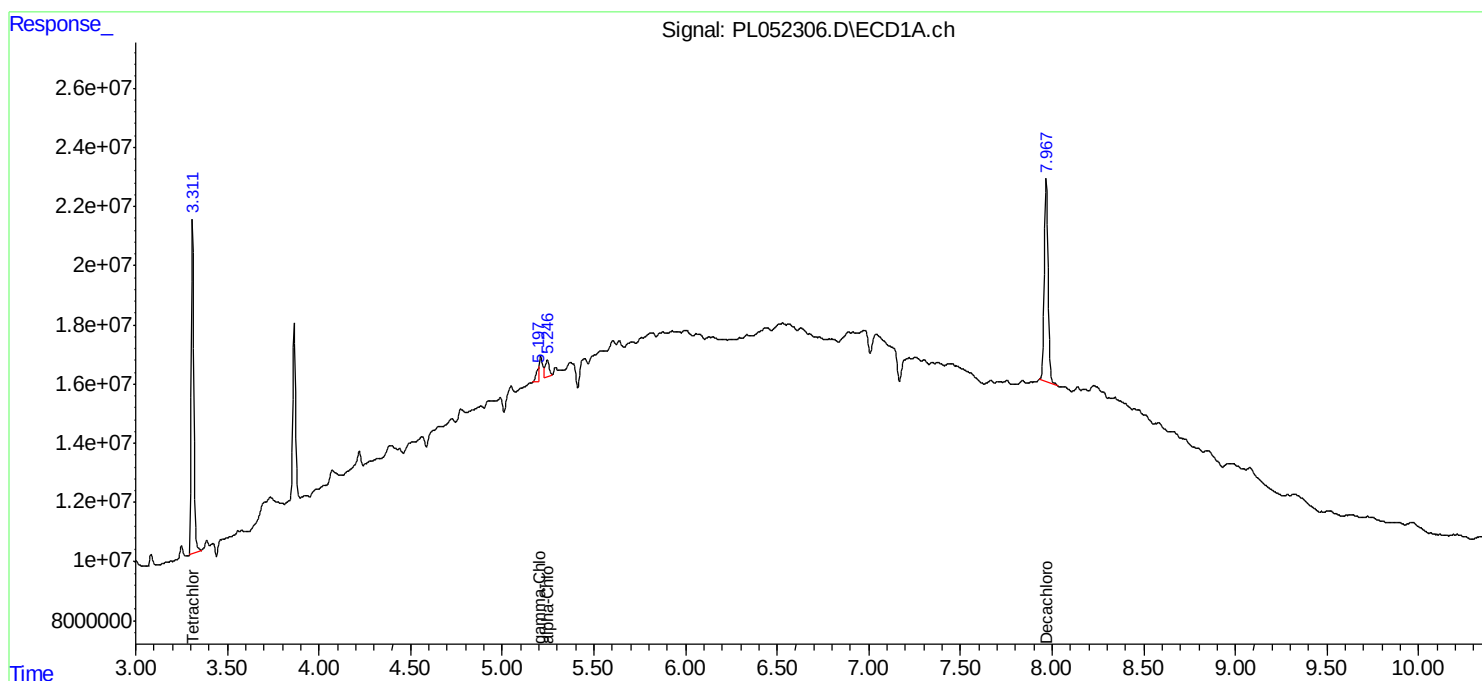

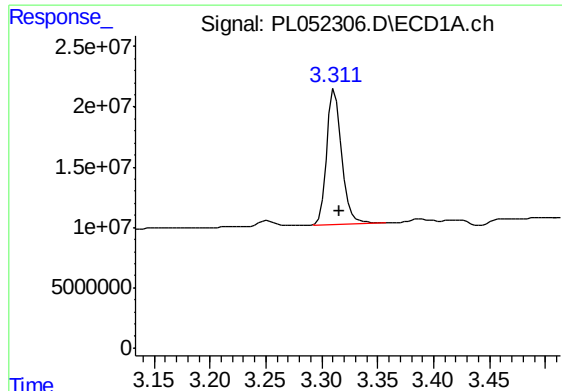


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 105915540
Conc: 12.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-058


Manual Integrations
APPROVED

Ankita
9/11/2019 8:56:13 AM

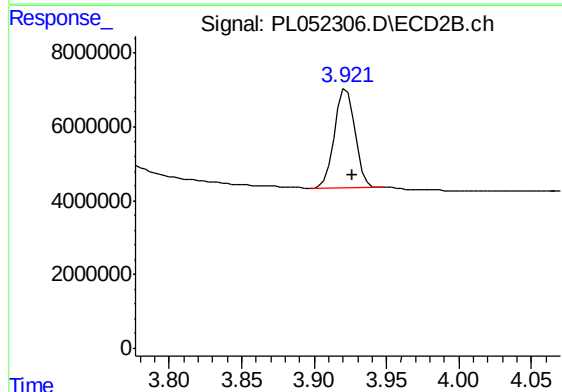


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.004 min
Response: 26581351
Conc: 12.17 ng/ml

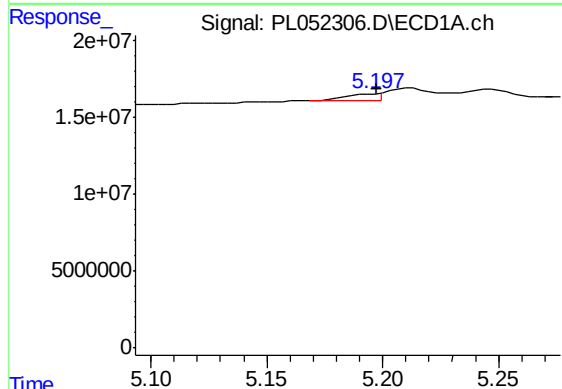


#10 gamma-Chlordane

R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 4127845
Conc: 0.28 ng/ml m

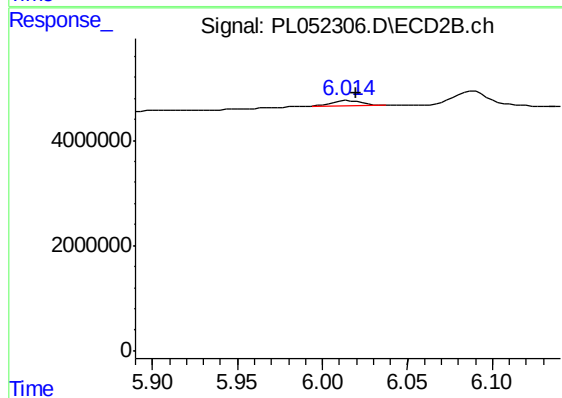

#10 gamma-Chlordane

R.T.: 6.014 min
Delta R.T.: -0.006 min
Response: 1240064
Conc: 0.34 ng/ml m

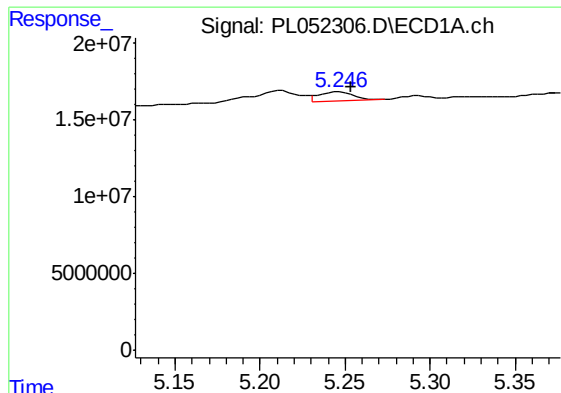


#11 alpha-Chlordane

R.T.: 5.247 min
Delta R.T.: -0.006 min
Response: 8052576
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-058


Manual Integrations
APPROVED

Ankita
9/11/2019 8:56:13 AM

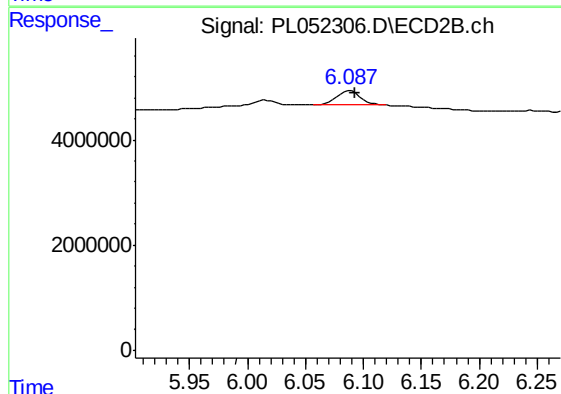


#11 alpha-Chlordane

R.T.: 6.087 min
Delta R.T.: -0.006 min
Response: 3857573
Conc: 1.12 ng/ml m

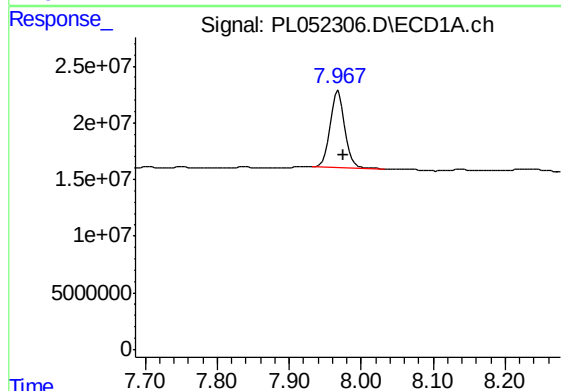

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.006 min
Response: 94790464
Conc: 7.81 ng/ml

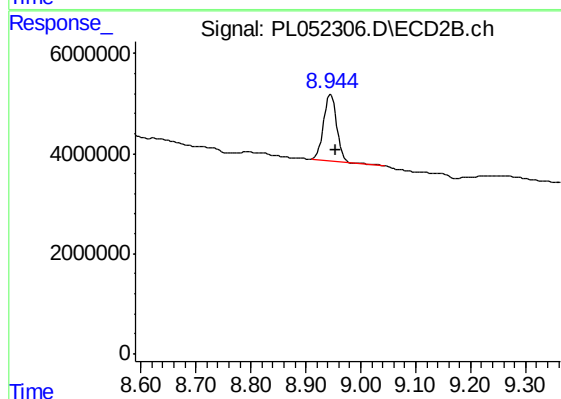

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.009 min
Response: 21617220
Conc: 7.10 ng/ml