

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
 Data File : PL052321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2019 21:25
 Operator : SG\AJ
 Sample : K4755-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-1-3

Manual Integrations
 APPROVED

Ankita
 9/10/2019 11:17:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 03:50:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.922	110.0E6	29282953	12.856	13.403
28)	SA Decachlor...	7.967	8.944	124.0E6	26562067	10.216	8.726m
Target Compounds							
17)	MA 4,4'-DDT	6.156	7.033	34019247	4081749	2.668	1.394m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL090919\
Data File : PL052321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2019 21:25
Operator : SG\AJ
Sample : K4755-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RO-1-3


Manual Integrations
APPROVED

Ankita
9/10/2019 11:17:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 03:50:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

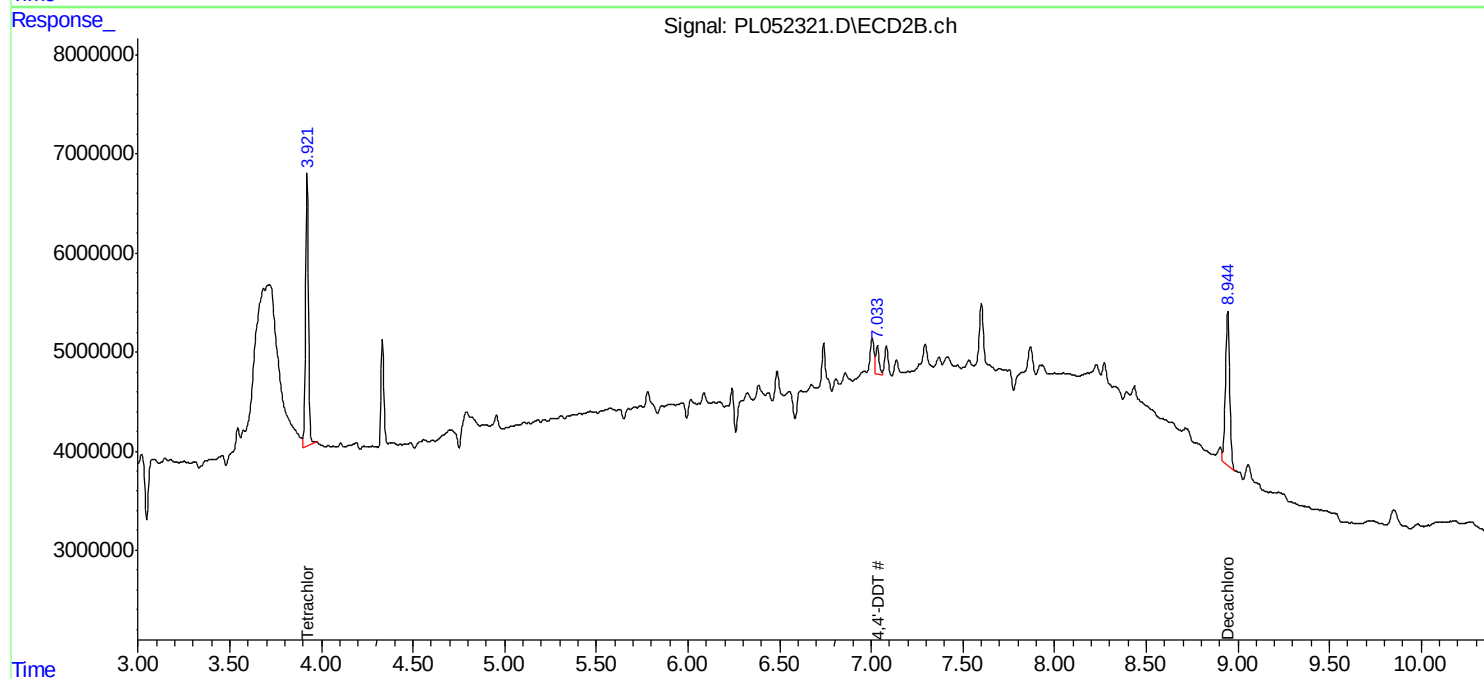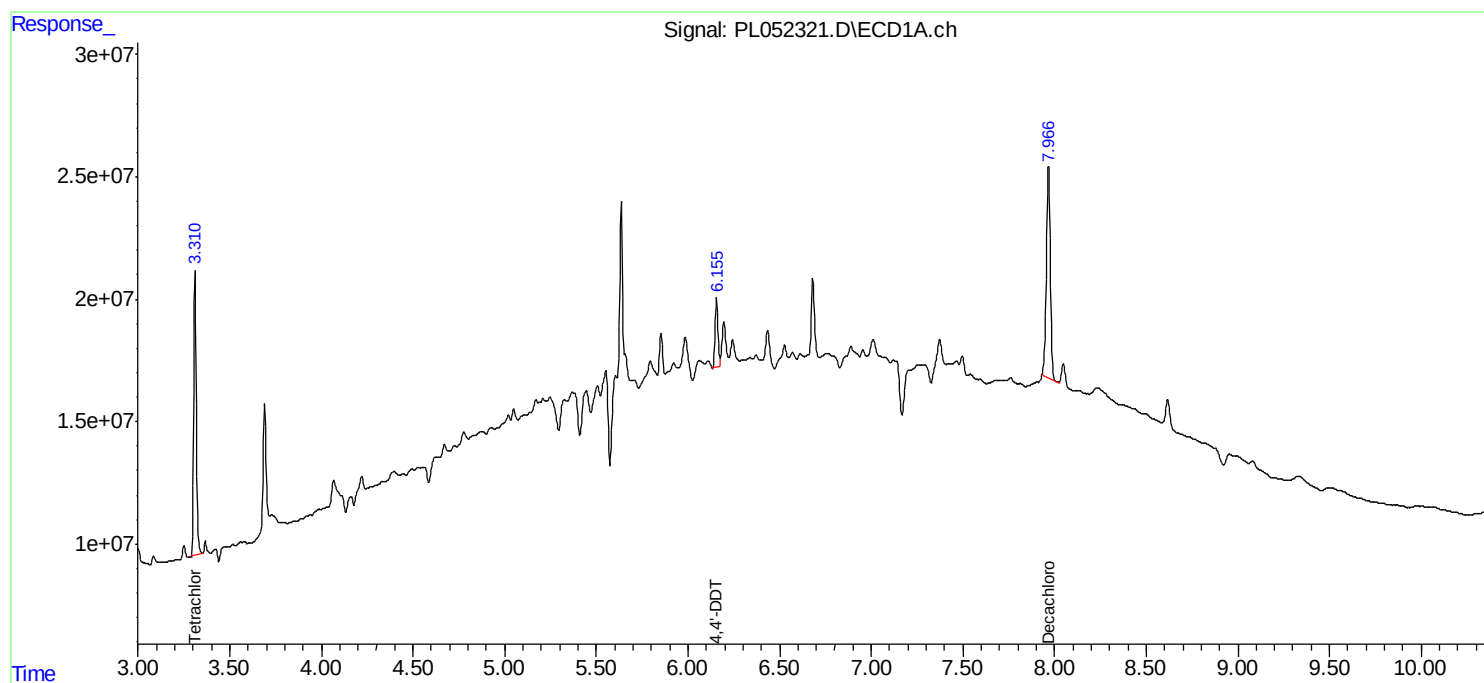

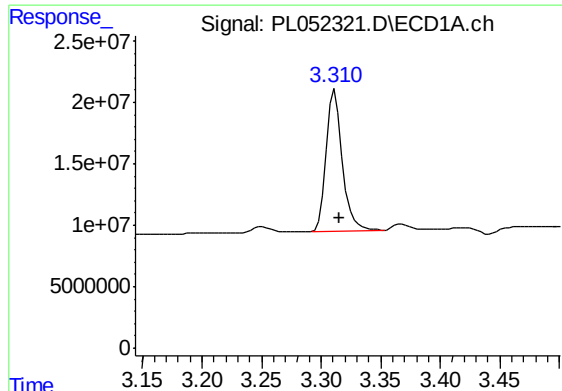


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.004 min
Response: 110027338
Conc: 12.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-1-3


Manual Integrations
APPROVED

Ankita
9/10/2019 11:17:29 AM

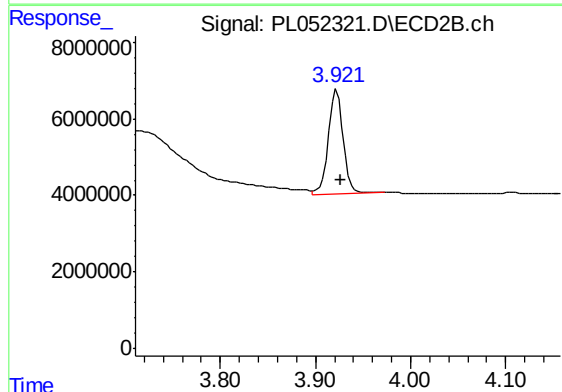


#1 Tetrachloro-m-xylene

R.T.: 3.922 min
Delta R.T.: -0.004 min
Response: 29282953
Conc: 13.40 ng/ml

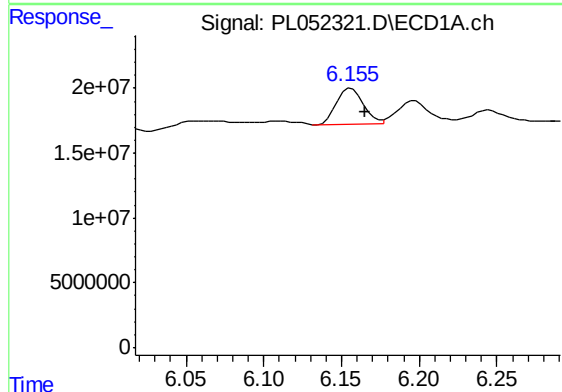


#17 4,4'-DDT

R.T.: 6.156 min
Delta R.T.: -0.008 min
Response: 34019247
Conc: 2.67 ng/ml

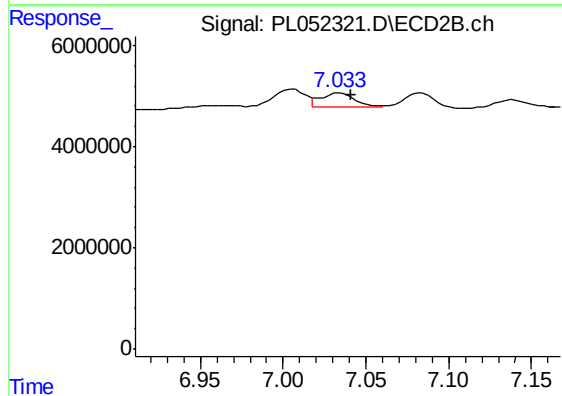

#17 4,4'-DDT

R.T.: 7.033 min
Delta R.T.: -0.008 min
Response: 4081749
Conc: 1.39 ng/ml m

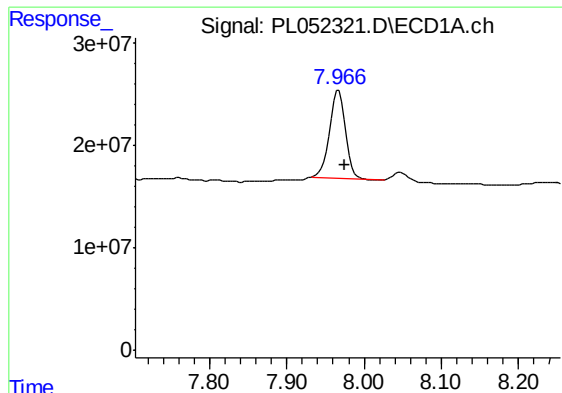


#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.007 min
Response: 123997965
Conc: 10.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-1-3

Manual Integrations
APPROVED

Ankita
9/10/2019 11:17:29 AM

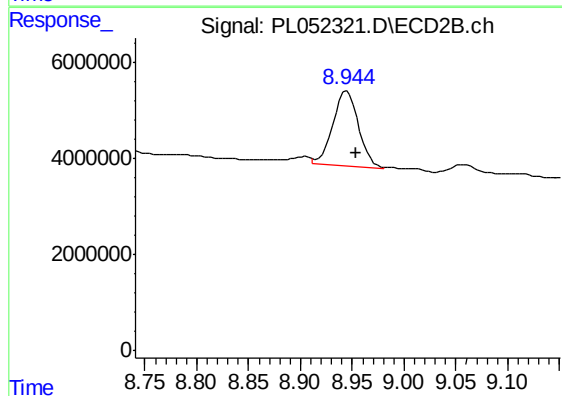

#28 Decachlorobiphenyl

R.T.: 8.944 min
Delta R.T.: -0.011 min
Response: 26562067
Conc: 8.73 ng/ml m