

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092225\
 Data File : PL097333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2025 19:20
 Operator : AR\AJ
 Sample : Q3065-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 01:48:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	2.825	73260928	111.6E6	16.183	16.968
28)	SA Decachlor...	9.000	7.983	51349548	80685272	15.693	14.176
Target Compounds							
8)	B Heptachlo...	5.651	4.793	53872486	47185246	9.374	5.949 #
9)	A Endosulfan I	0.000	5.175	0	414.7E6	N.D.	53.974 #
10)	B gamma-Chl...	5.905	5.043	9427462	18311682	1.668	2.097 #
12)	B 4,4'-DDE	6.134f	5.306	260.7E6	18397346	54.711	2.394 #
17)	MA 4,4'-DDT	6.976	6.119f	38109078	536.2E6	9.015	77.483 #
18)	B Endrin al...	0.000	6.170	0	24421072	N.D.	4.575 #
23)	Chlordane-1	4.696	3.824	14048708	23605880	66.288	92.880 #
25)	Chlordane-3	5.905	5.043	9427462	18311682	11.558	20.478 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092225\
Data File : PL097333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2025 19:20
Operator : AR\AJ
Sample : Q3065-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 01:48:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

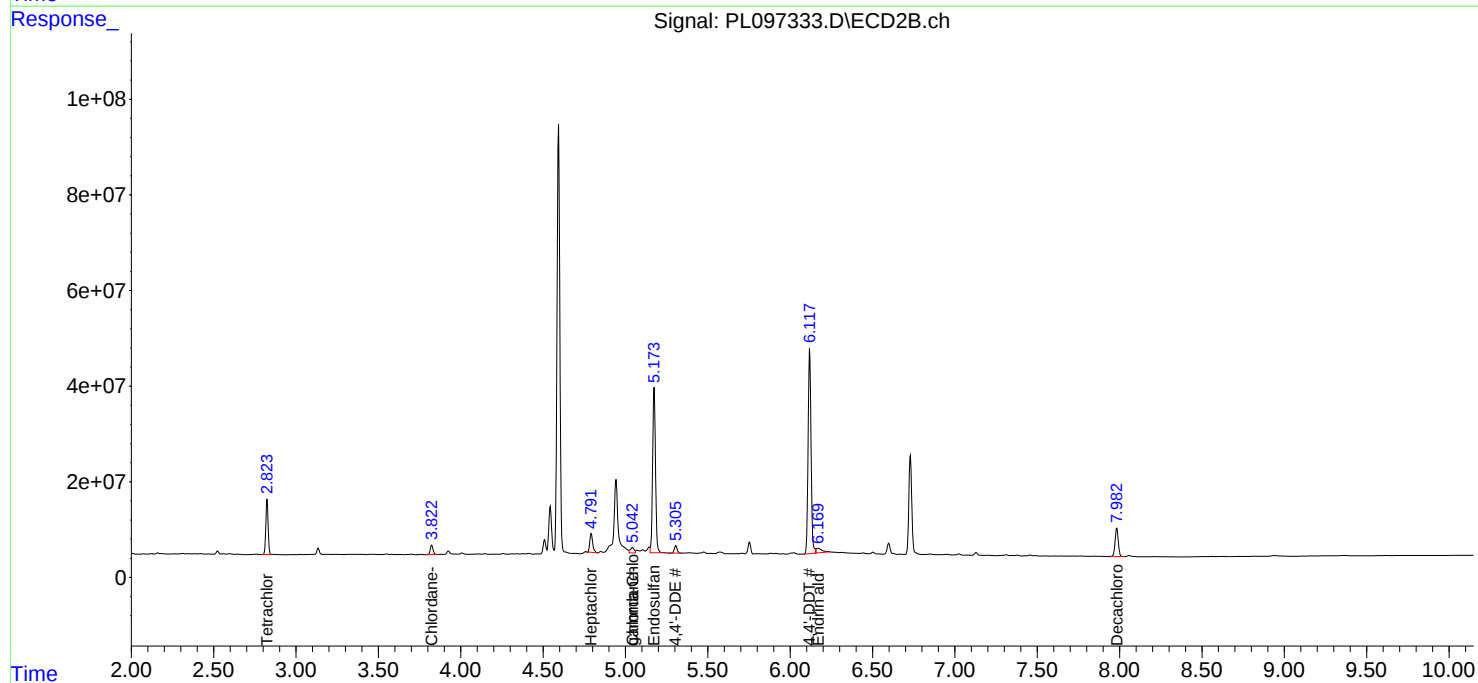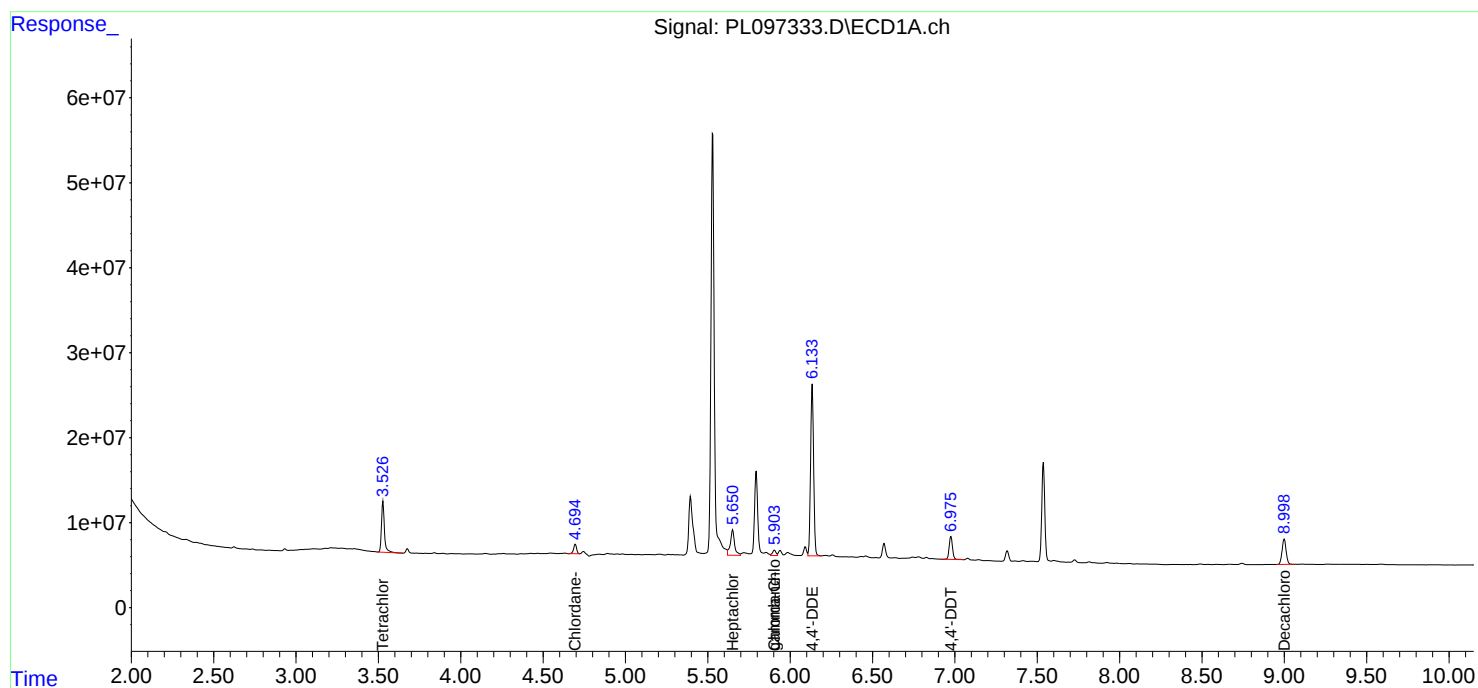


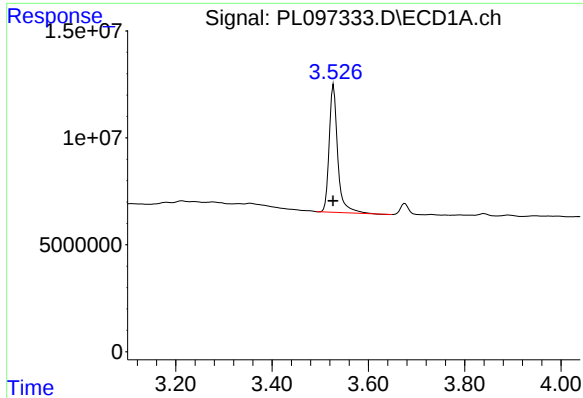

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 73260928
Conc: 16.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

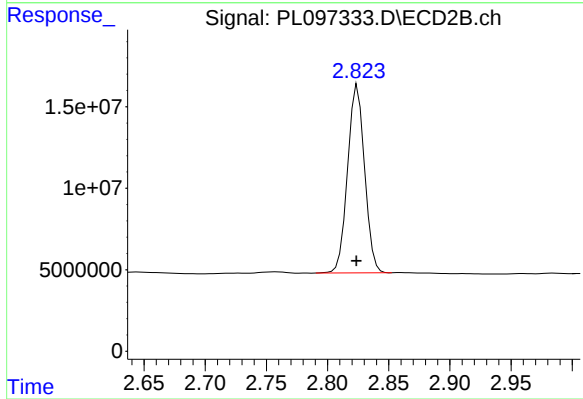


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: 0.001 min
Response: 111575510
Conc: 16.97 ng/ml

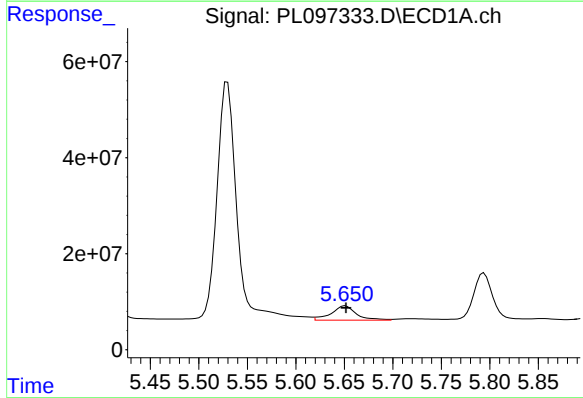


#8 Heptachlor epoxide

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 53872486
Conc: 9.37 ng/ml

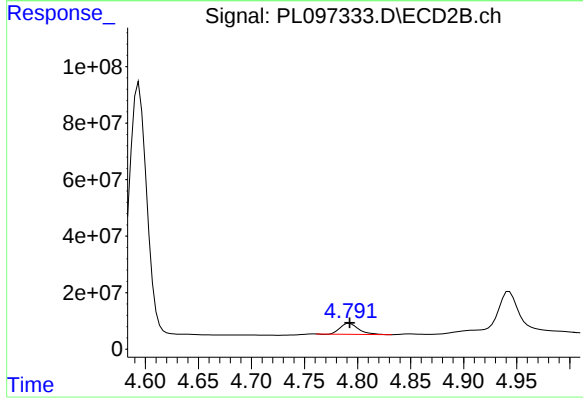

#8 Heptachlor epoxide


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 47185246
Conc: 5.95 ng/ml

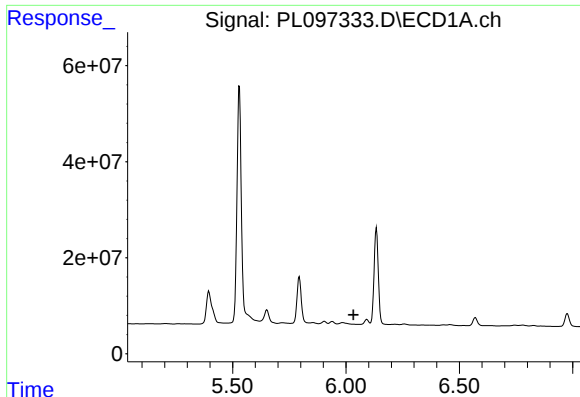

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

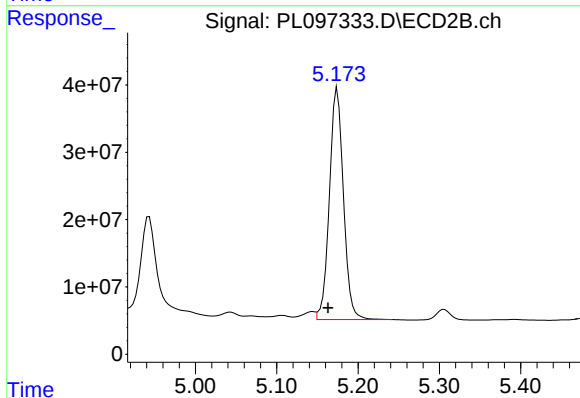


#9 Endosulfan I

R.T.: 5.175 min
Delta R.T.: 0.012 min
Response: 414716519
Conc: 53.97 ng/ml

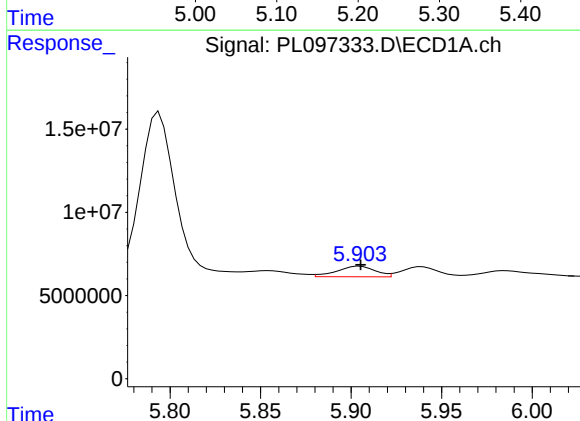


#10 gamma-Chlordane

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 9427462
Conc: 1.67 ng/ml

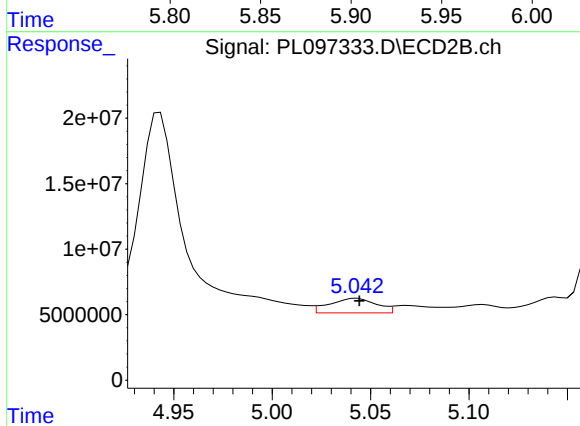

#10 gamma-Chlordane


R.T.: 5.043 min
Delta R.T.: -0.001 min
Response: 18311682
Conc: 2.10 ng/ml

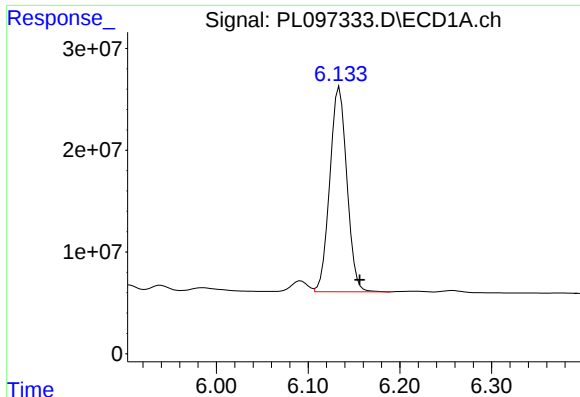

#12 4,4'-DDE


R.T.: 6.134 min
Delta R.T.: -0.022 min
Response: 260680312
Conc: 54.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

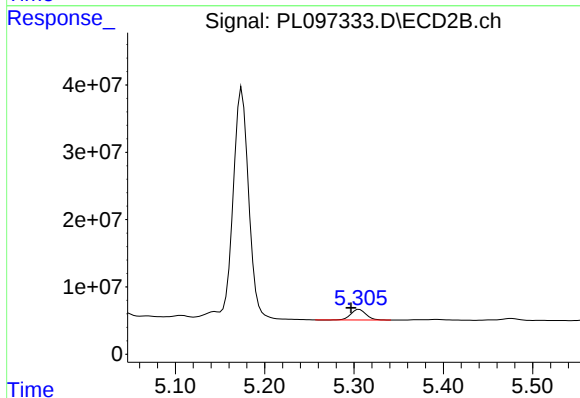


#12 4,4'-DDE

R.T.: 5.306 min
Delta R.T.: 0.009 min
Response: 18397346
Conc: 2.39 ng/ml

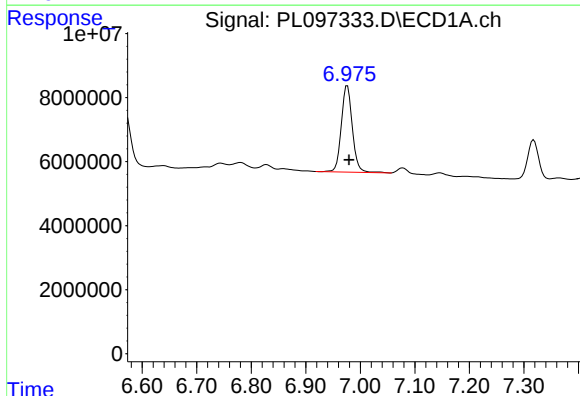


#17 4,4'-DDT

R.T.: 6.976 min
Delta R.T.: -0.003 min
Response: 38109078
Conc: 9.02 ng/ml

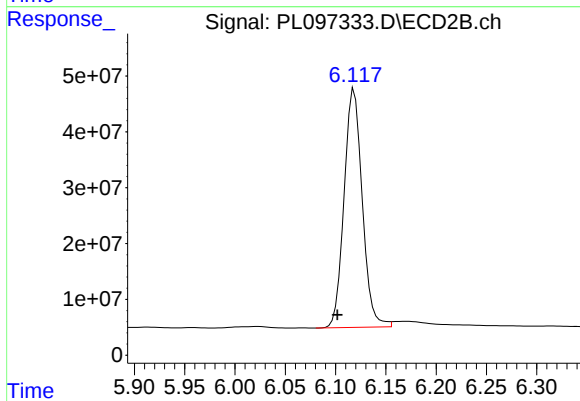

#17 4,4'-DDT


R.T.: 6.119 min
Delta R.T.: 0.017 min
Response: 536221228
Conc: 77.48 ng/ml

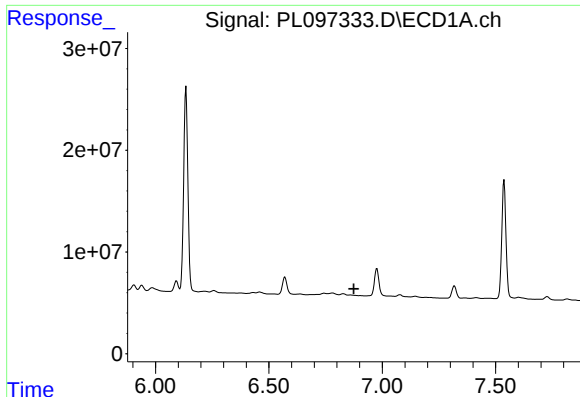

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

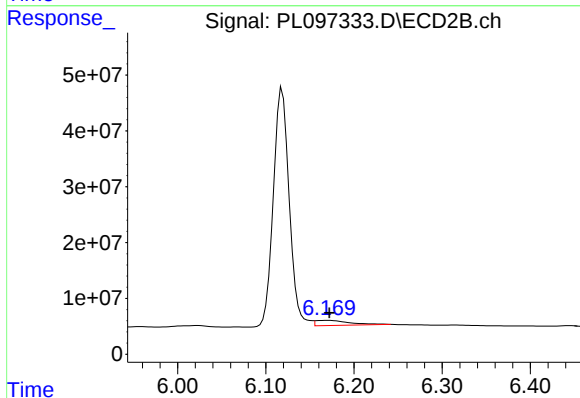


#18 Endrin aldehyde

R.T.: 6.170 min
Delta R.T.: -0.002 min
Response: 24421072
Conc: 4.58 ng/ml

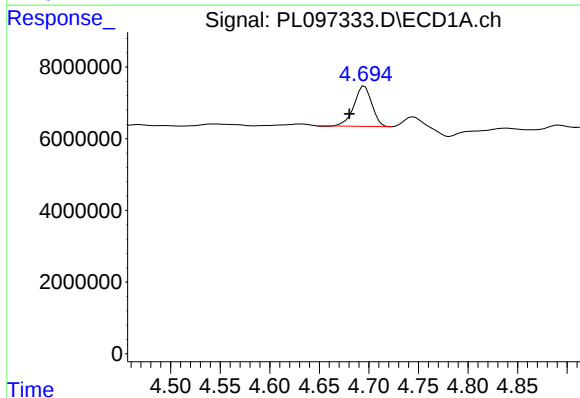


#23 Chlordane-1

R.T.: 4.696 min
Delta R.T.: 0.015 min
Response: 14048708
Conc: 66.29 ng/ml

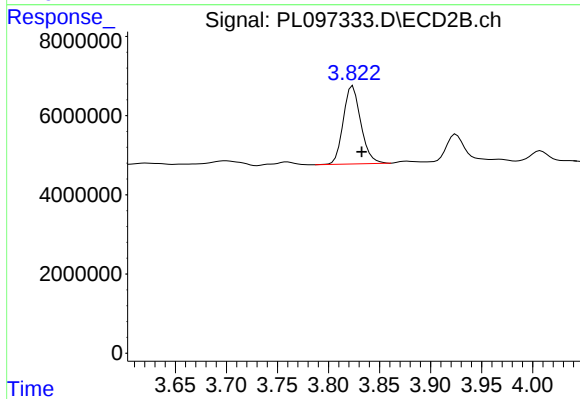

#23 Chlordane-1


R.T.: 3.824 min
Delta R.T.: -0.009 min
Response: 23605880
Conc: 92.88 ng/ml

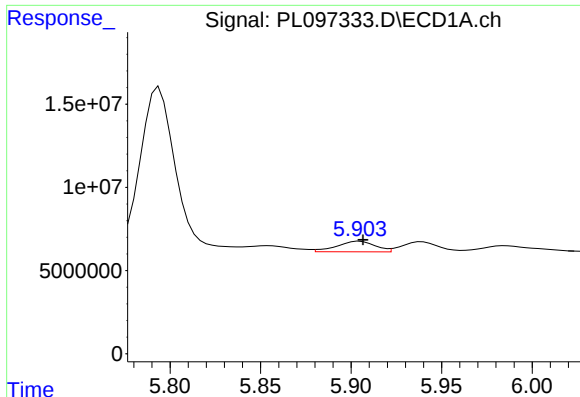

#25 Chlordane-3


R.T.: 5.905 min
Delta R.T.: -0.002 min
Response: 9427462
Conc: 11.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

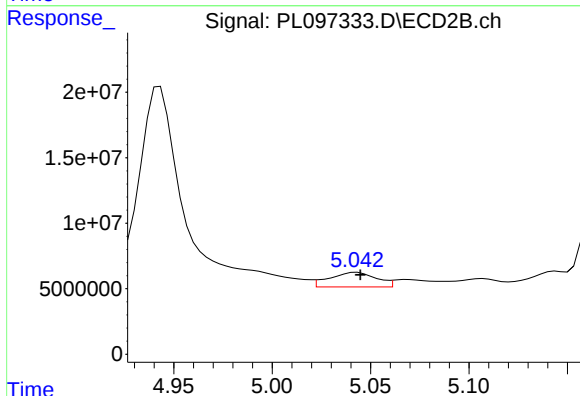


#25 Chlordane-3

R.T.: 5.043 min
Delta R.T.: -0.002 min
Response: 18311682
Conc: 20.48 ng/ml

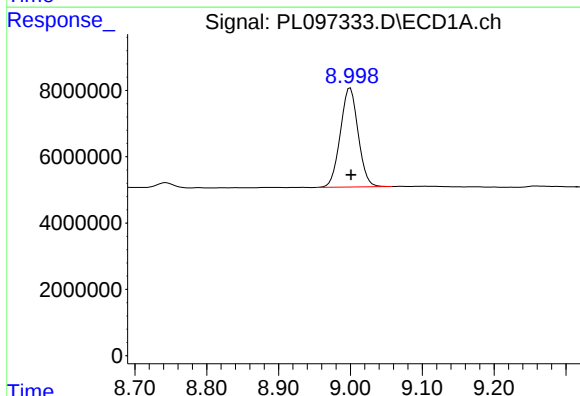

#28 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: 0.000 min
Response: 51349548
Conc: 15.69 ng/ml

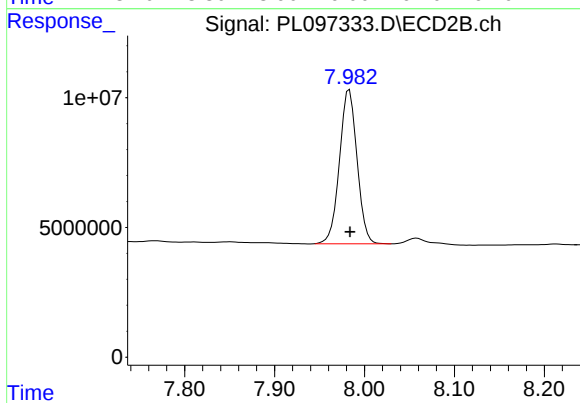

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: 0.000 min
Response: 80685272
Conc: 14.18 ng/ml