

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092225\
 Data File : PL097352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2025 00:05
 Operator : AR\AJ
 Sample : Q3155-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 01:50:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	2.825	51417330	73041005	11.358	11.108
28)	SA Decachlor...	9.000	7.983	37797116	58412252	11.551	10.263
Target Compounds							
9)	A Endosulfan I	0.000	5.176	0	16075726	N.D.	2.092 #
10)	B gamma-Chl...	5.905	5.045	31315190	35397194	5.539	4.053 #
11)	B alpha-Chl...	5.989	5.107	35948783	44414488	6.329	5.351
12)	B 4,4'-DDE	6.156	5.297	235.7E6	394.2E6	49.470	51.300
13)	MA Dieldrin	0.000	5.428	0	13809973	N.D.	1.689 #
14)	MA Endrin	0.000	5.713	0	20444645	N.D.	2.722 #
16)	A 4,4'-DDD	6.665	5.849	20804940	22397075	5.518	3.473 #
17)	MA 4,4'-DDT	6.978	6.101	87183723	130.5E6	20.624	18.861
18)	B Endrin al...	0.000	6.165	0	5335451	N.D.	1.000 #
20)	A Methoxychlor	0.000	6.653f	0	5337751	N.D.	1.416 #
25)	Chlordane-3	5.905	5.045	31315190	35397194	38.393	39.585
26)	Chlordane-4	5.989	5.107	35948783	44414488	35.941	58.322 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092225\
Data File : PL097352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2025 00:05
Operator : AR\AJ
Sample : Q3155-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 01:50:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

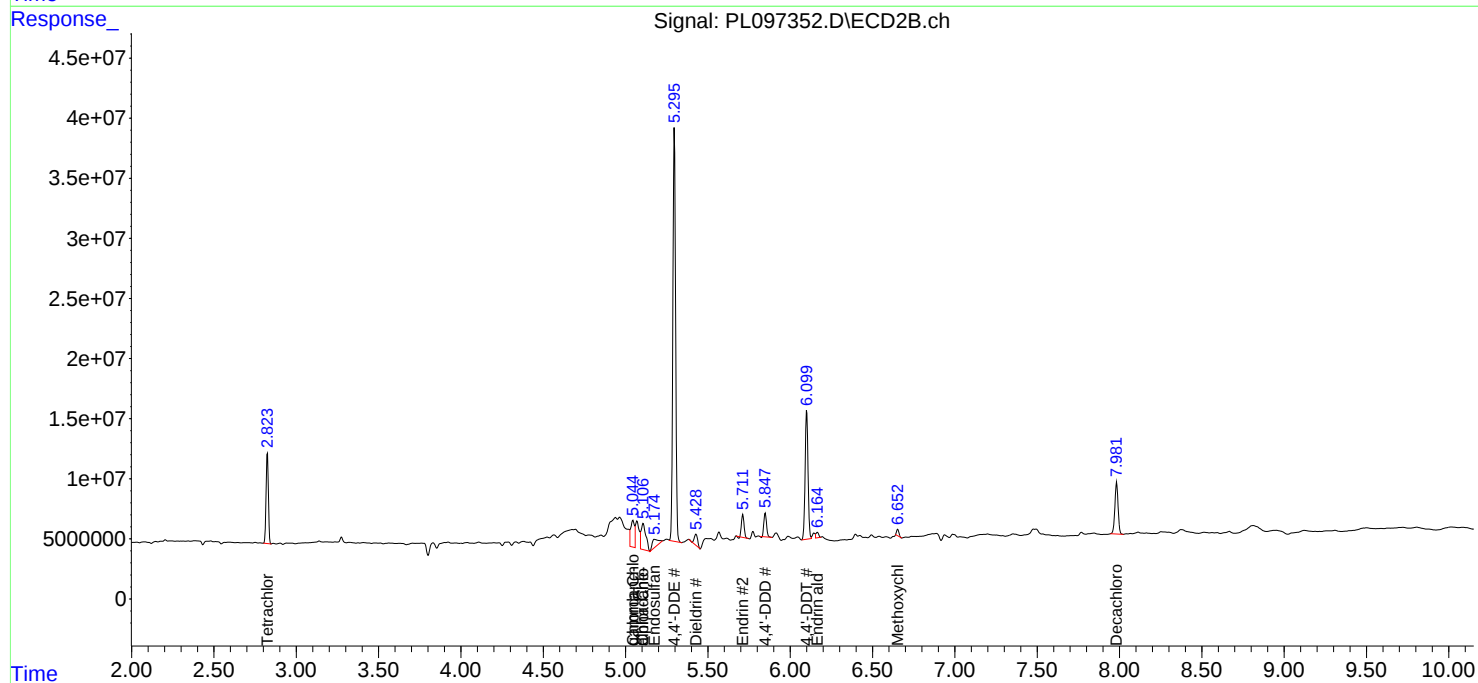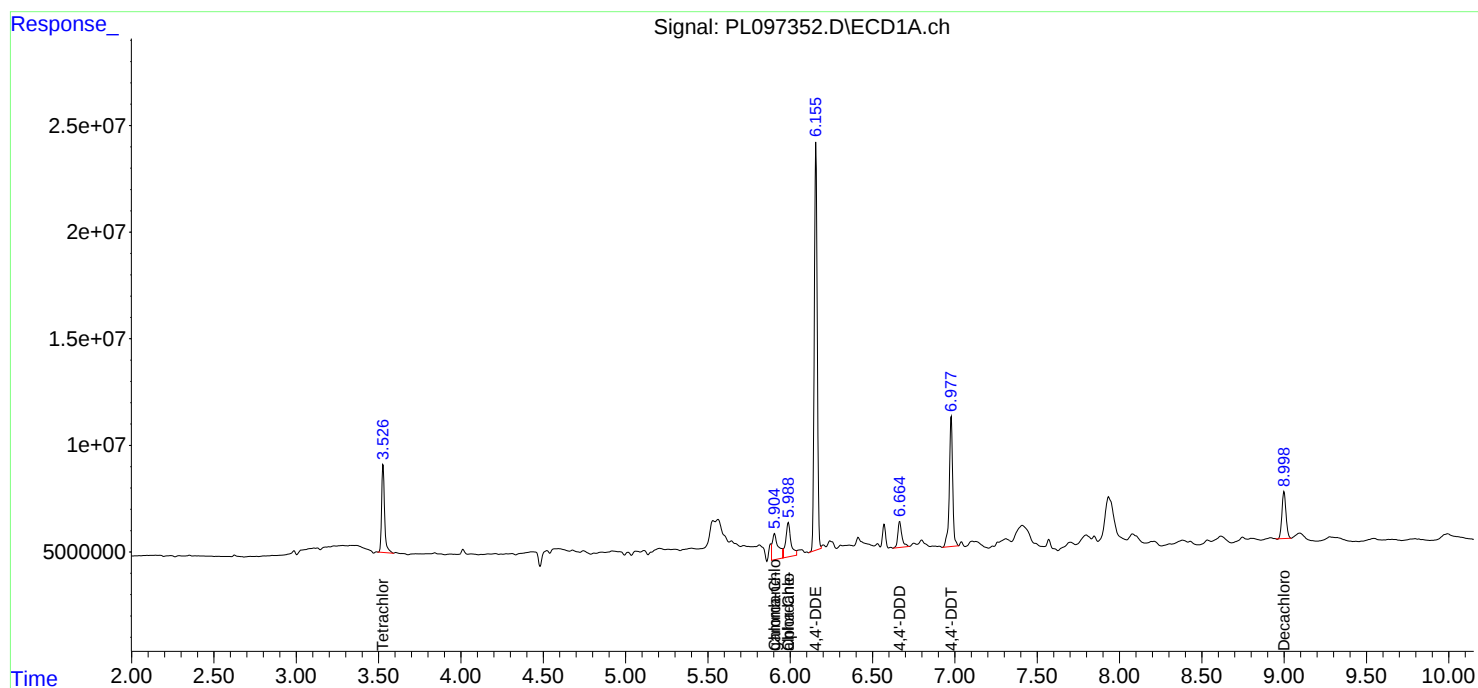


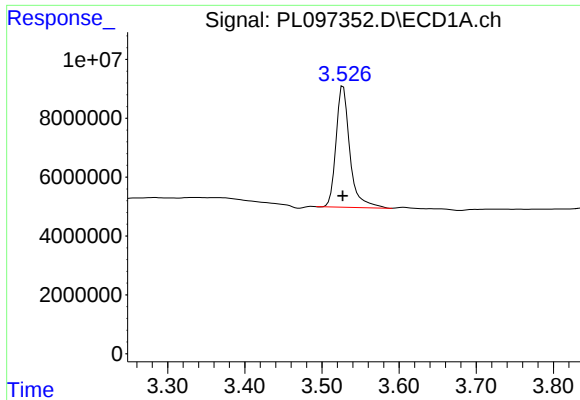

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 51417330
Conc: 11.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

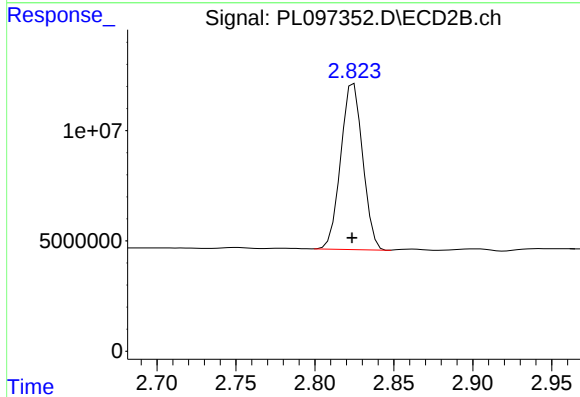


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: 0.001 min
Response: 73041005
Conc: 11.11 ng/ml

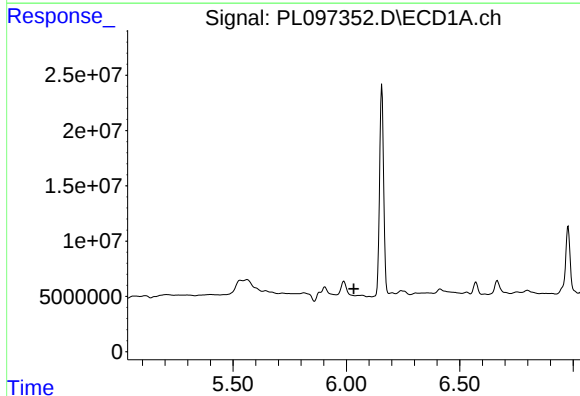


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

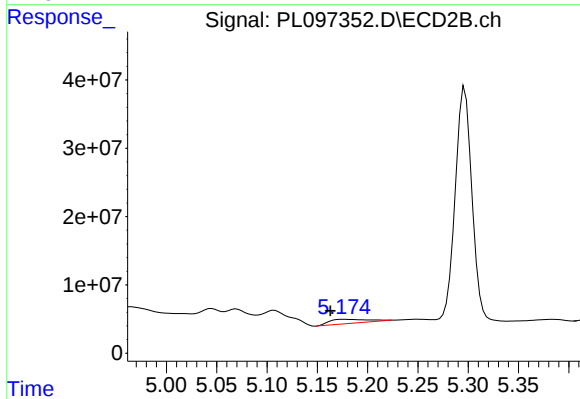

#9 Endosulfan I


R.T.: 5.176 min
Delta R.T.: 0.013 min
Response: 16075726
Conc: 2.09 ng/ml

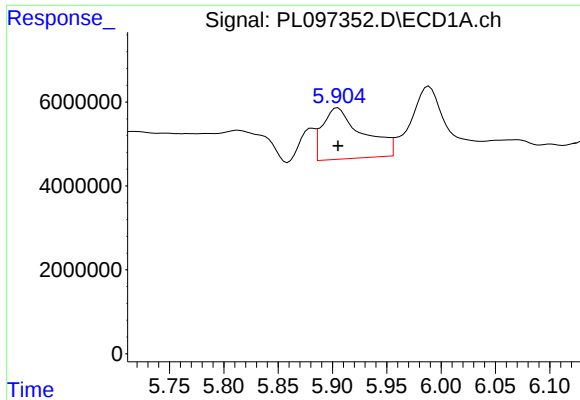

#10 gamma-Chlordane


R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 31315190
Conc: 5.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

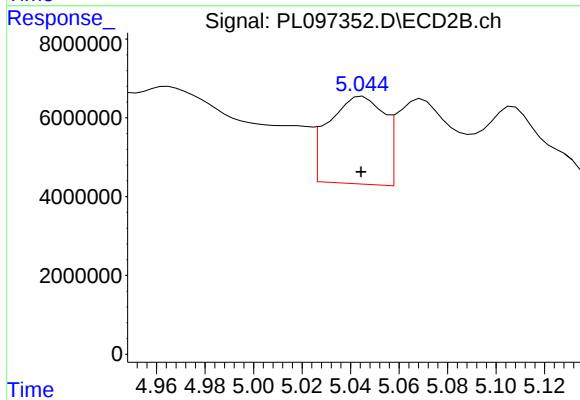


#10 gamma-Chlordane

R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 35397194
Conc: 4.05 ng/ml

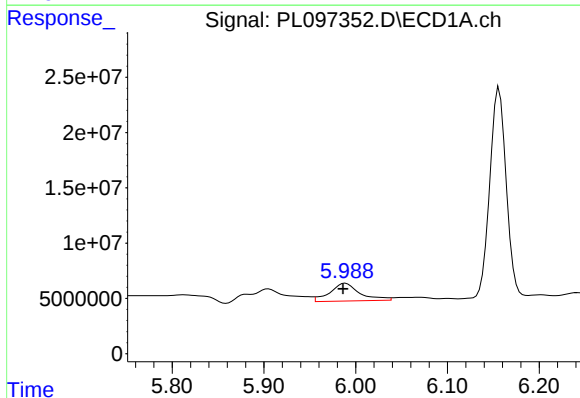


#11 alpha-Chlordane

R.T.: 5.989 min
Delta R.T.: 0.003 min
Response: 35948783
Conc: 6.33 ng/ml

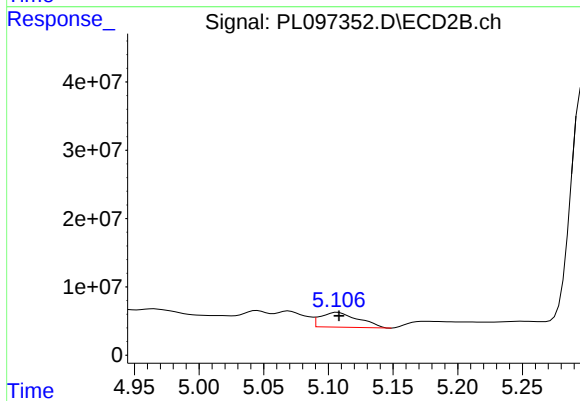

#11 alpha-Chlordane


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 44414488
Conc: 5.35 ng/ml

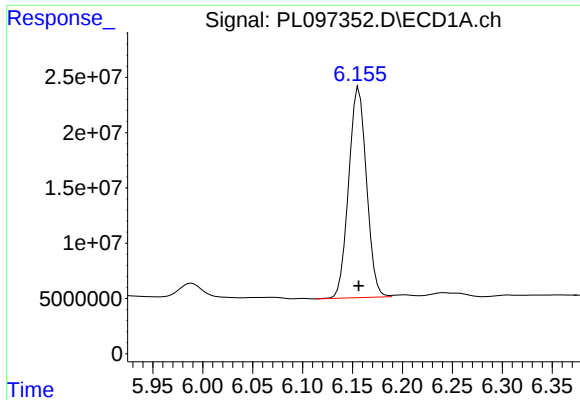

#12 4,4'-DDE


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 235708481
Conc: 49.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

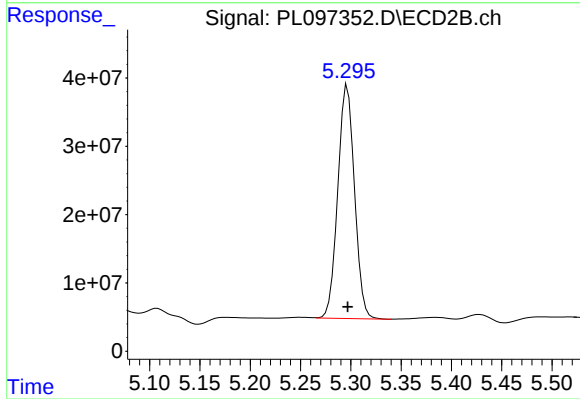


#12 4,4'-DDE

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 394225426
Conc: 51.30 ng/ml

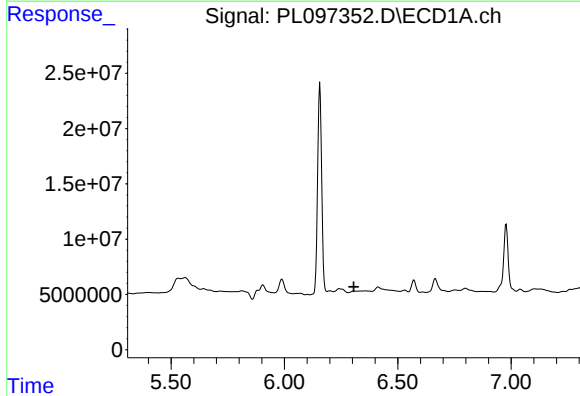


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

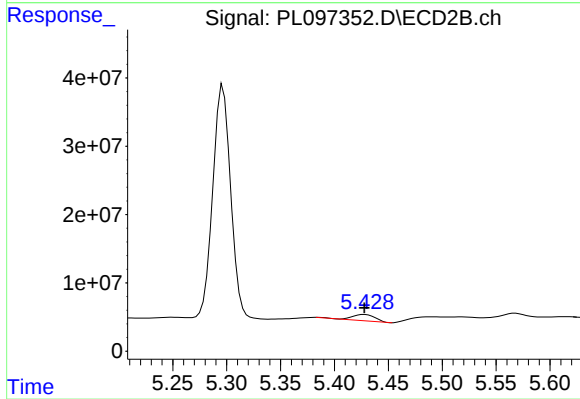

#13 Dieldrin


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 13809973
Conc: 1.69 ng/ml

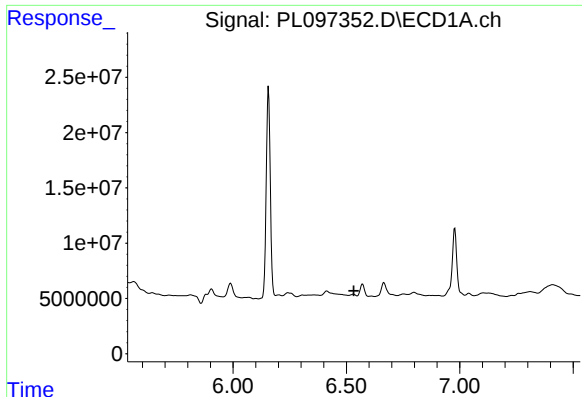

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

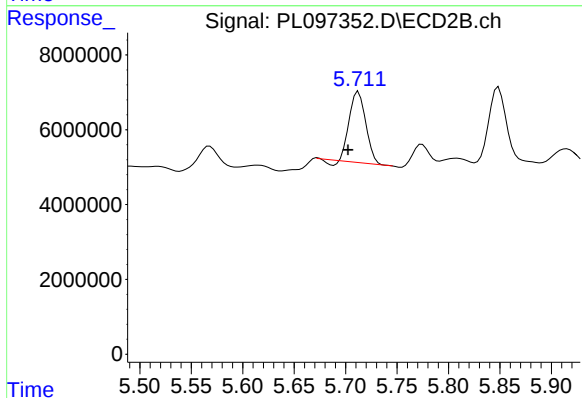


#14 Endrin

R.T.: 5.713 min
Delta R.T.: 0.010 min
Response: 20444645
Conc: 2.72 ng/ml

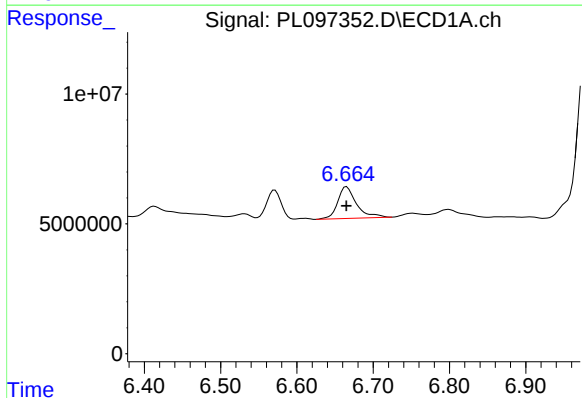


#16 4,4'-DDD

R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 20804940
Conc: 5.52 ng/ml

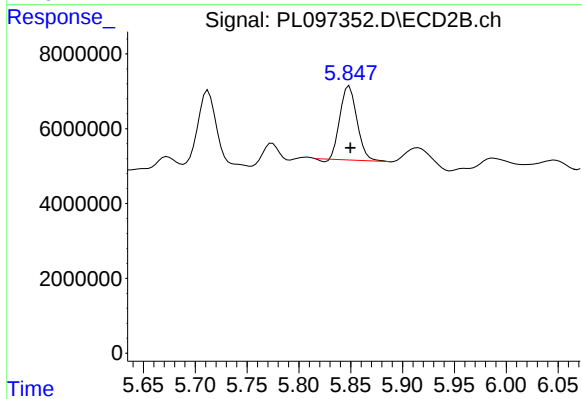

#16 4,4'-DDD


R.T.: 5.849 min
Delta R.T.: 0.000 min
Response: 22397075
Conc: 3.47 ng/ml

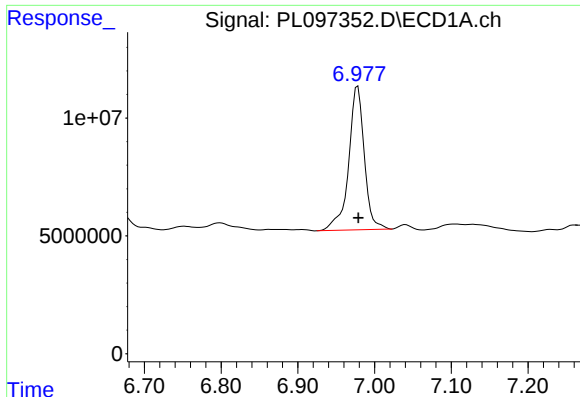

#17 4,4'-DDT


R.T.: 6.978 min
Delta R.T.: 0.000 min
Response: 87183723
Conc: 20.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

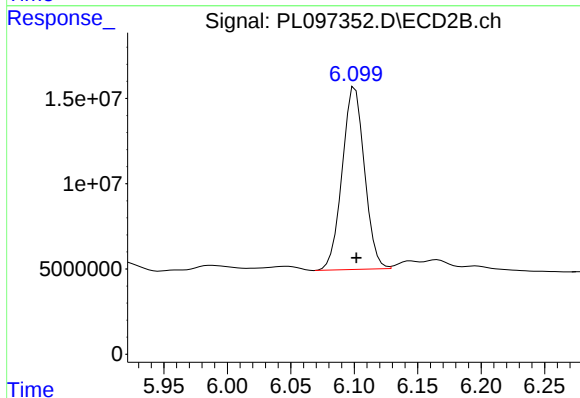


#17 4,4'-DDT

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 130524949
Conc: 18.86 ng/ml

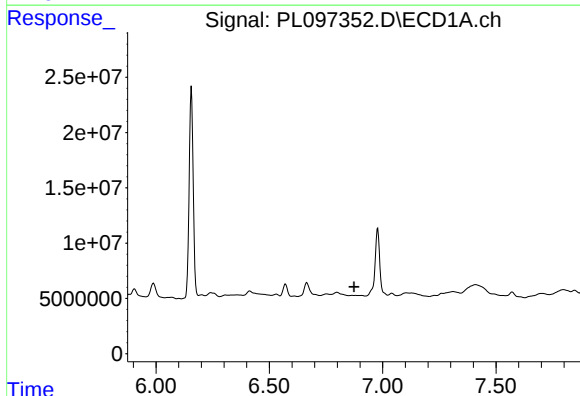


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.874 min
Response: 0
Conc: N.D.

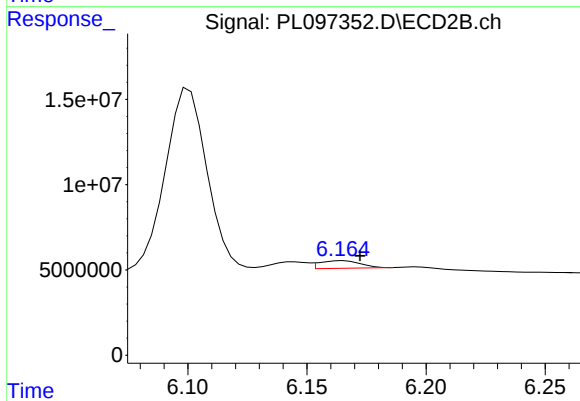

#18 Endrin aldehyde


R.T.: 6.165 min
Delta R.T.: -0.007 min
Response: 5335451
Conc: 1.00 ng/ml

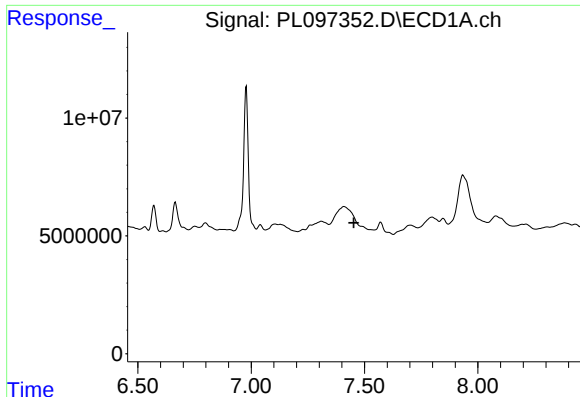

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

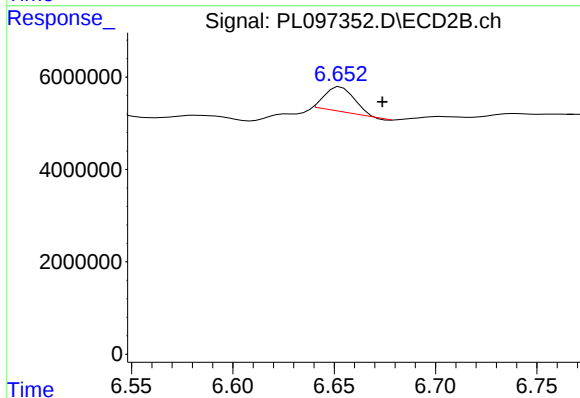


#20 Methoxychlor

R.T.: 6.653 min
Delta R.T.: -0.021 min
Response: 5337751
Conc: 1.42 ng/ml

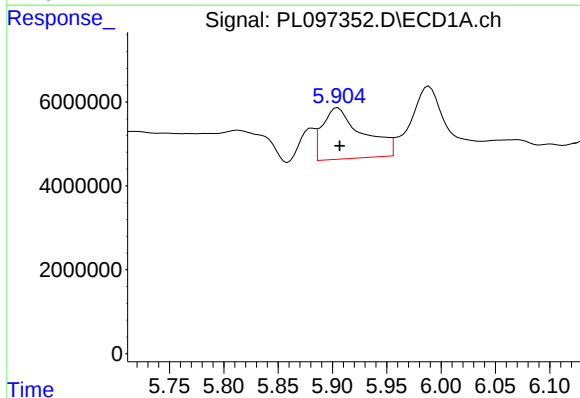


#25 Chlordane-3

R.T.: 5.905 min
Delta R.T.: -0.002 min
Response: 31315190
Conc: 38.39 ng/ml

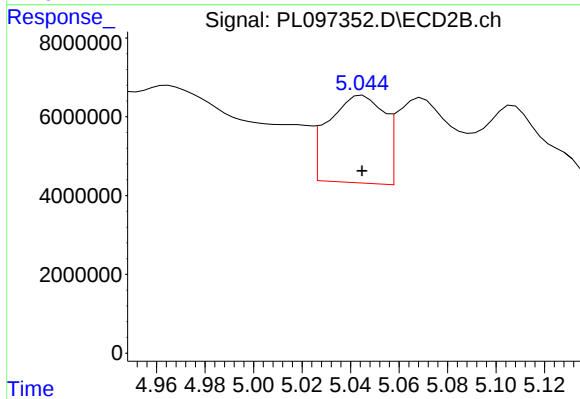

#25 Chlordane-3


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 35397194
Conc: 39.58 ng/ml

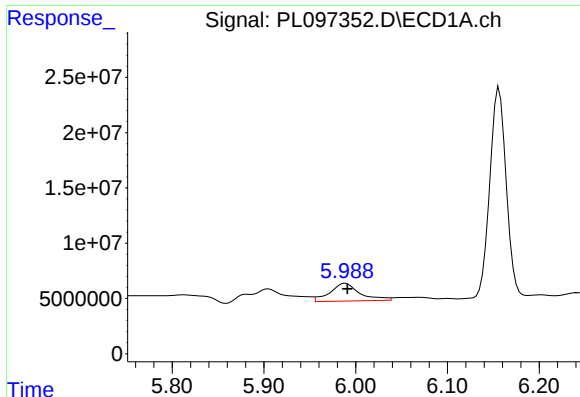

#26 Chlordane-4


R.T.: 5.989 min
Delta R.T.: -0.002 min
Response: 35948783
Conc: 35.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

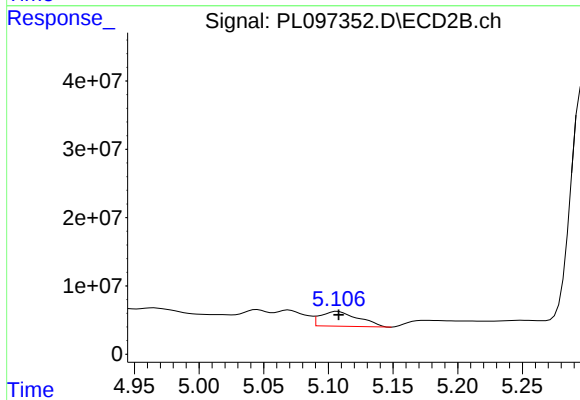


#26 Chlordane-4

R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 44414488
Conc: 58.32 ng/ml

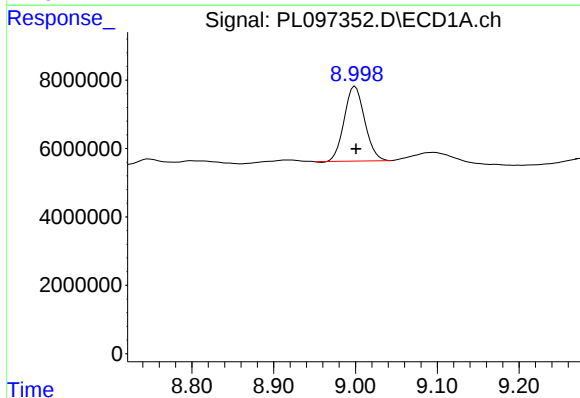

#28 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: -0.001 min
Response: 37797116
Conc: 11.55 ng/ml

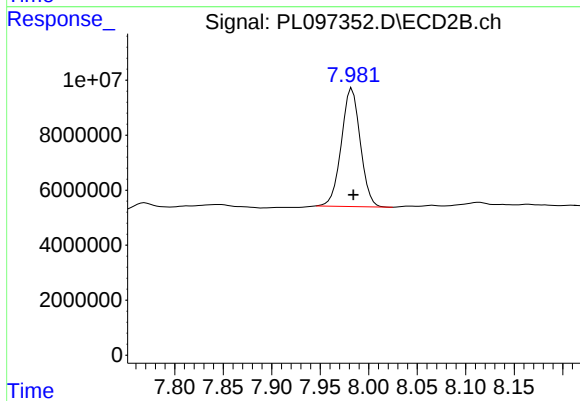

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.001 min
Response: 58412252
Conc: 10.26 ng/ml