

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092225\
 Data File : PL097353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2025 00:19
 Operator : AR\AJ
 Sample : Q3157-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 01:51:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.824	48703898	67319672	10.758	10.238
28)	SA Decachlor...	8.999	7.983	32744360	45492536	10.007	7.993
Target Compounds							
10)	B gamma-Chl...	5.905	5.044	24625259	38490412	4.356	4.407
11)	B alpha-Chl...	5.988	5.108	51334627	58157425	9.038	7.006
15)	B Endosulfa...	0.000	6.002	0	11932507	N.D.	1.678 #
23)	Chlordane-1	0.000	3.833	0	3432403	N.D.	13.505 #
24)	Chlordane-2	5.199	4.416	9896323	13737229	44.583	46.771
25)	Chlordane-3	5.905	5.044	24625259	38490412	30.191	43.044 #
26)	Chlordane-4	5.988	5.108	51334627	58157425	51.323	76.368 #
27)	Chlordane-5	6.826	6.002	7122422	11932507	42.488	40.023



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092225\
Data File : PL097353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2025 00:19
Operator : AR\AJ
Sample : Q3157-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 01:51:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

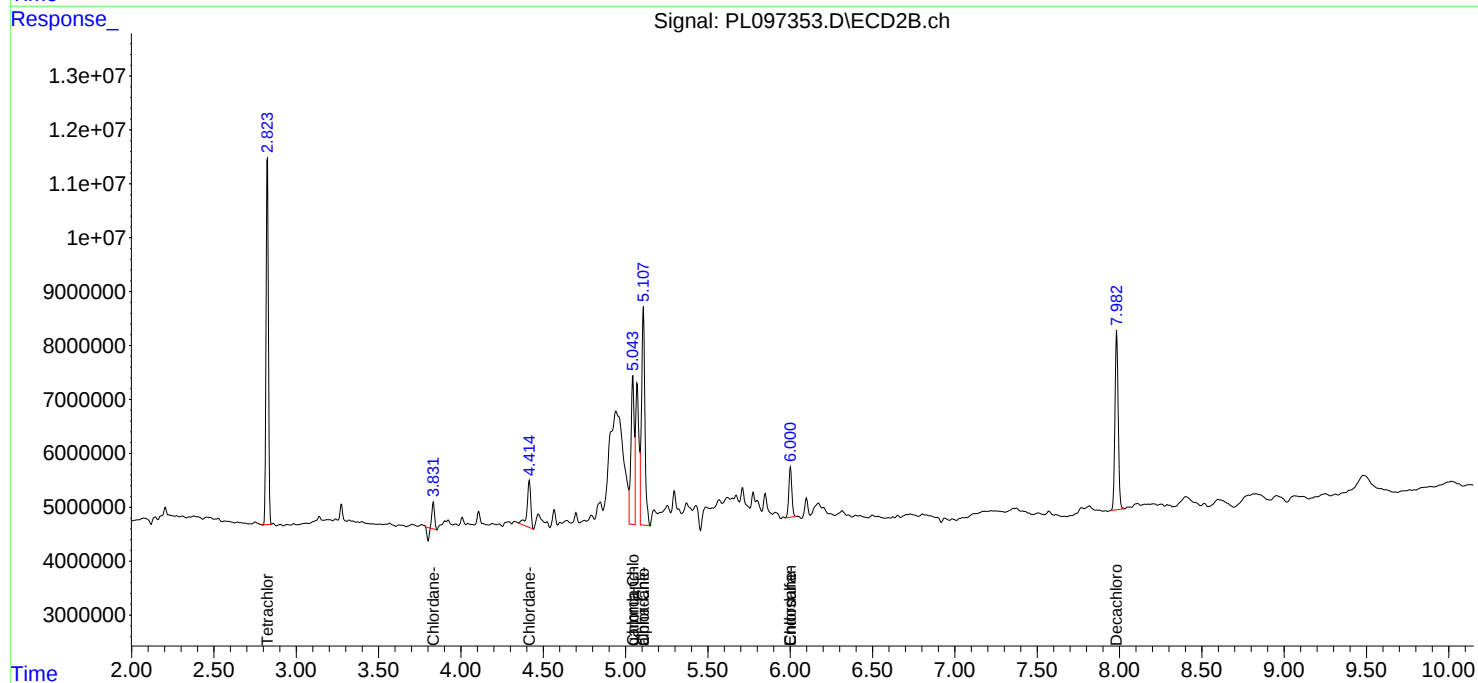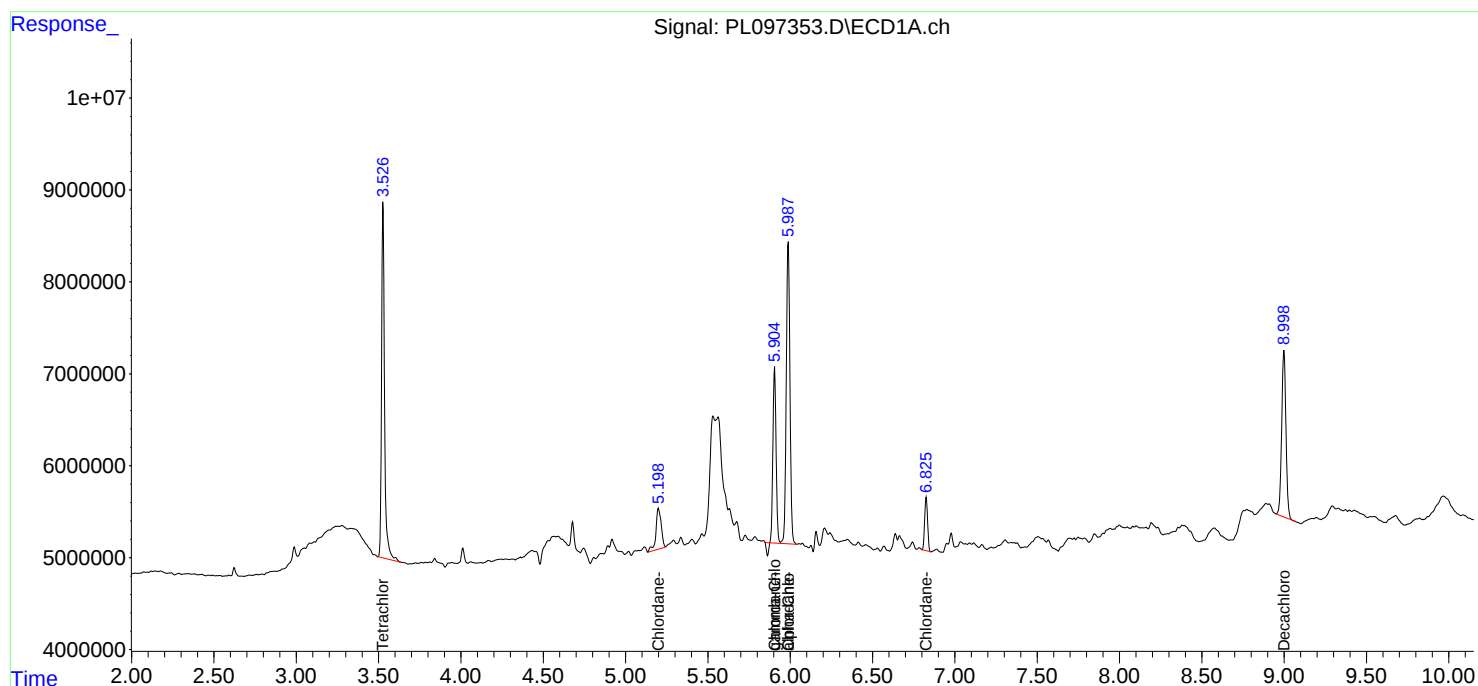


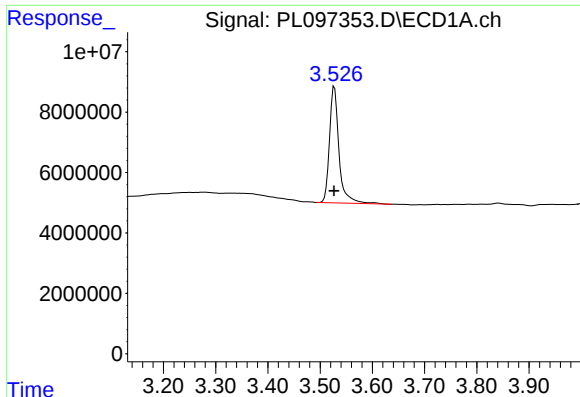

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 48703898
Conc: 10.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

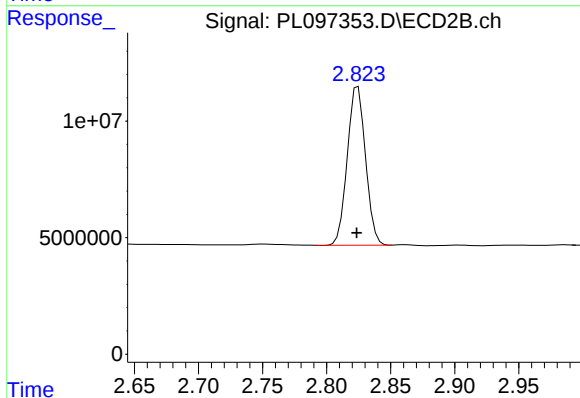


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.001 min
Response: 67319672
Conc: 10.24 ng/ml

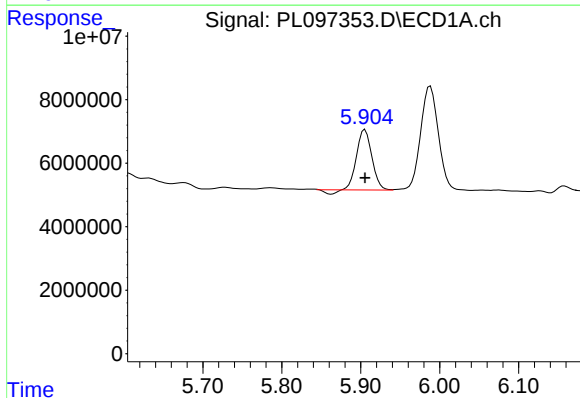


#10 gamma-Chlordane

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 24625259
Conc: 4.36 ng/ml

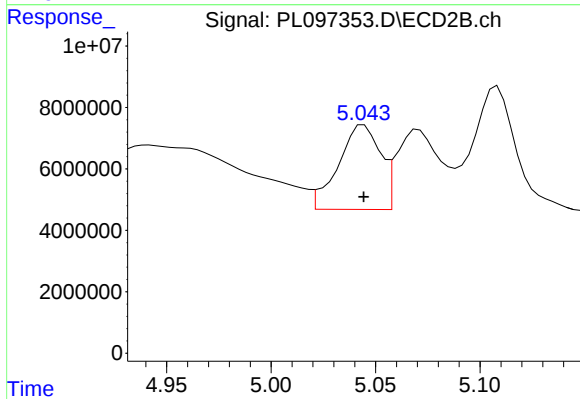

#10 gamma-Chlordane


R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 38490412
Conc: 4.41 ng/ml

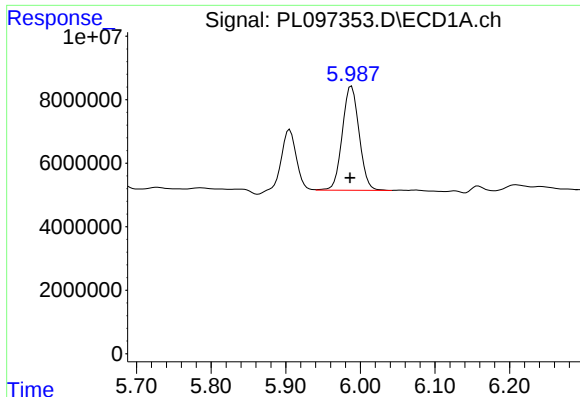

#11 alpha-Chlordane


R.T.: 5.988 min
Delta R.T.: 0.002 min
Response: 51334627
Conc: 9.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

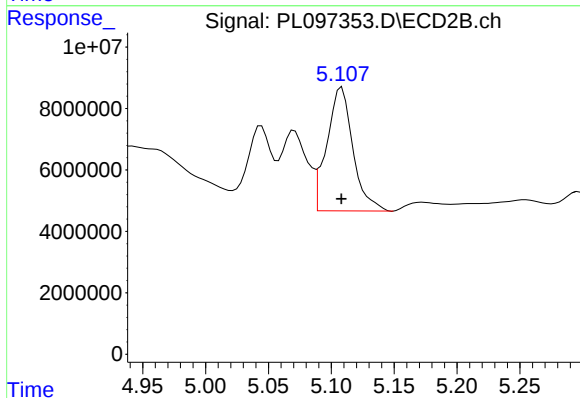


#11 alpha-Chlordane

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 58157425
Conc: 7.01 ng/ml

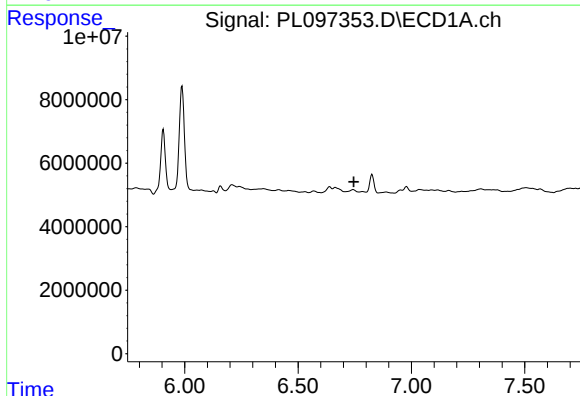


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.745 min
Response: 0
Conc: N.D.

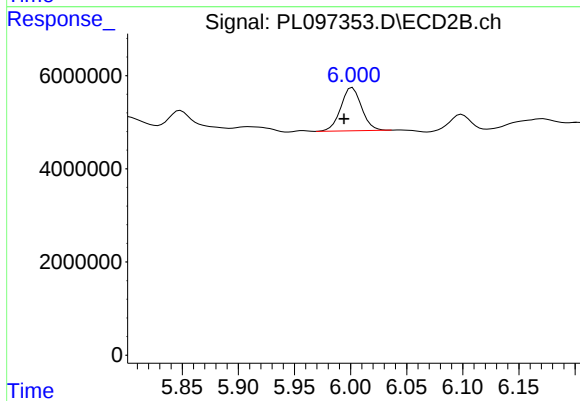

#15 Endosulfan II


R.T.: 6.002 min
Delta R.T.: 0.007 min
Response: 11932507
Conc: 1.68 ng/ml

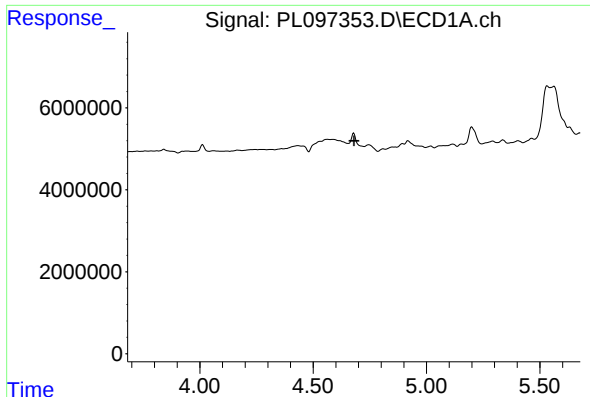

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

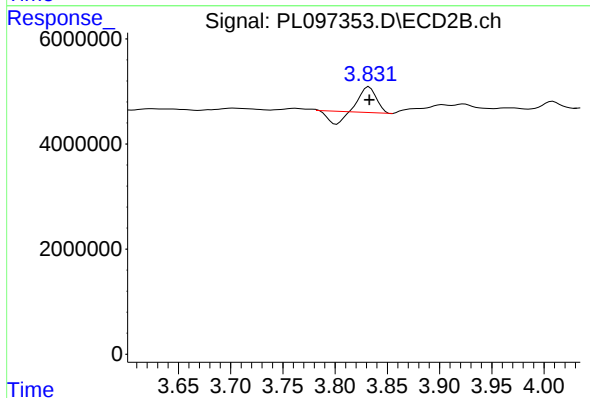


#23 Chlordane-1

R.T.: 3.833 min
Delta R.T.: 0.000 min
Response: 3432403
Conc: 13.51 ng/ml

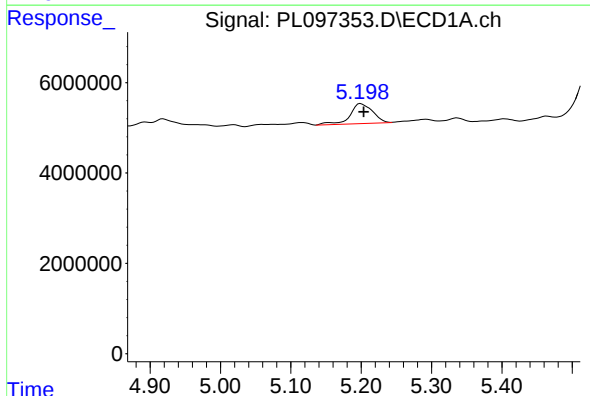


#24 Chlordane-2

R.T.: 5.199 min
Delta R.T.: -0.004 min
Response: 9896323
Conc: 44.58 ng/ml

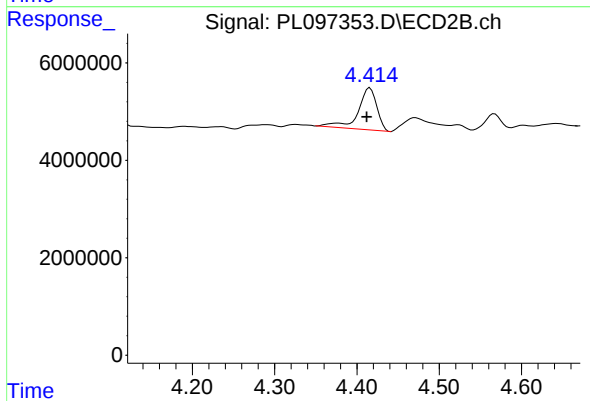

#24 Chlordane-2


R.T.: 4.416 min
Delta R.T.: 0.004 min
Response: 13737229
Conc: 46.77 ng/ml

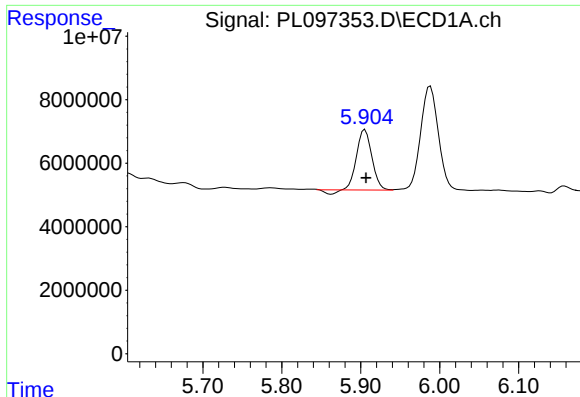

#25 Chlordane-3


R.T.: 5.905 min
Delta R.T.: -0.001 min
Response: 24625259
Conc: 30.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

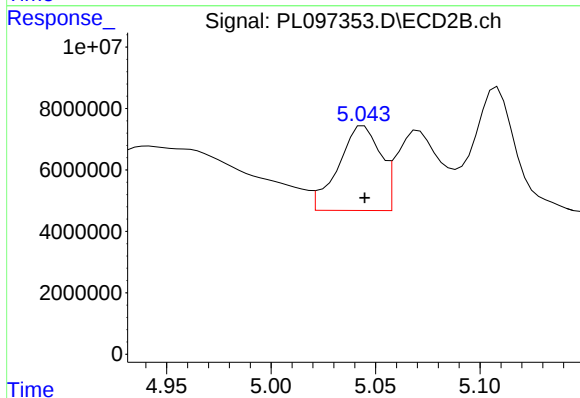


#25 Chlordane-3

R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 38490412
Conc: 43.04 ng/ml

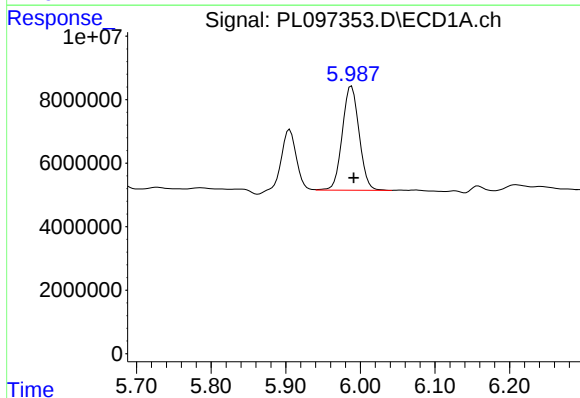


#26 Chlordane-4

R.T.: 5.988 min
Delta R.T.: -0.003 min
Response: 51334627
Conc: 51.32 ng/ml

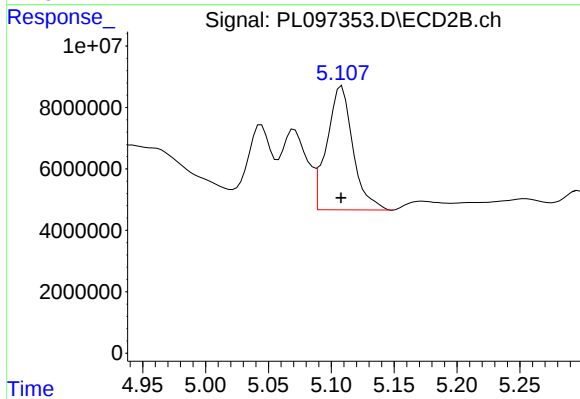

#26 Chlordane-4


R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 58157425
Conc: 76.37 ng/ml

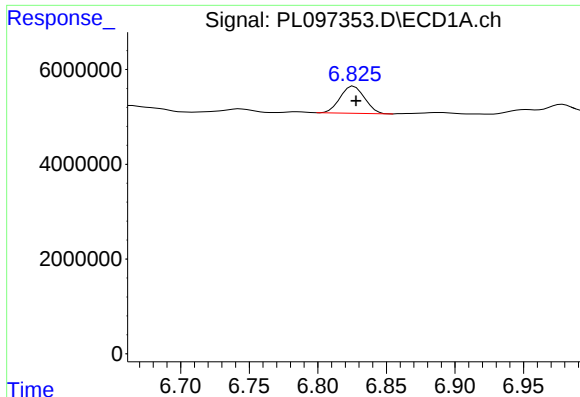

#27 Chlordane-5


R.T.: 6.826 min
Delta R.T.: -0.002 min
Response: 7122422
Conc: 42.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

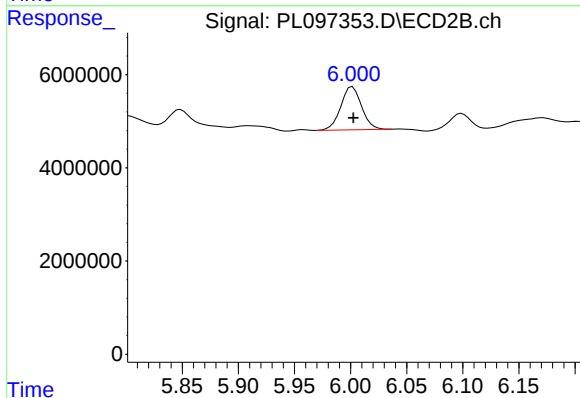


#27 Chlordane-5

R.T.: 6.002 min
Delta R.T.: 0.000 min
Response: 11932507
Conc: 40.02 ng/ml

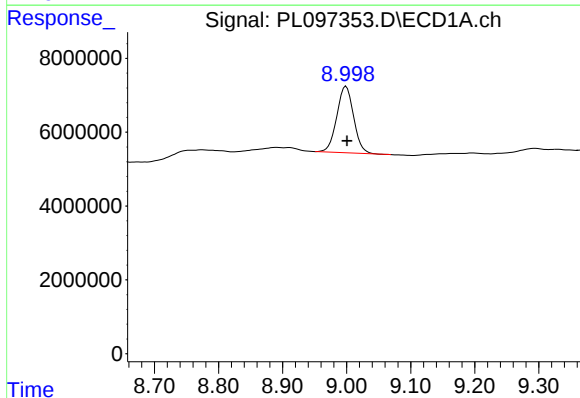

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.002 min
Response: 32744360
Conc: 10.01 ng/ml

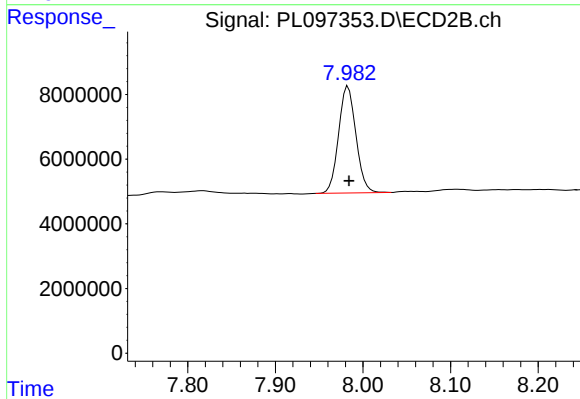

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.001 min
Response: 45492536
Conc: 7.99 ng/ml