

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
 Data File : PL062058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 13:26
 Operator : DD\AJ
 Sample : L4272-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 17:51:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	37654092	57815108	22.072	21.191
28)	SA Decachlor...	8.207	9.092	33183343	45689144	20.398	20.755
Target Compounds							
10)	B gamma-Chl...	5.418f	6.120	27645532	20324090	15.919	6.921 #
11)	B alpha-Chl...	5.453	6.196	8482535	45502787	4.883	15.150 #
14)	MA Endrin	0.000	6.739f	0	2144559	N.D.	0.879 #
15)	B Endosulfa...	0.000	6.942	0	3602451	N.D.	1.394 #
16)	A 4,4'-DDD	6.135	0.000	1055488	0	0.797	N.D. #
19)	B Endosulfa...	0.000	7.278	0	9616395	N.D.	4.107 #
25)	Chlordane-3	5.418f	6.120	27645532	20324090	175.883	55.464 #
26)	Chlordane-4	5.453	6.196	8482535	45502787	65.014	101.361 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
Data File : PL062058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 13:26
Operator : DD\AJ
Sample : L4272-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 17:51:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

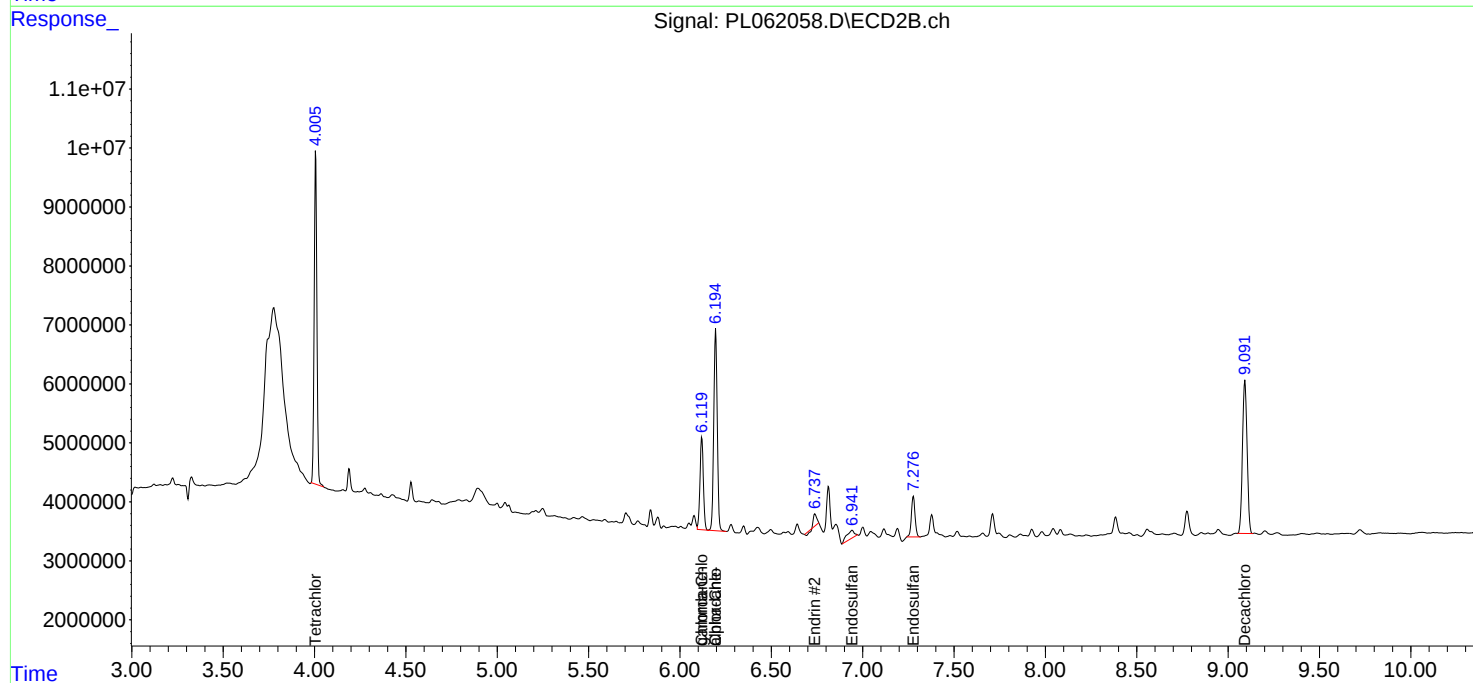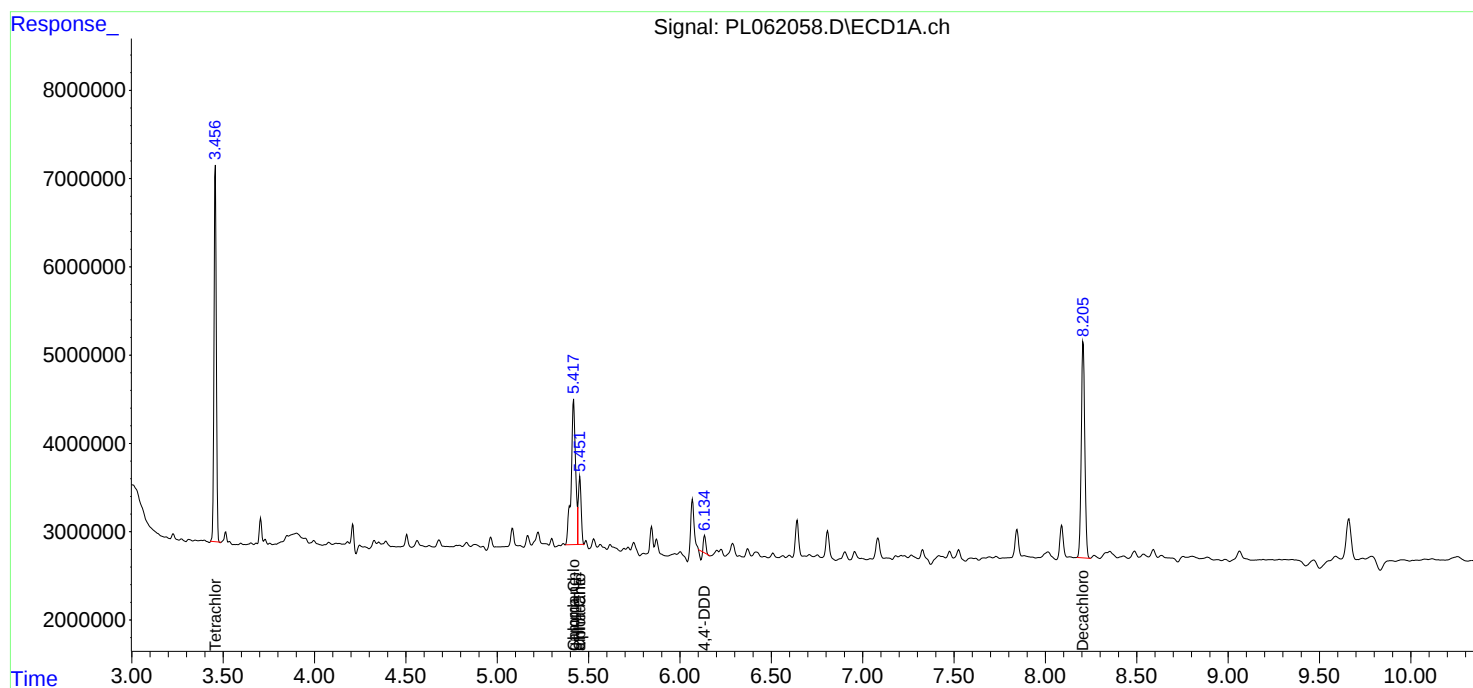


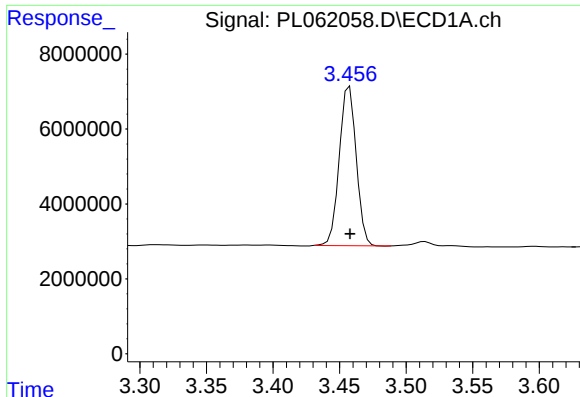

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 37654092
Conc: 22.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

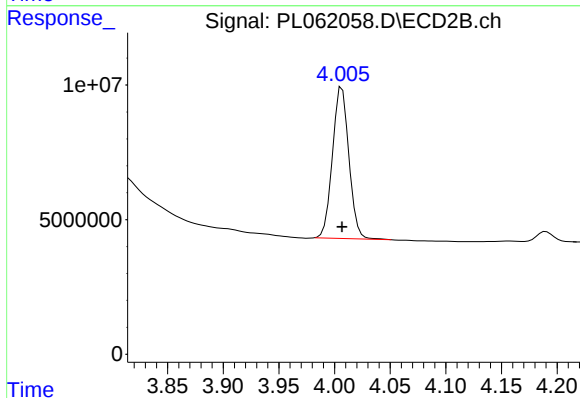


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 57815108
Conc: 21.19 ng/ml

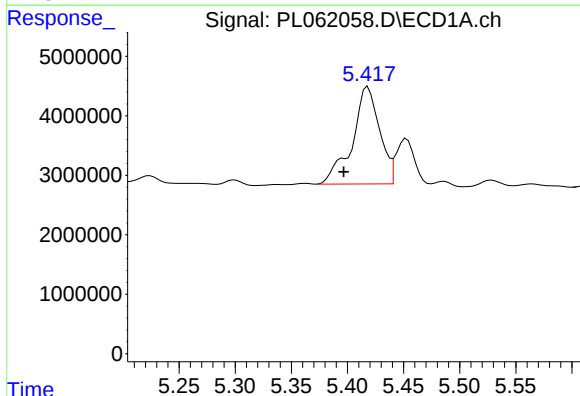


#10 gamma-Chlordane

R.T.: 5.418 min
Delta R.T.: 0.022 min
Response: 27645532
Conc: 15.92 ng/ml

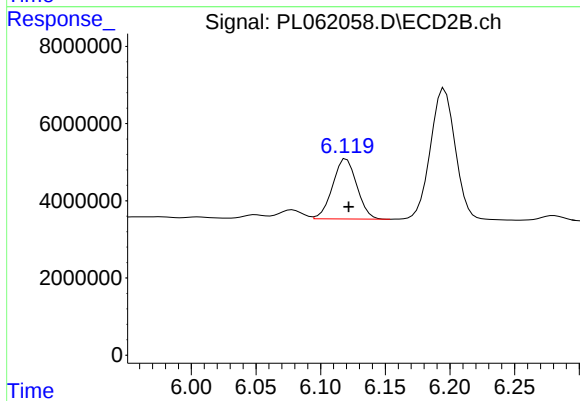

#10 gamma-Chlordane


R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 20324090
Conc: 6.92 ng/ml

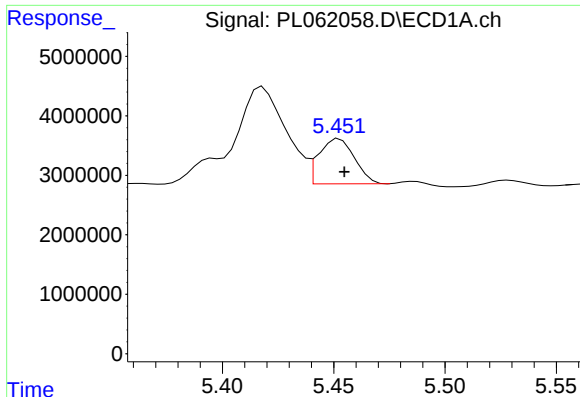

#11 alpha-Chlordane


R.T.: 5.453 min
Delta R.T.: -0.002 min
Response: 8482535
Conc: 4.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

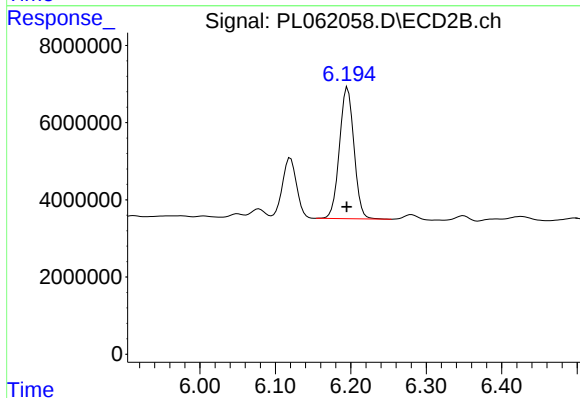


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.001 min
Response: 45502787
Conc: 15.15 ng/ml

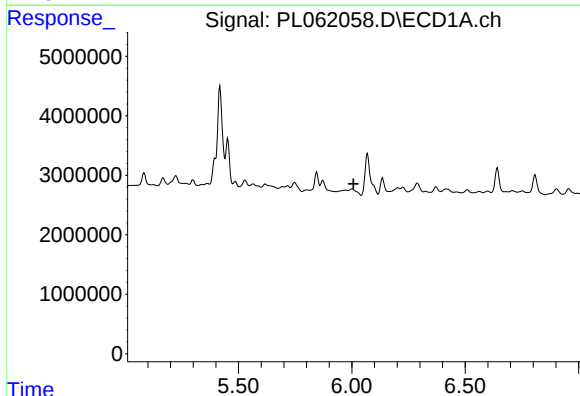


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.008 min
Response: 0
Conc: N.D.

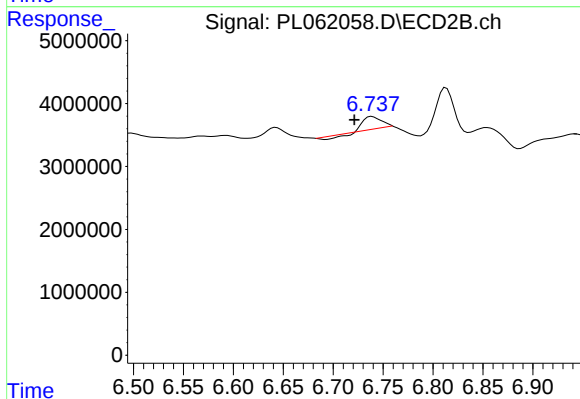

#14 Endrin


R.T.: 6.739 min
Delta R.T.: 0.018 min
Response: 2144559
Conc: 0.88 ng/ml

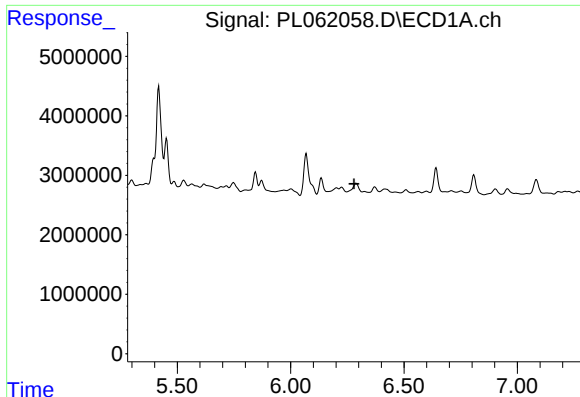

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

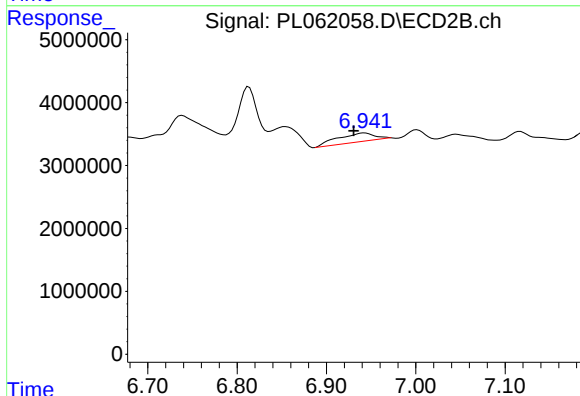


#15 Endosulfan II

R.T.: 6.942 min
Delta R.T.: 0.012 min
Response: 3602451
Conc: 1.39 ng/ml

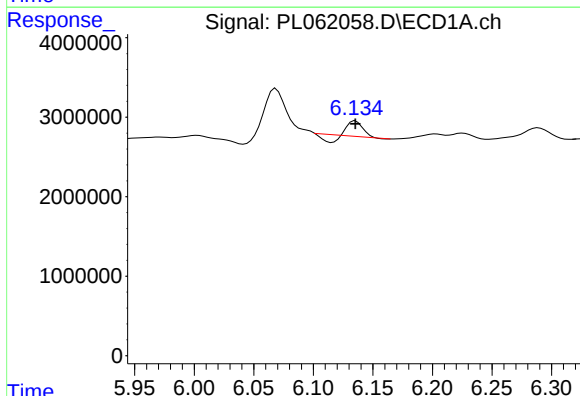


#16 4,4'-DDD

R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 1055488
Conc: 0.80 ng/ml

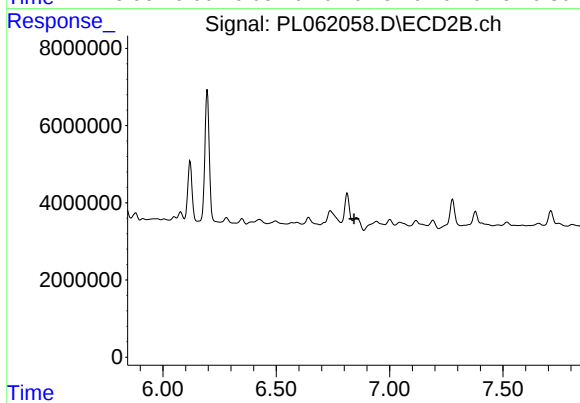

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.844 min
Response: 0
Conc: N.D.

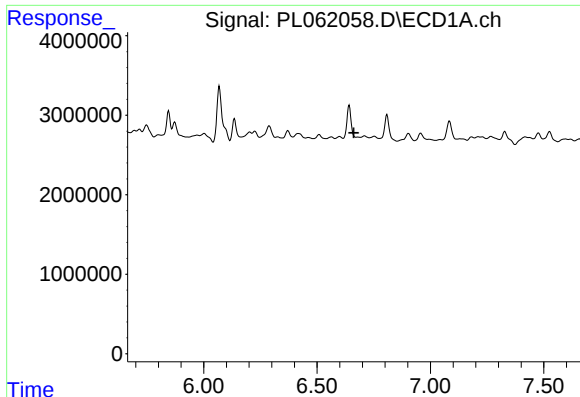

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

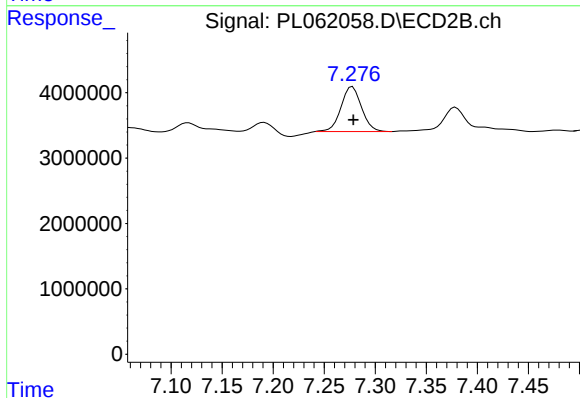


#19 Endosulfan Sulfate

R.T.: 7.278 min
Delta R.T.: 0.000 min
Response: 9616395
Conc: 4.11 ng/ml

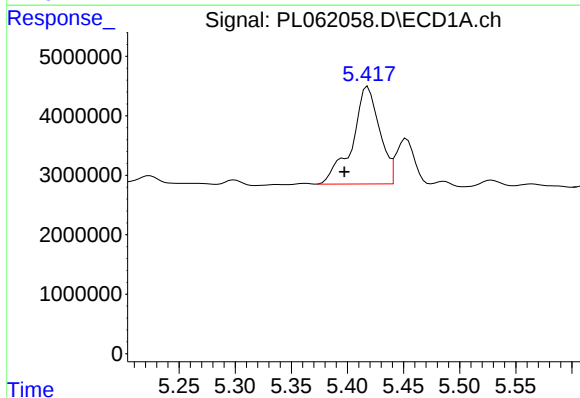


#25 Chlordane-3

R.T.: 5.418 min
Delta R.T.: 0.021 min
Response: 27645532
Conc: 175.88 ng/ml

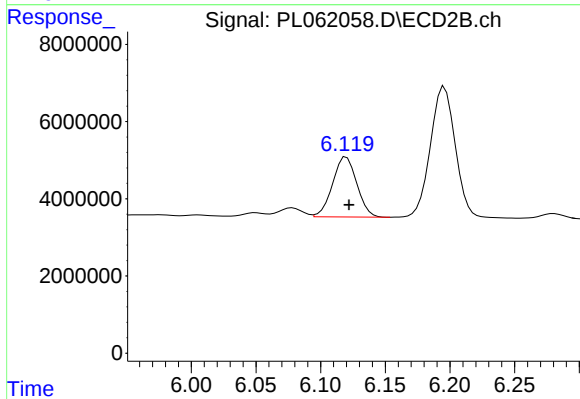

#25 Chlordane-3


R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 20324090
Conc: 55.46 ng/ml

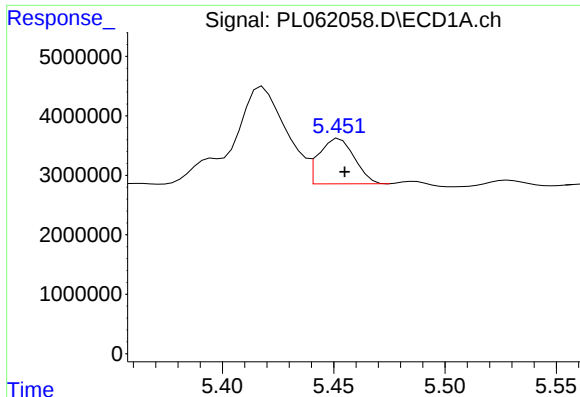

#26 Chlordane-4


R.T.: 5.453 min
Delta R.T.: -0.002 min
Response: 8482535
Conc: 65.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

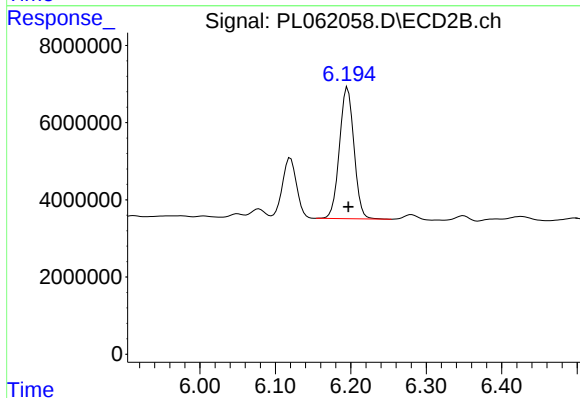


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 45502787
Conc: 101.36 ng/ml

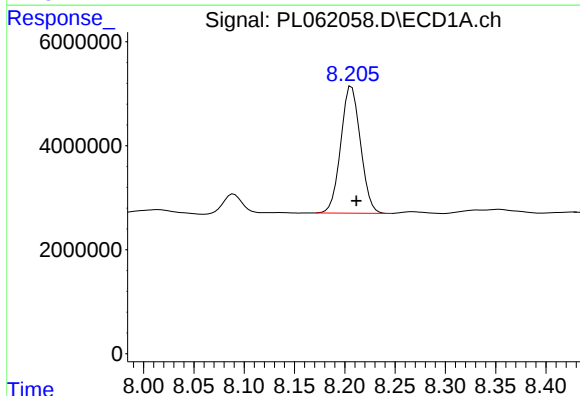

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.005 min
Response: 33183343
Conc: 20.40 ng/ml

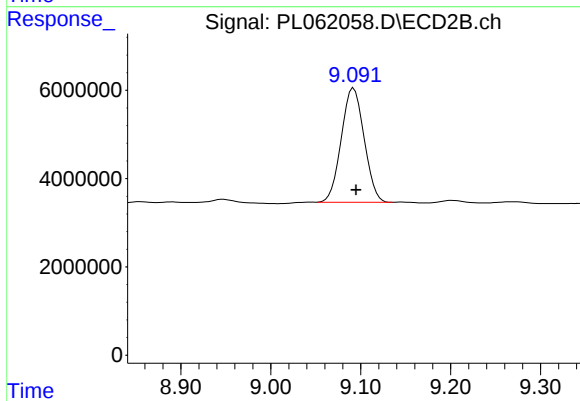

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.002 min
Response: 45689144
Conc: 20.75 ng/ml