

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
 Data File : PL062059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 13:40
 Operator : DD\AJ
 Sample : L4272-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 17:52:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	35903777	55002762	21.046	20.161
28)	SA Decachlor...	8.208	9.093	31612745	42612004	19.433	19.357
Target Compounds							
10)	B gamma-Chl...	5.418f	6.120	4343827	5441331	2.501	1.853 #
11)	B alpha-Chl...	0.000	6.196	0	10469191	N.D.	3.486 #
14)	MA Endrin	0.000	6.737f	0	5159061	N.D.	2.115 #
15)	B Endosulfa...	0.000	6.946f	0	9204115	N.D.	3.561 #
16)	A 4,4'-DDD	6.136	0.000	2337127	0	1.765	N.D. #
19)	B Endosulfa...	6.642f	7.279	6738625	28757269	4.356	12.281 #
22)	Mirex	7.328	0.000	7786292	0	5.554	N.D. #
25)	Chlordane-3	5.418f	6.120	4343827	5441331	27.636	14.849 #
26)	Chlordane-4	0.000	6.196	0	10469191	N.D.	23.321 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
Data File : PL062059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 13:40
Operator : DD\AJ
Sample : L4272-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 17:52:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

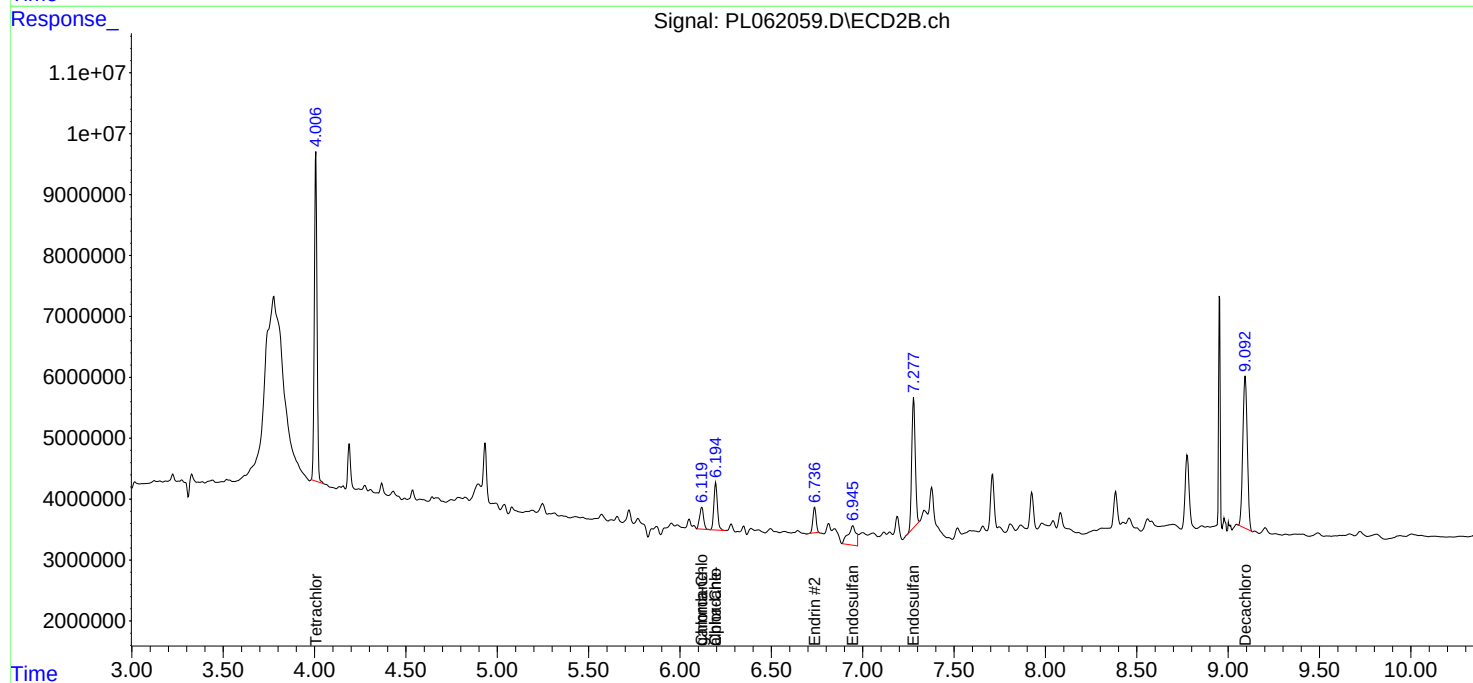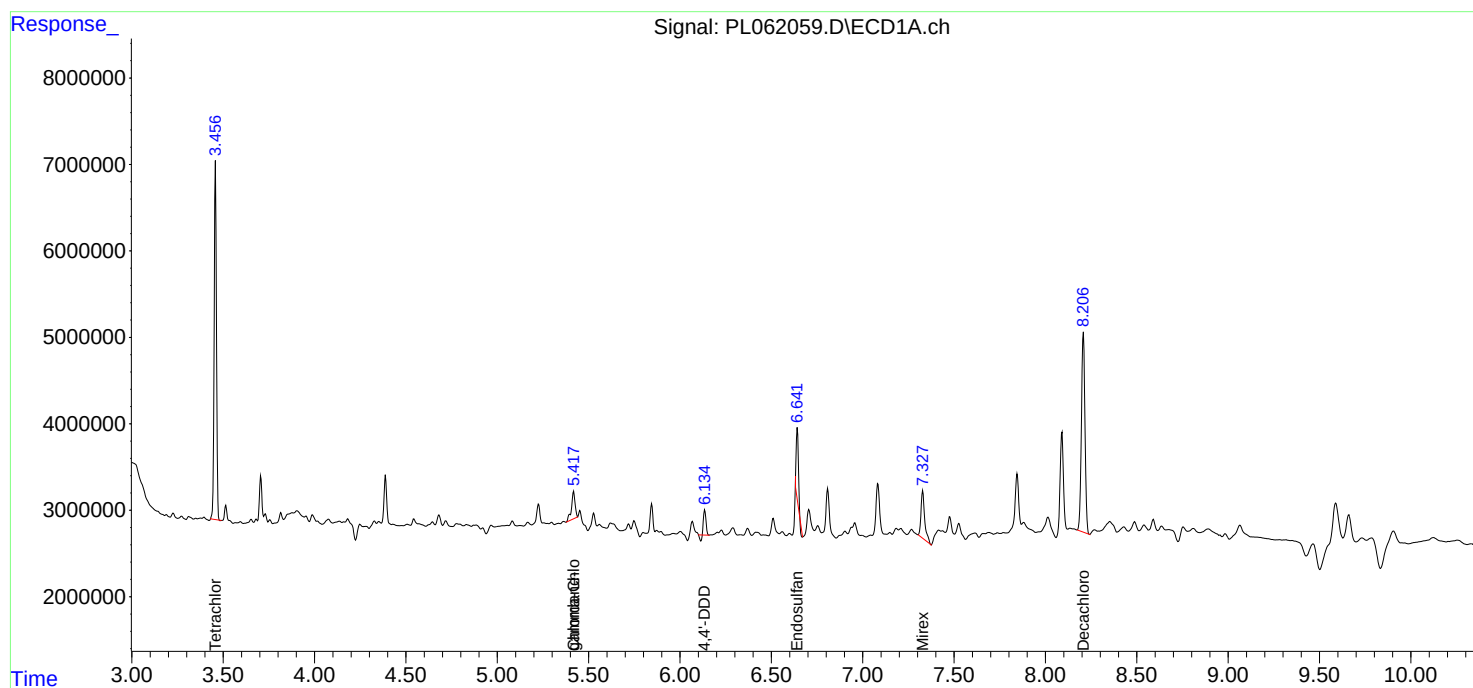


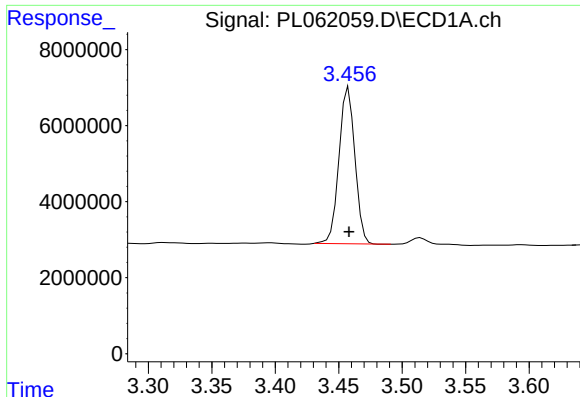

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 35903777
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

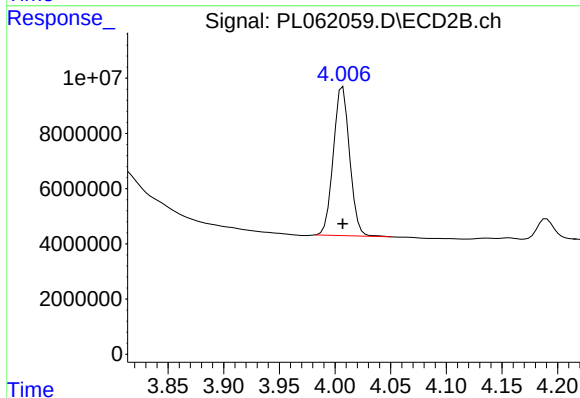


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 55002762
Conc: 20.16 ng/ml

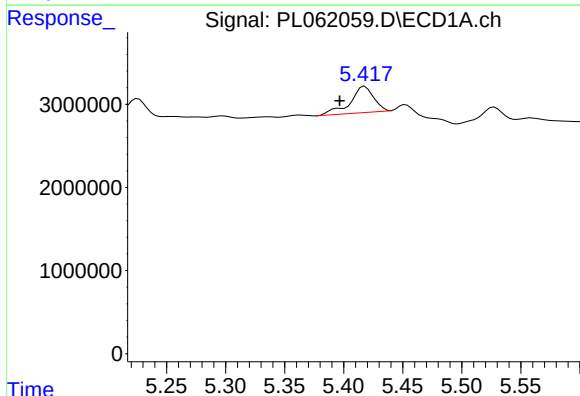


#10 gamma-Chlordane

R.T.: 5.418 min
Delta R.T.: 0.021 min
Response: 4343827
Conc: 2.50 ng/ml

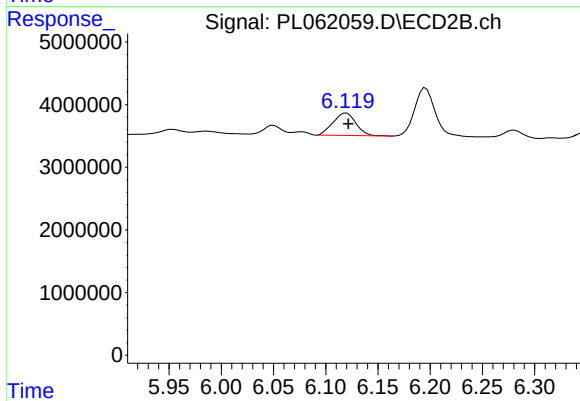

#10 gamma-Chlordane


R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 5441331
Conc: 1.85 ng/ml

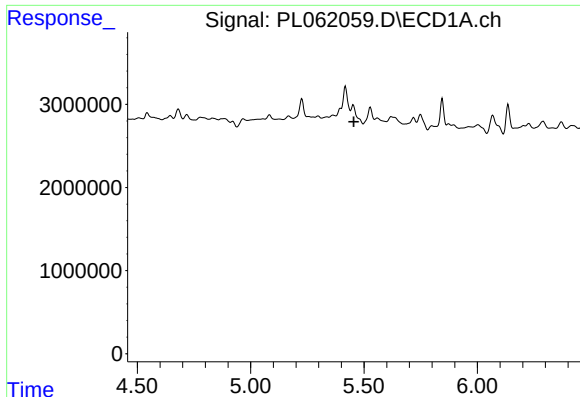

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

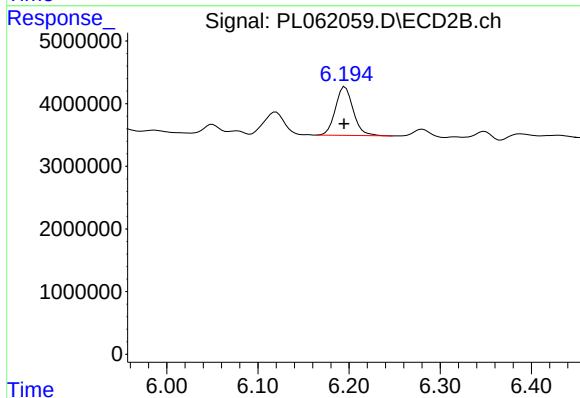


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.001 min
Response: 10469191
Conc: 3.49 ng/ml

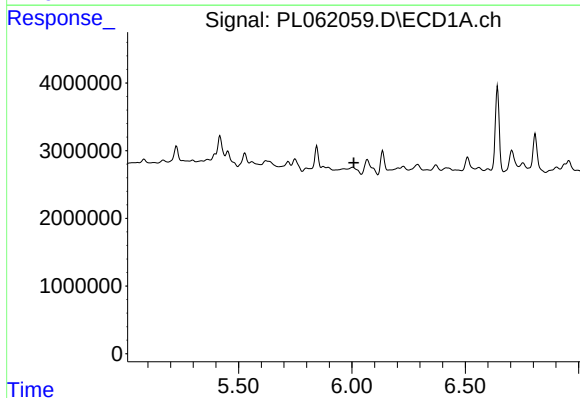


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.008 min
Response: 0
Conc: N.D.

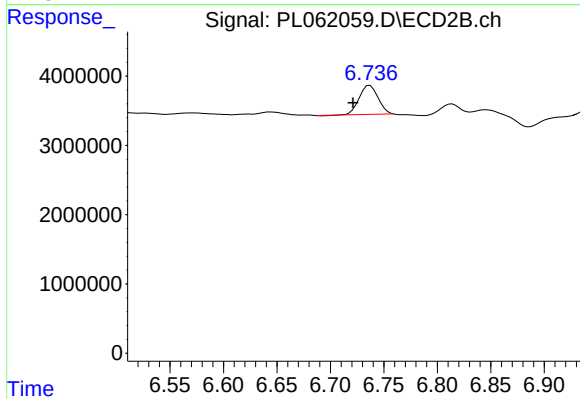

#14 Endrin


R.T.: 6.737 min
Delta R.T.: 0.016 min
Response: 5159061
Conc: 2.11 ng/ml

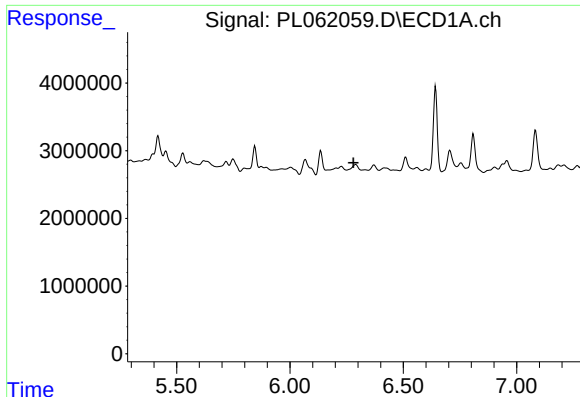

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

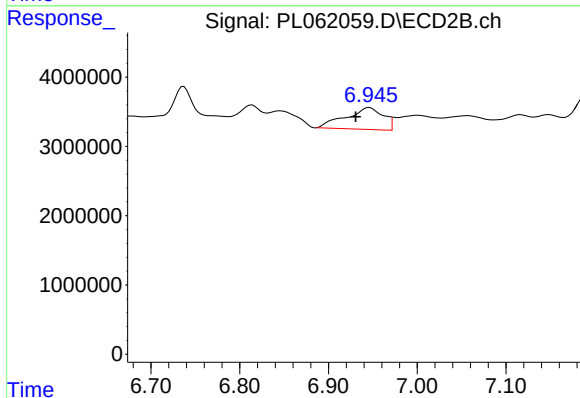


#15 Endosulfan II

R.T.: 6.946 min
Delta R.T.: 0.015 min
Response: 9204115
Conc: 3.56 ng/ml

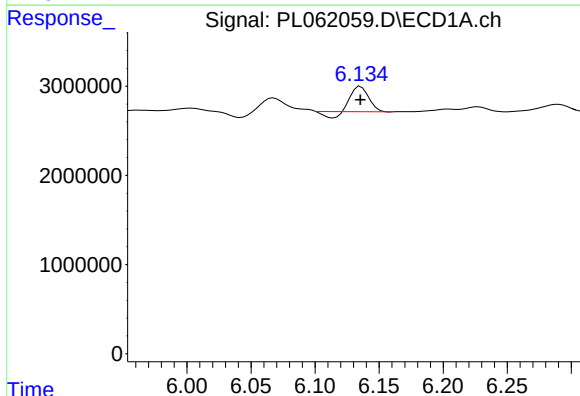


#16 4,4'-DDD

R.T.: 6.136 min
Delta R.T.: 0.000 min
Response: 2337127
Conc: 1.77 ng/ml

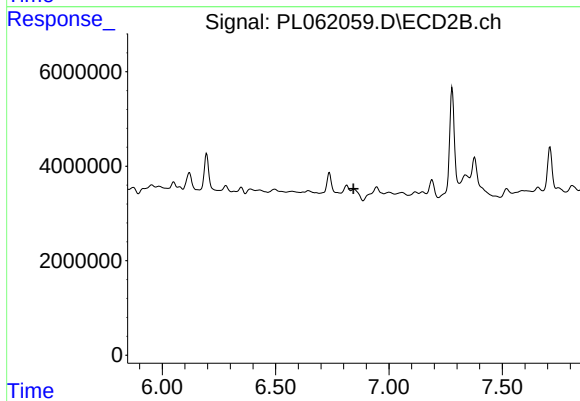

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.844 min
Response: 0
Conc: N.D.

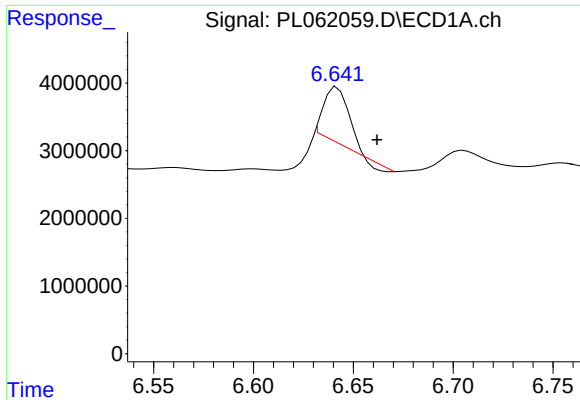

#19 Endosulfan Sulfate


R.T.: 6.642 min
Delta R.T.: -0.020 min
Response: 6738625
Conc: 4.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

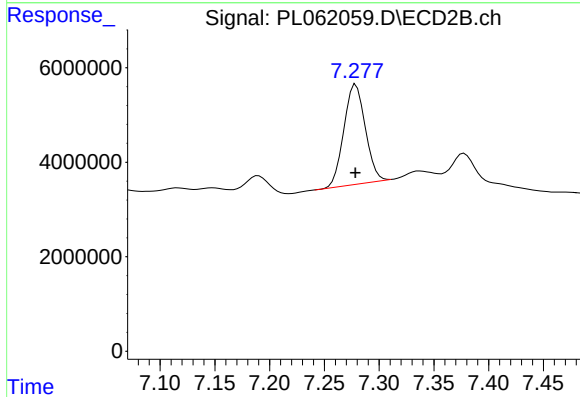


#19 Endosulfan Sulfate

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 28757269
Conc: 12.28 ng/ml

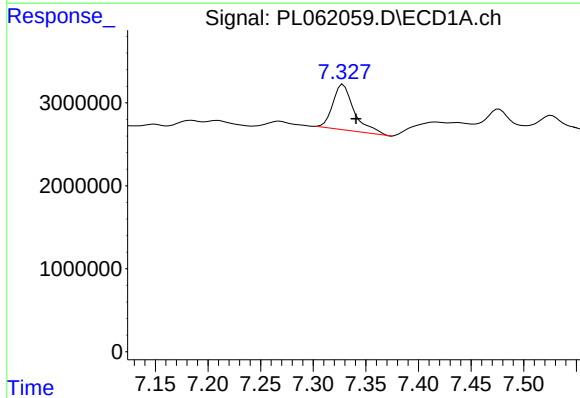


#22 Mirex

R.T.: 7.328 min
Delta R.T.: -0.012 min
Response: 7786292
Conc: 5.55 ng/ml

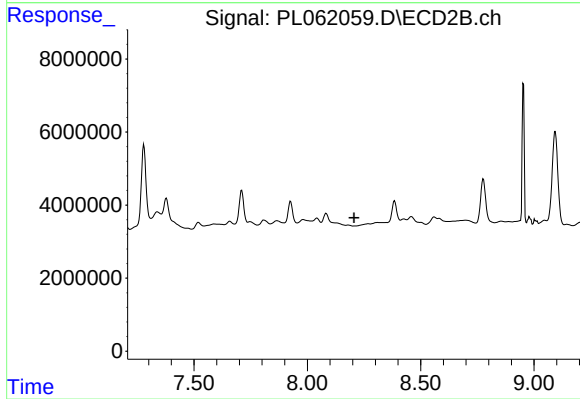

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.207 min
Response: 0
Conc: N.D.

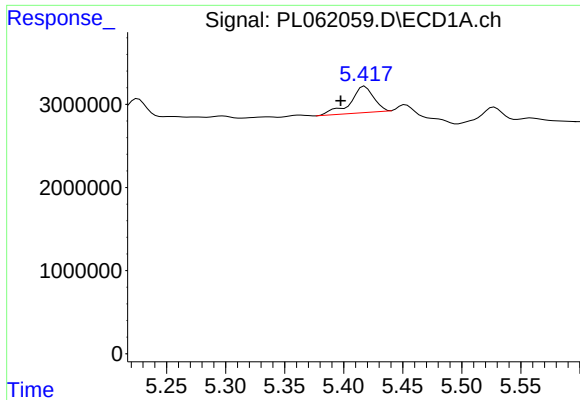

#25 Chlordane-3


R.T.: 5.418 min
Delta R.T.: 0.021 min
Response: 4343827
Conc: 27.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

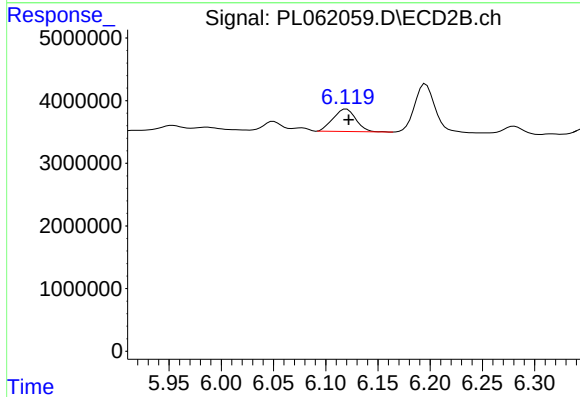


#25 Chlordane-3

R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 5441331
Conc: 14.85 ng/ml

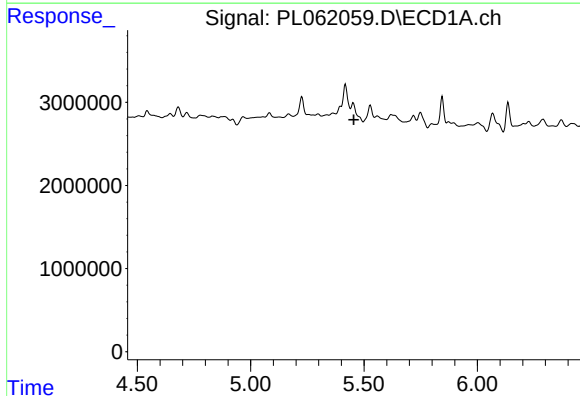


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

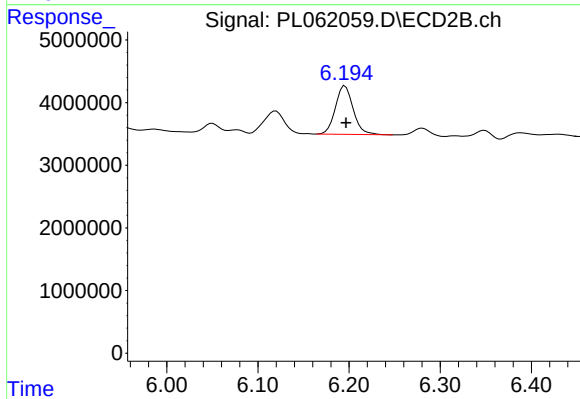

#26 Chlordane-4


R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 10469191
Conc: 23.32 ng/ml

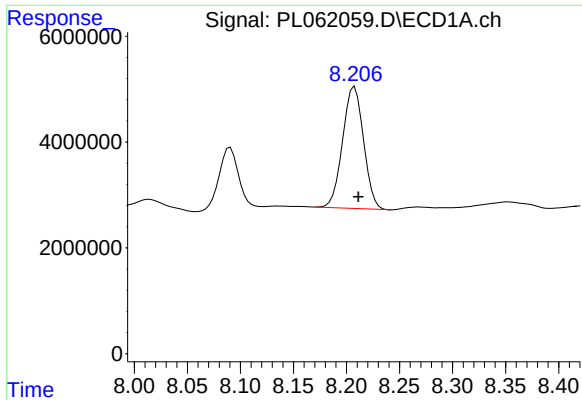

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.004 min
Response: 31612745
Conc: 19.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

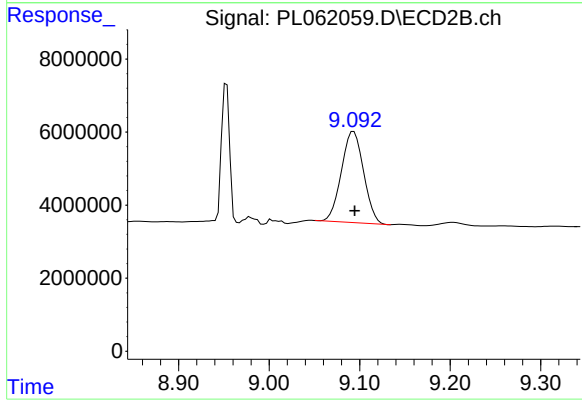

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.001 min
Response: 42612004
Conc: 19.36 ng/ml