

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
 Data File : PL062072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 16:47
 Operator : DD\AJ
 Sample : L4272-31
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 18:02:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	38828336	58547410	22.760	21.460
28)	SA Decachlor...	8.208	9.094	37378093	51789016	22.977	23.526
Target Compounds							
12)	B 4,4'-DDE	5.637f	0.000	2838219	0	1.806	N.D. #
15)	B Endosulfa...	0.000	6.946	0	9555511	N.D.	3.697 #
23)	Chlordane-1	4.330	0.000	2120807	0	42.831	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
Data File : PL062072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 16:47
Operator : DD\AJ
Sample : L4272-31
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 18:02:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

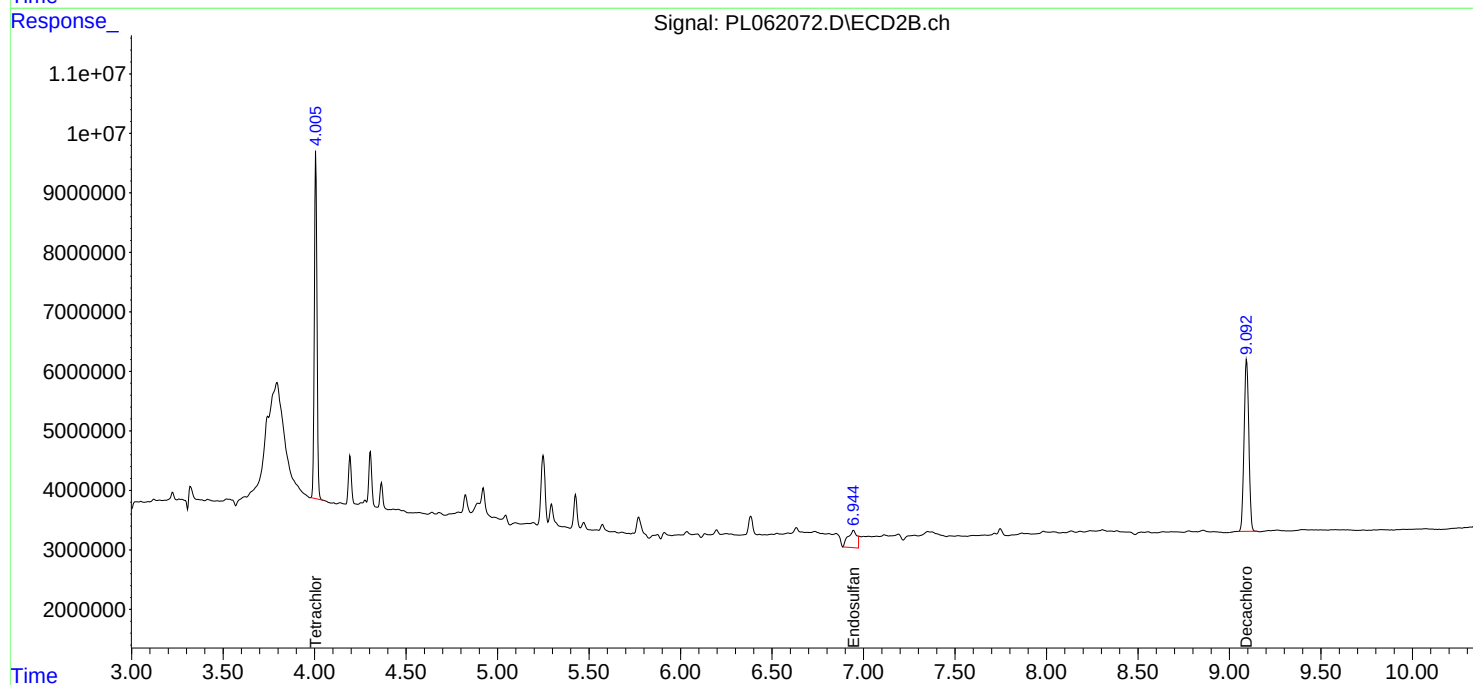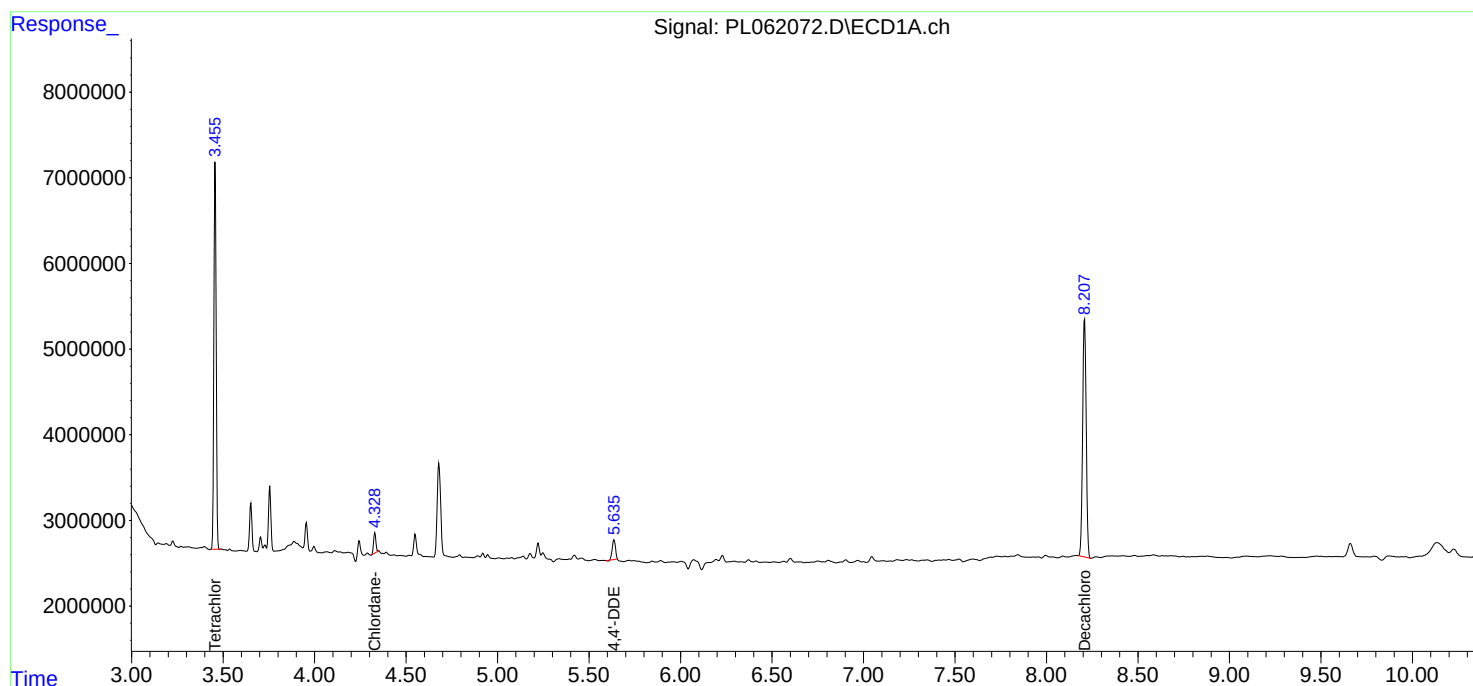


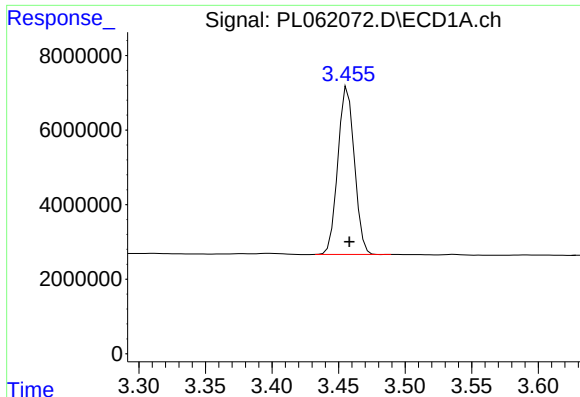

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 38828336
Conc: 22.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

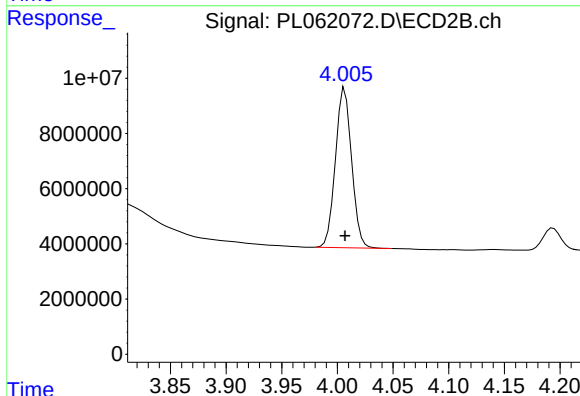


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 58547410
Conc: 21.46 ng/ml

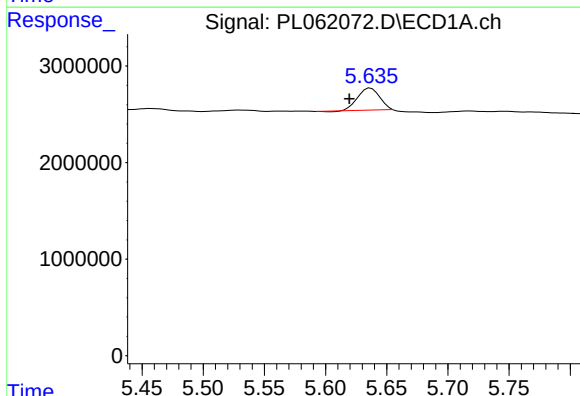


#12 4,4'-DDE

R.T.: 5.637 min
Delta R.T.: 0.017 min
Response: 2838219
Conc: 1.81 ng/ml

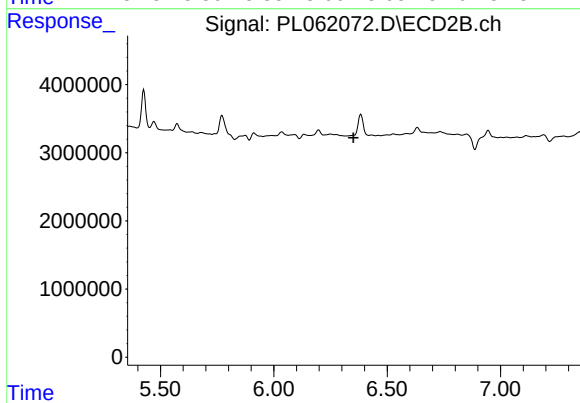

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

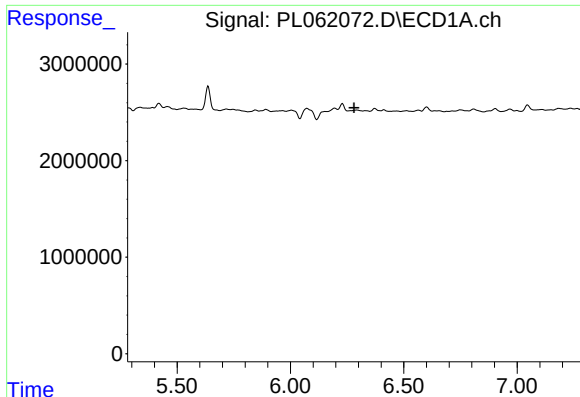

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

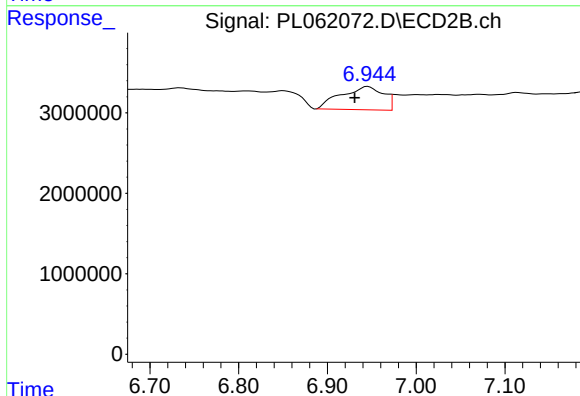


#15 Endosulfan II

R.T.: 6.946 min
Delta R.T.: 0.015 min
Response: 955511
Conc: 3.70 ng/ml

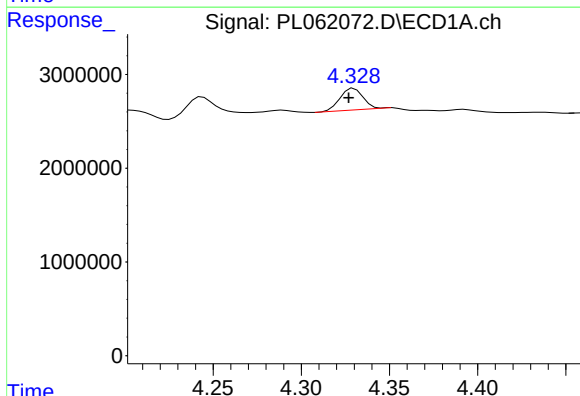


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.003 min
Response: 2120807
Conc: 42.83 ng/ml

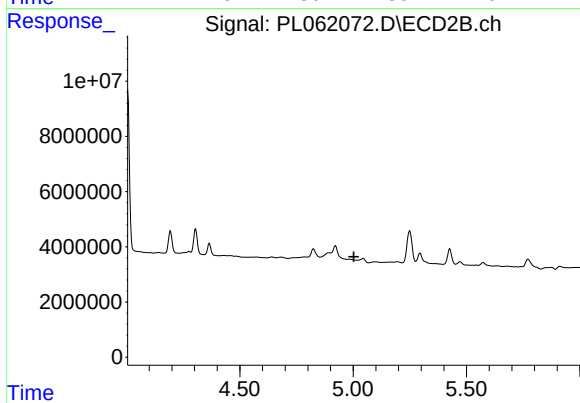

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

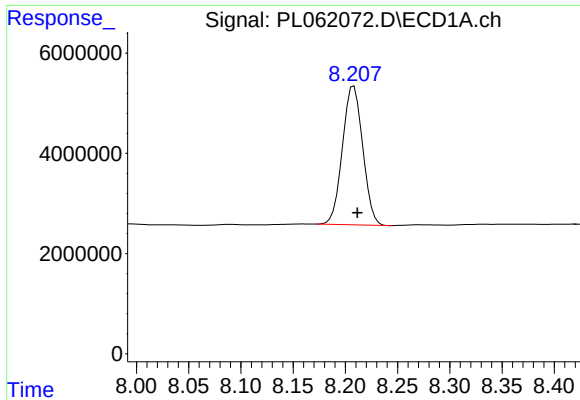

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.003 min
Response: 37378093
Conc: 22.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

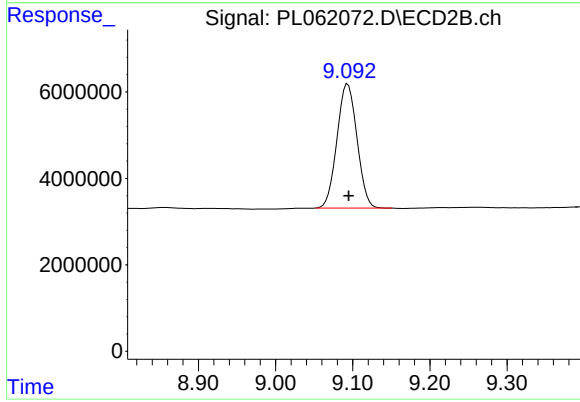

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 51789016
Conc: 23.53 ng/ml