

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
 Data File : PL062060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 13:55
 Operator : DD\AJ
 Sample : L4272-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-3-(6)

Manual Integrations
 APPROVED

Ankita
 10/8/2020 8:31:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 05:15:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.458	4.007	34599674	52820716	20.281	19.361
28) SA Decachlor...	8.208	9.093	28717789	39339883	17.653	17.871
Target Compounds						
10) B gamma-Chl...	5.394	6.120	580652	2282128	0.334m	0.777m#
11) B alpha-Chl...	5.452	6.194	1146698	3908305	0.660m	1.301m#
12) B 4,4'-DDE	5.618	6.349	606440	1654158	0.386m	0.606m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
Data File : PL062060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 13:55
Operator : DD\AJ
Sample : L4272-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MH-3-(6)


Manual Integrations
APPROVED

Ankita
10/8/2020 8:31:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 05:15:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm



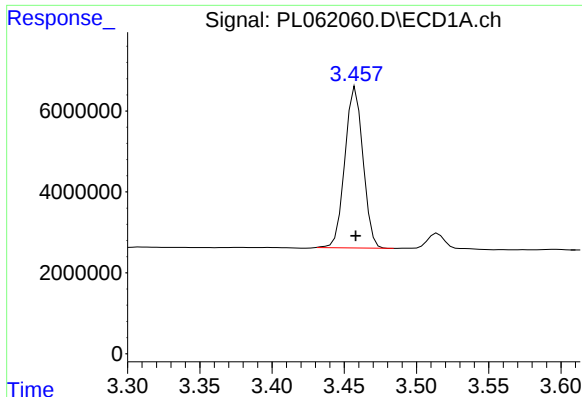


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 34599674
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-3-(6)


Manual Integrations
APPROVED

Ankita
10/8/2020 8:31:05 AM

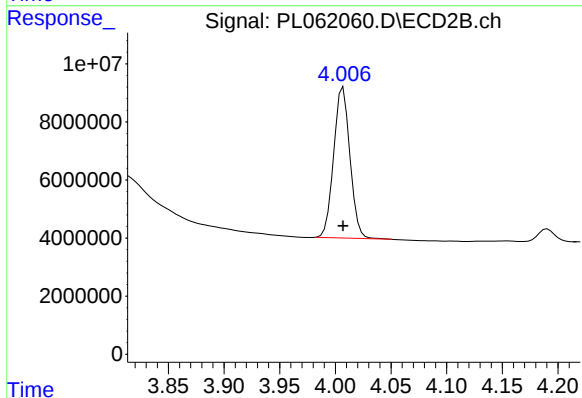


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 52820716
Conc: 19.36 ng/ml

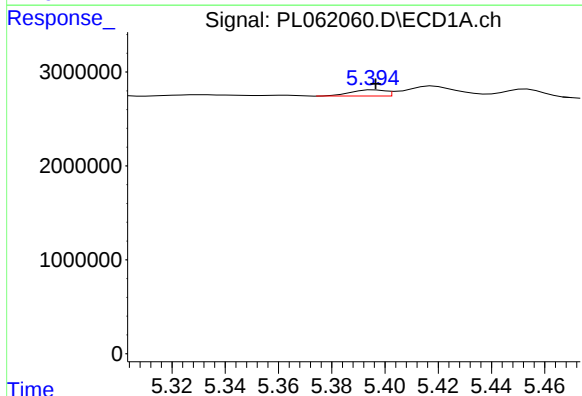


#10 gamma-Chlordane

R.T.: 5.394 min
Delta R.T.: -0.002 min
Response: 580652
Conc: 0.33 ng/ml m

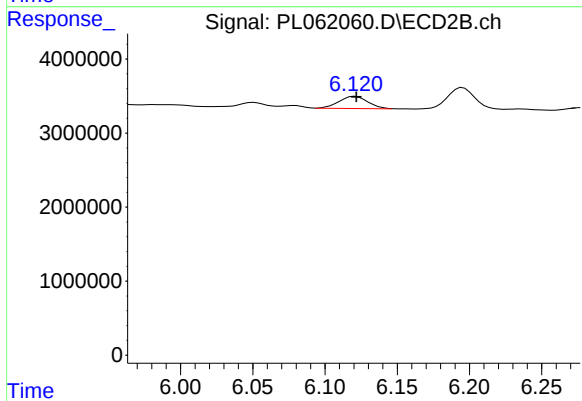

#10 gamma-Chlordane

R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 2282128
Conc: 0.78 ng/ml m

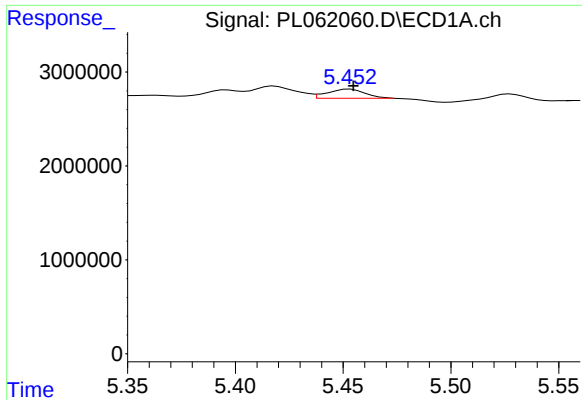


#11 alpha-Chlordane

R.T.: 5.452 min
Delta R.T.: -0.003 min
Response: 1146698
Conc: 0.66 ng/ml m

Instrument :
ECD_L
ClientSampleId :
MH-3-(6)


Manual Integrations
APPROVED

Ankita
10/8/2020 8:31:05 AM

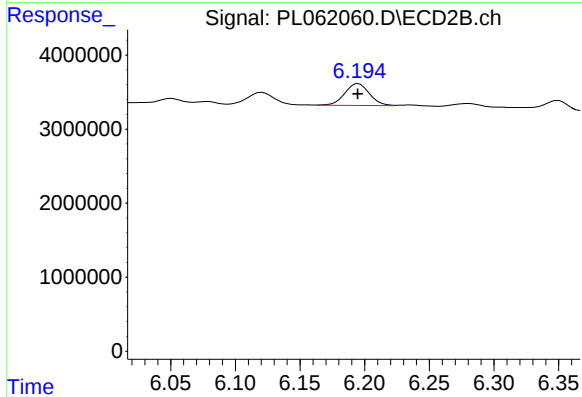


#11 alpha-Chlordane

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 3908305
Conc: 1.30 ng/ml m

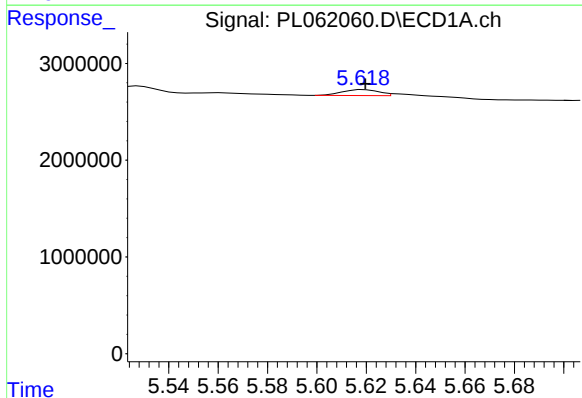


#12 4,4'-DDE

R.T.: 5.618 min
Delta R.T.: -0.002 min
Response: 606440
Conc: 0.39 ng/ml m

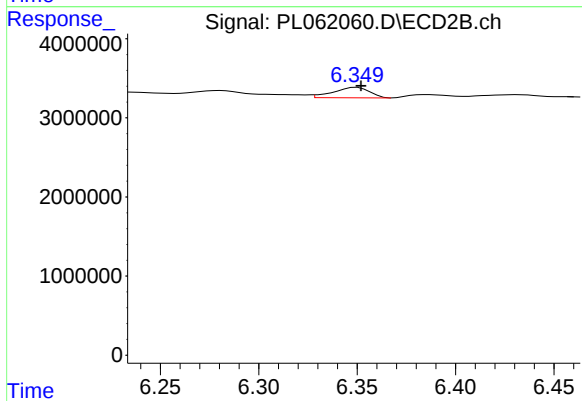

#12 4,4'-DDE

R.T.: 6.349 min
Delta R.T.: -0.003 min
Response: 1654158
Conc: 0.61 ng/ml m

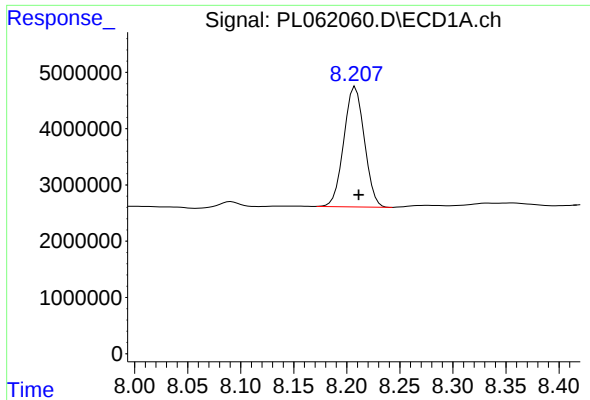


#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.003 min
Response: 28717789
Conc: 17.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-3-(6)

Manual Integrations
APPROVED

Ankita
10/8/2020 8:31:05 AM

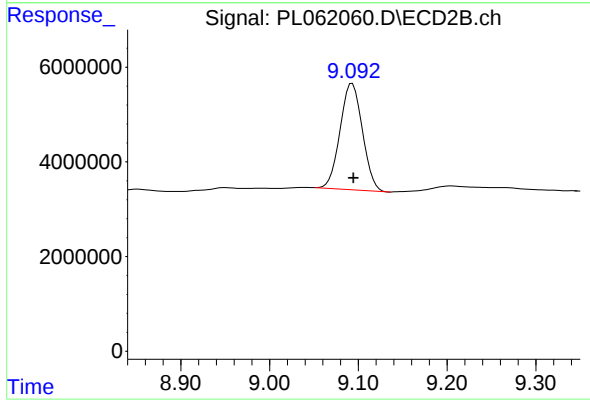

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.001 min
Response: 39339883
Conc: 17.87 ng/ml