

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
 Data File : PL062069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 16:04
 Operator : DD\AJ
 Sample : L4272-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SC-1-(6.5)

Manual Integrations
 APPROVED

Ankita
 10/8/2020 8:31:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 05:09:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.008	36881497	55332037	21.619	20.281
28)	SA Decachlor...	8.213	9.098	29417434	40744378	18.083	18.509
Target Compounds							
11)	B alpha-Chl...	5.457	6.198	963496	4151694	0.555m	1.382 #
12)	B 4,4'-DDE	5.622	6.351	756052	1762473	0.481m	0.646m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100620\
Data File : PL062069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 16:04
Operator : DD\AJ
Sample : L4272-22
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SC-1-(6.5)


Manual Integrations
APPROVED

Ankita
10/8/2020 8:31:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 05:09:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

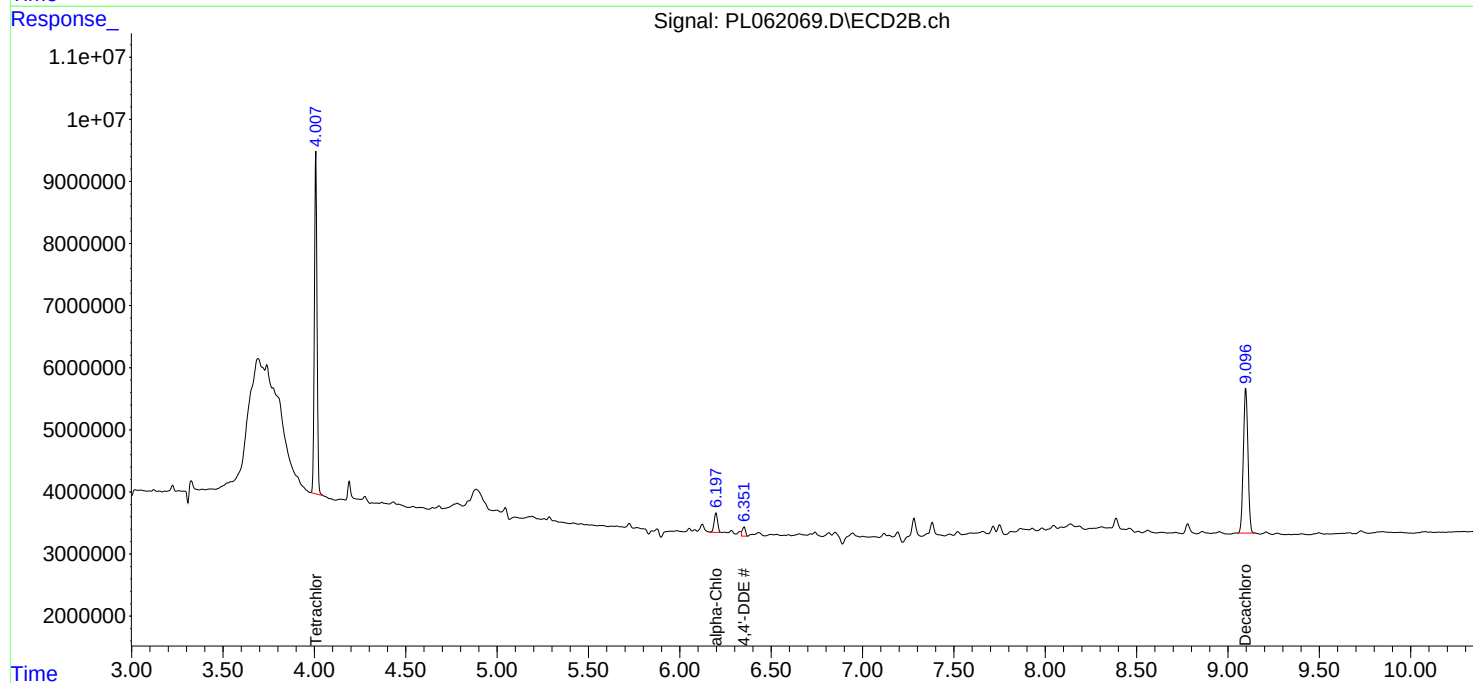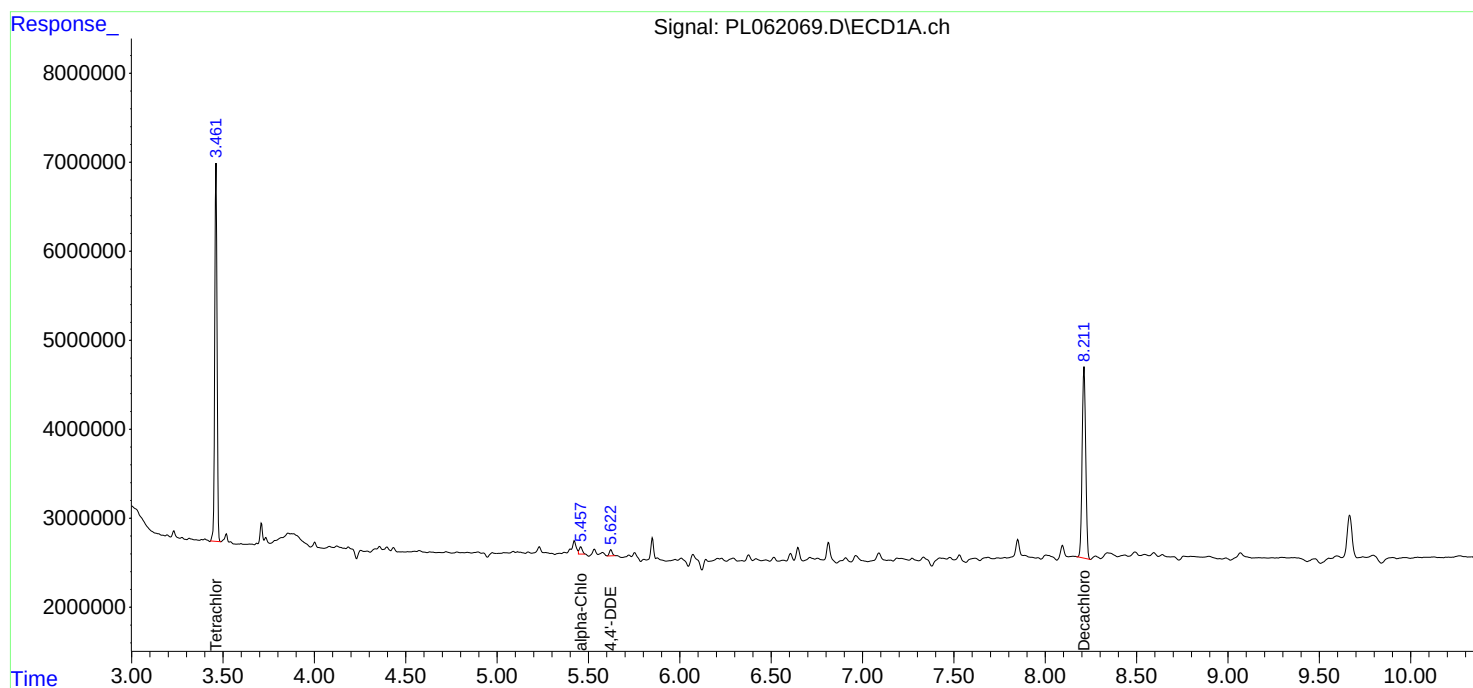

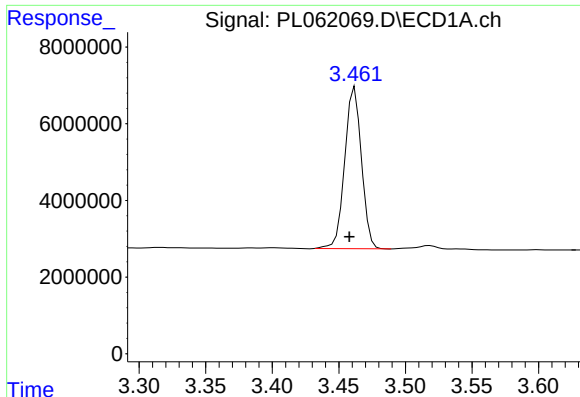


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: 0.004 min
Response: 36881497
Conc: 21.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-1-(6.5)


Manual Integrations
APPROVED

Ankita
10/8/2020 8:31:15 AM

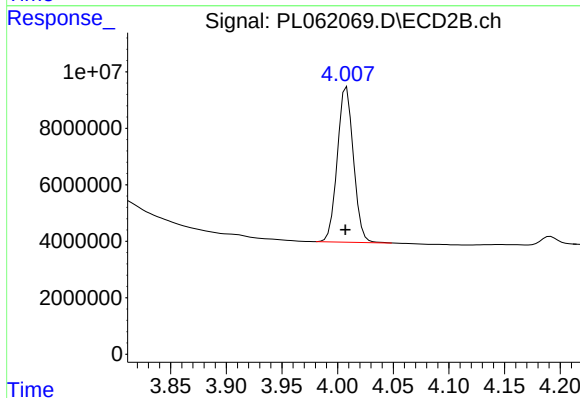


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.001 min
Response: 55332037
Conc: 20.28 ng/ml

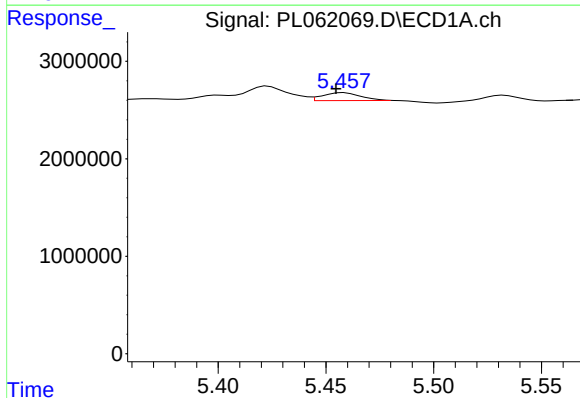


#11 alpha-Chlordane

R.T.: 5.457 min
Delta R.T.: 0.002 min
Response: 963496
Conc: 0.55 ng/ml m

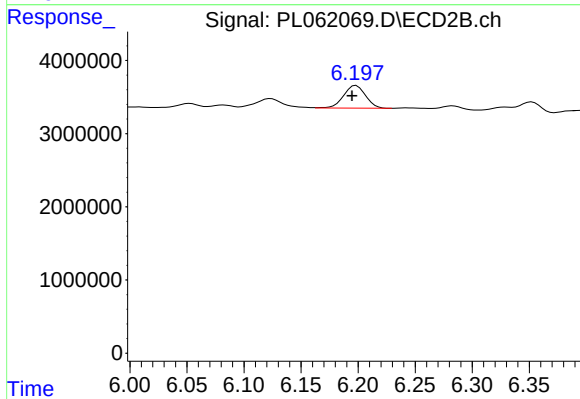

#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.004 min
Response: 4151694
Conc: 1.38 ng/ml

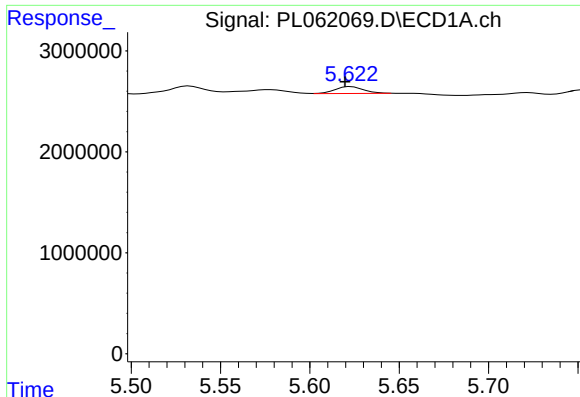


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: 0.002 min
Response: 756052
Conc: 0.48 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SC-1-(6.5)


Manual Integrations
APPROVED

Ankita
10/8/2020 8:31:15 AM

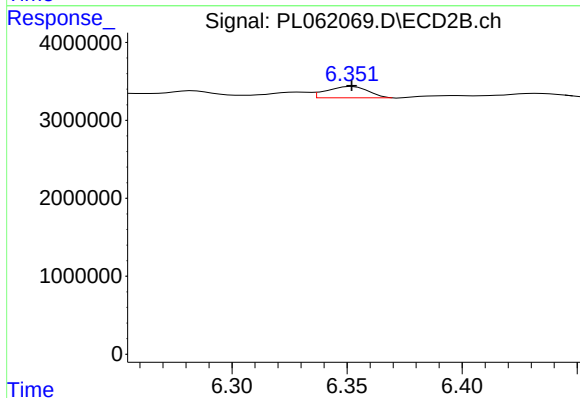


#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1762473
Conc: 0.65 ng/ml m

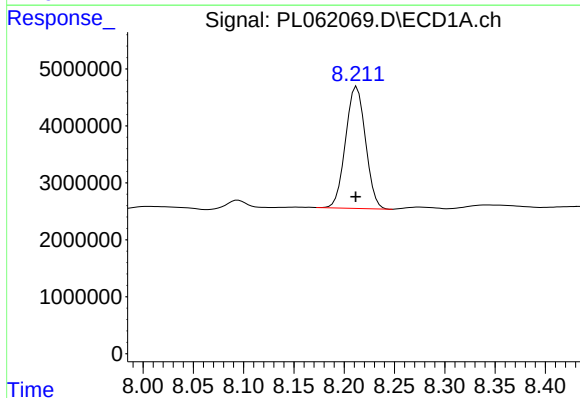

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.001 min
Response: 29417434
Conc: 18.08 ng/ml

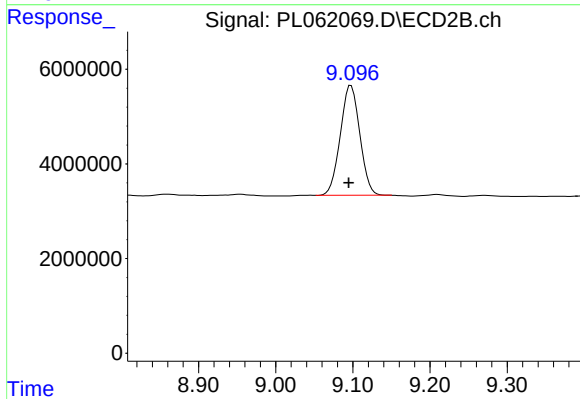

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.003 min
Response: 40744378
Conc: 18.51 ng/ml