

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100822\
 Data File : PL078202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 11:02
 Operator : AR\AJ
 Sample : N4956-10MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8S9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/10/2022
 Supervised By : Ankita Jodhani 10/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 23:39:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.621	32704527	50007067	18.541	14.863
27)	SA Decachlor...	8.905	7.718	41533487	65802727	27.402	24.301
Target Compounds							
2)	A alpha-BHC	3.882	3.113	114.3E6	195.2E6	45.484	38.892
3)	MA gamma-BHC...	4.217	3.437	105.3E6	193.1E6	43.635	42.181
4)	MA Heptachlor	4.791	3.768	107.7E6	169.9E6	44.656m	36.980
5)	MB Aldrin	5.133	4.042	100.6E6	177.0E6	46.070	39.670
6)	B beta-BHC	4.429	3.737	47144280	76505856	40.077m	38.535
7)	B delta-BHC	4.674	3.960	30127856	72625718	12.333	15.450 #
8)	B Heptachlo...	5.566	4.541	90795886	166.7E6	42.915	42.247
9)	A Endosulfan I	5.952	4.906	82869630	147.1E6	46.647	40.690
10)	B trans-Chl...	5.821	4.790	88313090	157.2E6	45.222	38.887
11)	B cis-Chlor...	5.899	4.853	89164039	156.8E6	47.259	40.651
12)	B 4,4'-DDE	6.079	5.047	170.2E6	306.4E6	90.818	81.598
13)	MA Dieldrin	6.229	5.170	196.1E6	300.9E6	105.456	77.360 #
14)	MA Endrin	6.461	5.442	160.0E6	294.1E6	99.244	91.187
15)	B Endosulfa...	6.689	5.738	151.3E6	271.0E6	93.813	85.690
16)	A 4,4'-DDD	6.603	5.600	136.6E6	251.7E6	100.702	83.333
17)	MA 4,4'-DDT	6.913	5.848	131.9E6	258.7E6	90.601	85.645
18)	B Endrin al...	6.821	5.918	116.5E6	206.6E6	86.539	79.912
19)	B Endosulfa...	7.053	6.141	109.1E6	217.2E6	73.501	70.071
20)	A Methoxychlor	7.394	6.425	350.0E6	606.3E6	466.732	407.418
21)	B Endrin ke...	7.541	6.640	156.5E6	288.7E6	97.366	86.887

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100822\
Data File : PL078202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 11:02
Operator : AR\AJ
Sample : N4956-10MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 23:39:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

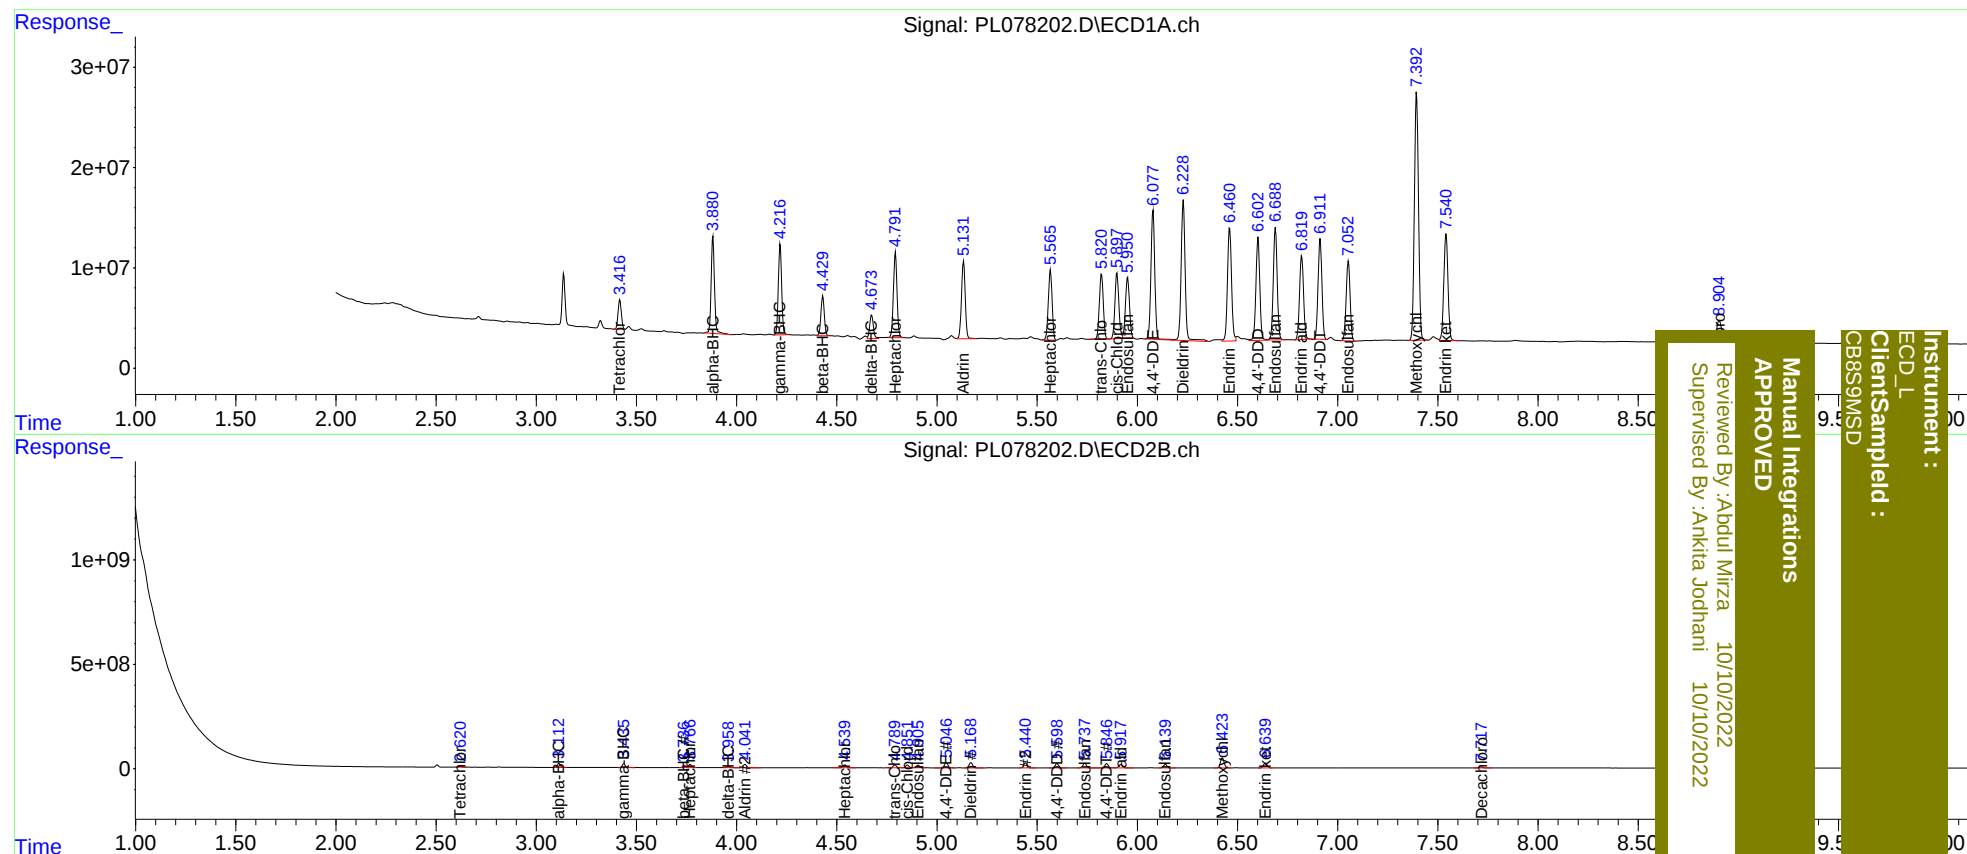

Instrument :
ECD_L
ClientSampled :
CB8S9MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 10/10/2022
Supervised By :Ankita Jodhani 10/10/2022