

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
 Data File : PL078340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 18:00
 Operator : AR\AJ
 Sample : N5105-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 23:34:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	2.621	15377926	25072878	9.305	9.486
28)	SA Decachlor...	8.901	7.715	11593308	15648097	7.510	7.198
Target Compounds							
8)	B Heptachlo...	5.573	4.530	146360	371700	0.096	0.126 #
10)	B gamma-Chl...	0.000	4.793	0	2838802	N.D.	0.948 #
12)	B 4,4'-DDE	6.072	5.045	440790	1918897	0.262	0.671 #
14)	MA Endrin	0.000	5.461f	0	334920	N.D.	0.145 #
15)	B Endosulfa...	6.706f	5.708f	550191	658075	0.410	0.269 #
20)	A Methoxychlor	0.000	6.436	0	226443	N.D.	0.179 #
21)	B Endrin ke...	7.567f	0.000	2103029	0	1.348	N.D. #
25)	Chlordane-3	0.000	4.793	0	2838802	N.D.	9.278 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
Data File : PL078340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 18:00
Operator : AR\AJ
Sample : N5105-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 23:34:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

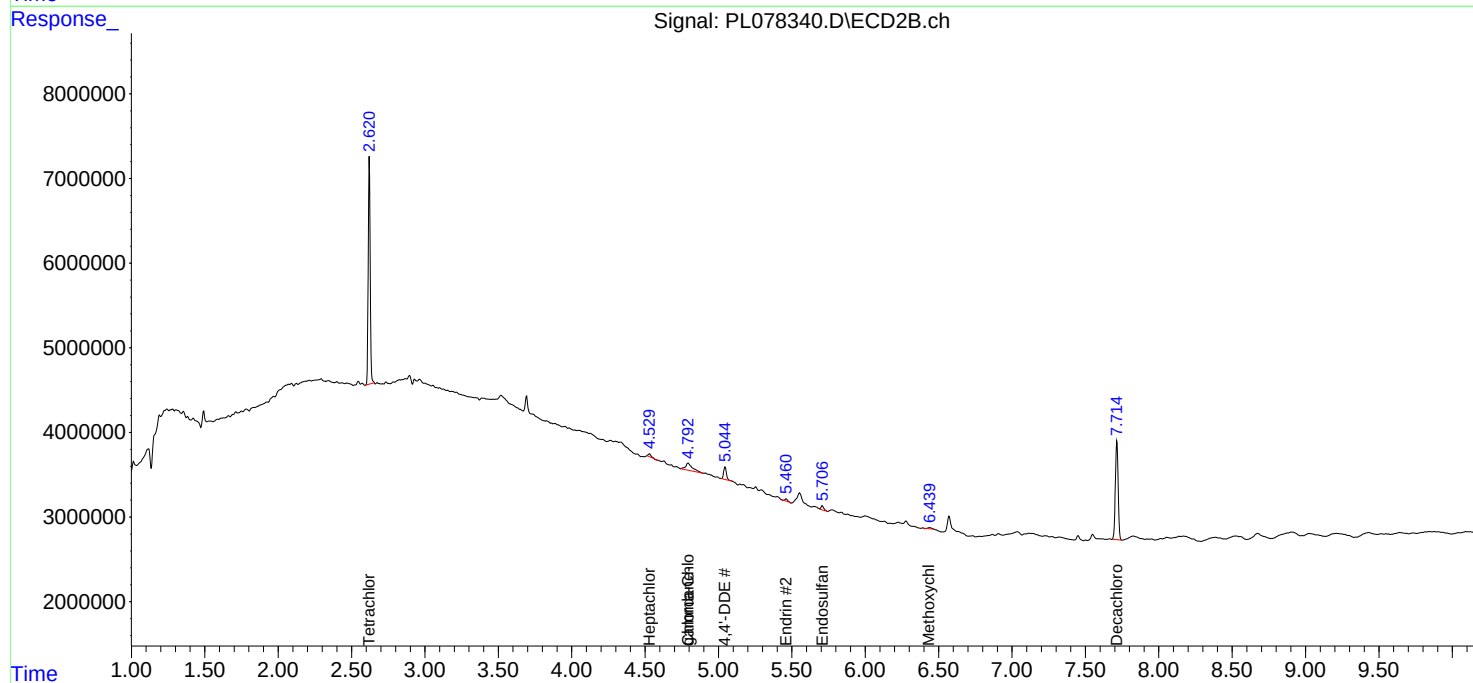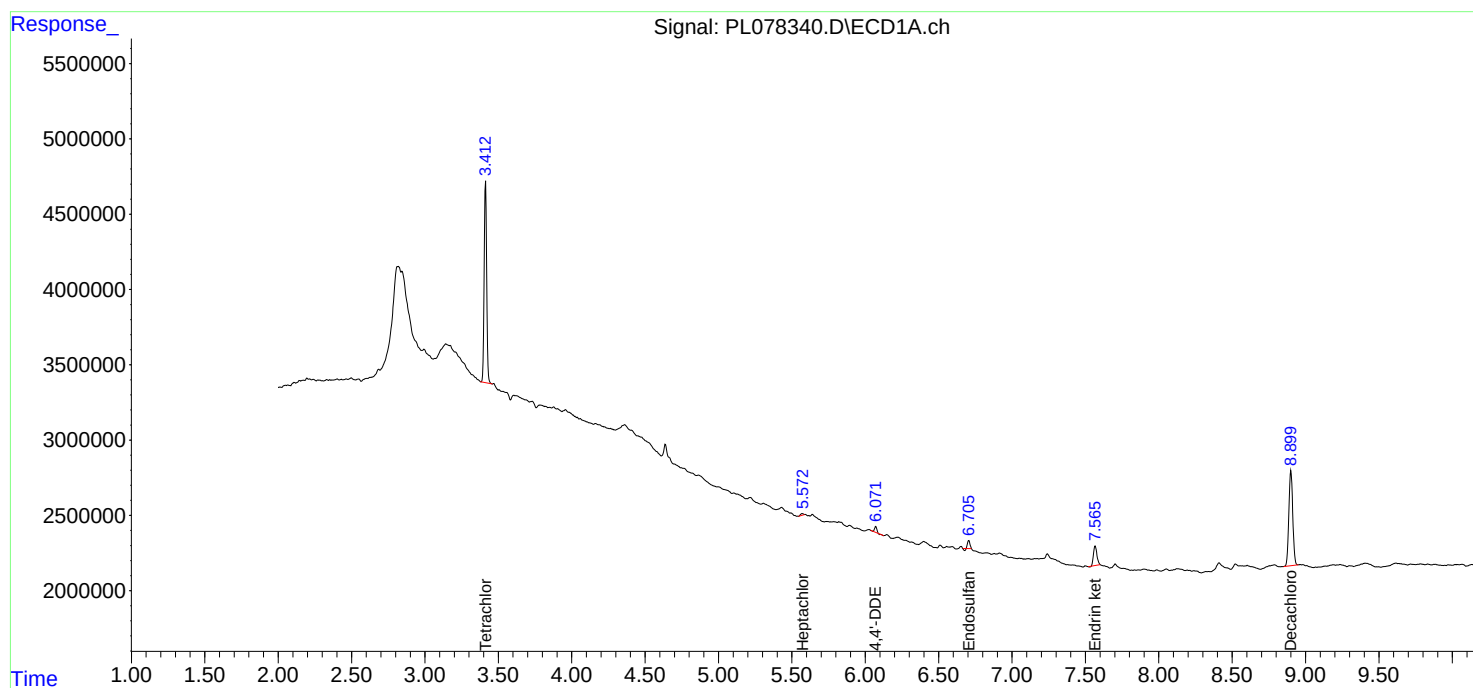


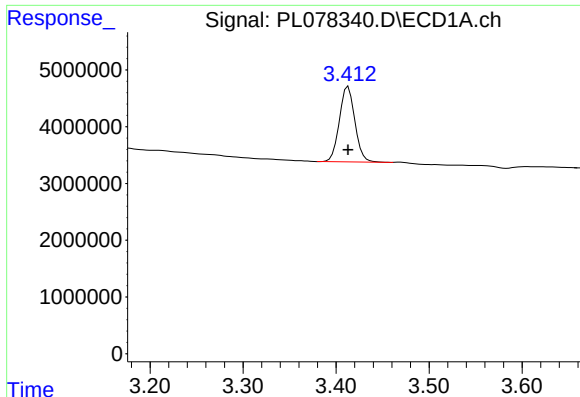

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 15377926
Conc: 9.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-6

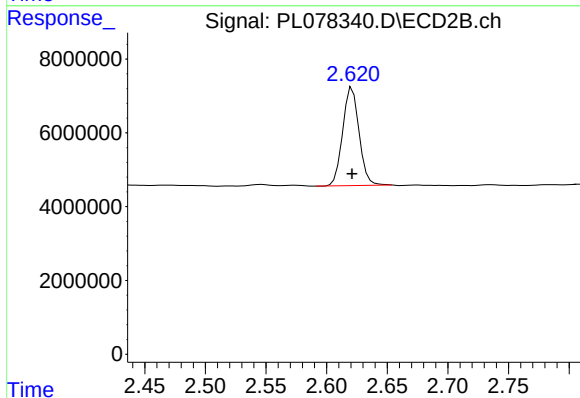


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 25072878
Conc: 9.49 ng/ml

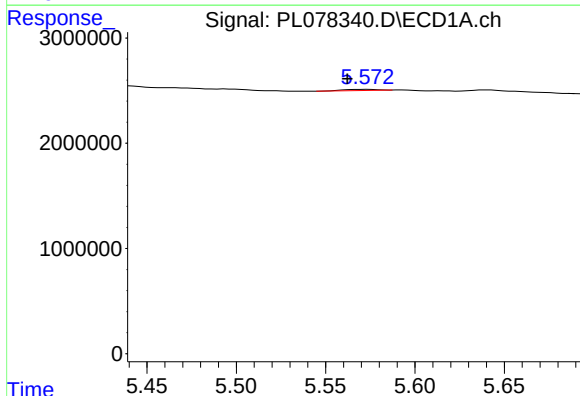


#8 Heptachlor epoxide

R.T.: 5.573 min
Delta R.T.: 0.011 min
Response: 146360
Conc: 0.10 ng/ml

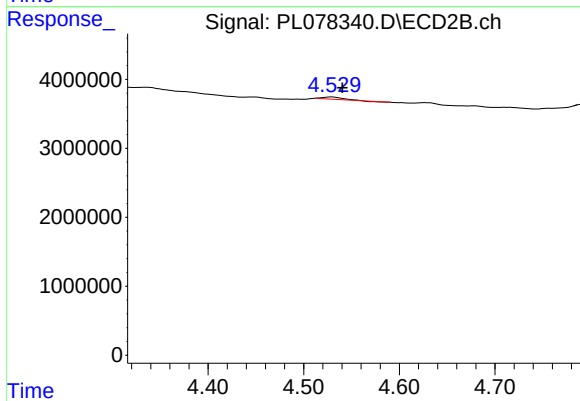

#8 Heptachlor epoxide


R.T.: 4.530 min
Delta R.T.: -0.010 min
Response: 371700
Conc: 0.13 ng/ml

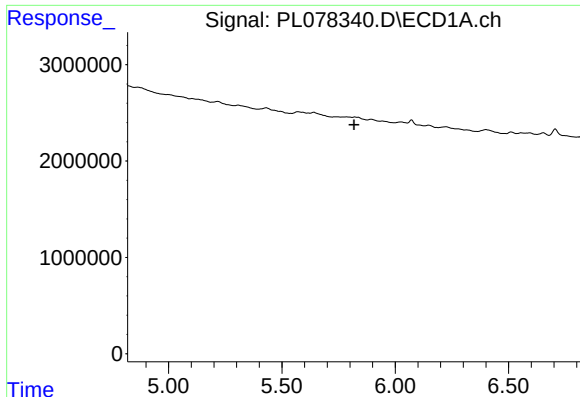

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.818 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-6

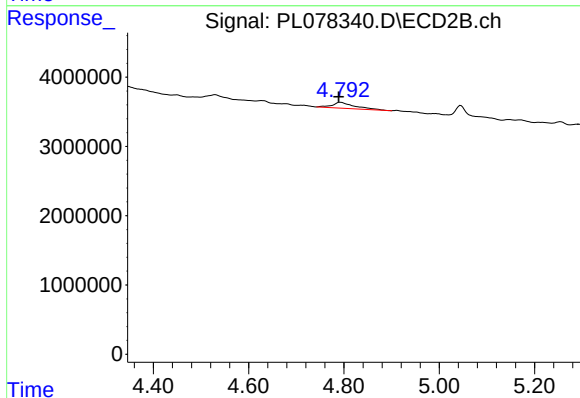


#10 gamma-Chlordane

R.T.: 4.793 min
Delta R.T.: 0.004 min
Response: 2838802
Conc: 0.95 ng/ml

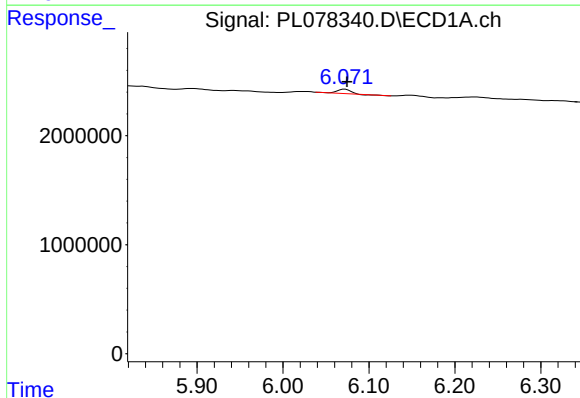


#12 4,4'-DDE

R.T.: 6.072 min
Delta R.T.: -0.003 min
Response: 440790
Conc: 0.26 ng/ml

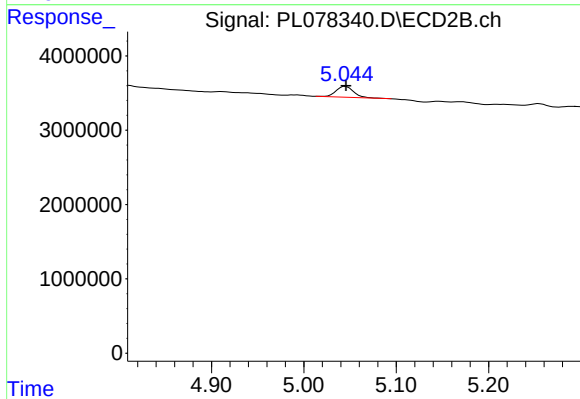

#12 4,4'-DDE


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 1918897
Conc: 0.67 ng/ml

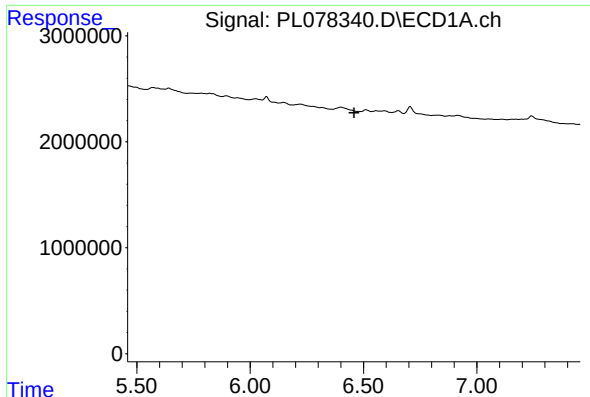

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-6

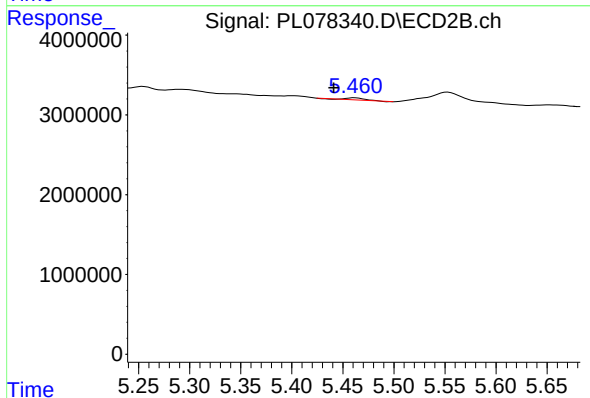


#14 Endrin

R.T.: 5.461 min
Delta R.T.: 0.020 min
Response: 334920
Conc: 0.15 ng/ml

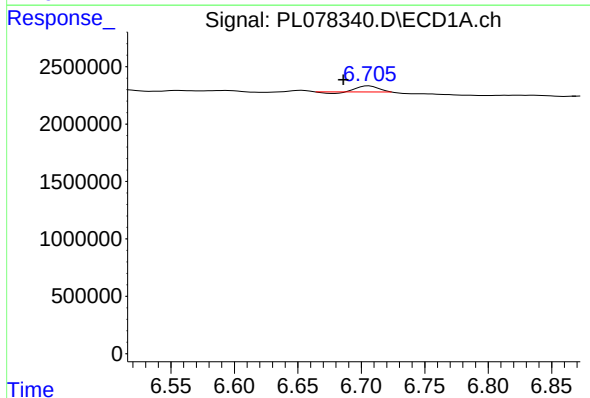


#15 Endosulfan II

R.T.: 6.706 min
Delta R.T.: 0.020 min
Response: 550191
Conc: 0.41 ng/ml

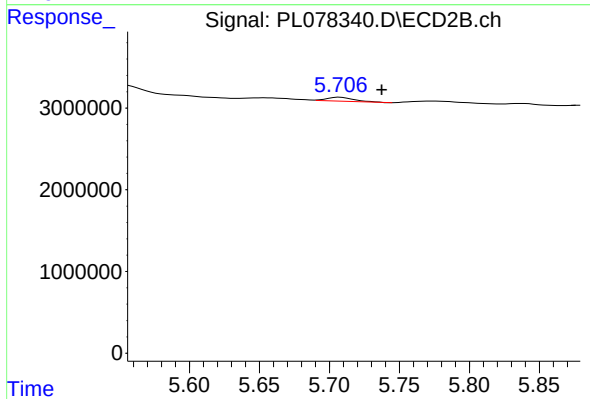

#15 Endosulfan II


R.T.: 5.708 min
Delta R.T.: -0.030 min
Response: 658075
Conc: 0.27 ng/ml

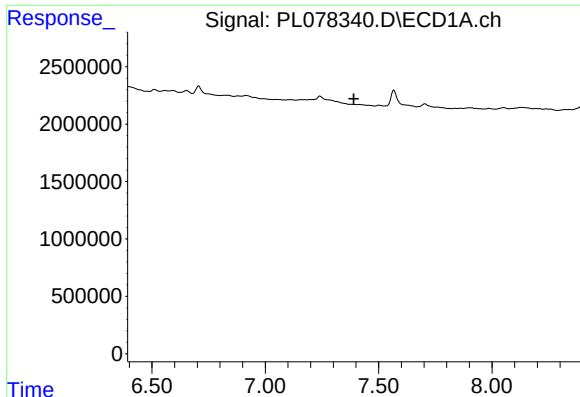

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-6

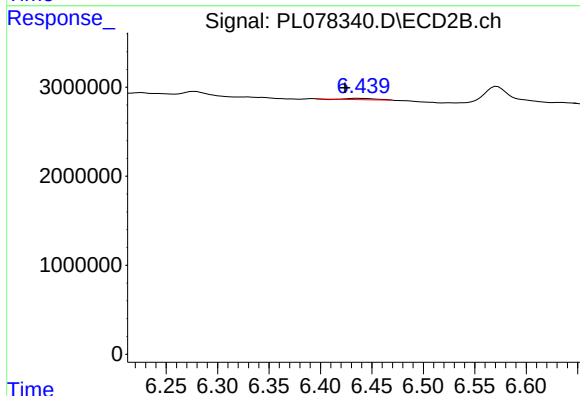


#20 Methoxychlor

R.T.: 6.436 min
Delta R.T.: 0.012 min
Response: 226443
Conc: 0.18 ng/ml

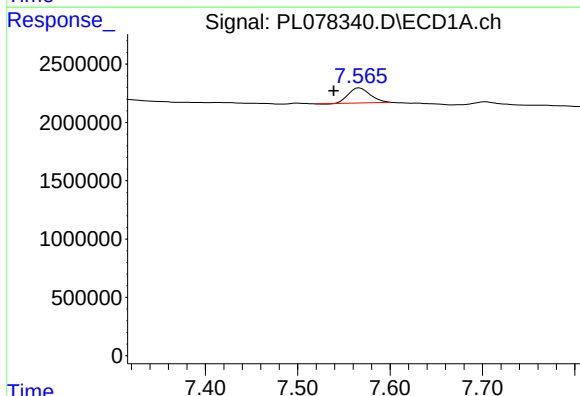


#21 Endrin ketone

R.T.: 7.567 min
Delta R.T.: 0.028 min
Response: 2103029
Conc: 1.35 ng/ml

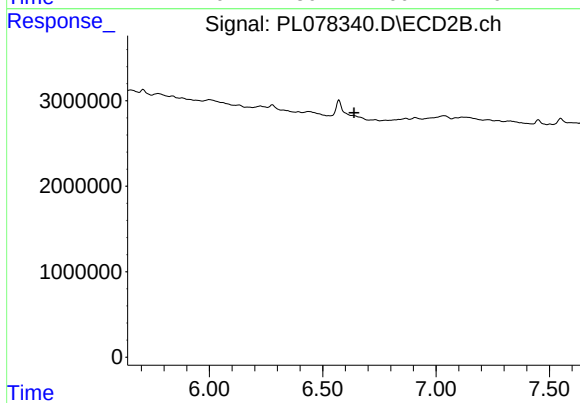

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.638 min
Response: 0
Conc: N.D.

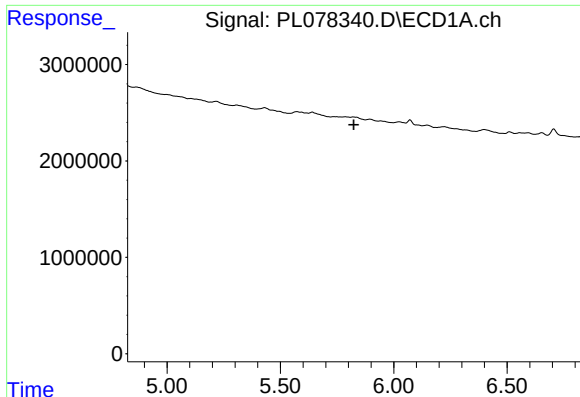

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-6

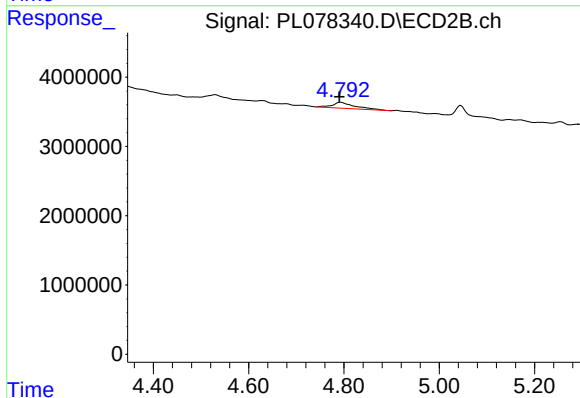


#25 Chlordane-3

R.T.: 4.793 min
Delta R.T.: 0.002 min
Response: 2838802
Conc: 9.28 ng/ml

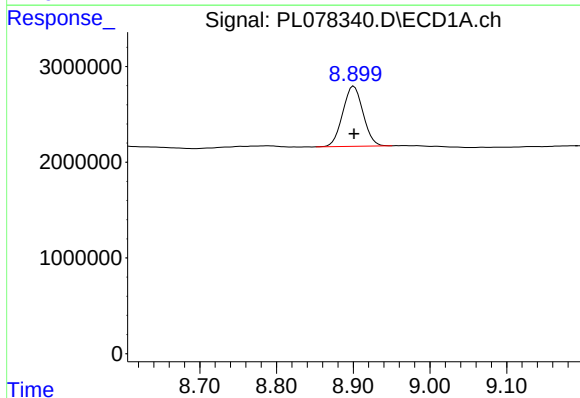

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 11593308
Conc: 7.51 ng/ml

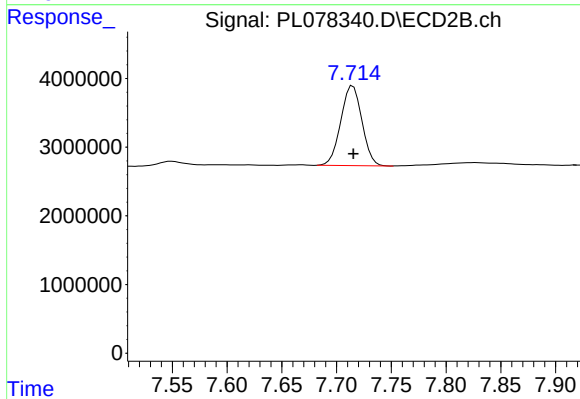

#28 Decachlorobiphenyl

R.T.: 7.715 min
Delta R.T.: 0.000 min
Response: 15648097
Conc: 7.20 ng/ml