

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
 Data File : PL078342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 18:27
 Operator : AR\AJ
 Sample : N5105-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 23:35:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	2.620	16808834	27438653	10.171	10.381
28)	SA Decachlor...	8.900	7.714	16719262	22303549	10.830	10.260
Target Compounds							
8)	B Heptachlo...	5.572	0.000	260435	0	0.171	N.D. #
10)	B gamma-Chl...	0.000	4.790	0	1008238	N.D.	0.337 #
12)	B 4,4'-DDE	6.073	5.044	771507	2110513	0.458	0.738 #
14)	MA Endrin	0.000	5.460f	0	520242	N.D.	0.226 #
15)	B Endosulfa...	6.705f	0.000	765100	0	0.571	N.D. #
17)	MA 4,4'-DDT	6.910	5.843	658792	390033	0.450	0.172 #
21)	B Endrin ke...	7.567f	0.000	1986284	0	1.273	N.D. #
25)	Chlordane-3	0.000	4.790	0	1008238	N.D.	3.295 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
Data File : PL078342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 18:27
Operator : AR\AJ
Sample : N5105-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 23:35:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

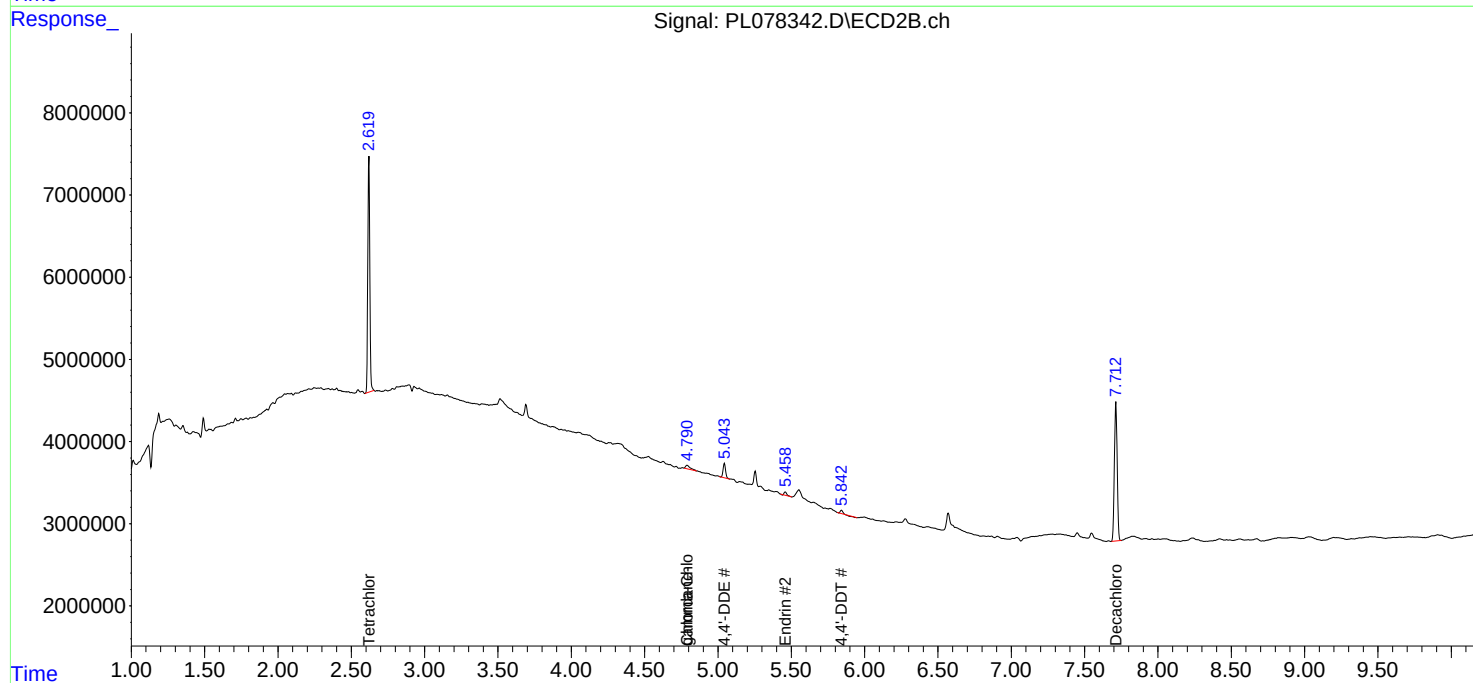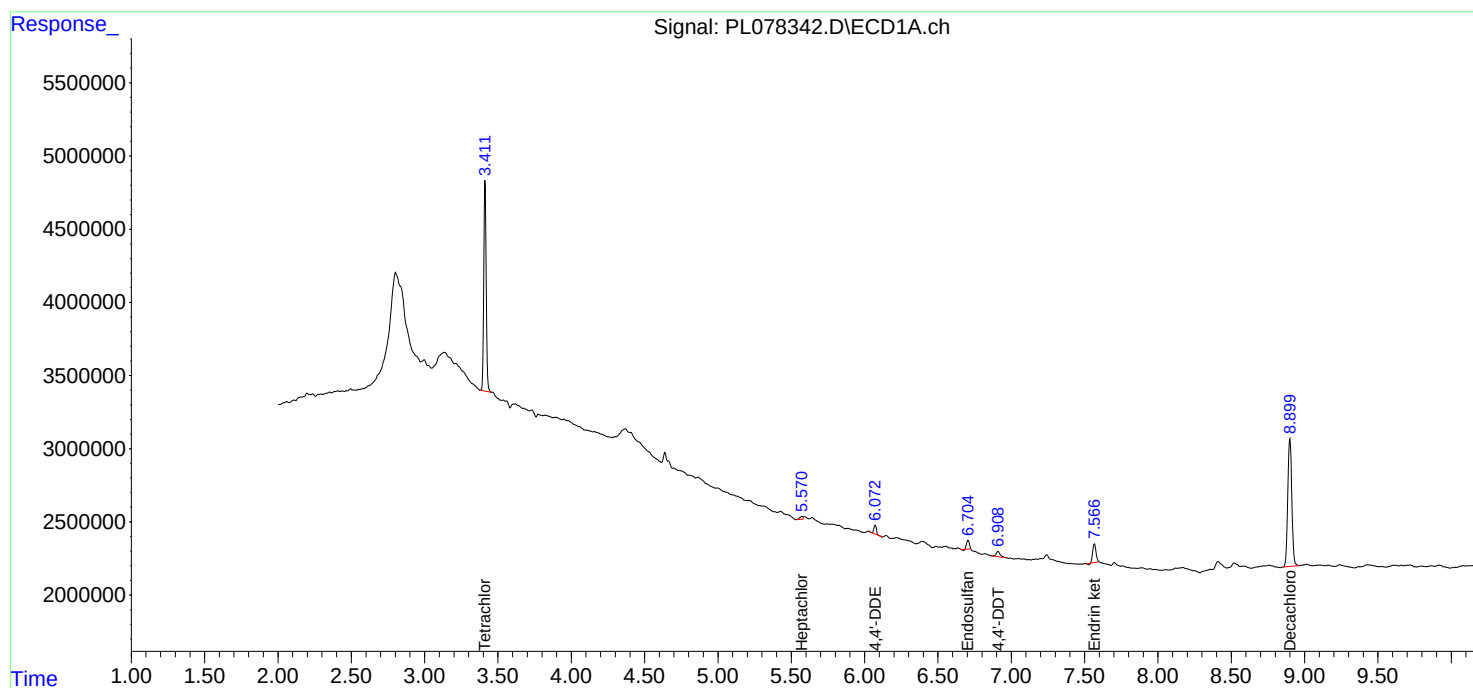


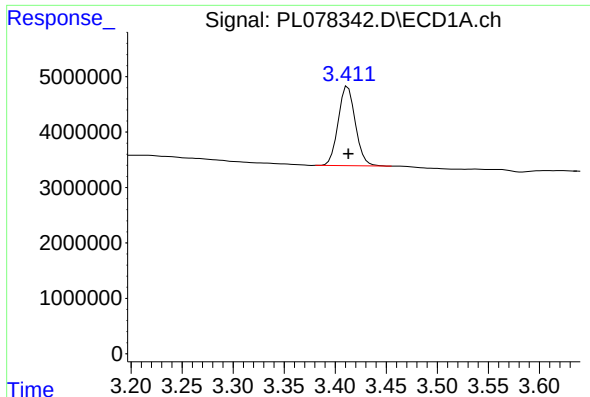

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 16808834
Conc: 10.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-4

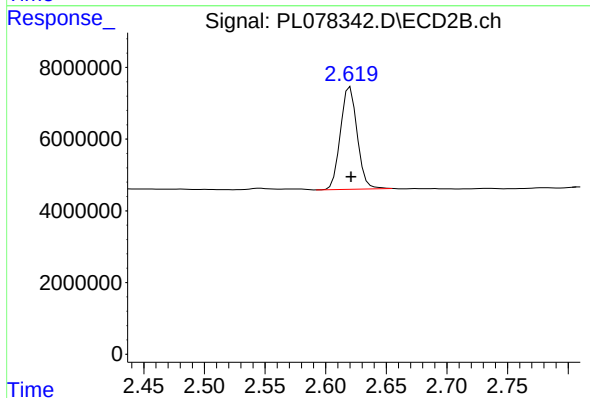


#1 Tetrachloro-m-xylene

R.T.: 2.620 min
Delta R.T.: 0.000 min
Response: 27438653
Conc: 10.38 ng/ml

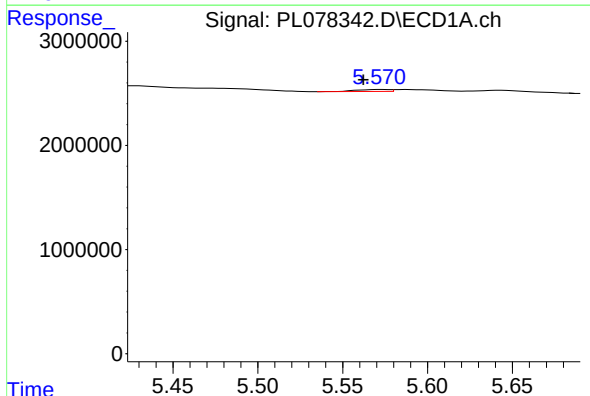


#8 Heptachlor epoxide

R.T.: 5.572 min
Delta R.T.: 0.010 min
Response: 260435
Conc: 0.17 ng/ml

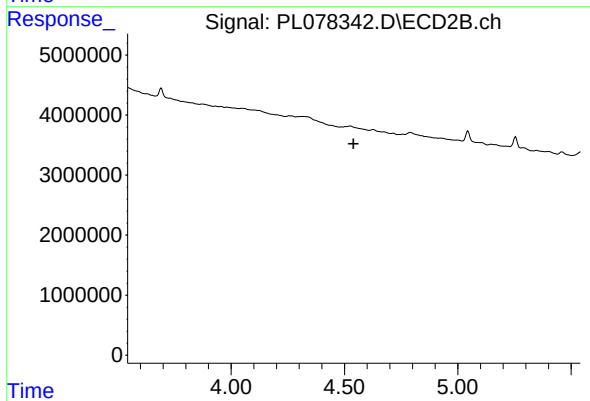

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.540 min
Response: 0
Conc: N.D.

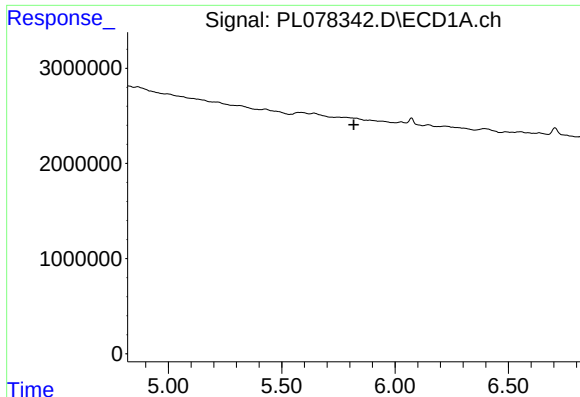

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.818 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-4

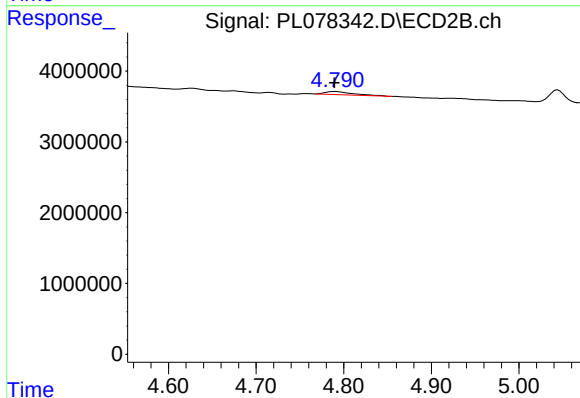


#10 gamma-Chlordane

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 1008238
Conc: 0.34 ng/ml

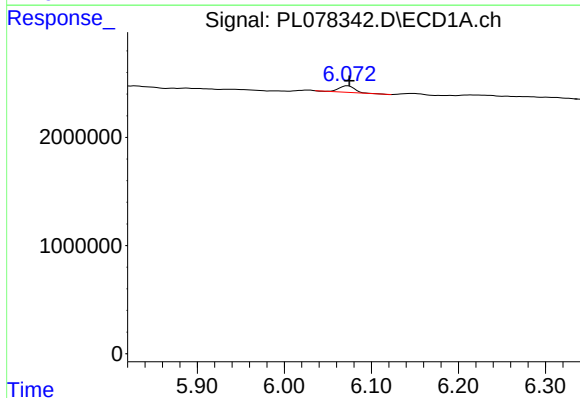


#12 4,4'-DDE

R.T.: 6.073 min
Delta R.T.: -0.002 min
Response: 771507
Conc: 0.46 ng/ml

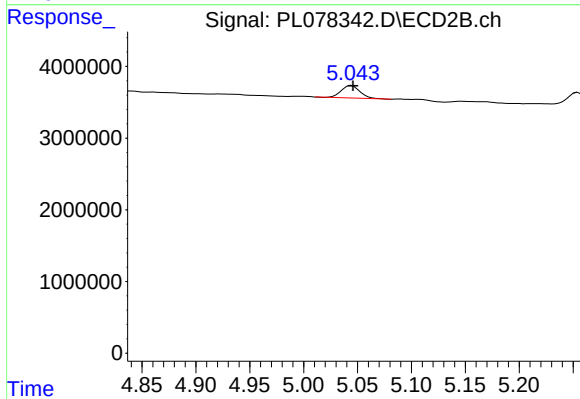

#12 4,4'-DDE


R.T.: 5.044 min
Delta R.T.: -0.001 min
Response: 2110513
Conc: 0.74 ng/ml

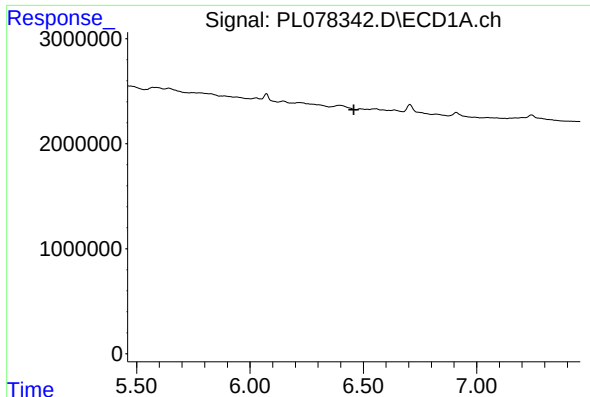

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-4

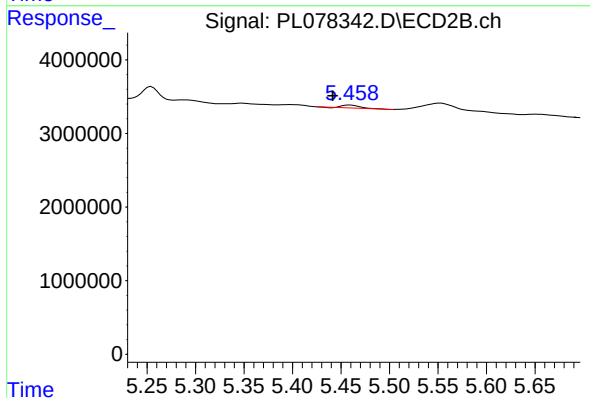


#14 Endrin

R.T.: 5.460 min
Delta R.T.: 0.018 min
Response: 520242
Conc: 0.23 ng/ml

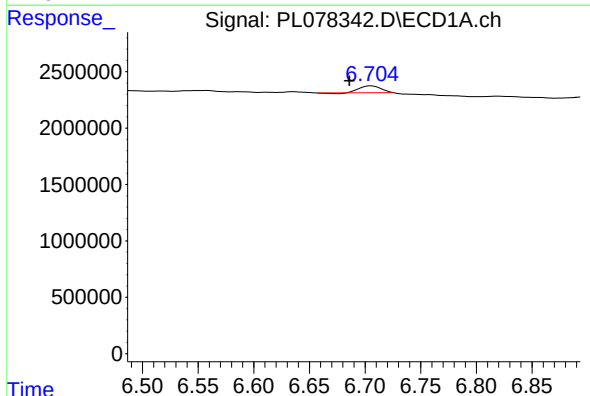


#15 Endosulfan II

R.T.: 6.705 min
Delta R.T.: 0.020 min
Response: 765100
Conc: 0.57 ng/ml

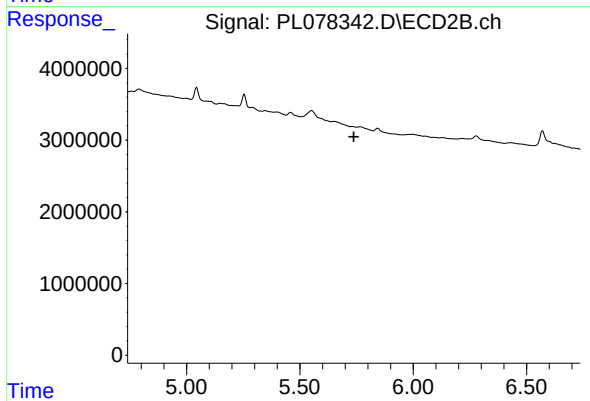

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

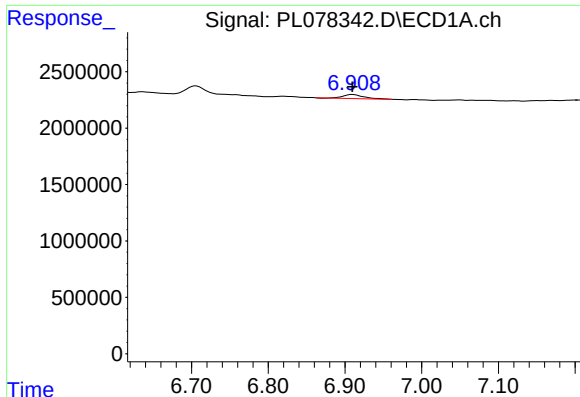

#17 4,4'-DDT


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 658792
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-4

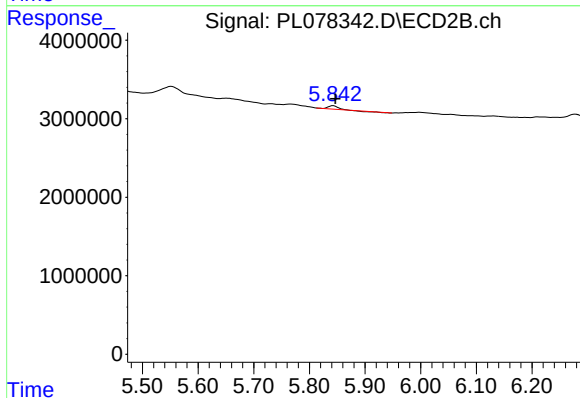


#17 4,4'-DDT

R.T.: 5.843 min
Delta R.T.: -0.004 min
Response: 390033
Conc: 0.17 ng/ml

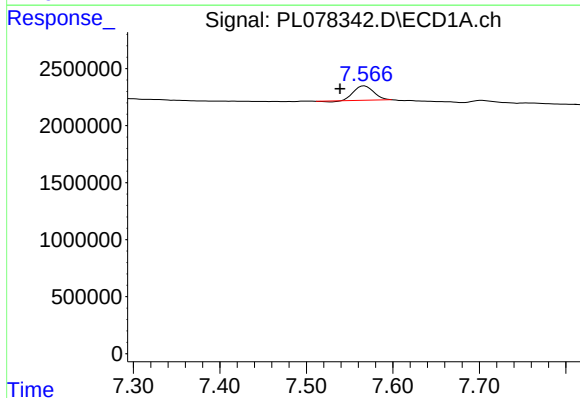


#21 Endrin ketone

R.T.: 7.567 min
Delta R.T.: 0.028 min
Response: 1986284
Conc: 1.27 ng/ml

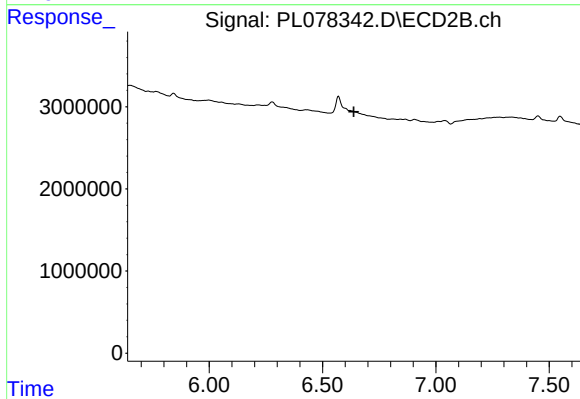

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.638 min
Response: 0
Conc: N.D.

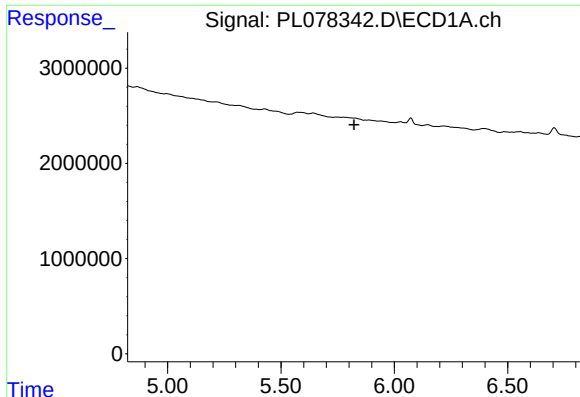

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-4

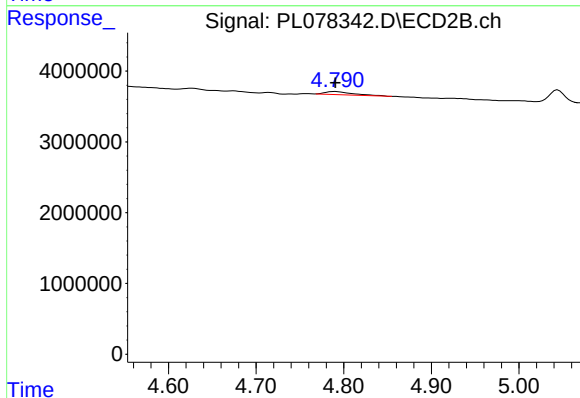


#25 Chlordane-3

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 1008238
Conc: 3.30 ng/ml

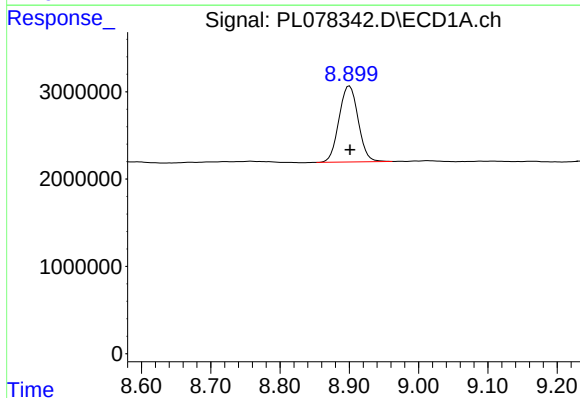

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.000 min
Response: 16719262
Conc: 10.83 ng/ml

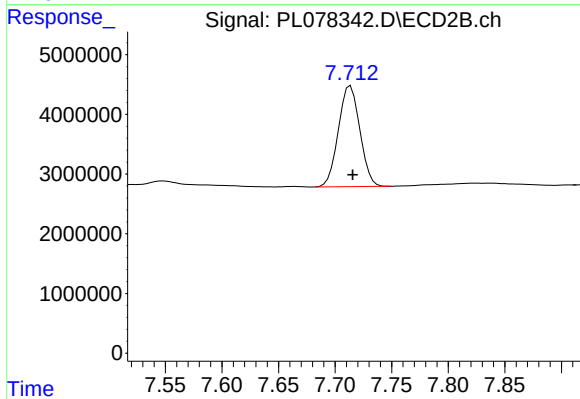

#28 Decachlorobiphenyl

R.T.: 7.714 min
Delta R.T.: -0.002 min
Response: 22303549
Conc: 10.26 ng/ml