

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
 Data File : PL078346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 19:23
 Operator : AR\AJ
 Sample : PB148164TB
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB148164TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 23:36:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	2.621	33409547	53215122	20.216	20.132
28)	SA Decachlor...	8.899	7.713	29512710	42931326	19.117	19.749
Target Compounds							
8)	B Heptachlo...	5.584f	4.529	267807	293898	0.176	0.100 #
10)	B gamma-Chl...	0.000	4.791	0	860700	N.D.	0.288 #
12)	B 4,4'-DDE	0.000	5.047	0	361121	N.D.	0.126 #
14)	MA Endrin	0.000	5.464f	0	75439	N.D.	0.033 #
15)	B Endosulfa...	6.706f	0.000	709613	0	0.529	N.D. #
20)	A Methoxychlor	0.000	6.439	0	382504	N.D.	0.303 #
21)	B Endrin ke...	7.566f	0.000	2216019	0	1.420	N.D. #
25)	Chlordane-3	0.000	4.791	0	860700	N.D.	2.813 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
Data File : PL078346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 19:23
Operator : AR\AJ
Sample : PB148164TB
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB148164TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 23:36:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

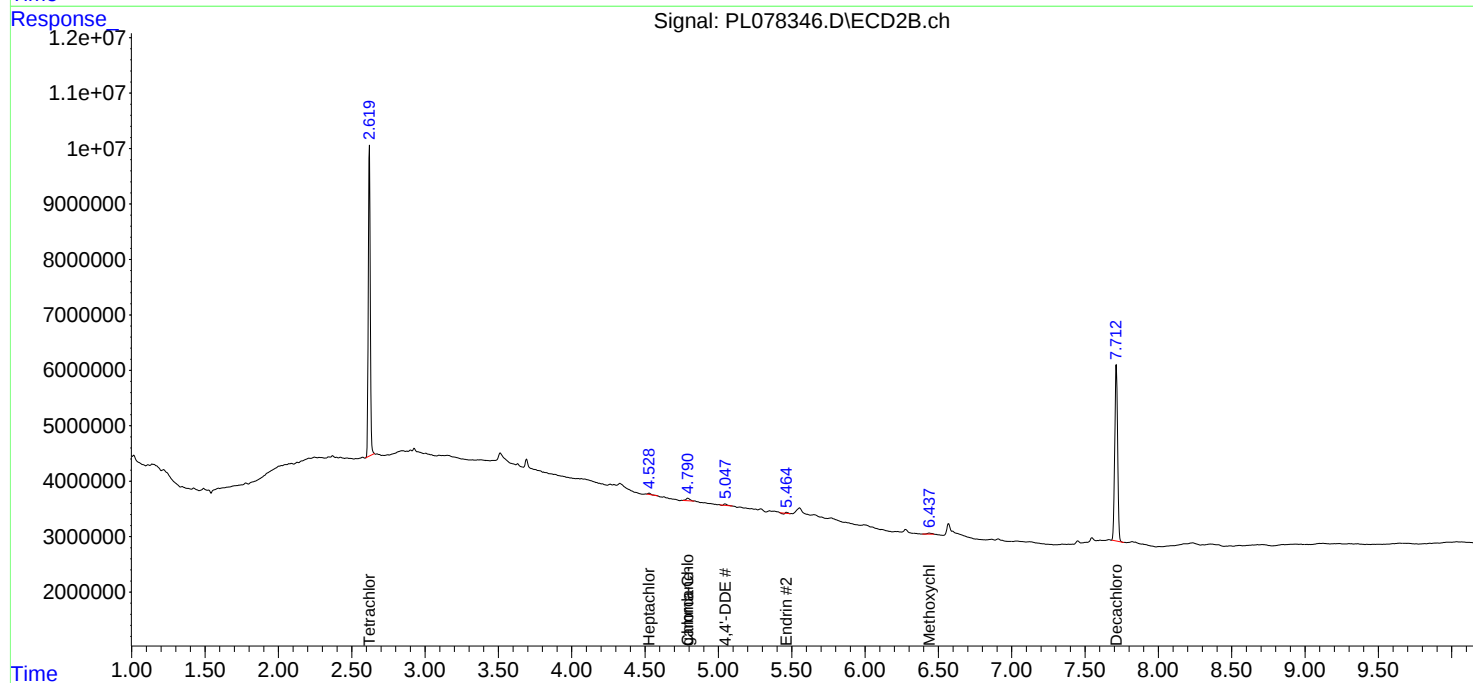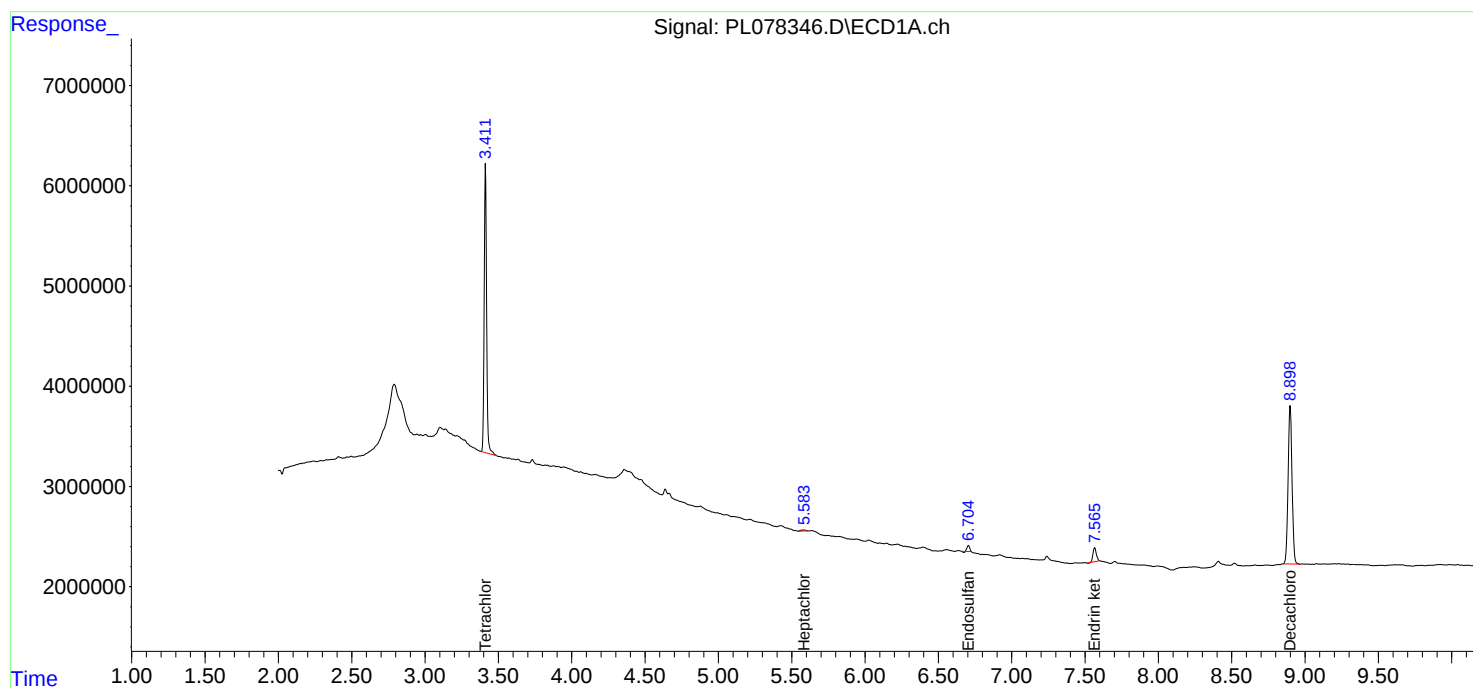


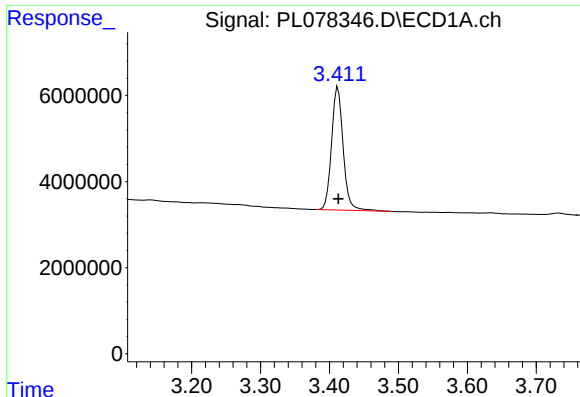

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 33409547
Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB148164TB

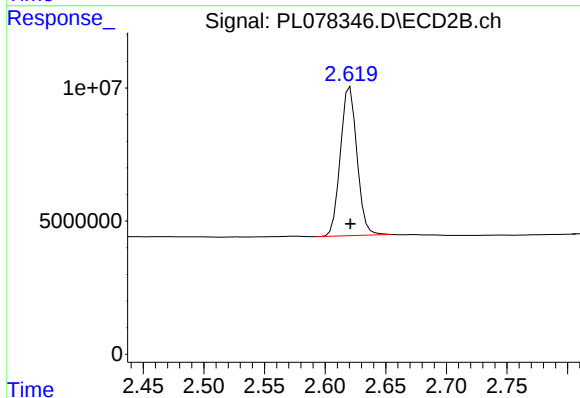


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 53215122
Conc: 20.13 ng/ml

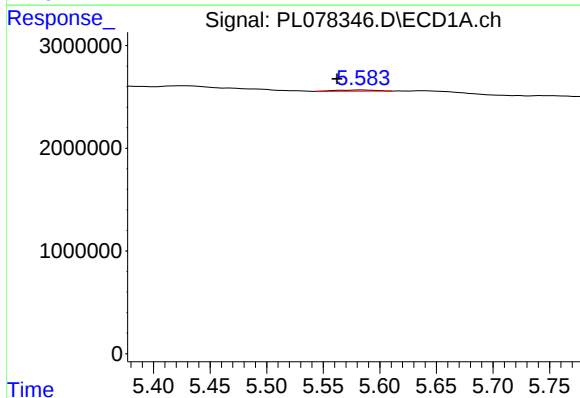


#8 Heptachlor epoxide

R.T.: 5.584 min
Delta R.T.: 0.022 min
Response: 267807
Conc: 0.18 ng/ml

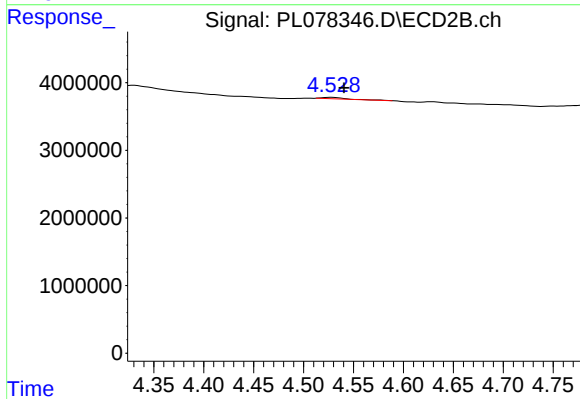

#8 Heptachlor epoxide

R.T.: 4.529 min
Delta R.T.: -0.011 min
Response: 293898
Conc: 0.10 ng/ml

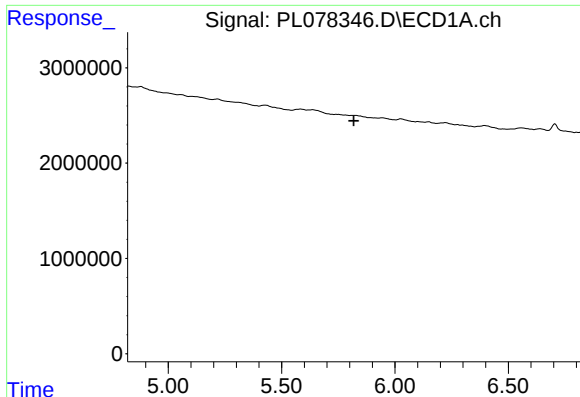


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.818 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB148164TB

#10 gamma-Chlordane

R.T.: 4.791 min
Delta R.T.: 0.002 min
Response: 860700
Conc: 0.29 ng/ml

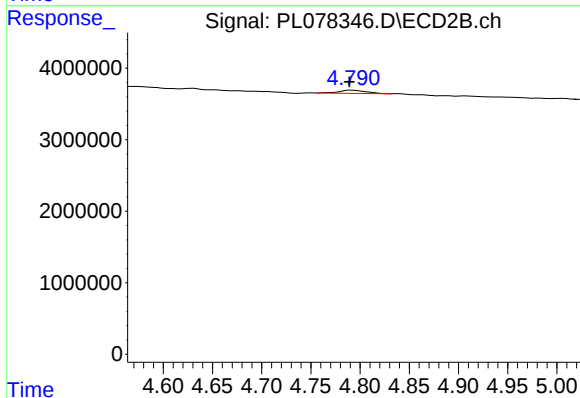



#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.075 min
Response: 0
Conc: N.D.

#12 4,4'-DDE

R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 361121
Conc: 0.13 ng/ml

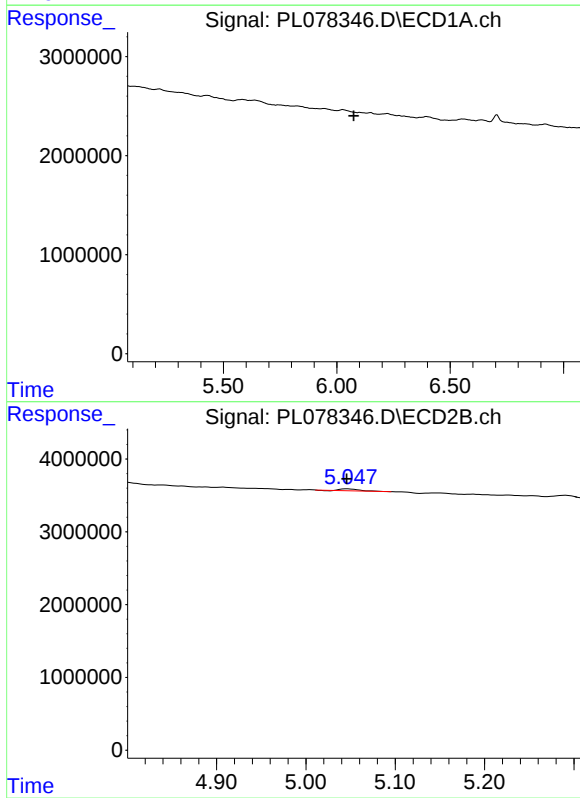


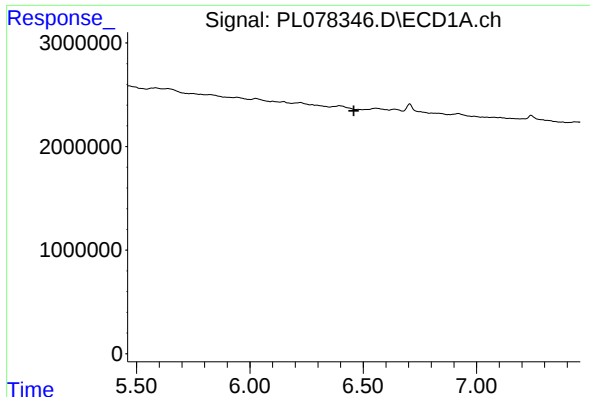

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB148164TB

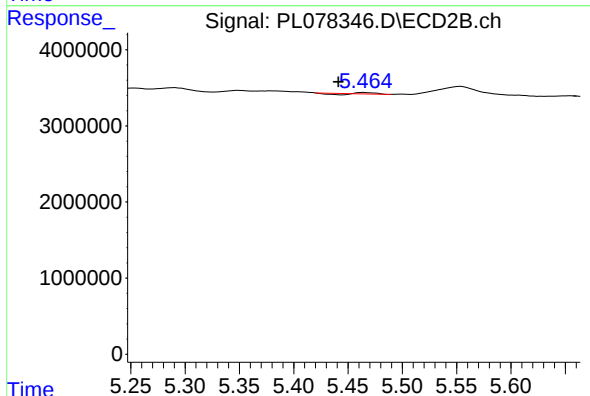


#14 Endrin

R.T.: 5.464 min
Delta R.T.: 0.023 min
Response: 75439
Conc: 0.03 ng/ml

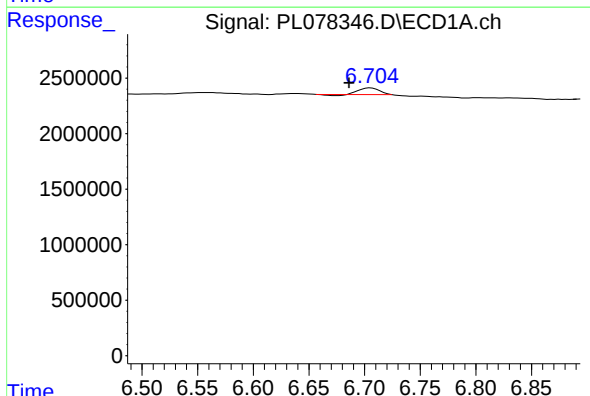


#15 Endosulfan II

R.T.: 6.706 min
Delta R.T.: 0.020 min
Response: 709613
Conc: 0.53 ng/ml

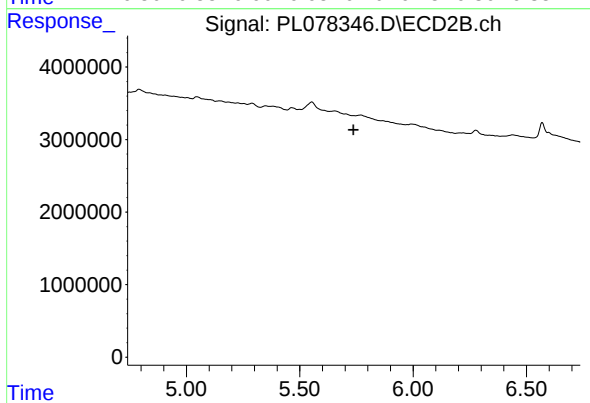

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

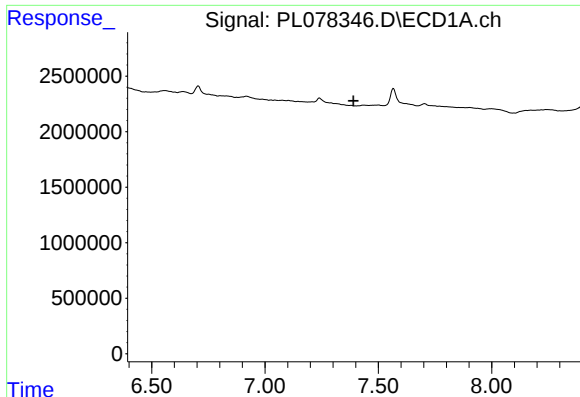

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB148164TB

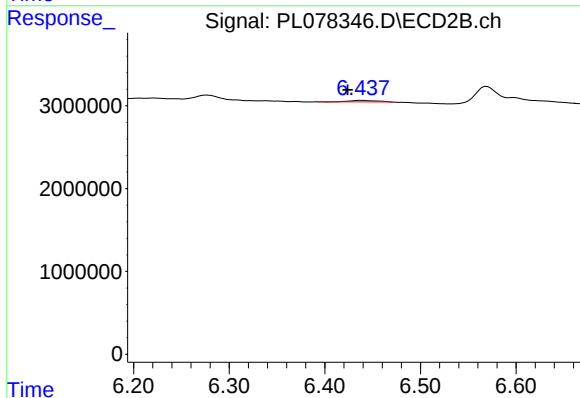


#20 Methoxychlor

R.T.: 6.439 min
Delta R.T.: 0.015 min
Response: 382504
Conc: 0.30 ng/ml

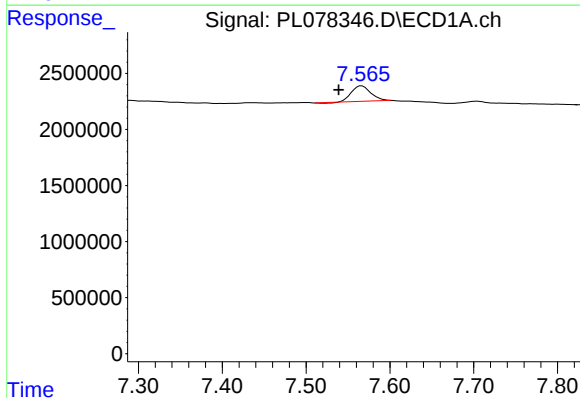


#21 Endrin ketone

R.T.: 7.566 min
Delta R.T.: 0.027 min
Response: 2216019
Conc: 1.42 ng/ml

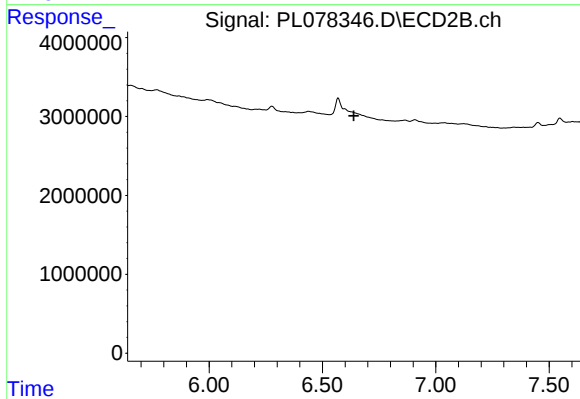

#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.638 min
Response: 0
Conc: N.D.

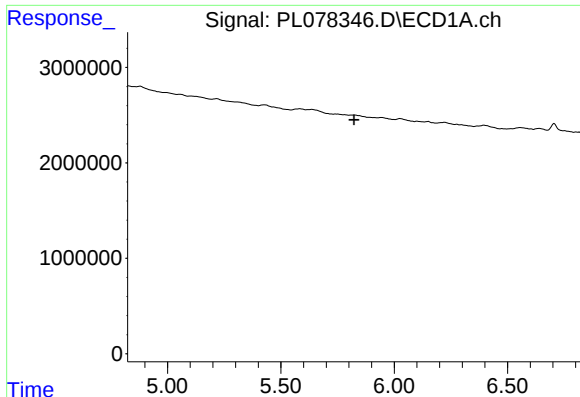


#25 Chlorordane-3

R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB148164TB

#25 Chlorordane-3

R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 860700
Conc: 2.81 ng/ml

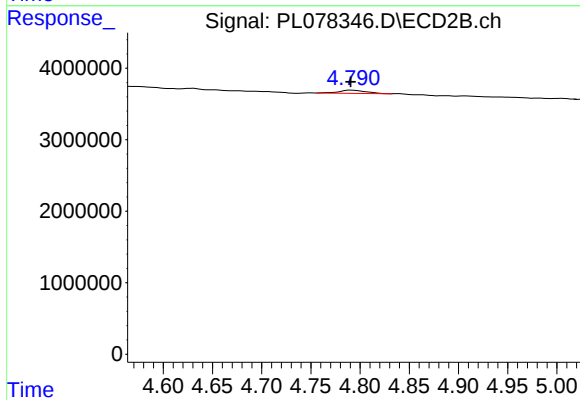

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: -0.002 min
Response: 29512710
Conc: 19.12 ng/ml

#28 Decachlorobiphenyl

R.T.: 7.713 min
Delta R.T.: -0.002 min
Response: 42931326
Conc: 19.75 ng/ml