

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
 Data File : PL078316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 11:35
 Operator : AR\AJ
 Sample : N5101-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-2-101122

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/14/2022
 Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 01:31:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.621	17085438	29577747	10.338m	11.190
28)	SA Decachlor...	8.911	7.720	19328894	26673326	12.520	12.270

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101322\
Data File : PL078316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 11:35
Operator : AR\AJ
Sample : N5101-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-2-101122


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/14/2022
Supervised By : Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:31:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

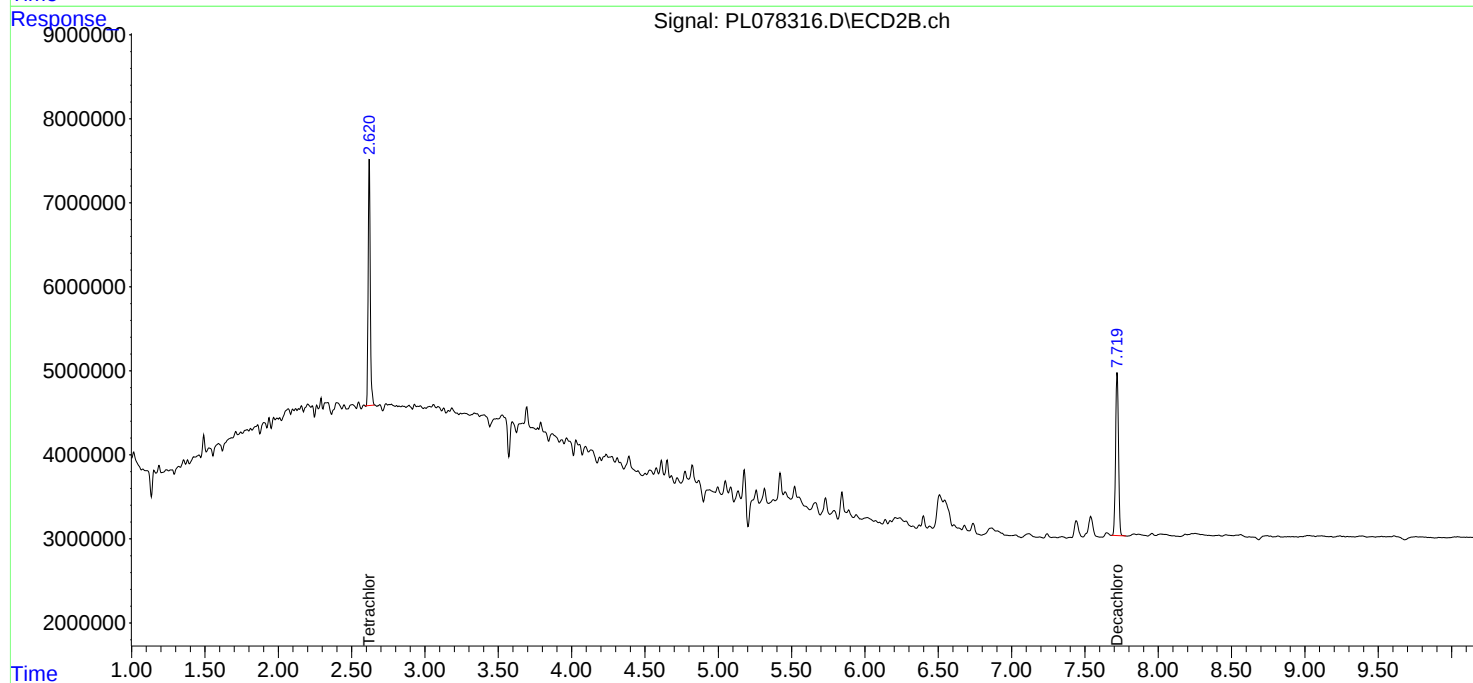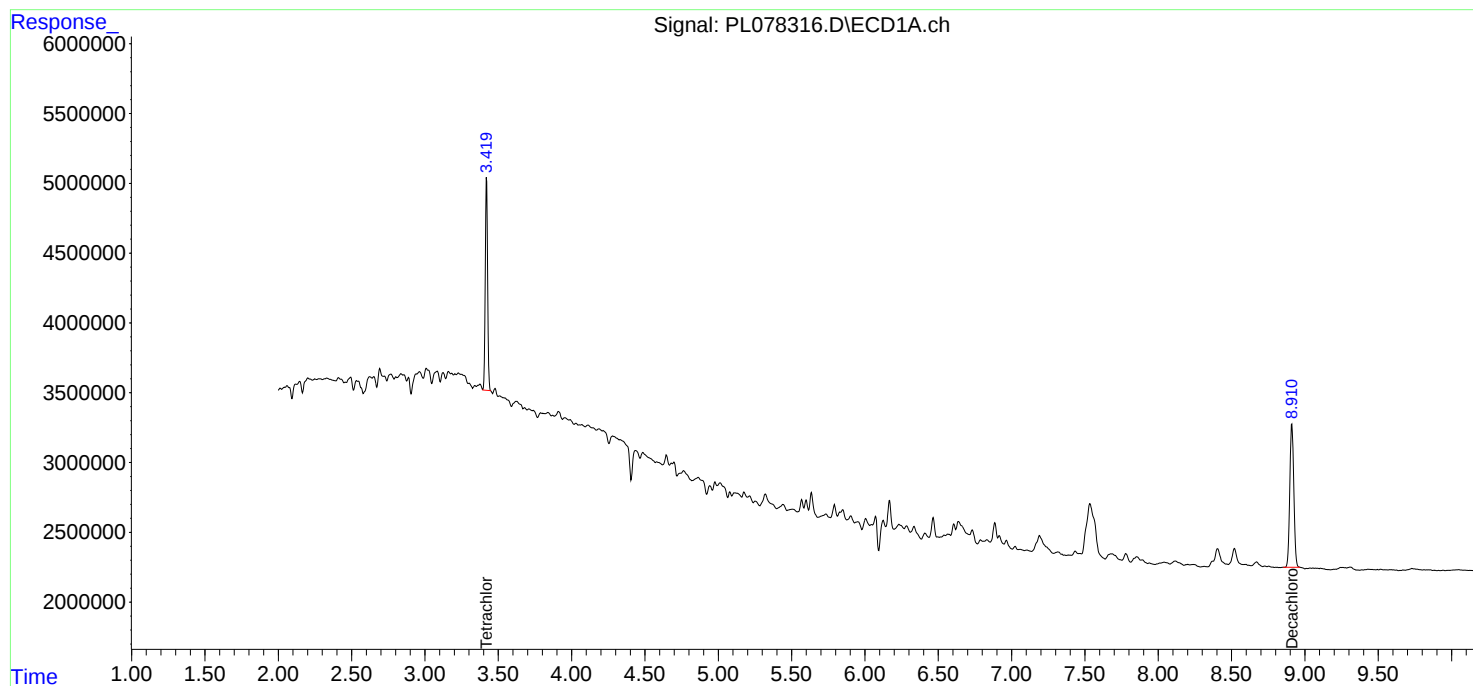

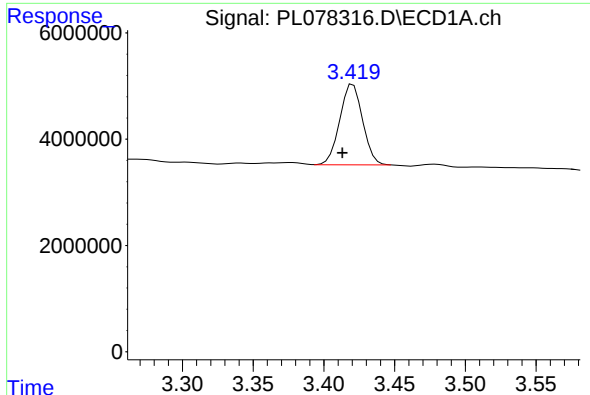


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: 0.006 min
Response: 17085438
Conc: 10.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-2-101122


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

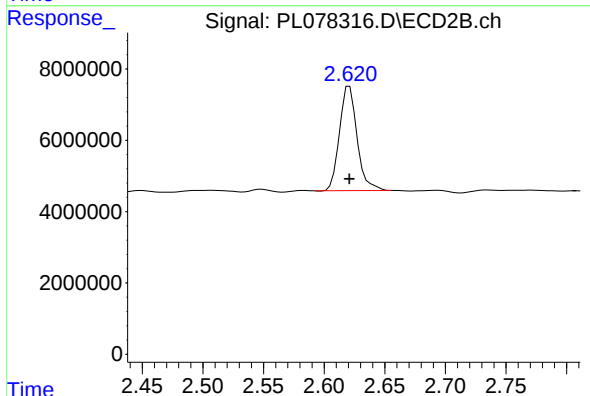


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 29577747
Conc: 11.19 ng/ml

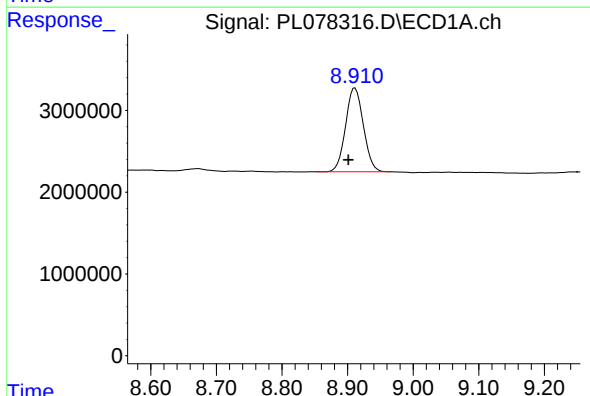

#28 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.010 min
Response: 19328894
Conc: 12.52 ng/ml

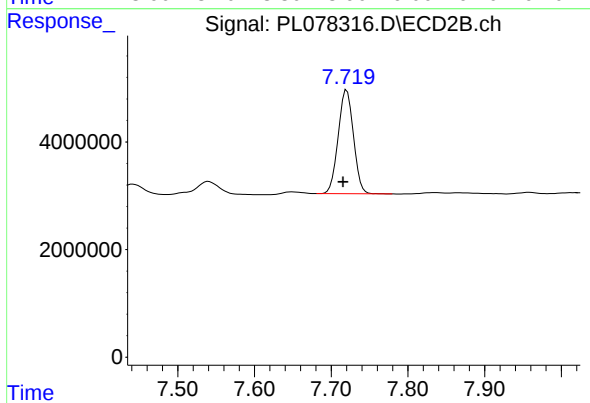

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: 0.005 min
Response: 26673326
Conc: 12.27 ng/ml