

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111620\
 Data File : PL063029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2020 12:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 00:53:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.951	33485322	61387872	19.467	20.889
28)	SA Decachlor...	8.129	8.992	35004119	44868899	21.819	21.438
Target Compounds							
2)	A alpha-BHC	3.853	0.000	2474162	0	0.970	N.D. #
7)	B delta-BHC	0.000	4.998	0	7948785	N.D.	2.271 #
8)	B Heptachlo...	5.117	5.827	8002065	22412887	4.386	6.921 #
18)	B Endrin al...	0.000	6.947f	0	4217745	N.D.	1.849 #
19)	B Endosulfa...	0.000	7.223f	0	2554387	N.D.	1.065 #
22)	Mirex	7.283f	0.000	7338076	0	5.176	N.D. #
23)	Chlordane-1	4.288f	0.000	18754961	0	363.821	N.D. #
24)	Chlordane-2	0.000	5.377f	0	5918900	N.D.	54.284 #
27)	Chlordane-5	0.000	6.947f	0	4217745	N.D.	56.542 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111620\
Data File : PL063029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2020 12:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 00:53:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

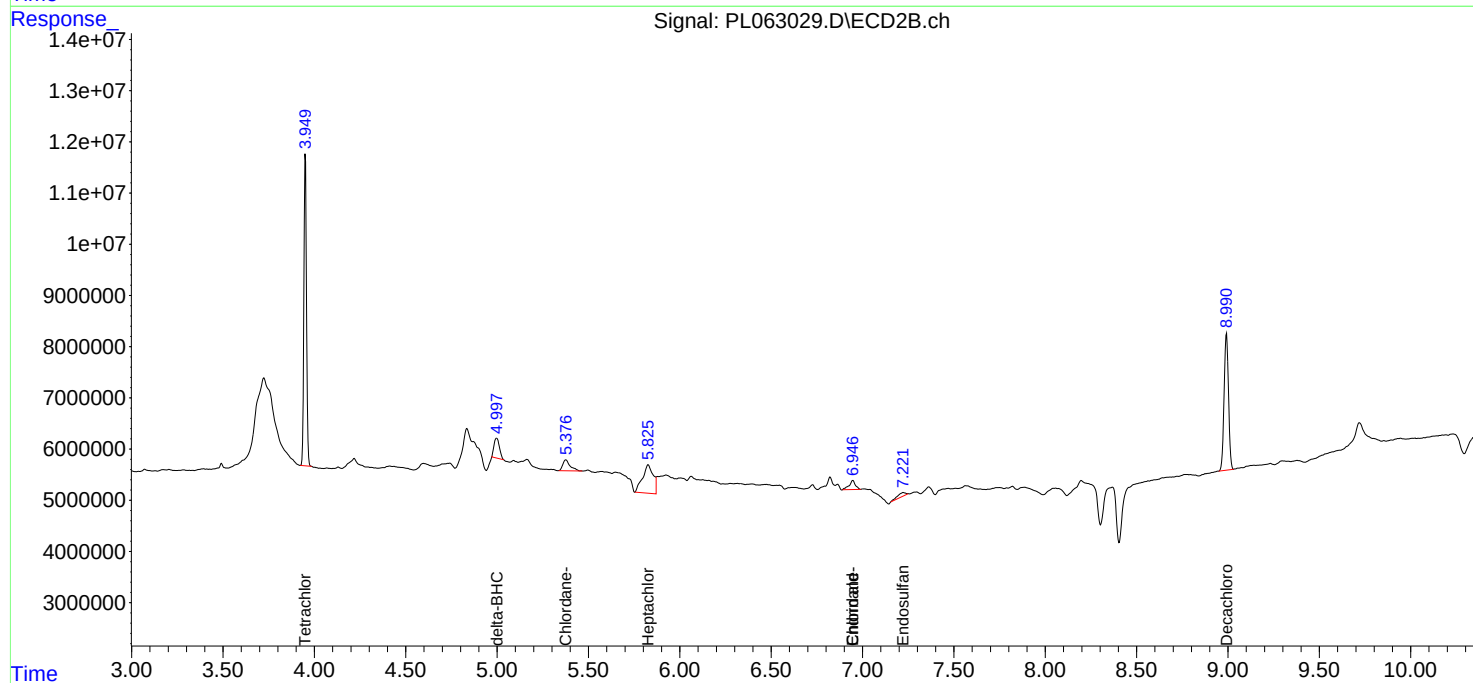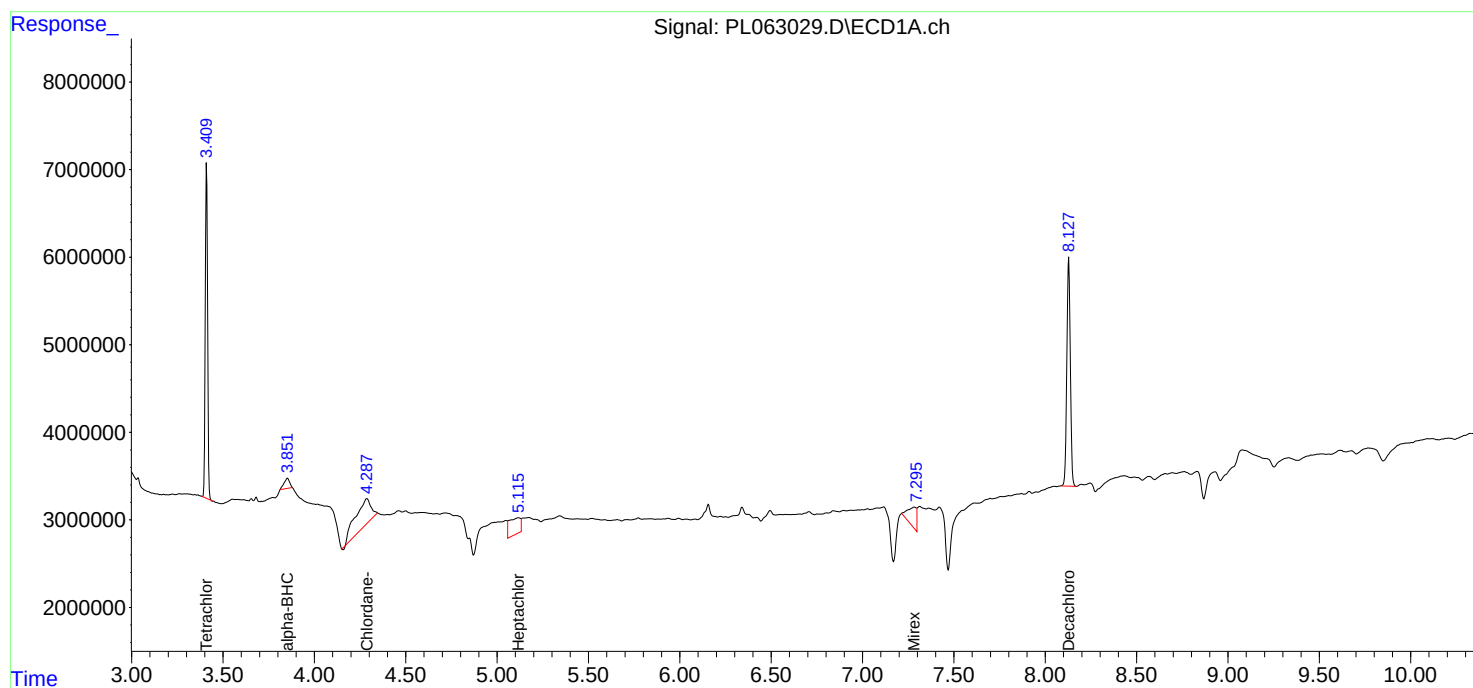


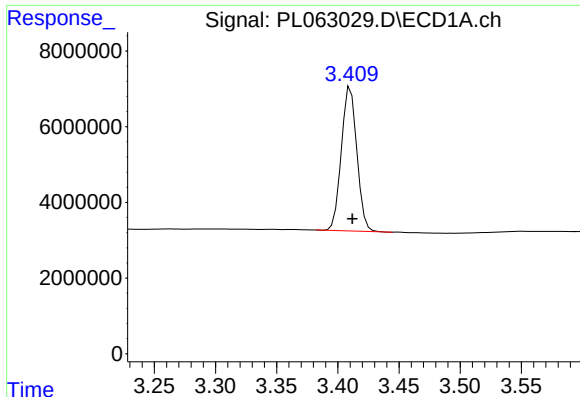

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 33485322
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

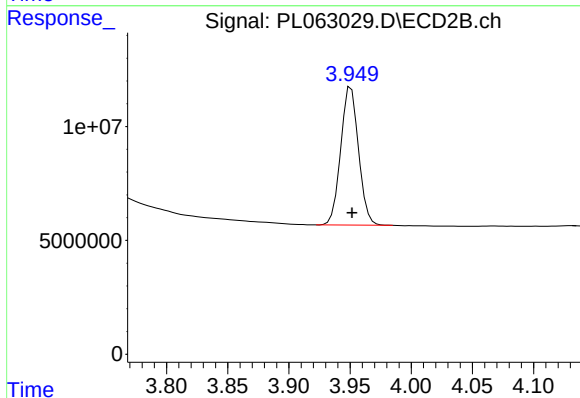


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 61387872
Conc: 20.89 ng/ml

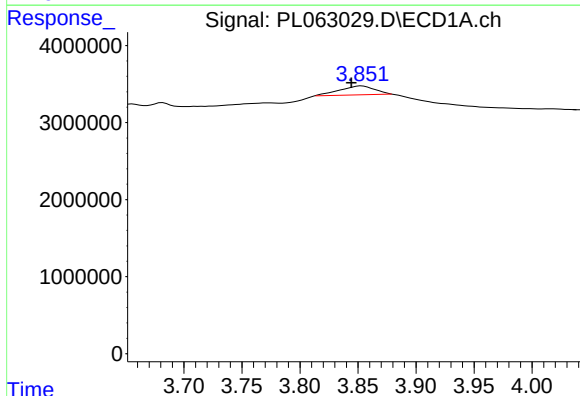


#2 alpha-BHC

R.T.: 3.853 min
Delta R.T.: 0.009 min
Response: 2474162
Conc: 0.97 ng/ml

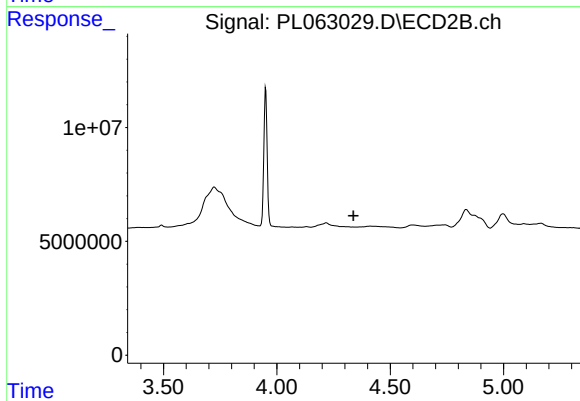

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.338 min
Response: 0
Conc: N.D.

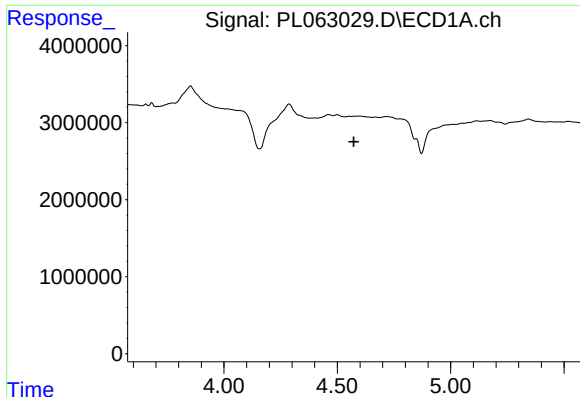

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

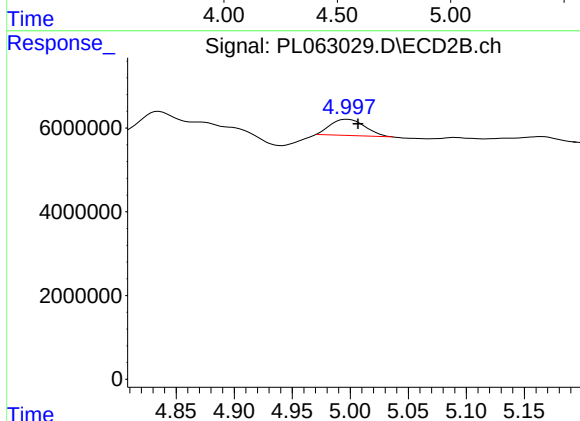


#7 delta-BHC

R.T.: 4.998 min
Delta R.T.: -0.009 min
Response: 7948785
Conc: 2.27 ng/ml

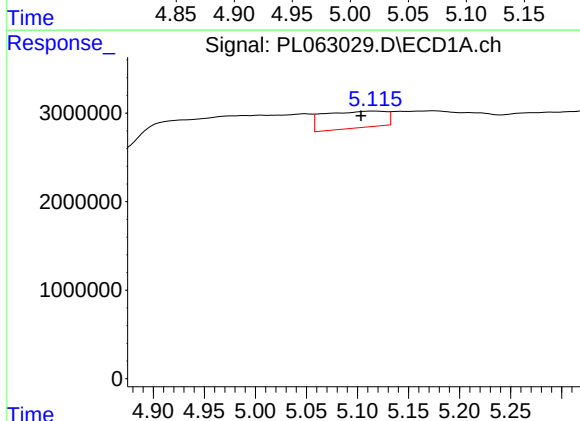


#8 Heptachlor epoxide

R.T.: 5.117 min
Delta R.T.: 0.014 min
Response: 8002065
Conc: 4.39 ng/ml

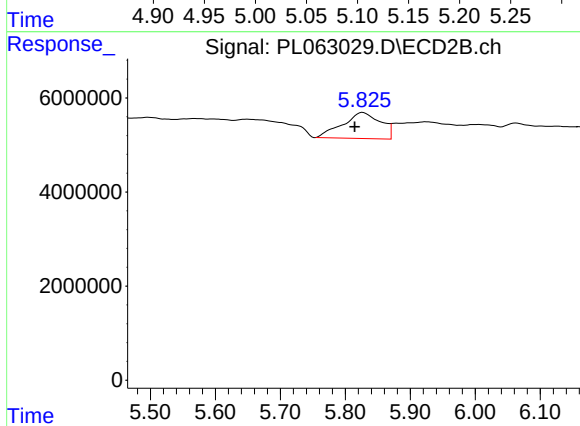

#8 Heptachlor epoxide


R.T.: 5.827 min
Delta R.T.: 0.012 min
Response: 22412887
Conc: 6.92 ng/ml

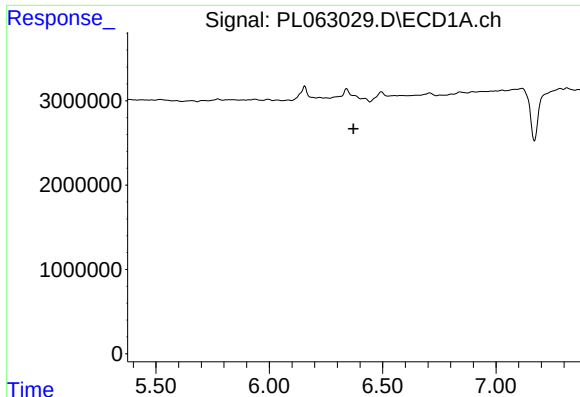

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

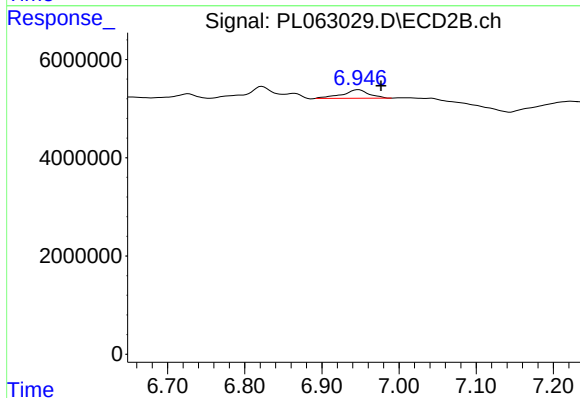


#18 Endrin aldehyde

R.T.: 6.947 min
Delta R.T.: -0.029 min
Response: 4217745
Conc: 1.85 ng/ml

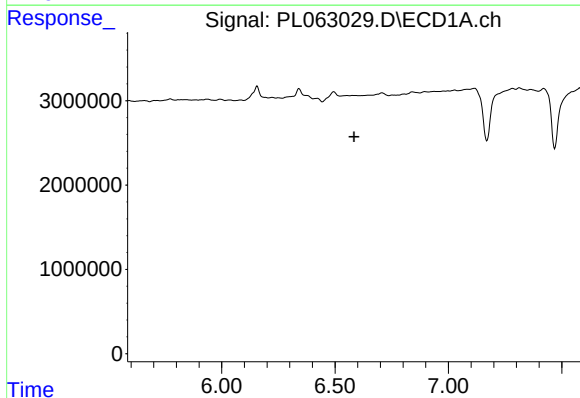


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

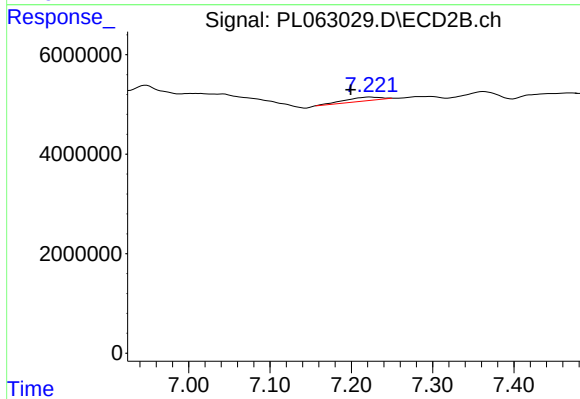

#19 Endosulfan Sulfate


R.T.: 7.223 min
Delta R.T.: 0.023 min
Response: 2554387
Conc: 1.06 ng/ml

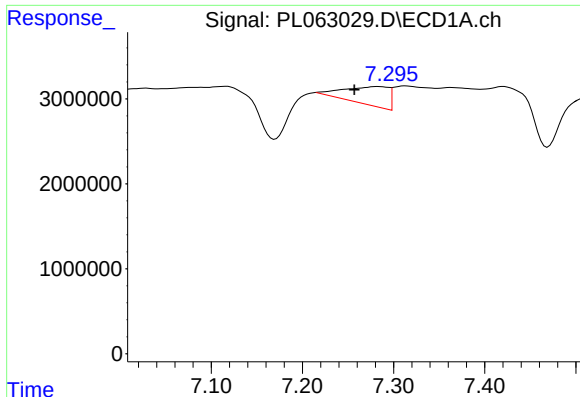

#22 Mirex


R.T.: 7.283 min
Delta R.T.: 0.026 min
Response: 7338076
Conc: 5.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

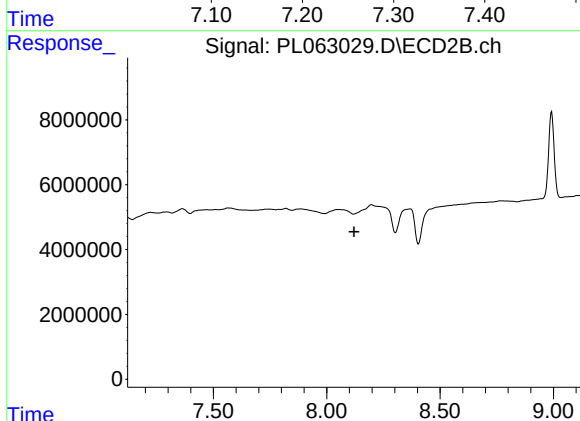


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

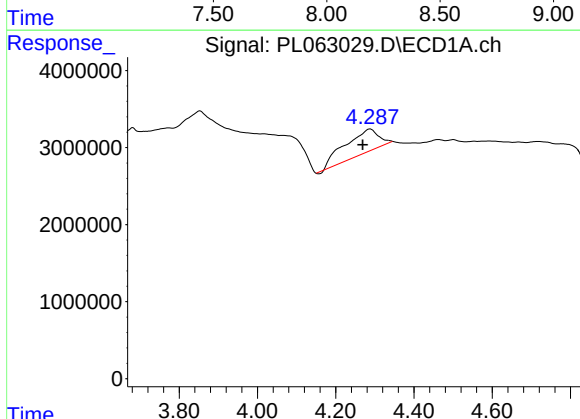


#23 Chlordane-1

R.T.: 4.288 min
Delta R.T.: 0.019 min
Response: 18754961
Conc: 363.82 ng/ml

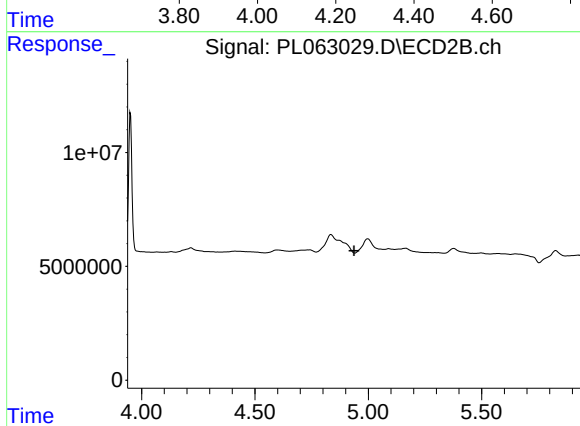

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

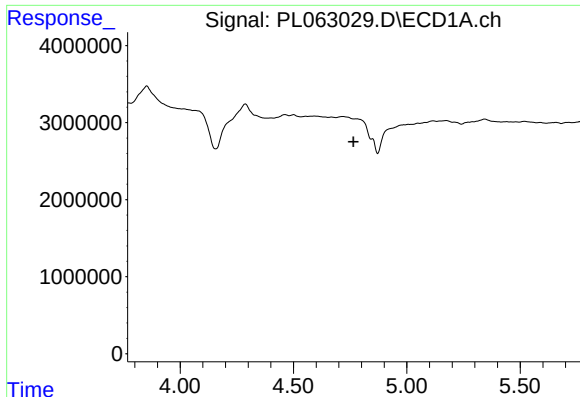

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

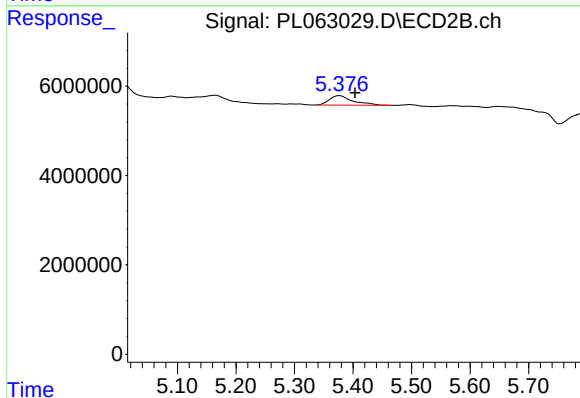


#24 Chlordane-2

R.T.: 5.377 min
Delta R.T.: -0.027 min
Response: 5918900
Conc: 54.28 ng/ml

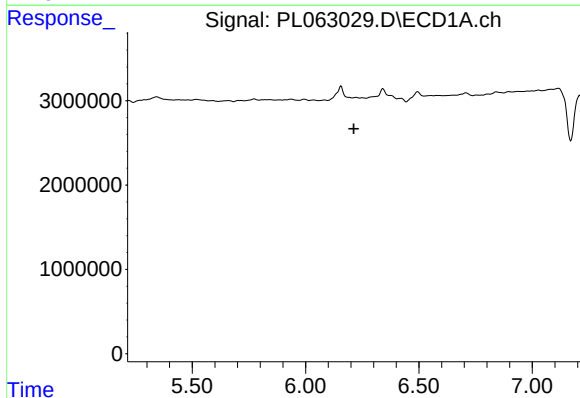


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.213 min
Response: 0
Conc: N.D.

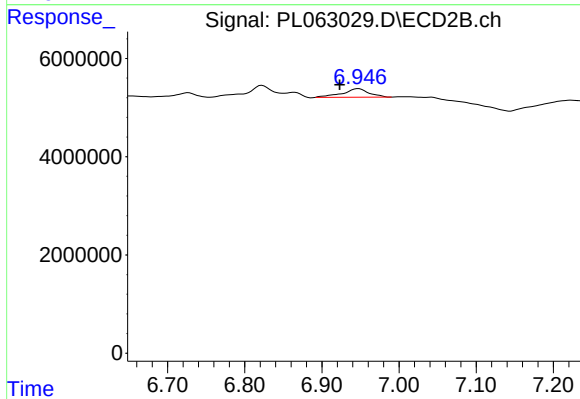

#27 Chlordane-5


R.T.: 6.947 min
Delta R.T.: 0.024 min
Response: 4217745
Conc: 56.54 ng/ml

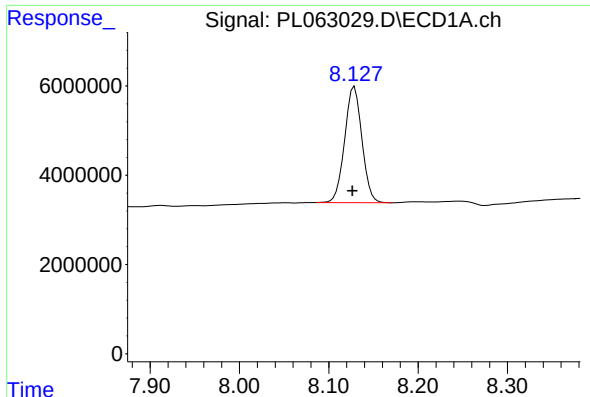

#28 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: 0.002 min
Response: 35004119
Conc: 21.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

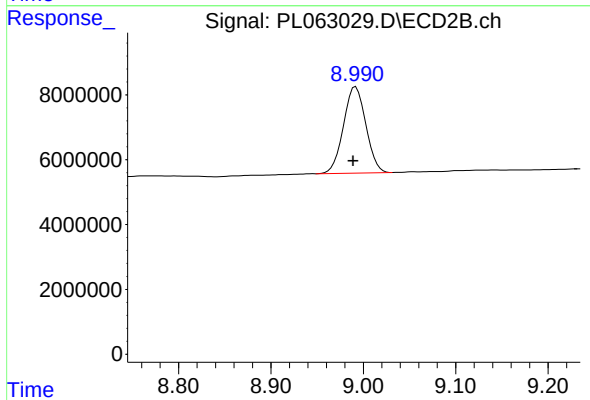

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 44868899
Conc: 21.44 ng/ml