

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111620\
 Data File : PL063030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2020 12:27
 Operator : DD\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 00:53:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	32819510	59940029	19.080	20.397
28)	SA Decachlor...	8.127	8.993	35054775	45208673	21.851	21.600
Target Compounds							
2)	A alpha-BHC	3.843	4.337	21308096	40672252	8.357	9.154
3)	MA gamma-BHC...	4.122	4.620	17943955	37238310	7.746	8.918
6)	B beta-BHC	4.372	4.792	9046194	19047537	9.471	10.115
7)	B delta-BHC	0.000	4.997	0	4662041	N.D.	1.332 #
8)	B Heptachlo...	5.130f	5.814	7968702	22450553	4.367	6.932 #
14)	MA Endrin	5.934	6.644	76355247	128.7E6	45.893	46.096
15)	B Endosulfa...	0.000	6.825f	0	1368361	N.D.	0.479 #
16)	A 4,4'-DDD	6.064	6.770	1018651	2635419	0.720	1.029 #
17)	MA 4,4'-DDT	6.303	7.068	137.2E6	232.6E6	102.779	103.611
19)	B Endosulfa...	0.000	7.222f	0	2548132	N.D.	1.062 #
20)	A Methoxychlor	6.846	7.528	199.4E6	303.5E6	231.503	245.626
21)	B Endrin ke...	7.071	7.669	13271412	1642331	7.361	0.693 #
23)	Chlordane-1	4.296f	0.000	14619886	0	283.606	N.D. #
24)	Chlordane-2	0.000	5.380f	0	3310776	N.D.	30.364 #
27)	Chlordane-5	0.000	6.946f	0	6728741	N.D.	90.204 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111620\
Data File : PL063030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2020 12:27
Operator : DD\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 00:53:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

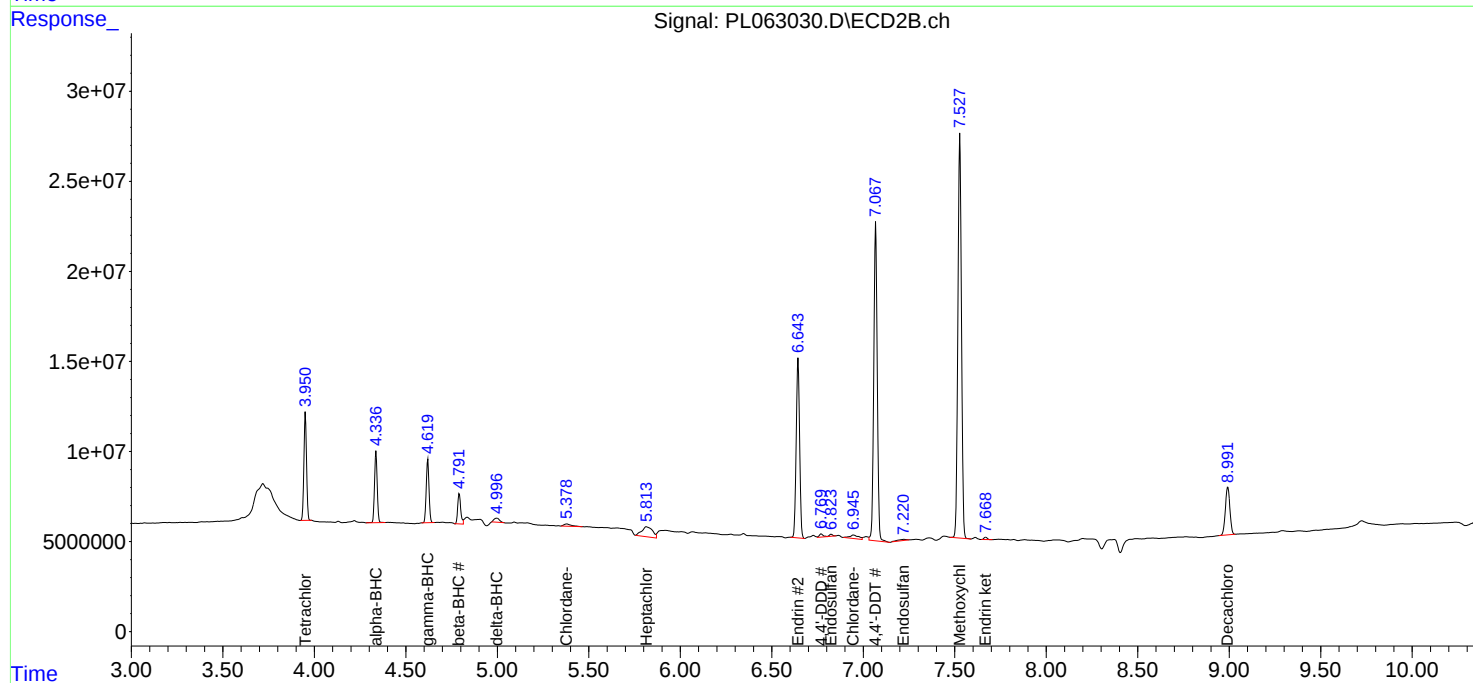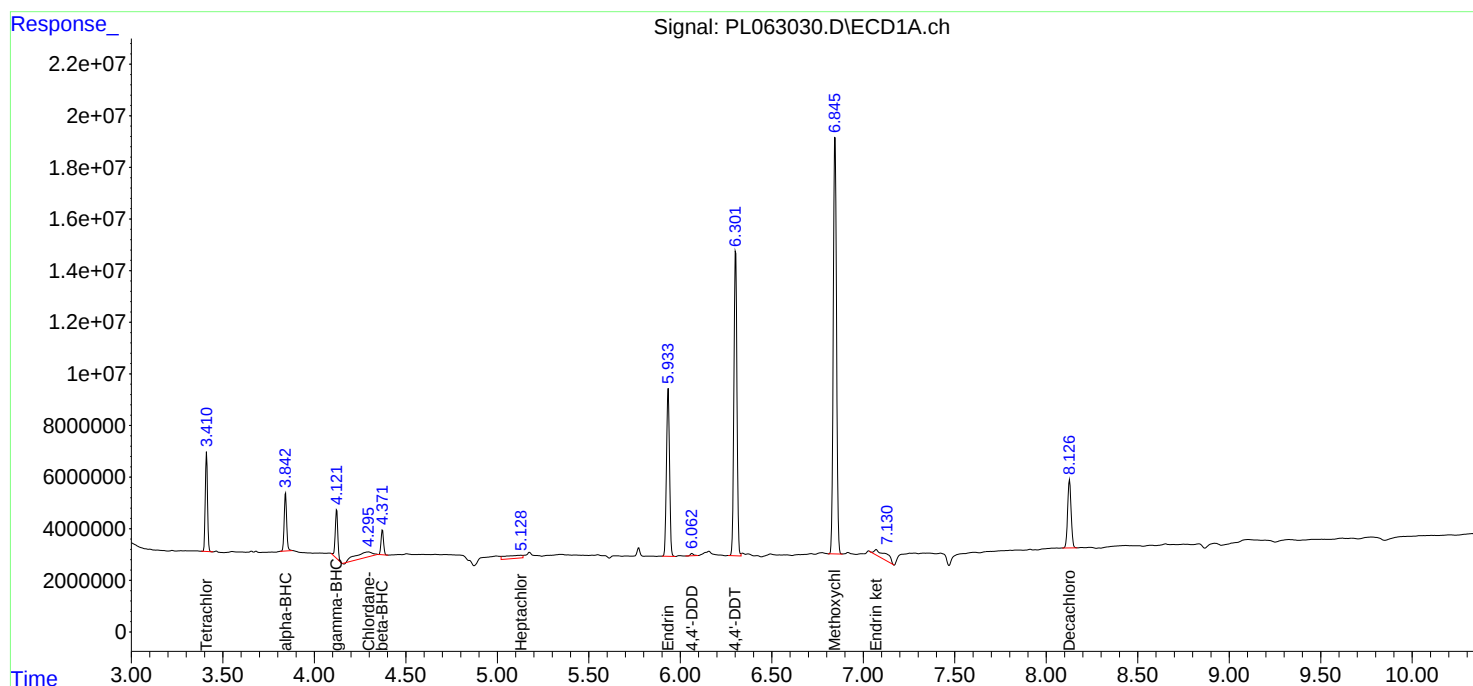


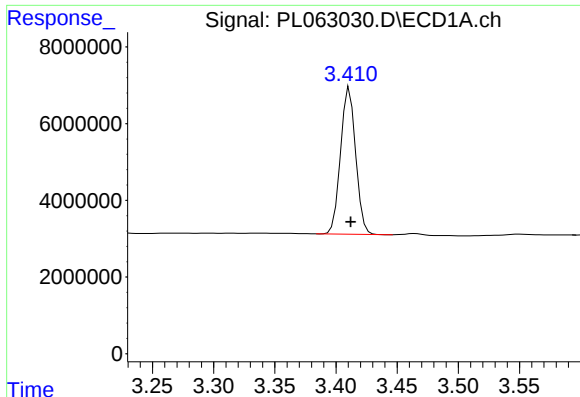

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 32819510
Conc: 19.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

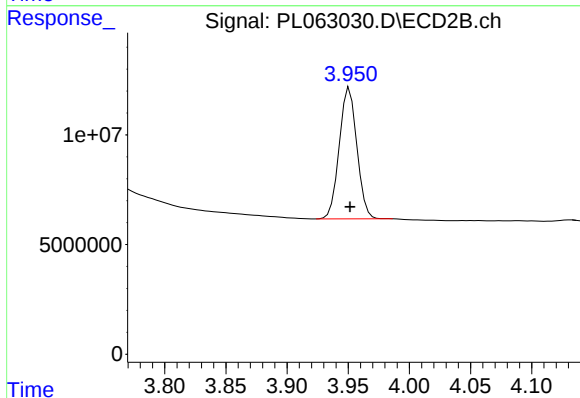


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 59940029
Conc: 20.40 ng/ml

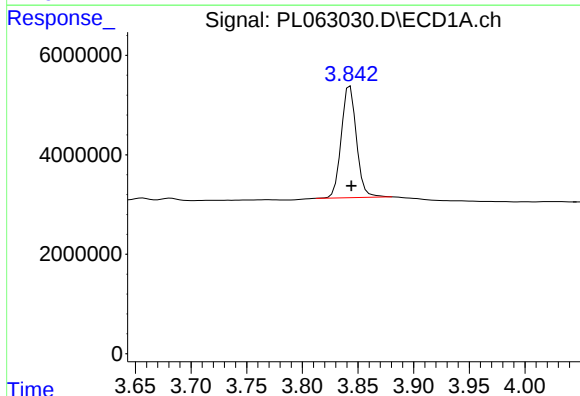


#2 alpha-BHC

R.T.: 3.843 min
Delta R.T.: -0.001 min
Response: 21308096
Conc: 8.36 ng/ml

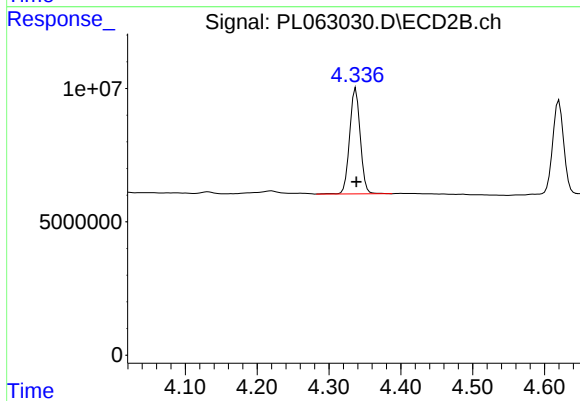

#2 alpha-BHC


R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 40672252
Conc: 9.15 ng/ml

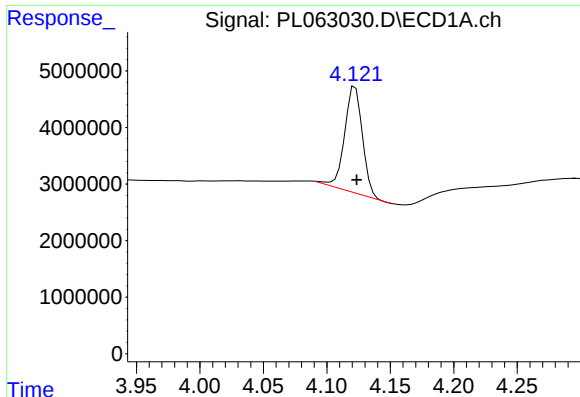

#3 gamma-BHC (Lindane)


R.T.: 4.122 min
Delta R.T.: -0.001 min
Response: 17943955
Conc: 7.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

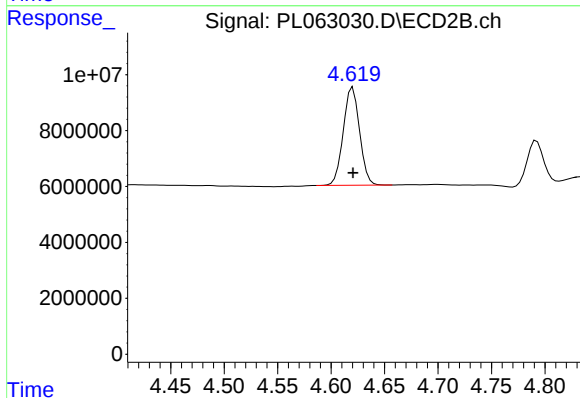


#3 gamma-BHC (Lindane)

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 37238310
Conc: 8.92 ng/ml

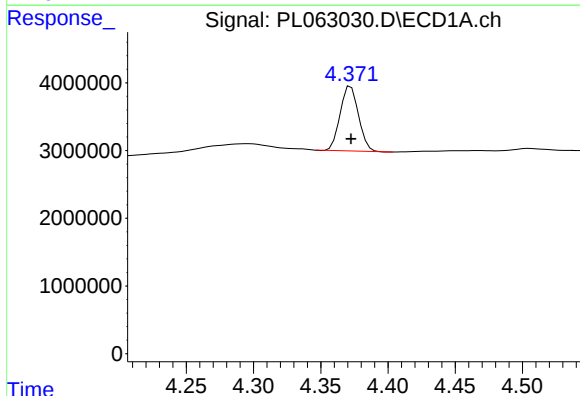


#6 beta-BHC

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 9046194
Conc: 9.47 ng/ml

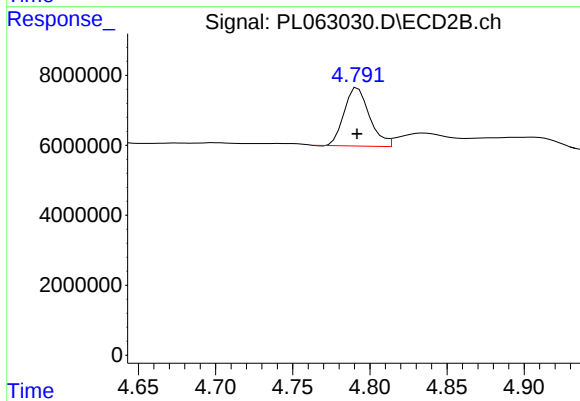

#6 beta-BHC


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 19047537
Conc: 10.12 ng/ml

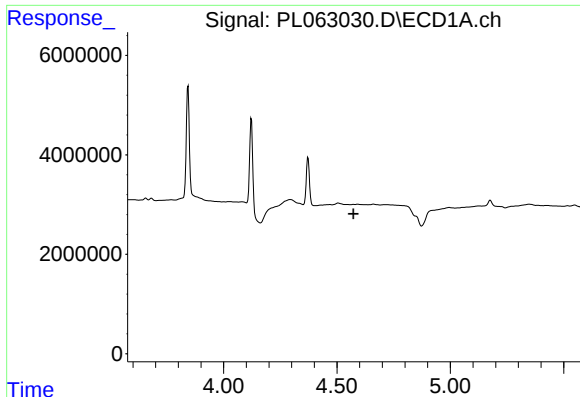

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

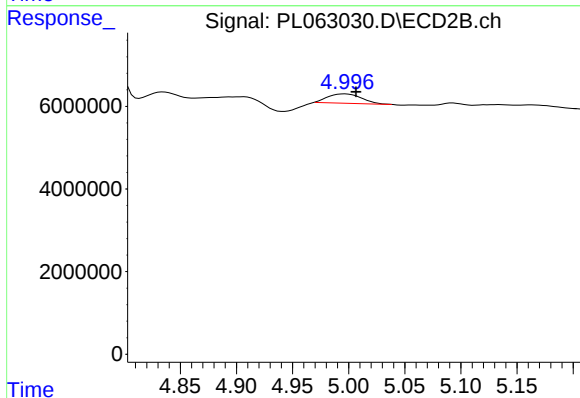


#7 delta-BHC

R.T.: 4.997 min
Delta R.T.: -0.010 min
Response: 4662041
Conc: 1.33 ng/ml

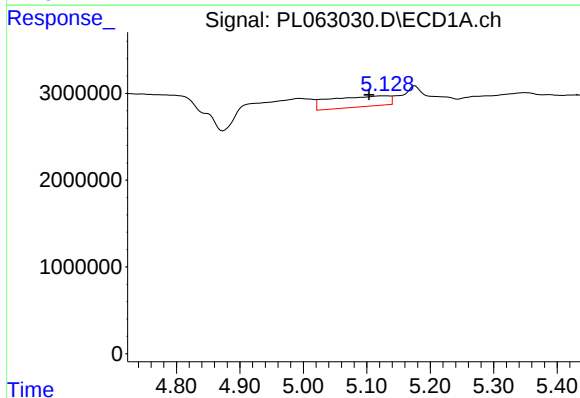


#8 Heptachlor epoxide

R.T.: 5.130 min
Delta R.T.: 0.027 min
Response: 7968702
Conc: 4.37 ng/ml

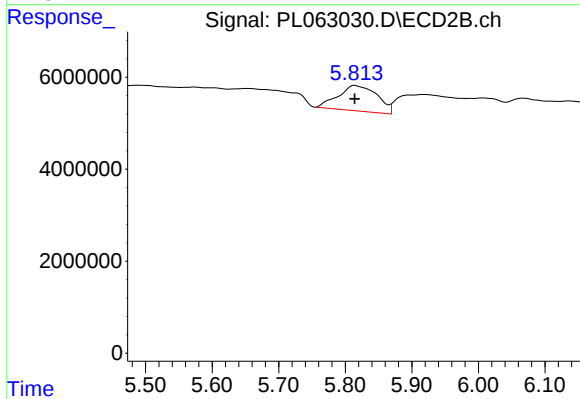

#8 Heptachlor epoxide


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 22450553
Conc: 6.93 ng/ml

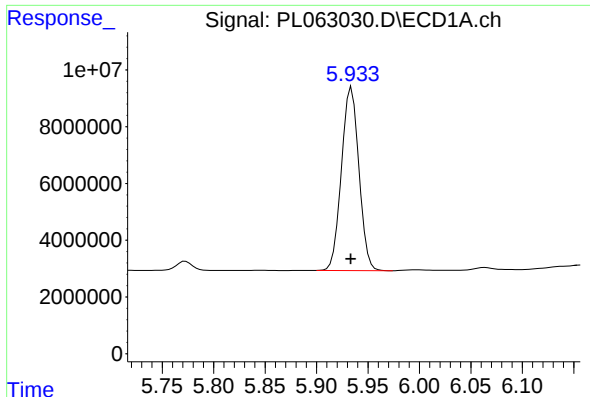

#14 Endrin


R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 76355247
Conc: 45.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

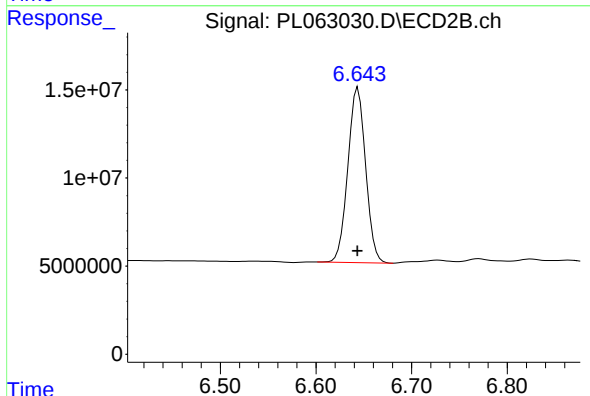


#14 Endrin

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 128660013
Conc: 46.10 ng/ml

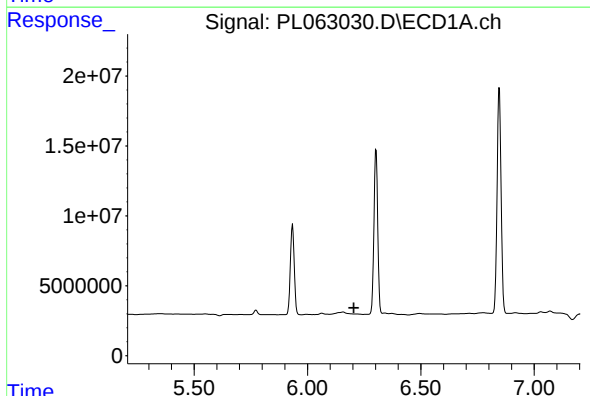


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

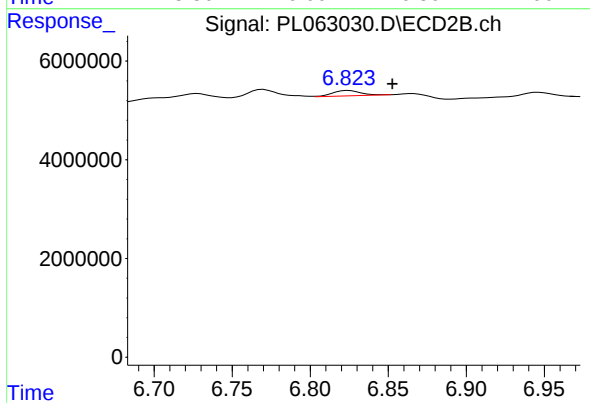

#15 Endosulfan II


R.T.: 6.825 min
Delta R.T.: -0.028 min
Response: 1368361
Conc: 0.48 ng/ml

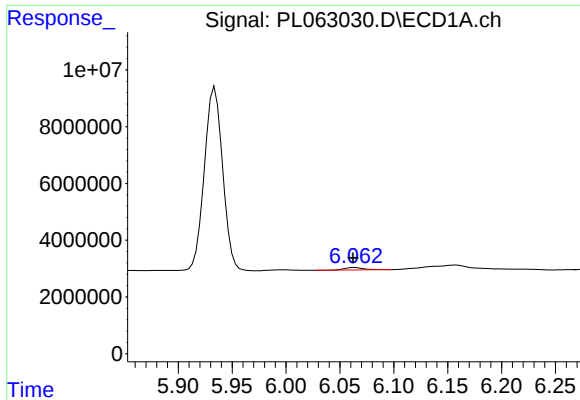

#16 4,4'-DDD


R.T.: 6.064 min
Delta R.T.: 0.002 min
Response: 1018651
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

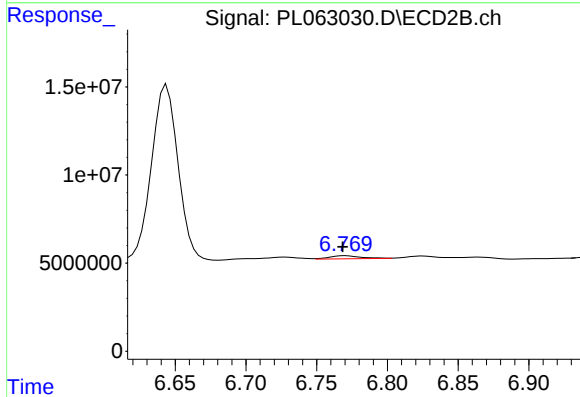


#16 4,4'-DDD

R.T.: 6.770 min
Delta R.T.: 0.002 min
Response: 2635419
Conc: 1.03 ng/ml

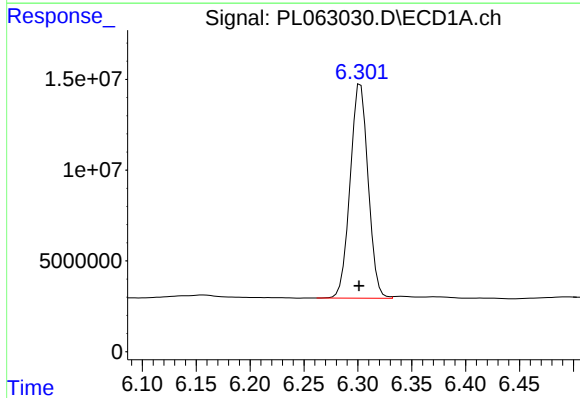


#17 4,4'-DDT

R.T.: 6.303 min
Delta R.T.: 0.001 min
Response: 137164633
Conc: 102.78 ng/ml

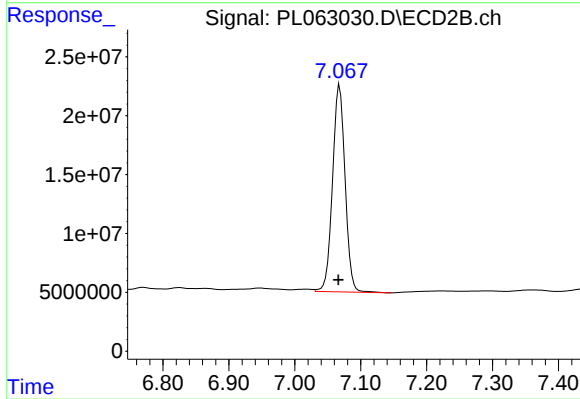

#17 4,4'-DDT


R.T.: 7.068 min
Delta R.T.: 0.002 min
Response: 232634322
Conc: 103.61 ng/ml

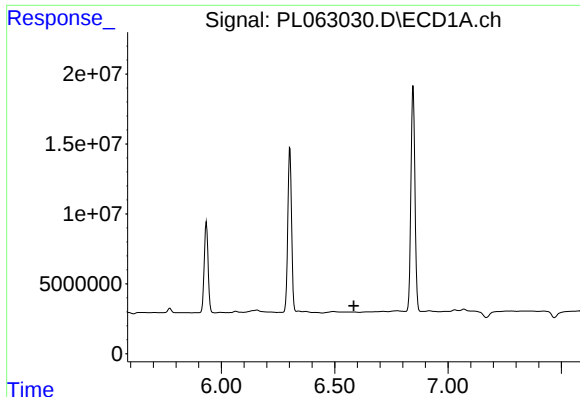

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

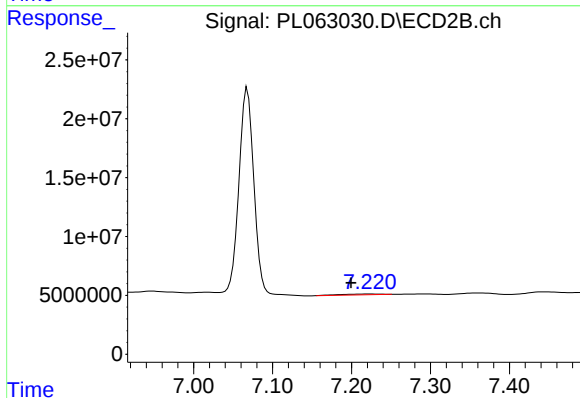


#19 Endosulfan Sulfate

R.T.: 7.222 min
Delta R.T.: 0.022 min
Response: 2548132
Conc: 1.06 ng/ml

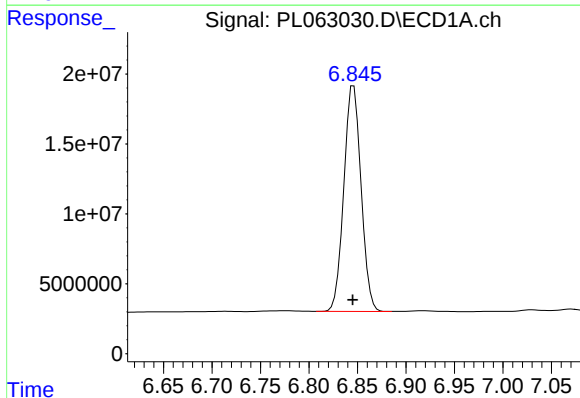


#20 Methoxychlor

R.T.: 6.846 min
Delta R.T.: 0.001 min
Response: 199392100
Conc: 231.50 ng/ml

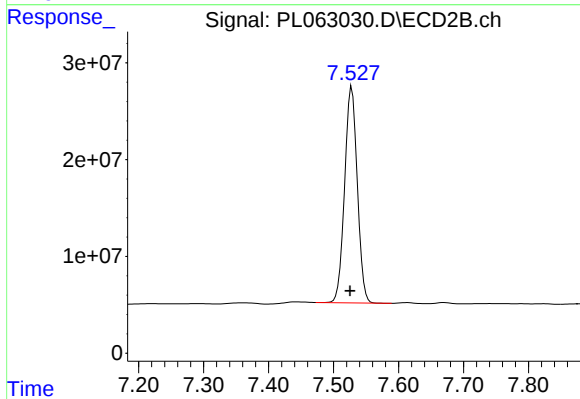

#20 Methoxychlor


R.T.: 7.528 min
Delta R.T.: 0.003 min
Response: 303472010
Conc: 245.63 ng/ml

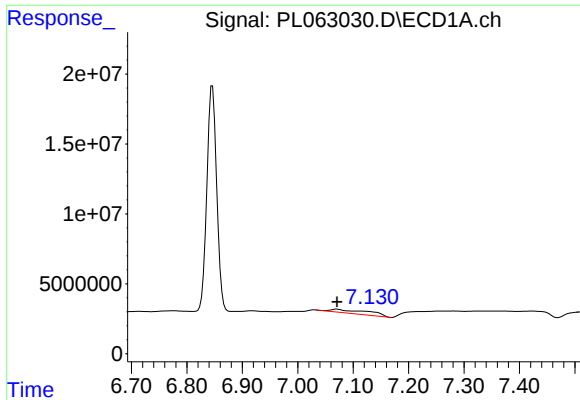

#21 Endrin ketone


R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 13271412
Conc: 7.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

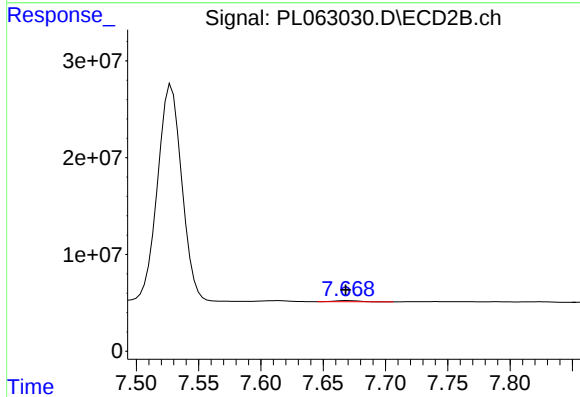


#21 Endrin ketone

R.T.: 7.669 min
Delta R.T.: 0.001 min
Response: 1642331
Conc: 0.69 ng/ml

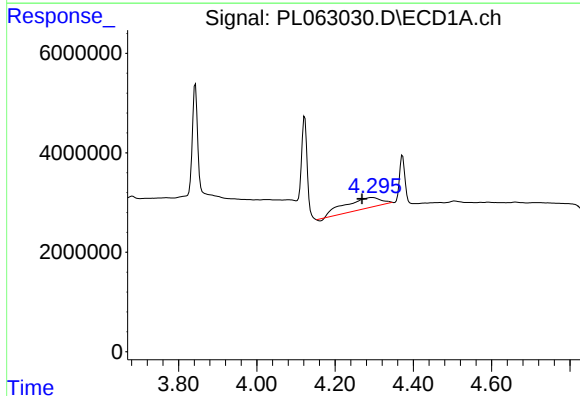


#23 Chlordane-1

R.T.: 4.296 min
Delta R.T.: 0.027 min
Response: 14619886
Conc: 283.61 ng/ml

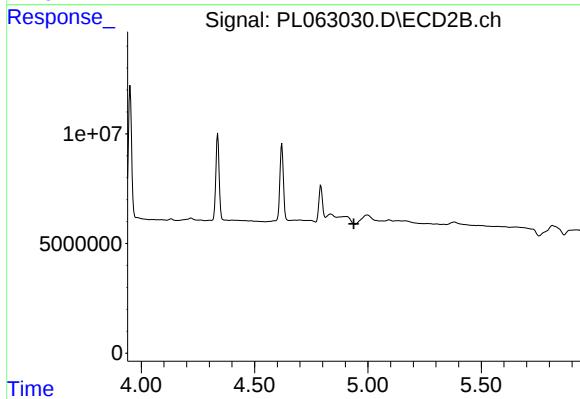

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

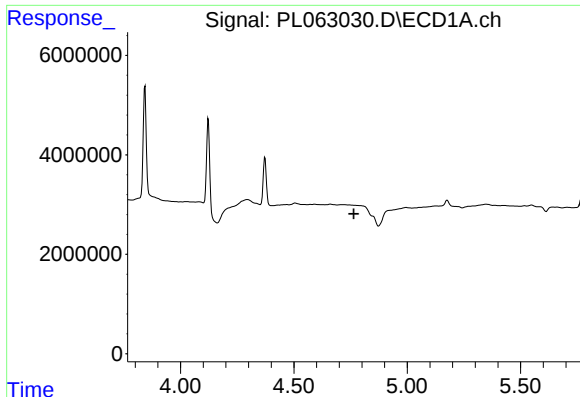

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

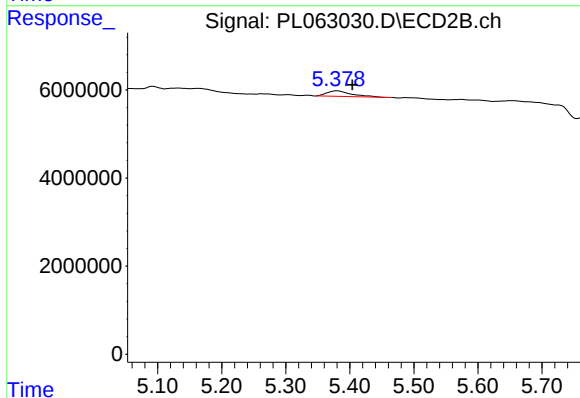


#24 Chlordane-2

R.T.: 5.380 min
Delta R.T.: -0.024 min
Response: 3310776
Conc: 30.36 ng/ml

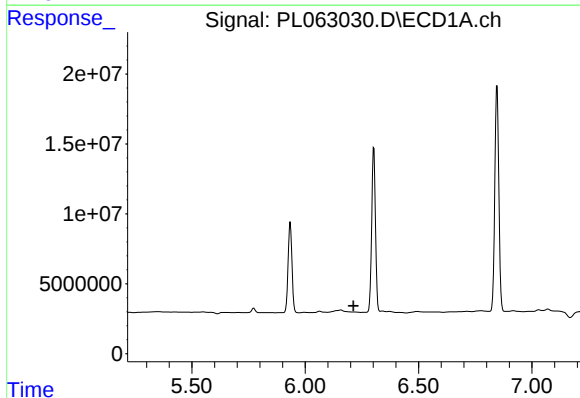


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.213 min
Response: 0
Conc: N.D.

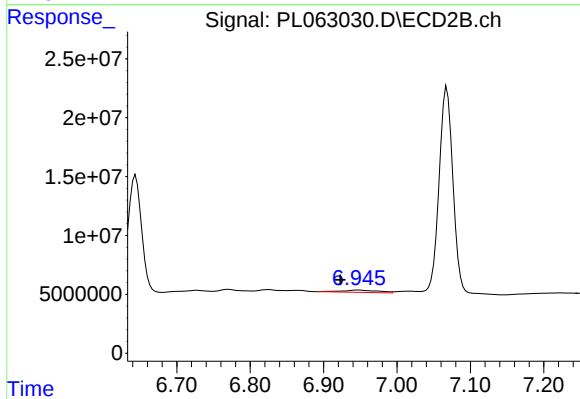

#27 Chlordane-5


R.T.: 6.946 min
Delta R.T.: 0.023 min
Response: 6728741
Conc: 90.20 ng/ml

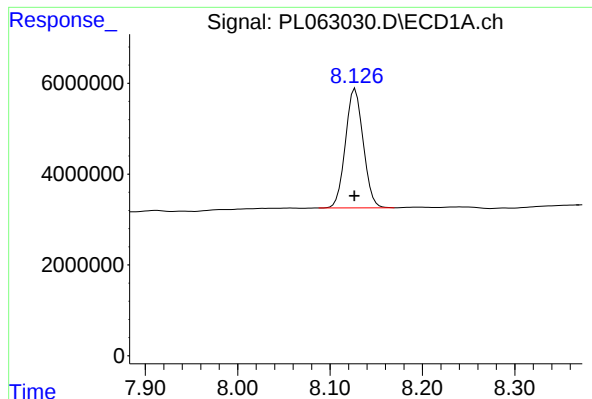

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 35054775
Conc: 21.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

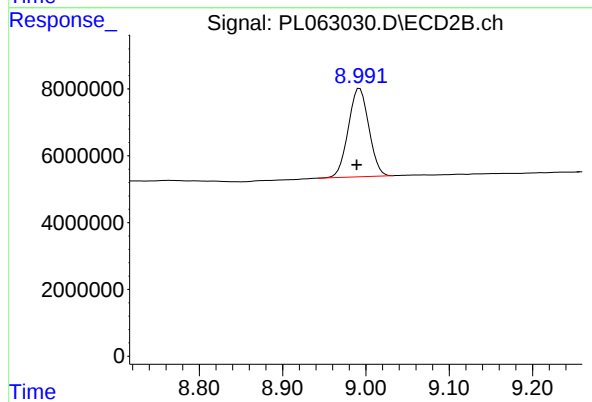

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.004 min
Response: 45208673
Conc: 21.60 ng/ml